

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 4:15
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 05:10:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.221	4.043	28655635	679.0E6	20.535	23.427
28) SA	Decachlor...	7.818	9.158	30510399	417.8E6	22.893	26.865
Target Compounds							
2) A	alpha-BHC	3.661f	0.000	331718	0	0.146	N.D. #
3) MA	gamma-BHC...	3.925f	0.000	1989325	0	0.910	N.D. #
8) B	Heptachlo...	4.870f	5.926	614381	139.3E6	0.323	4.316 #
9) A	Endosulfan I	0.000	6.282	0	21685860	N.D.	0.742 #
10) B	gamma-Chl...	0.000	6.168	0	120.1E6	N.D.	3.754 #
11) B	alpha-Chl...	0.000	6.242	0	16865023	N.D.	0.537 #
25)	Chlordane-3	0.000	6.168	0	120.1E6	N.D.	27.216 #
26)	Chlordane-4	0.000	6.242	0	16865023	N.D.	3.317 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 4:15
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 05:10:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

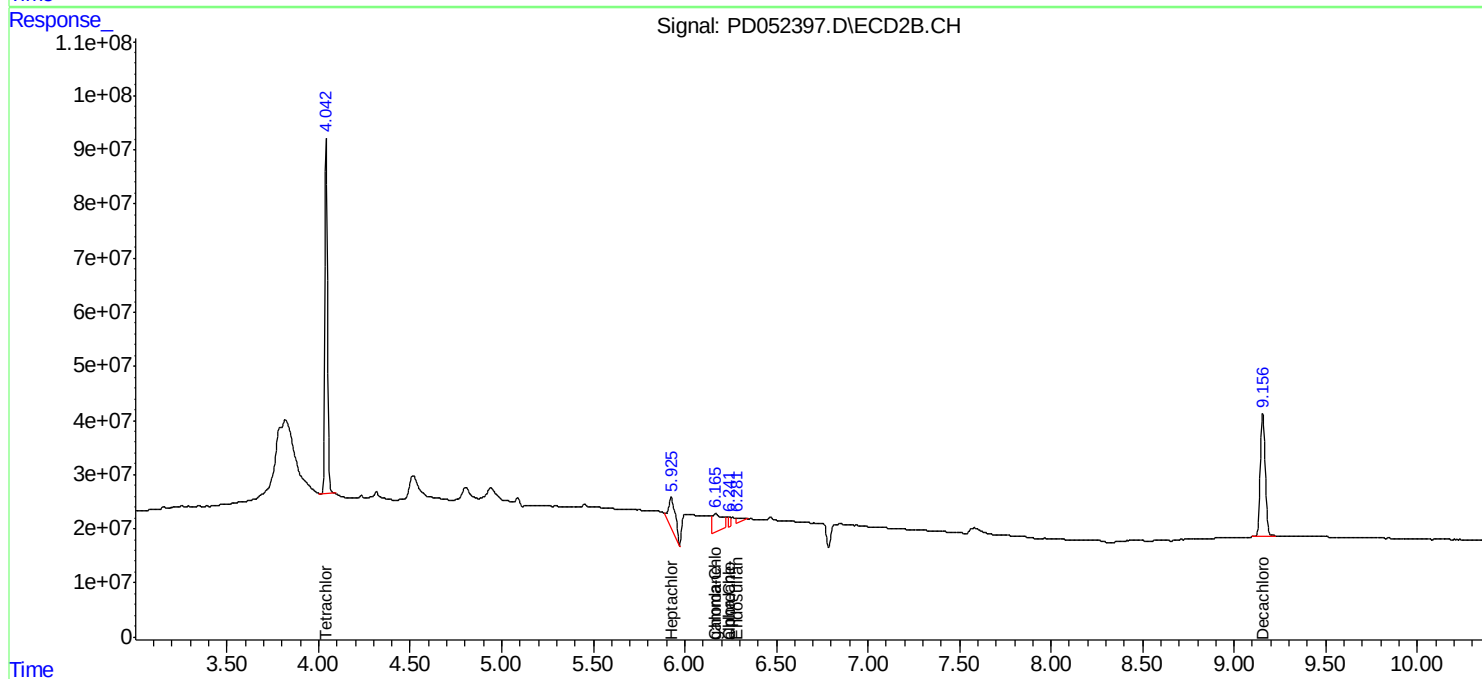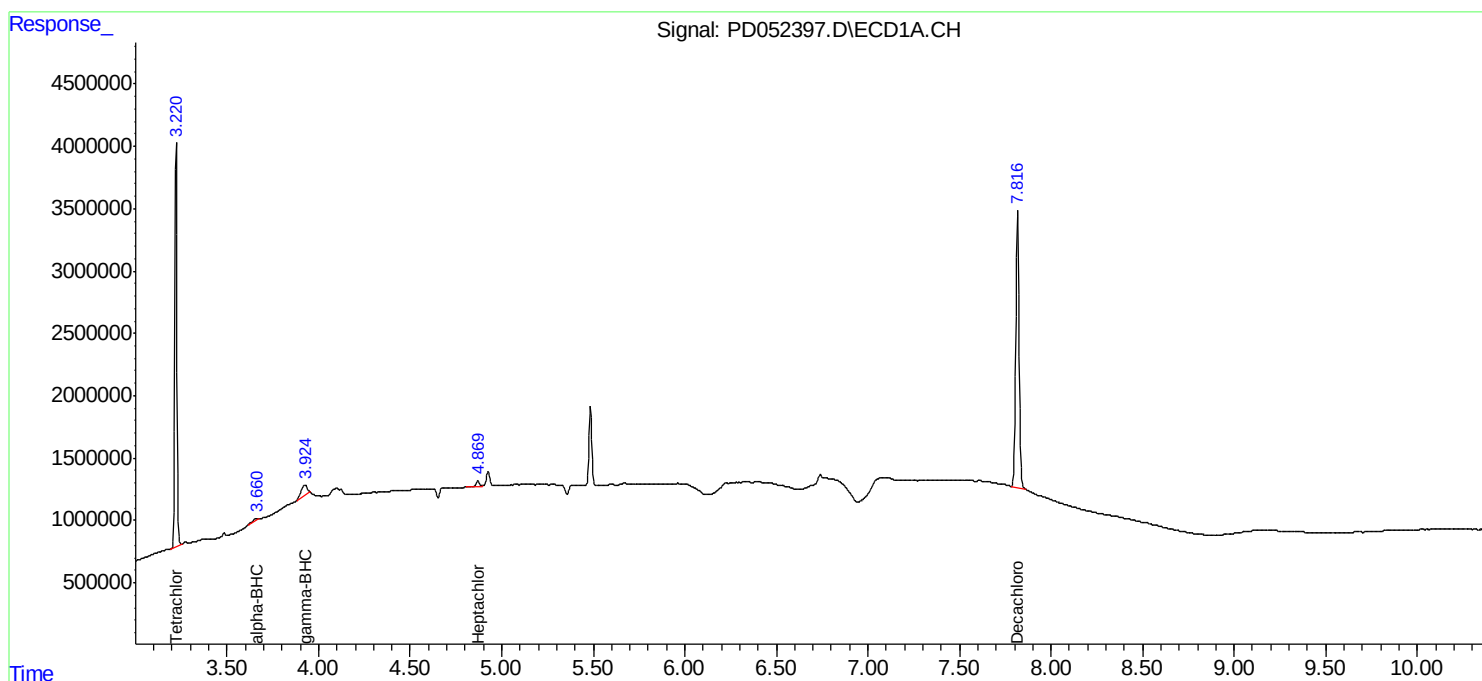


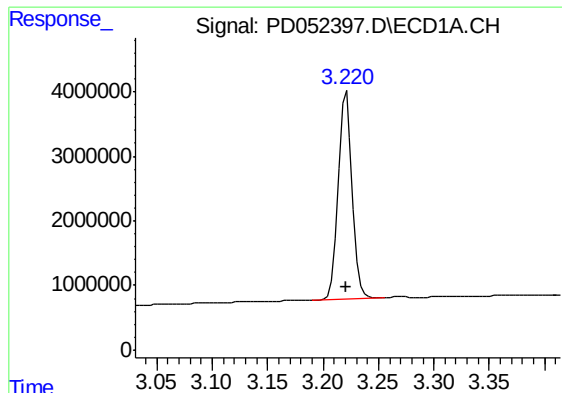

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28655635
Conc: 20.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

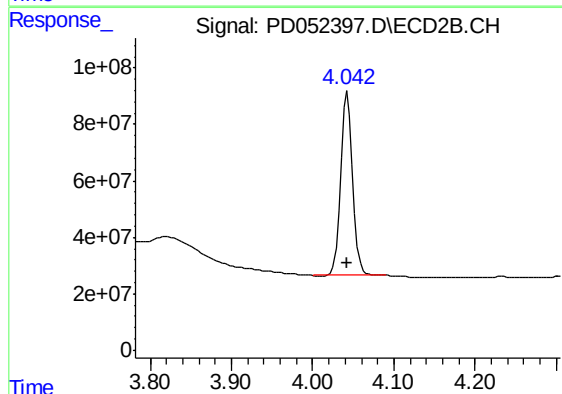


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 679004662
Conc: 23.43 ng/ml

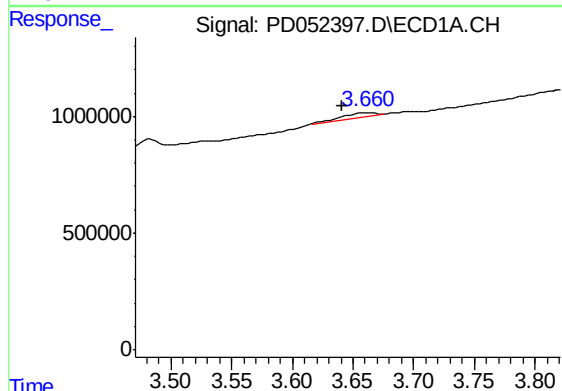


#2 alpha-BHC

R.T.: 3.661 min
Delta R.T.: 0.020 min
Response: 331718
Conc: 0.15 ng/ml

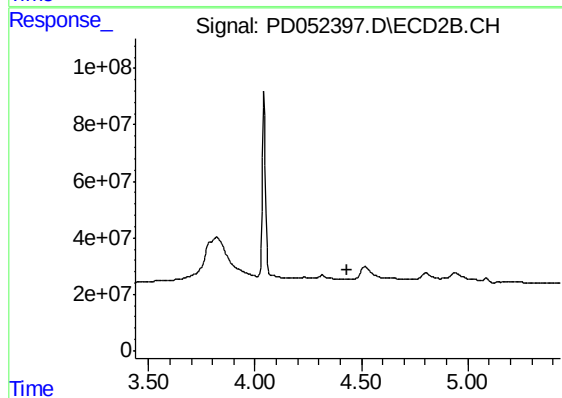

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

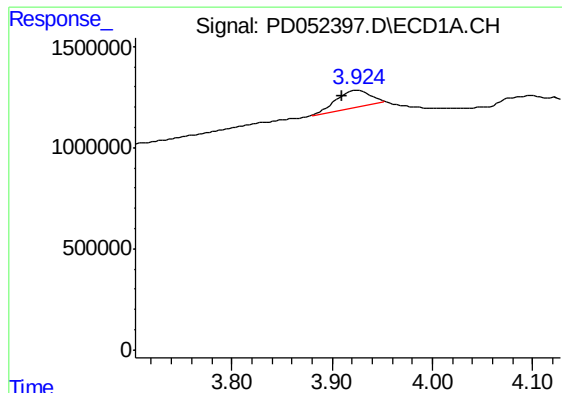

#3 gamma-BHC (Lindane)


R.T.: 3.925 min
Delta R.T.: 0.016 min
Response: 1989325
Conc: 0.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

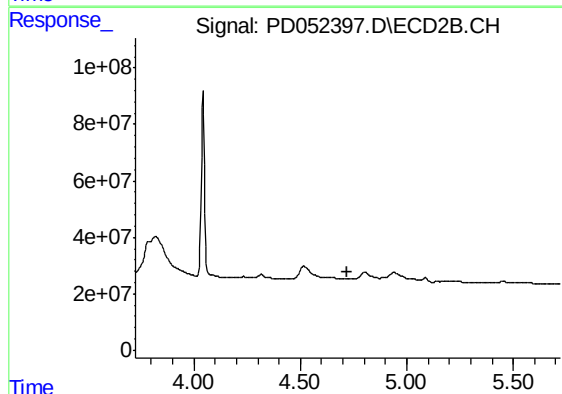


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

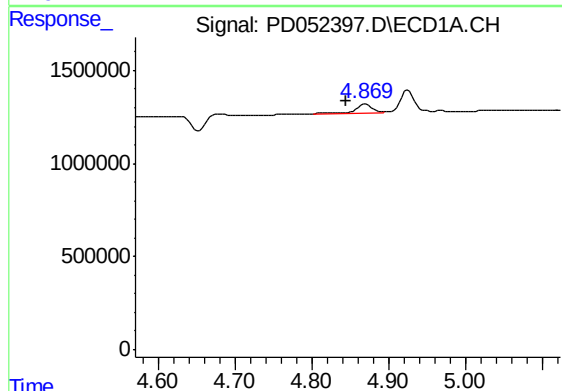


#8 Heptachlor epoxide

R.T.: 4.870 min
Delta R.T.: 0.024 min
Response: 614381
Conc: 0.32 ng/ml

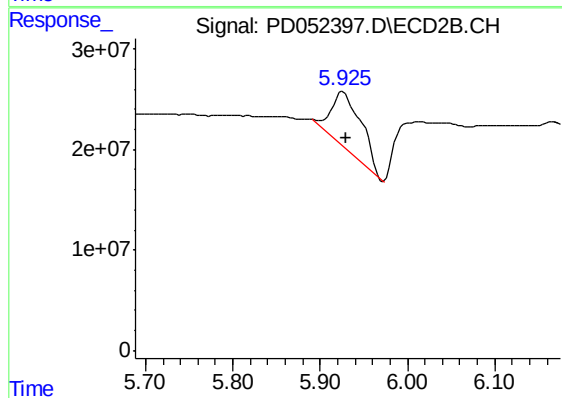

#8 Heptachlor epoxide


R.T.: 5.926 min
Delta R.T.: -0.004 min
Response: 139300460
Conc: 4.32 ng/ml

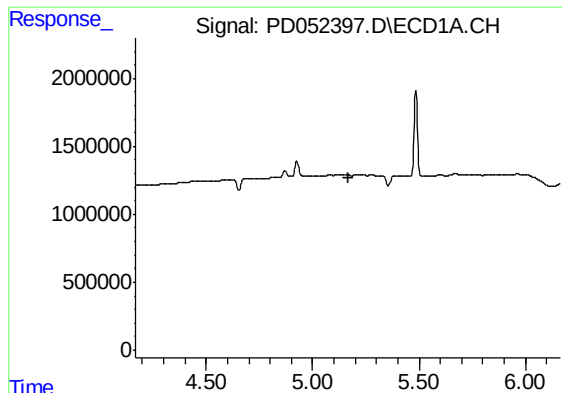

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

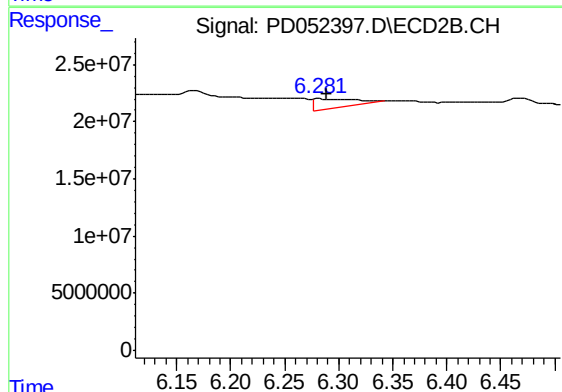


#9 Endosulfan I

R.T.: 6.282 min
Delta R.T.: -0.007 min
Response: 21685860
Conc: 0.74 ng/ml

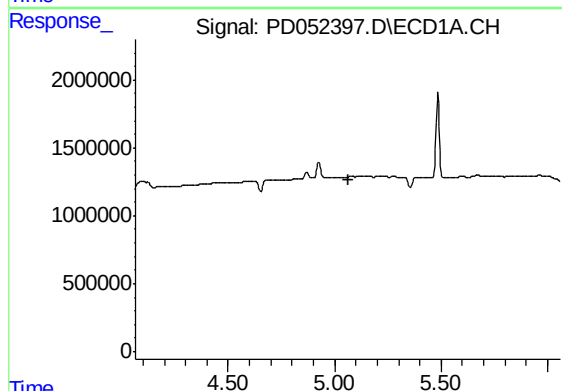


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

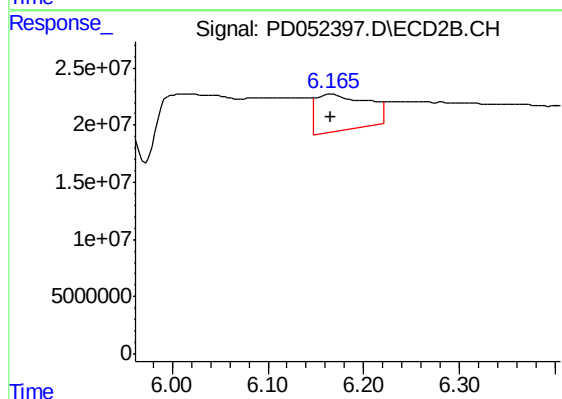

#10 gamma-Chlordane


R.T.: 6.168 min
Delta R.T.: 0.002 min
Response: 120099813
Conc: 3.75 ng/ml

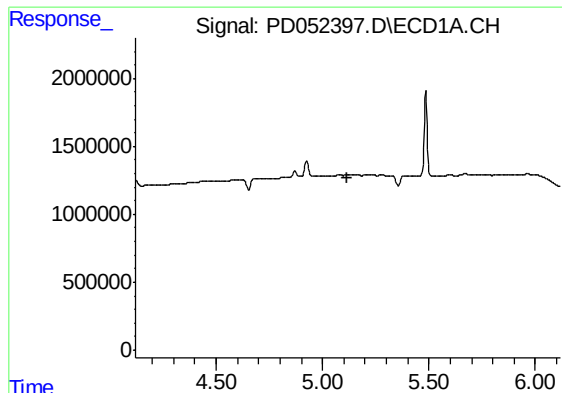

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

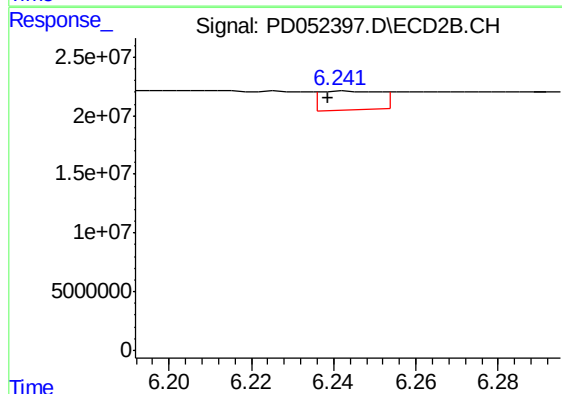


#11 alpha-Chlordane

R.T.: 6.242 min
Delta R.T.: 0.003 min
Response: 16865023
Conc: 0.54 ng/ml

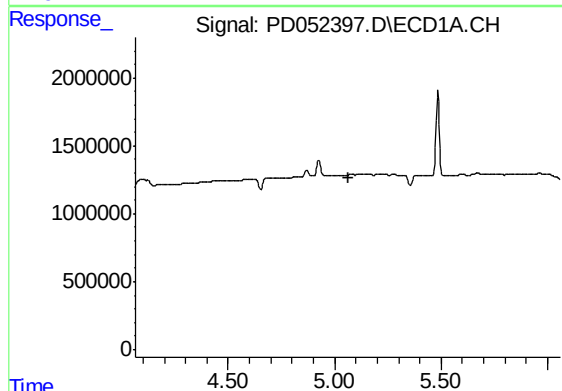


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

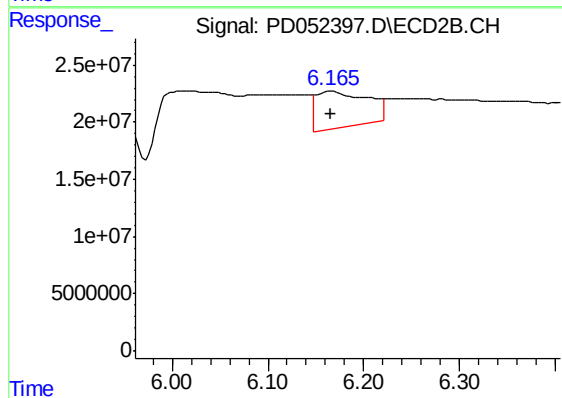

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: 0.002 min
Response: 120099813
Conc: 27.22 ng/ml

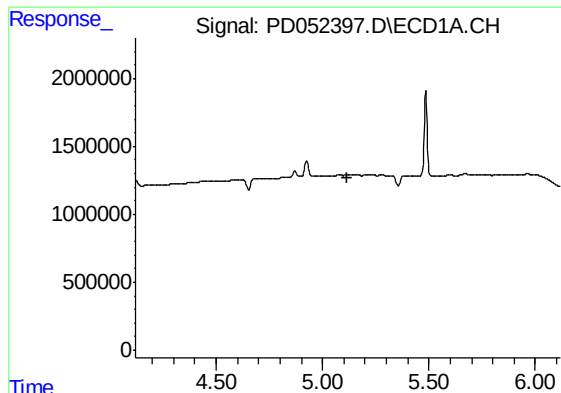

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

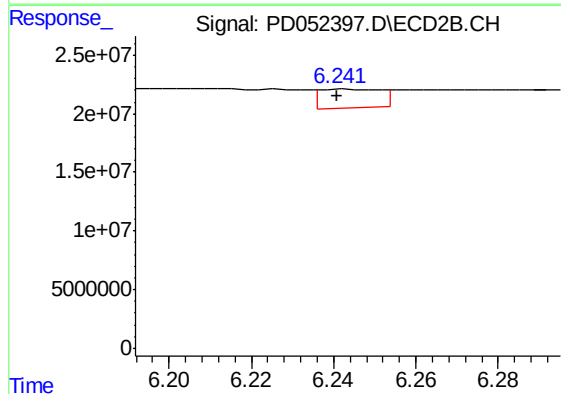


#26 Chlordane-4

R.T.: 6.242 min
Delta R.T.: 0.001 min
Response: 16865023
Conc: 3.32 ng/ml

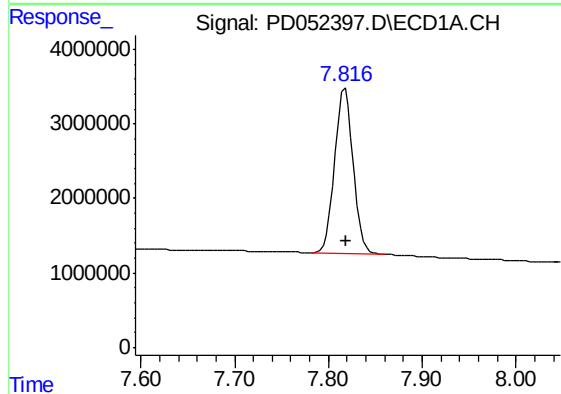

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 30510399
Conc: 22.89 ng/ml

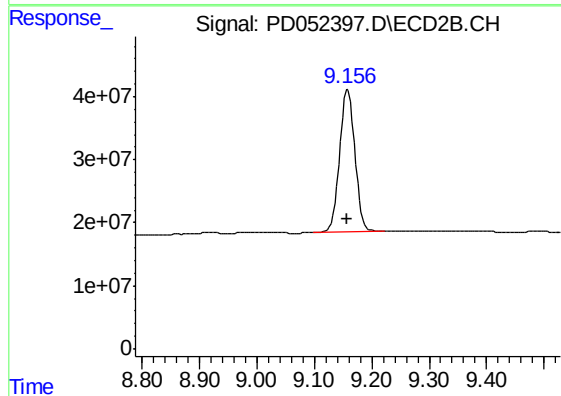

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.001 min
Response: 417794454
Conc: 26.87 ng/ml