

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052407.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 7:04
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 07:56:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	28195207	647.1E6	20.205	22.328
28)	SA Decachlor...	7.817	9.158	30130115	421.6E6	22.607	27.109
Target Compounds							
3)	MA gamma-BHC...	3.924	0.000	1848730	0	0.846	N.D. #
8)	B Heptachlo...	4.869f	5.926	657233	171.5E6	0.346	5.312 #
9)	A Endosulfan I	0.000	6.282	0	29883295	N.D.	1.023 #
10)	B gamma-Chl...	0.000	6.167	0	170.4E6	N.D.	5.326 #
11)	B alpha-Chl...	0.000	6.253	0	38064055	N.D.	1.213 #
17)	MA 4,4'-DDT	0.000	7.169f	0	1077788	N.D.	0.058 #
25)	Chlordane-3	0.000	6.167	0	170.4E6	N.D.	38.611 #
26)	Chlordane-4	0.000	6.253	0	38064055	N.D.	7.485 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052407.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 7:04
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 07:56:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

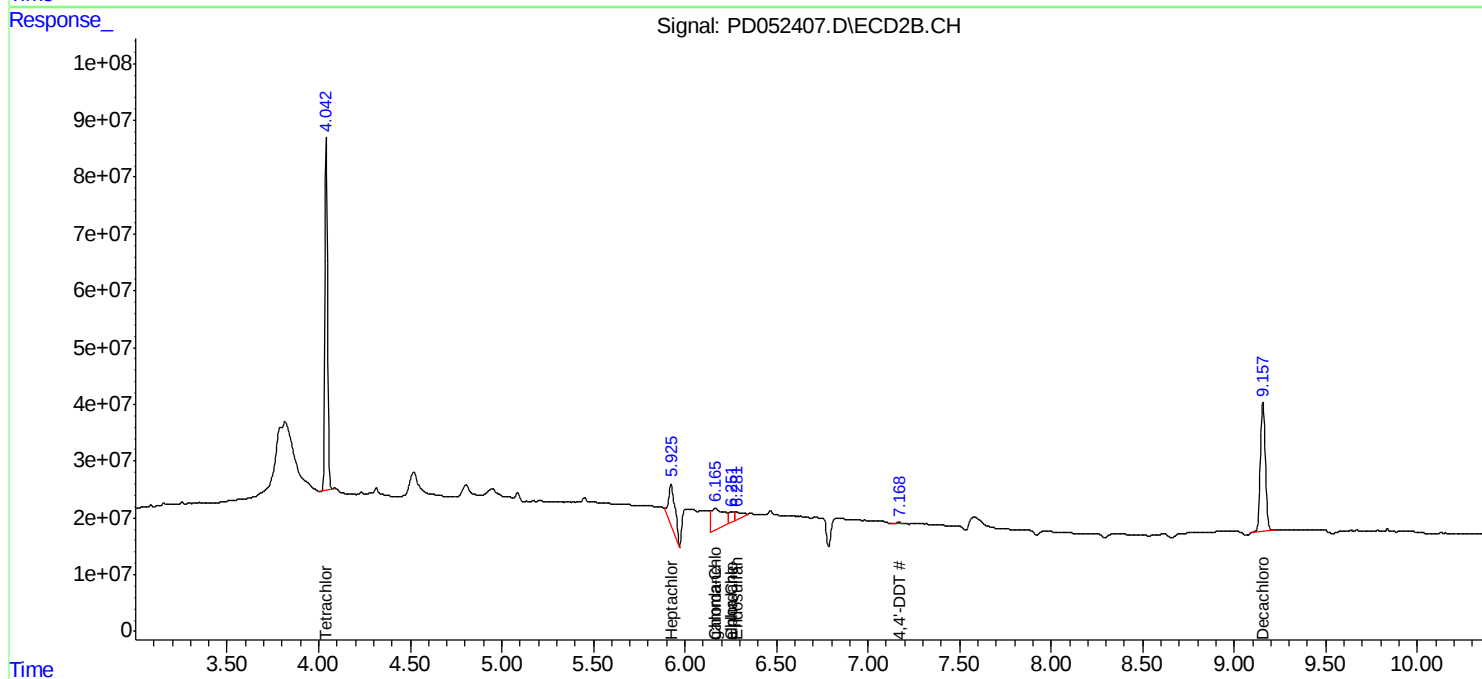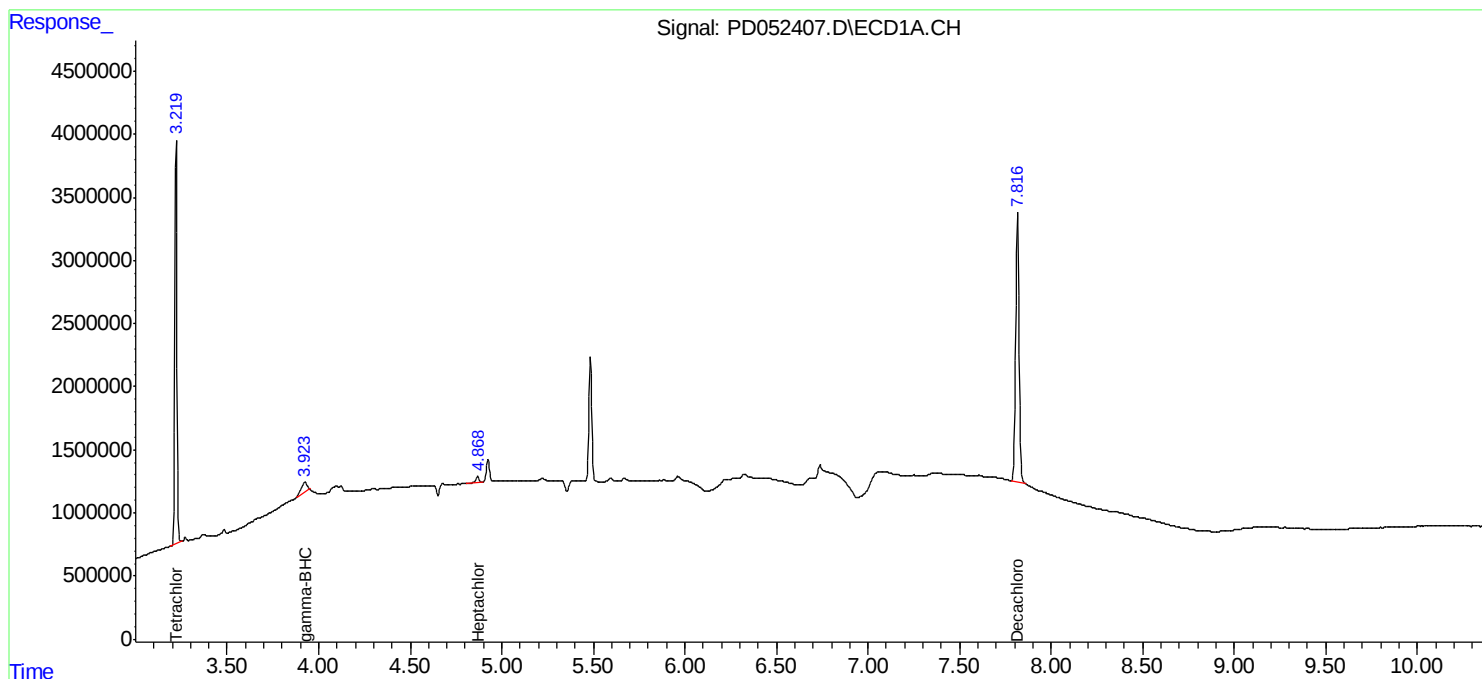


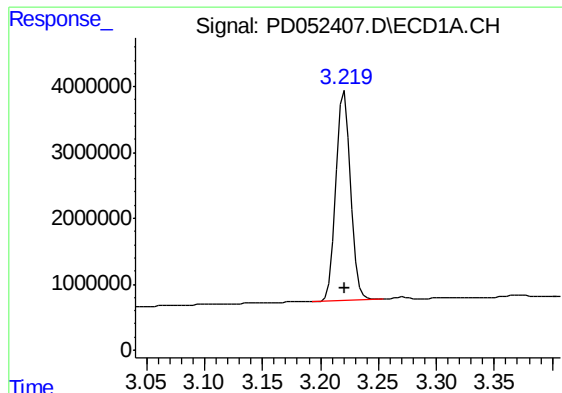

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28195207
Conc: 20.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

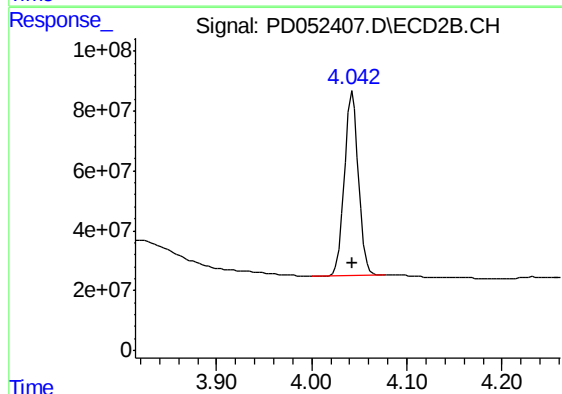


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 647145148
Conc: 22.33 ng/ml

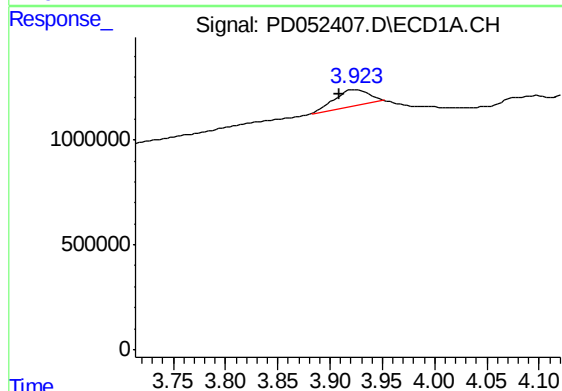


#3 gamma-BHC (Lindane)

R.T.: 3.924 min
Delta R.T.: 0.015 min
Response: 1848730
Conc: 0.85 ng/ml

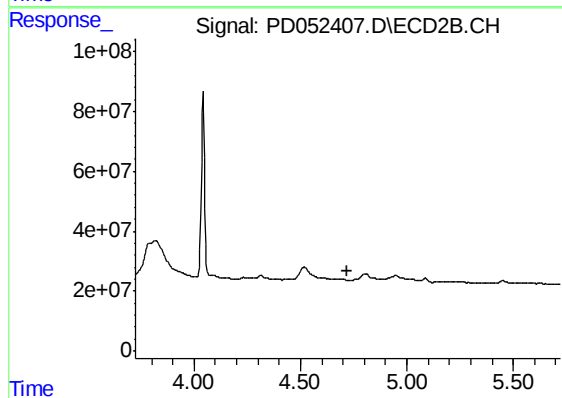

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

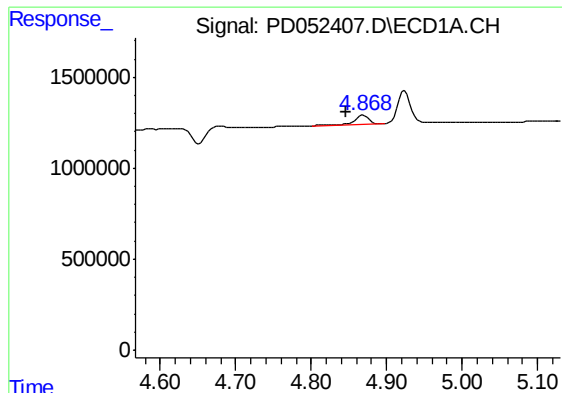

#8 Heptachlor epoxide


R.T.: 4.869 min
Delta R.T.: 0.023 min
Response: 657233
Conc: 0.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

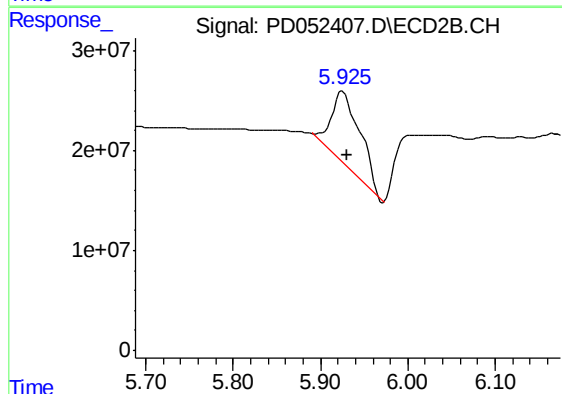


#8 Heptachlor epoxide

R.T.: 5.926 min
Delta R.T.: -0.005 min
Response: 171472139
Conc: 5.31 ng/ml

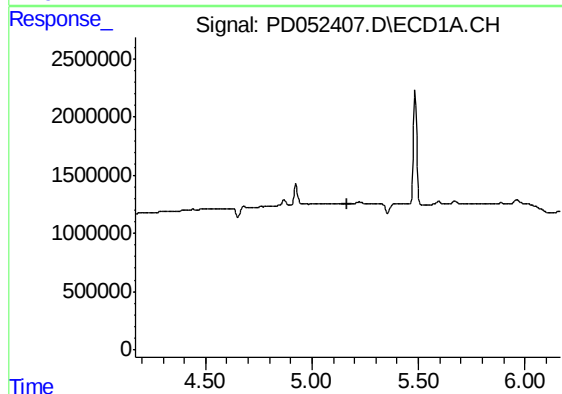


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

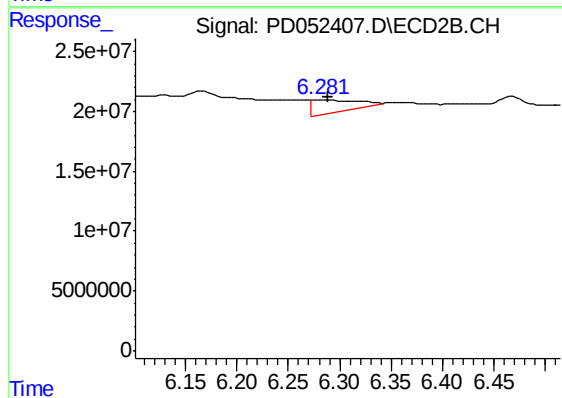

#9 Endosulfan I


R.T.: 6.282 min
Delta R.T.: -0.007 min
Response: 29883295
Conc: 1.02 ng/ml

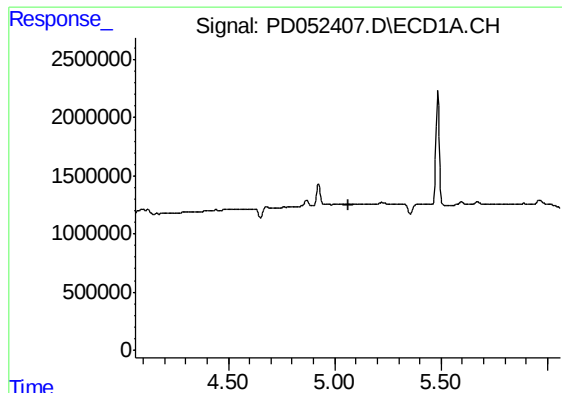

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

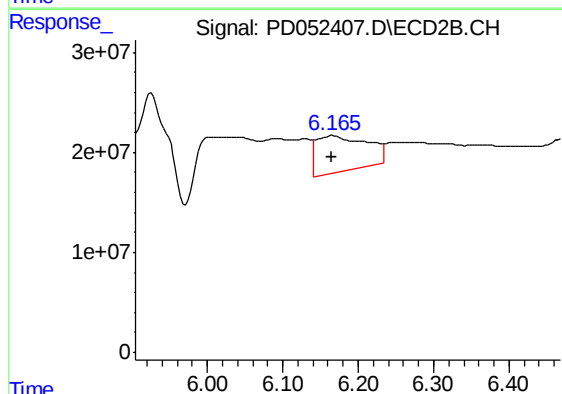


#10 gamma-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.001 min
Response: 170383934
Conc: 5.33 ng/ml

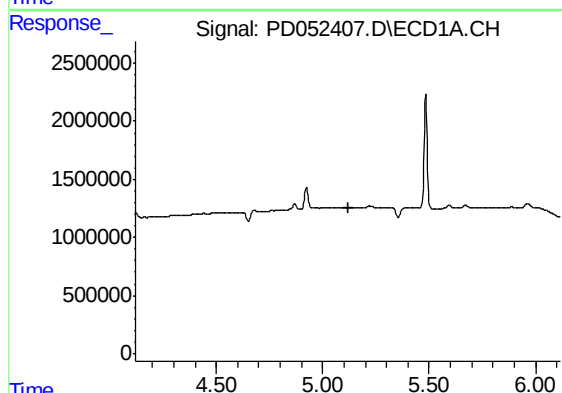


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

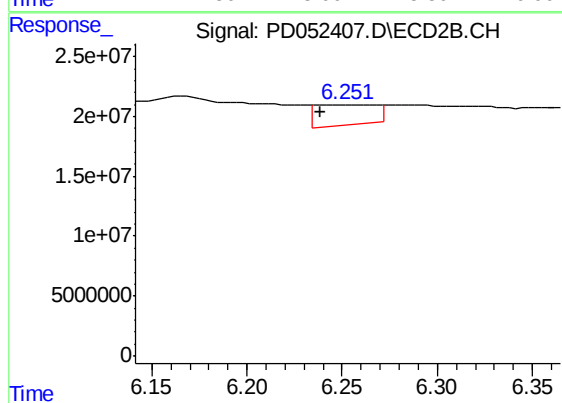

#11 alpha-Chlordane


R.T.: 6.253 min
Delta R.T.: 0.015 min
Response: 38064055
Conc: 1.21 ng/ml

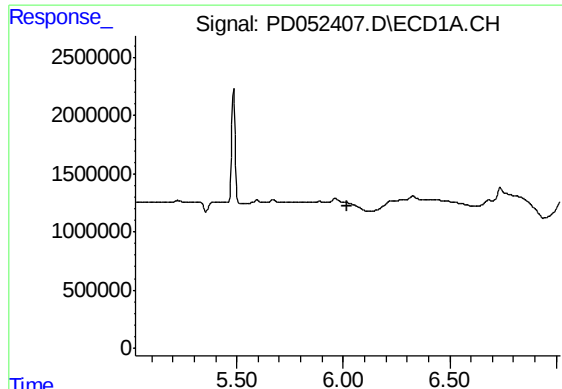

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

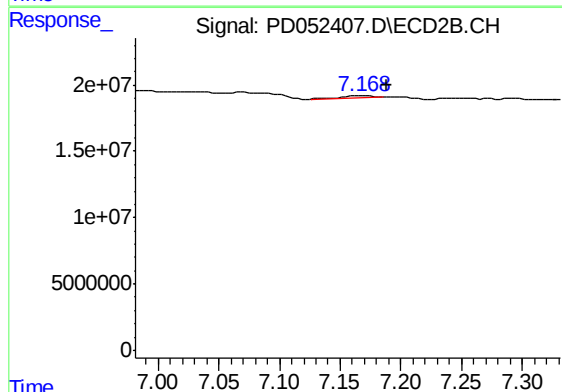


#17 4,4'-DDT

R.T.: 7.169 min
Delta R.T.: -0.019 min
Response: 1077788
Conc: 0.06 ng/ml

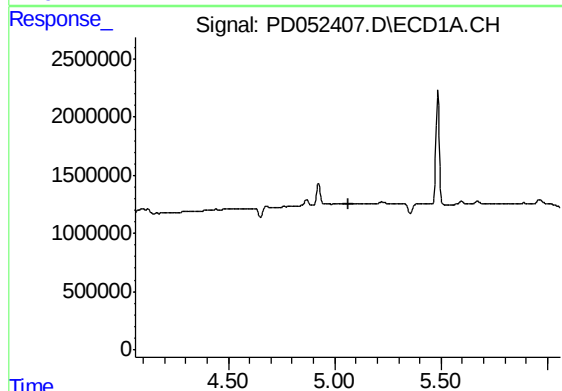


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.064 min
Response: 0
Conc: N.D.

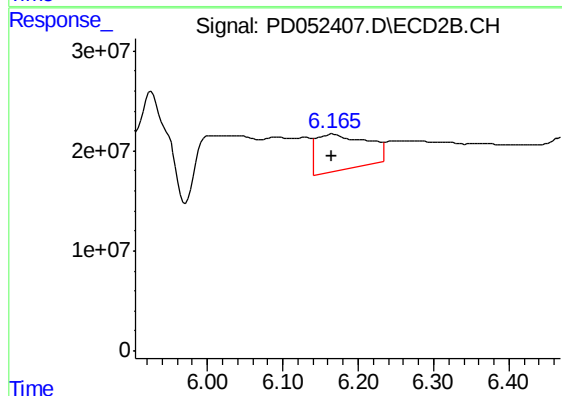

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 170383934
Conc: 38.61 ng/ml

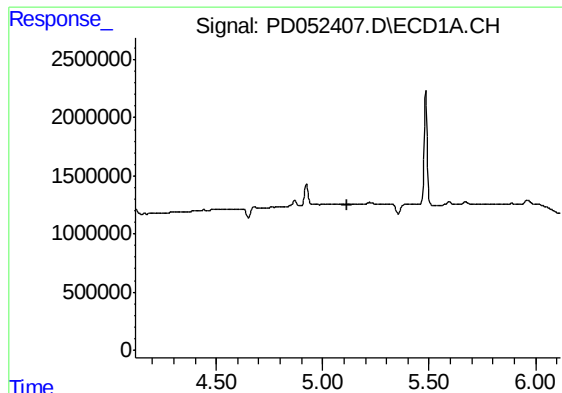

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

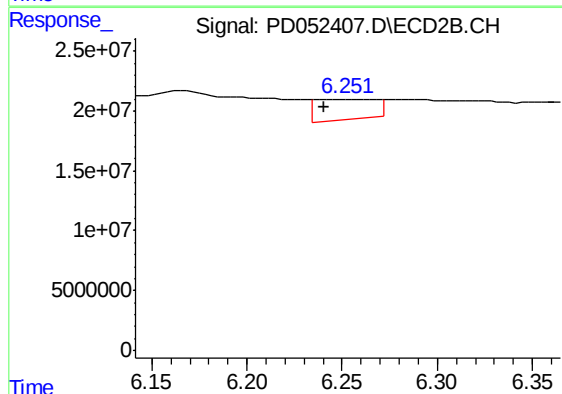


#26 Chlordane-4

R.T.: 6.253 min
Delta R.T.: 0.013 min
Response: 38064055
Conc: 7.49 ng/ml

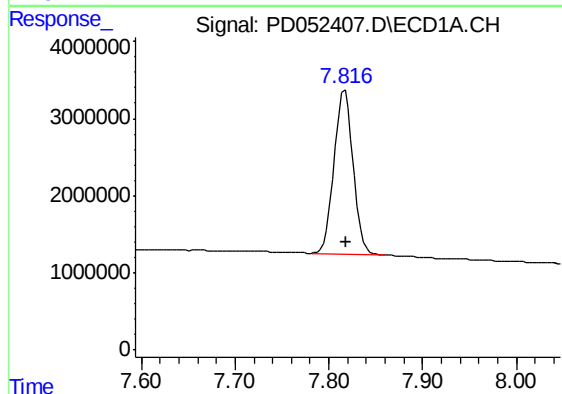

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.001 min
Response: 30130115
Conc: 22.61 ng/ml

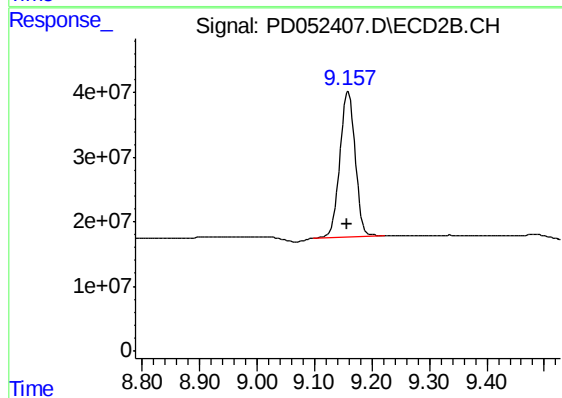

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.002 min
Response: 421588680
Conc: 27.11 ng/ml