

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052360.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 23:04
 Operator : AJ\SJ
 Sample : MDL-CHL-S-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-CHL-S-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 04:38:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	29423695	672.9E6	21.086	23.218
28)	SA Decachlor...	7.820	9.161	30801818	362.4E6	23.111	23.303
Target Compounds							
23)	Chlordane-1	4.043	5.045	1805001	47008700	28.745	30.643
24)	Chlordane-2	4.523	5.517	2410925	47508063	32.398	33.923
25)	Chlordane-3	5.063	6.166	5539473	151.9E6	25.050	34.429 #
26)	Chlordane-4	5.119	6.241	5422145	179.9E6	25.565	35.375 #
27)	Chlordane-5	5.923	7.051	1229370	38386750	18.904	41.607 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052360.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 23:04
Operator : AJ\SJ
Sample : MDL-CHL-S-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 04:38:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

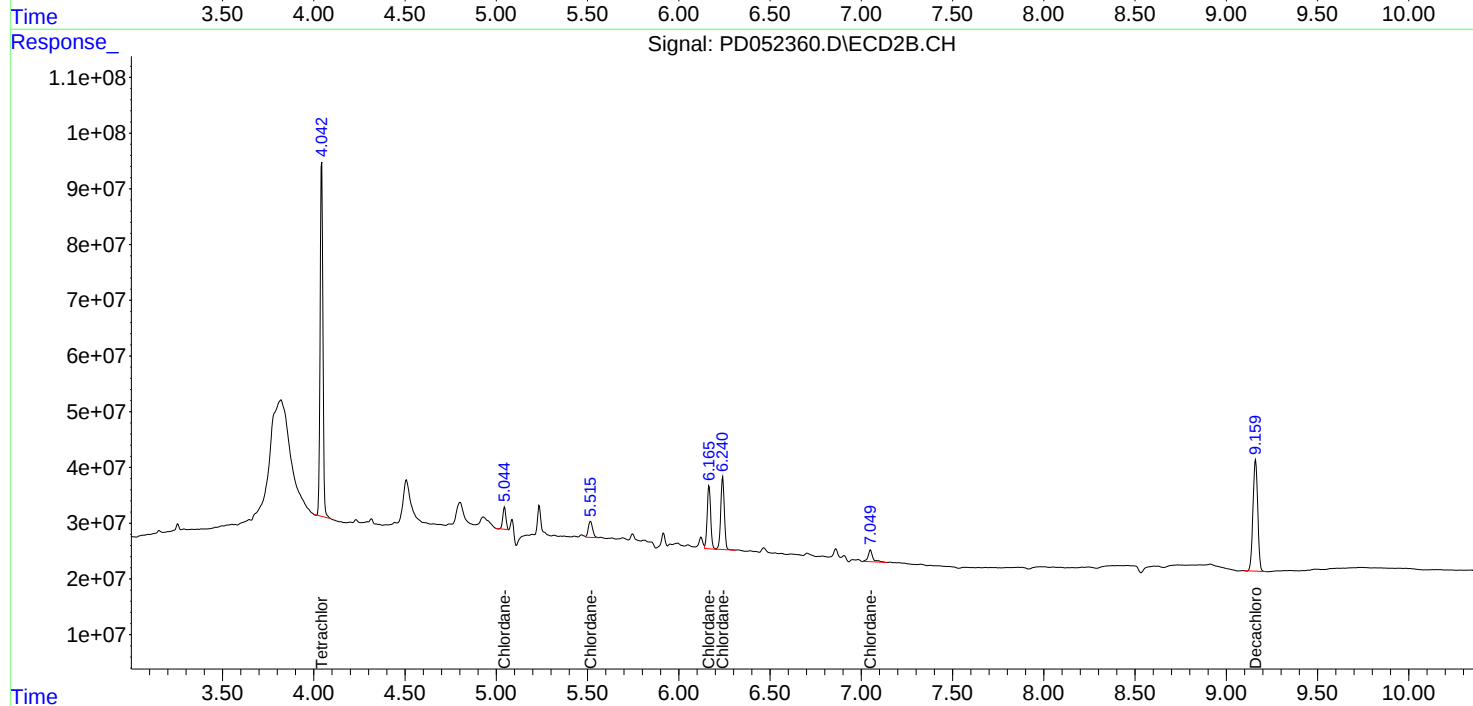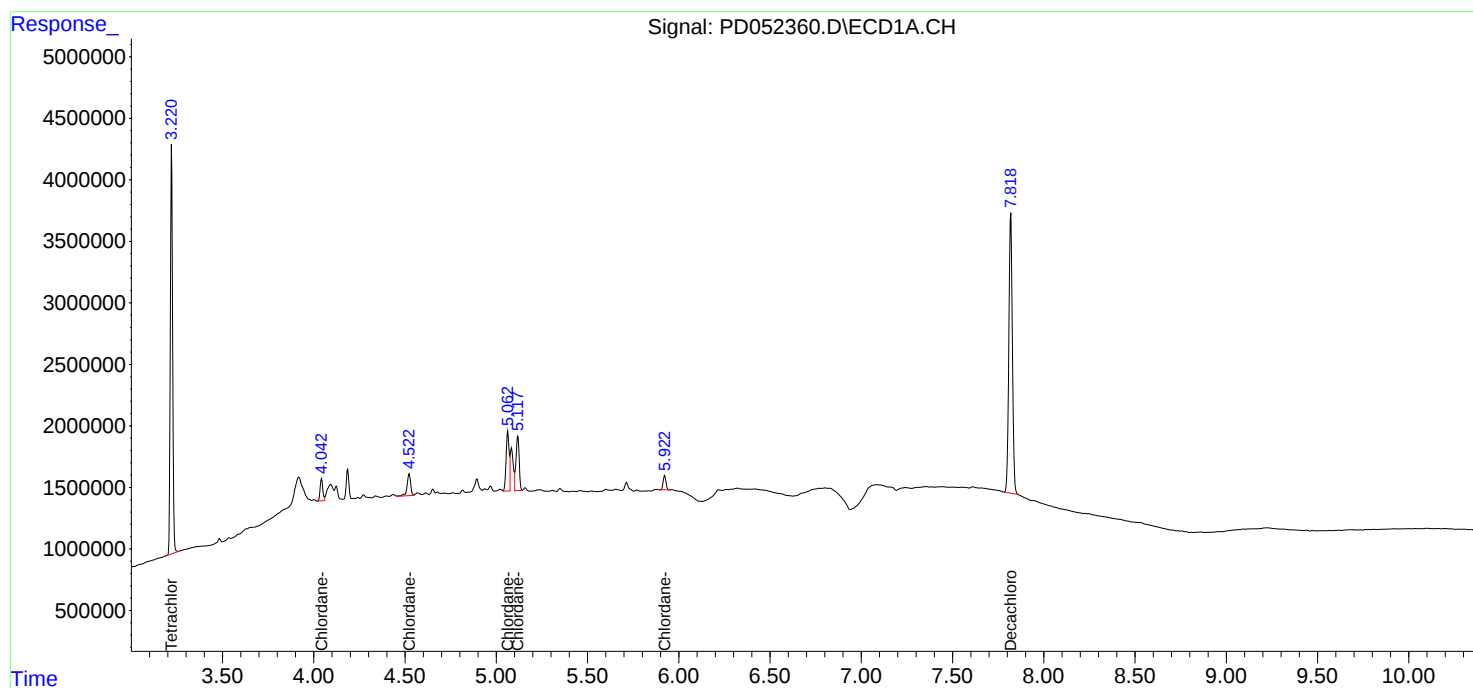


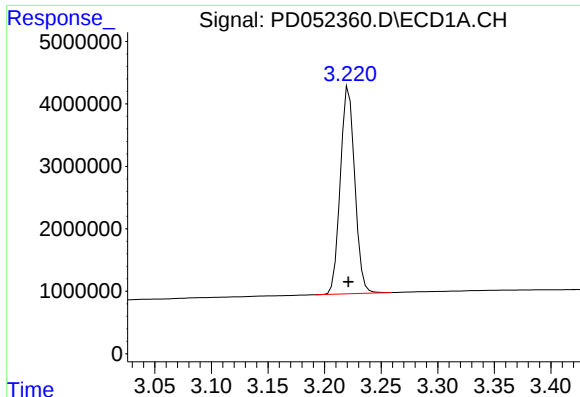

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 29423695
Conc: 21.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-04

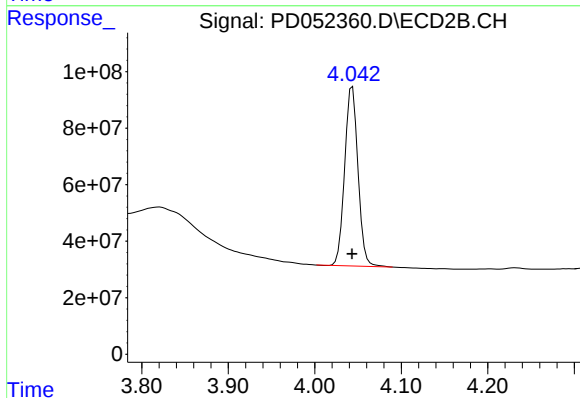


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 672945035
Conc: 23.22 ng/ml

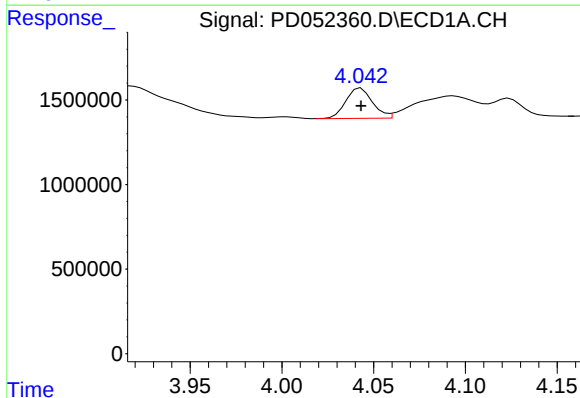


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1805001
Conc: 28.74 ng/ml

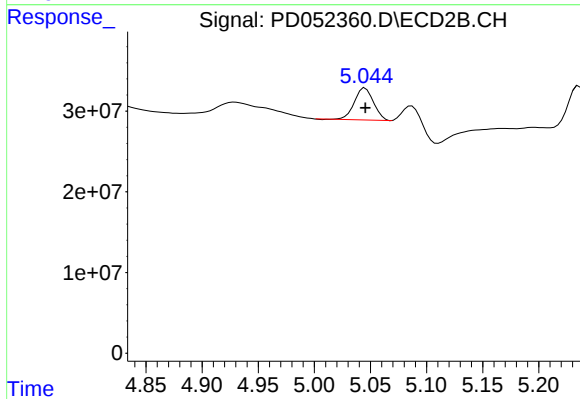

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 47008700
Conc: 30.64 ng/ml

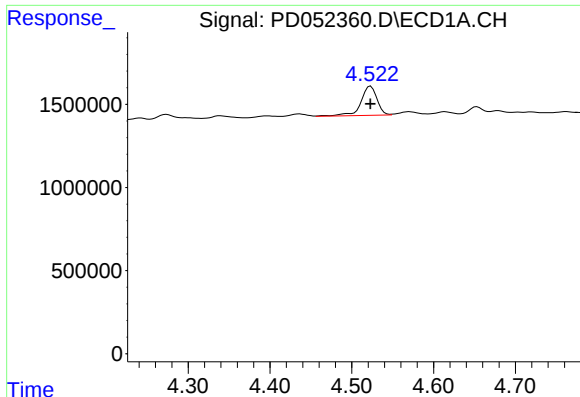

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 2410925
Conc: 32.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-04

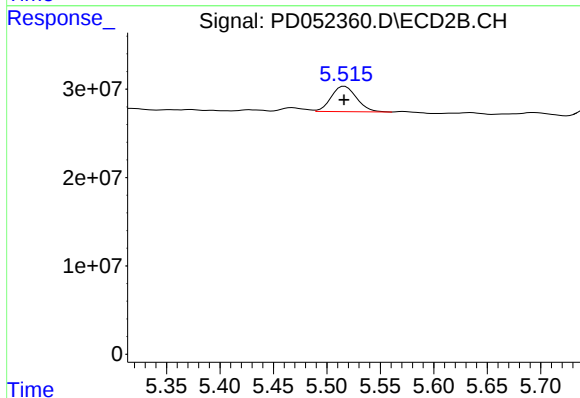


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 47508063
Conc: 33.92 ng/ml

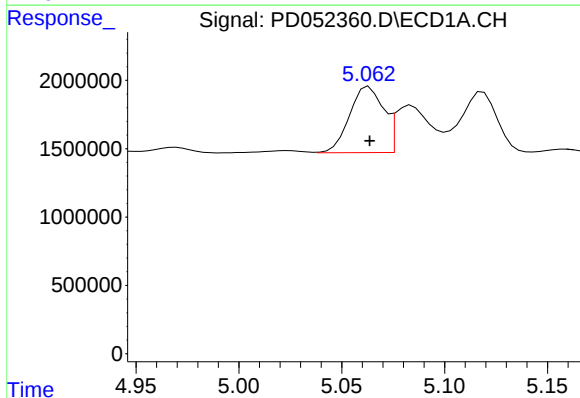


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 5539473
Conc: 25.05 ng/ml

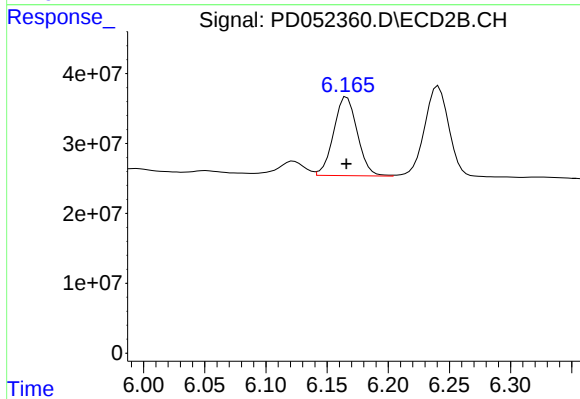

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 151927886
Conc: 34.43 ng/ml

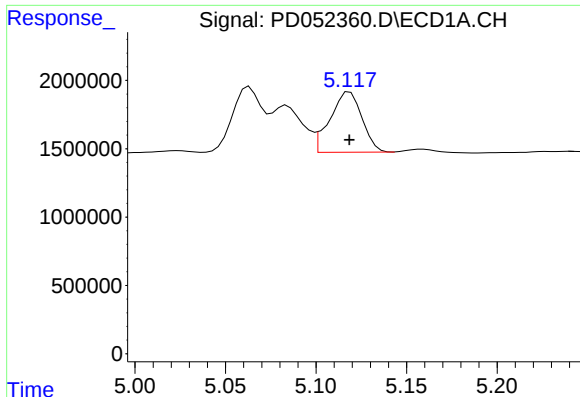

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 5422145
Conc: 25.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-04

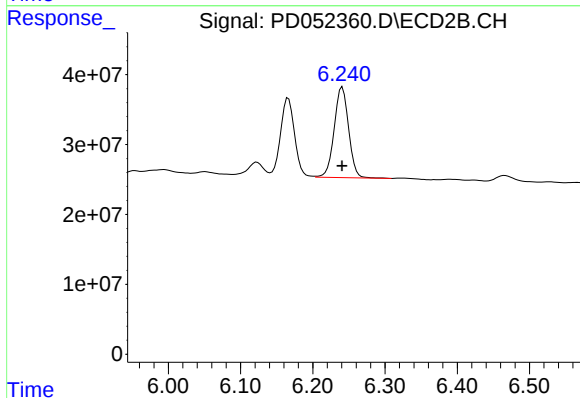


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 179884560
Conc: 35.37 ng/ml

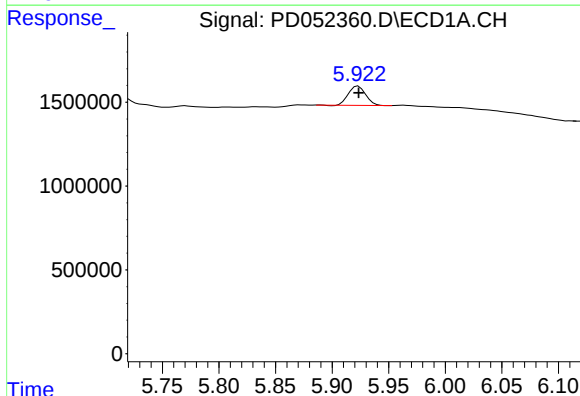


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1229370
Conc: 18.90 ng/ml

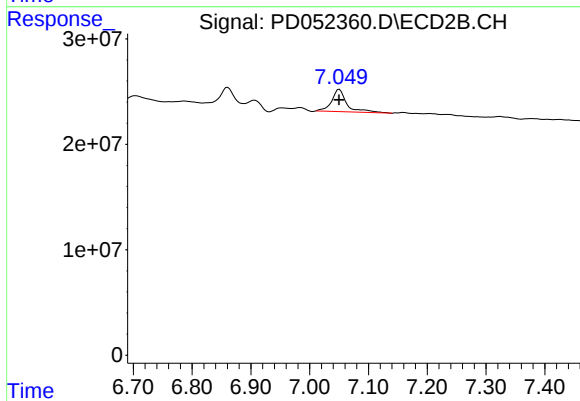

#27 Chlordane-5


R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 38386750
Conc: 41.61 ng/ml

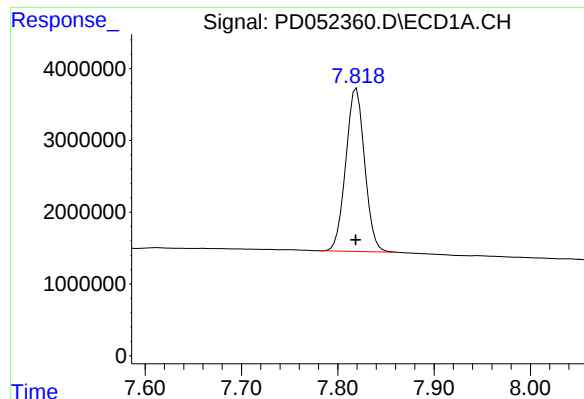

#28 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: 0.000 min
Response: 30801818
Conc: 23.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-04

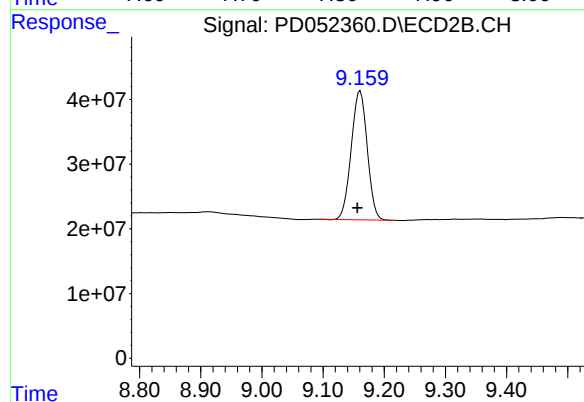

#28 Decachlorobiphenyl

R.T.: 9.161 min
Delta R.T.: 0.004 min
Response: 362396975
Conc: 23.30 ng/ml