

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052361.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 23:18
 Operator : AJ\SJ
 Sample : MDL-CHL-S-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-CHL-S-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:42:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	29081524	660.7E6	20.841	22.797
28)	SA Decachlor...	7.819	9.159	30573804	391.1E6	22.940	25.148
Target Compounds							
23)	Chlordane-1	4.043	5.045	1779781	45190291	28.343	29.457
24)	Chlordane-2	4.523	5.515	2154279	48163421	28.949	34.391
25)	Chlordane-3	5.063	6.166	5404669	150.1E6	24.440	34.022 #
26)	Chlordane-4	5.118	6.240	5374369	178.5E6	25.340	35.105 #
27)	Chlordane-5	5.923	7.050	1238469	27646689	19.044	29.966 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052361.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 23:18
Operator : AJ\SJ
Sample : MDL-CHL-S-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:42:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

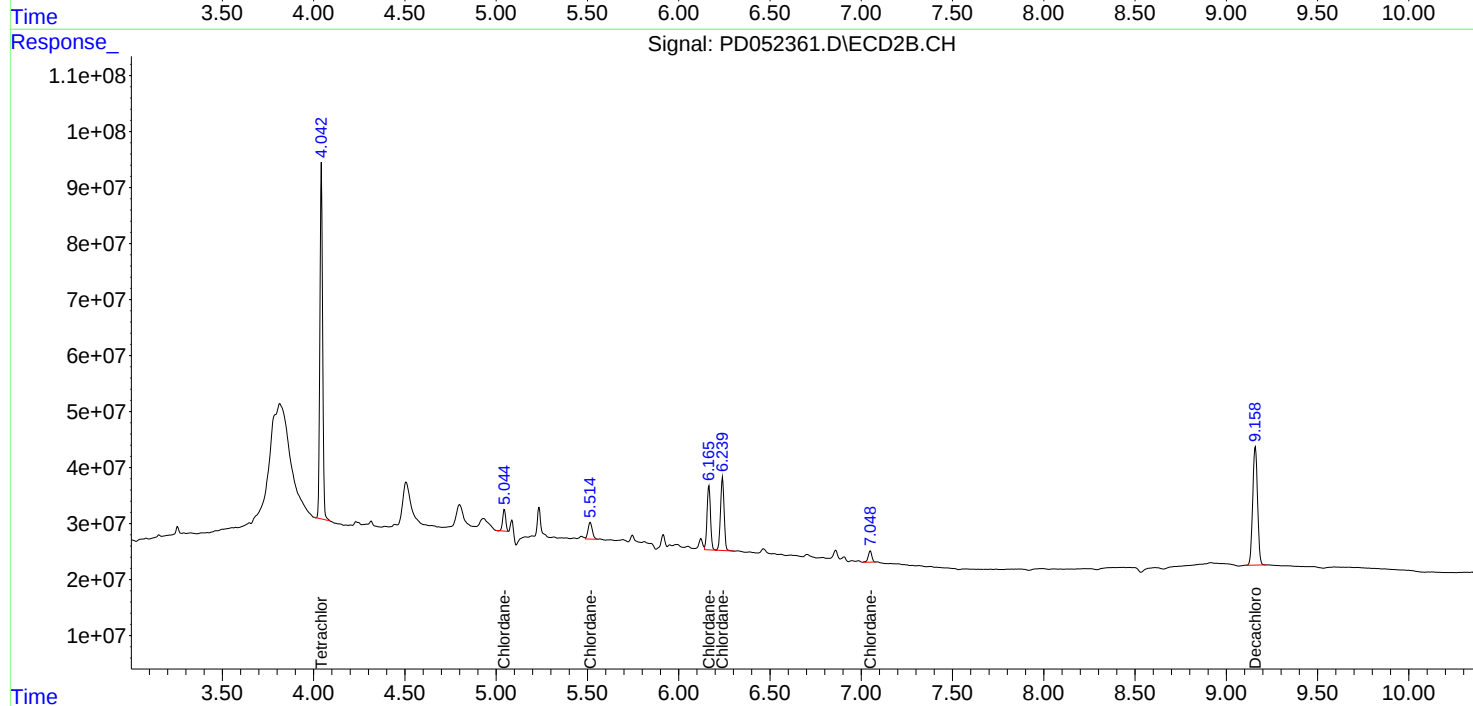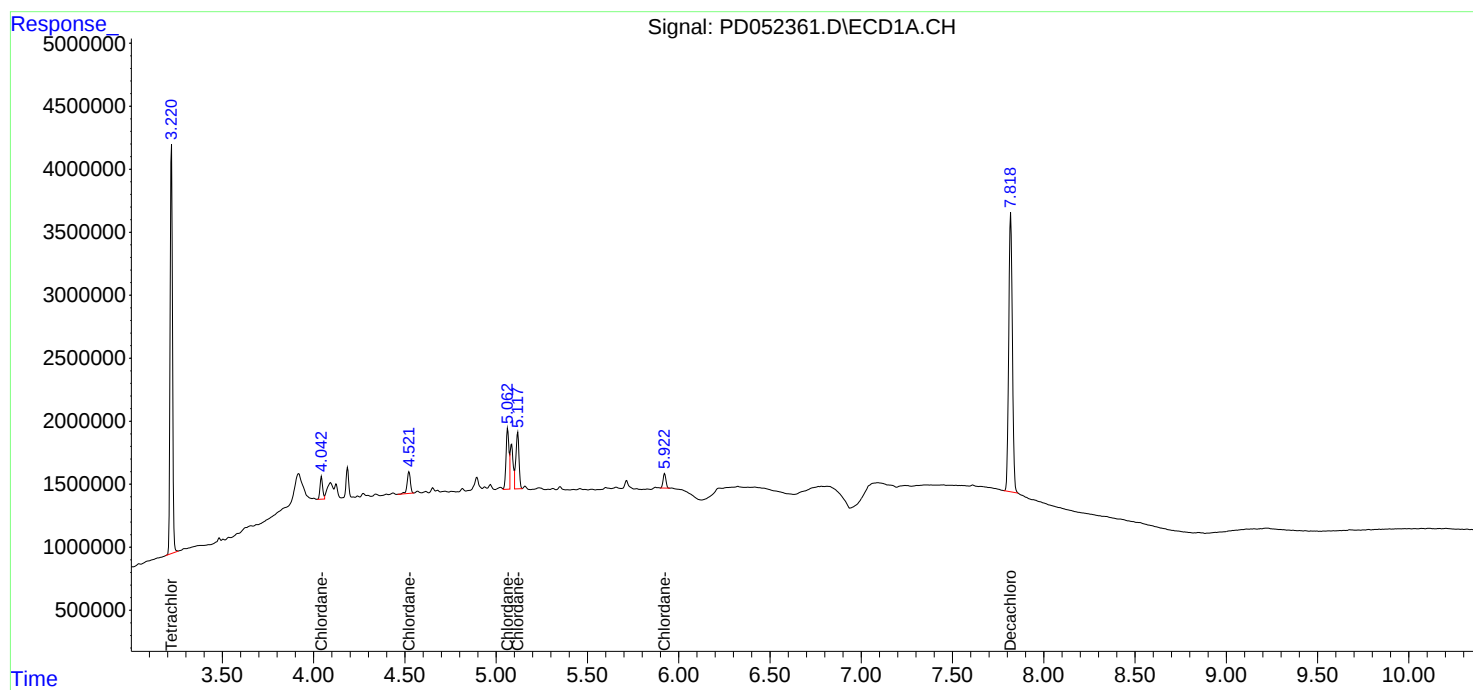


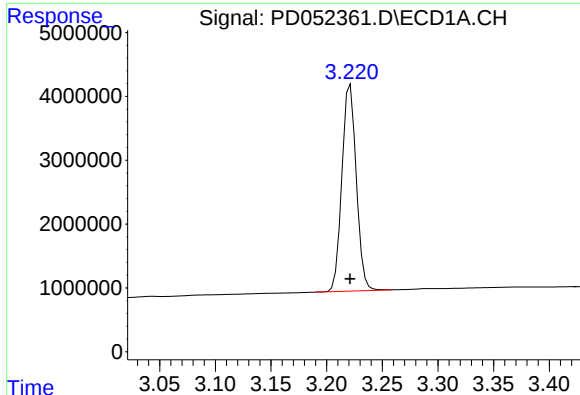

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 29081524
Conc: 20.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-05

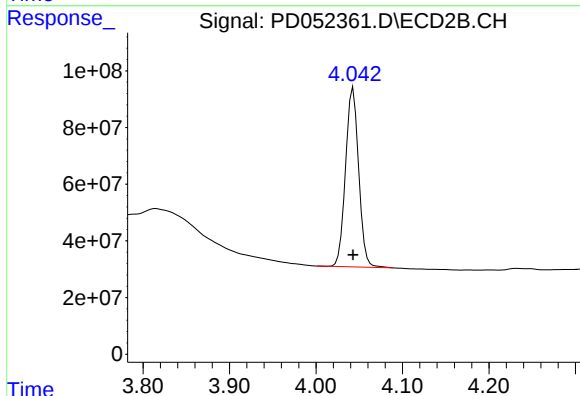


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 660740735
Conc: 22.80 ng/ml

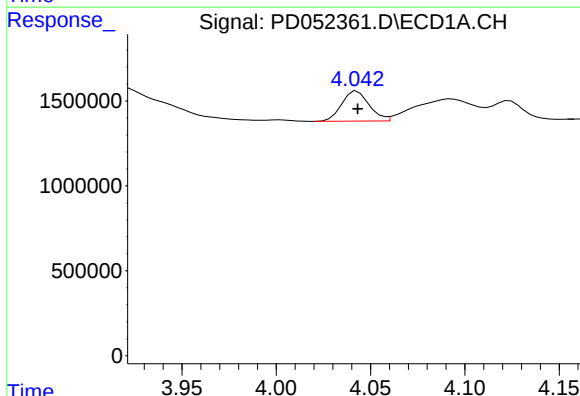


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1779781
Conc: 28.34 ng/ml

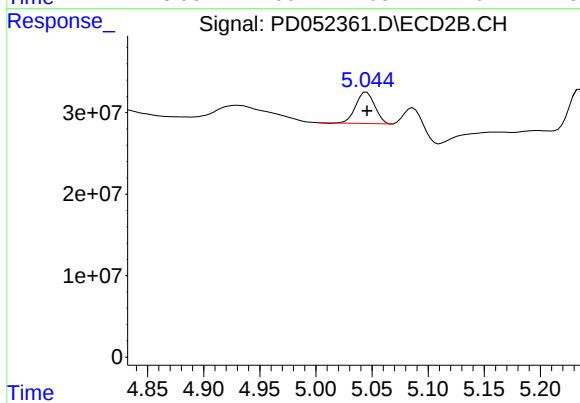

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 45190291
Conc: 29.46 ng/ml

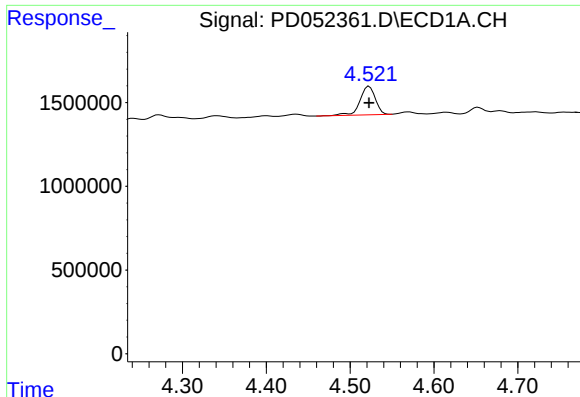

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 2154279
Conc: 28.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-05

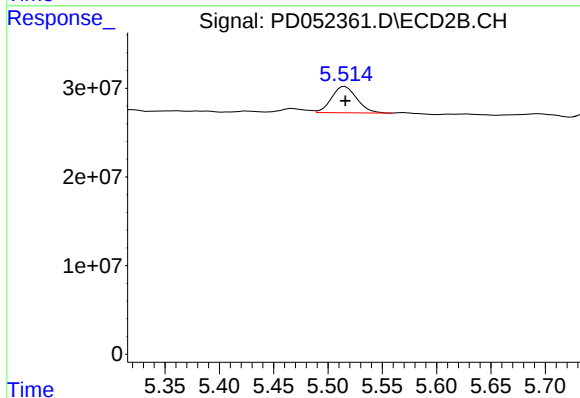


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 48163421
Conc: 34.39 ng/ml

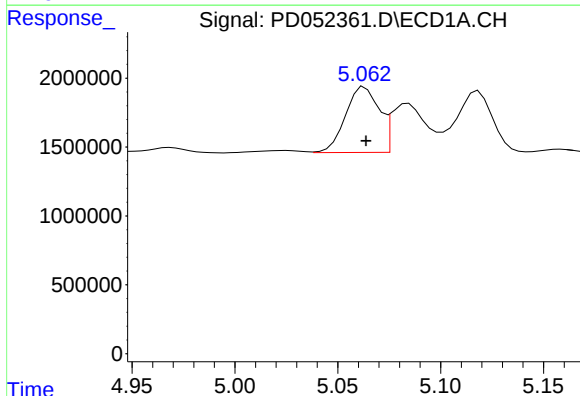


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 5404669
Conc: 24.44 ng/ml

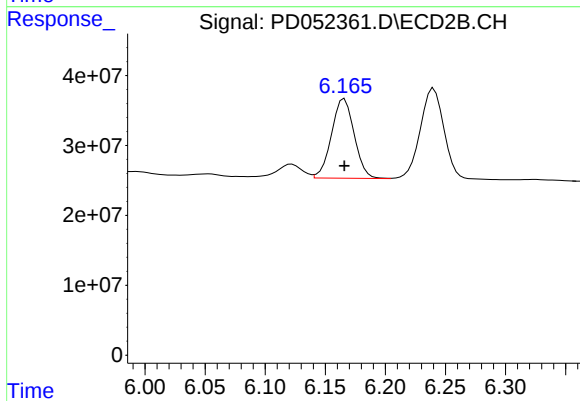

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 150131502
Conc: 34.02 ng/ml

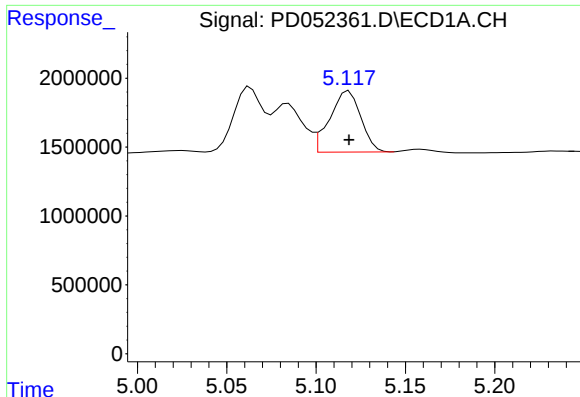

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 5374369
Conc: 25.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-05

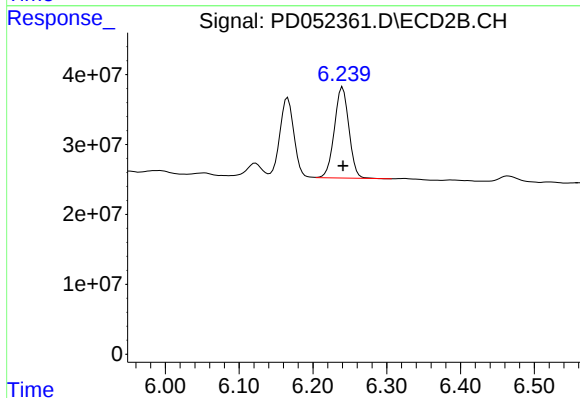


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 178514533
Conc: 35.11 ng/ml

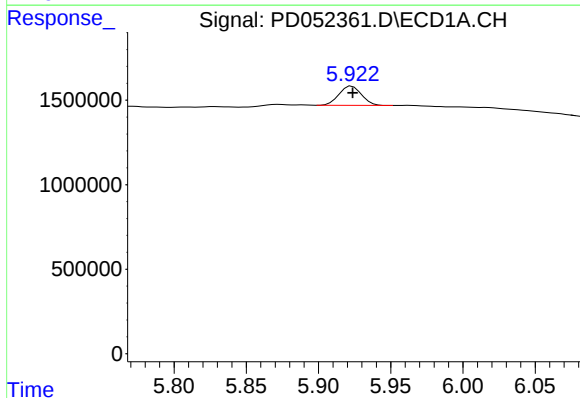


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1238469
Conc: 19.04 ng/ml

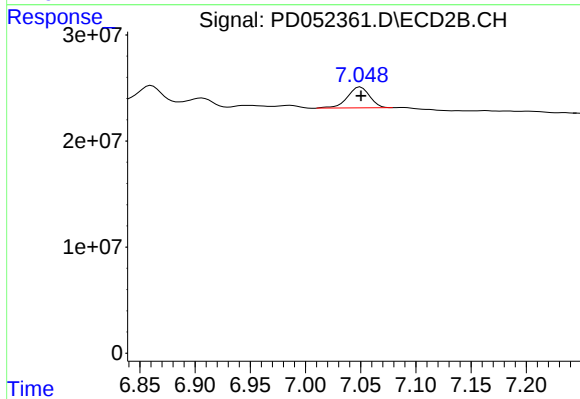

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 27646689
Conc: 29.97 ng/ml

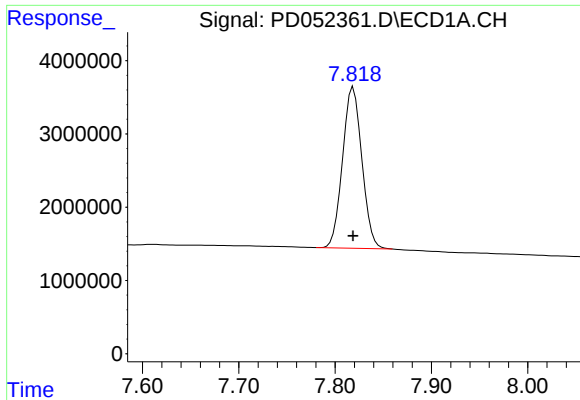

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 30573804
Conc: 22.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-05

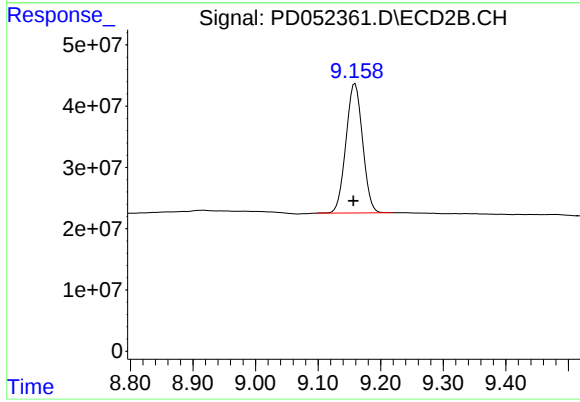

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 391090799
Conc: 25.15 ng/ml