

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052364.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2019 00:00
 Operator : AJ\SJ
 Sample : MDL-CHL-W-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-CHL-W-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:43:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	28456168	632.5E6	20.392	21.821
28)	SA Decachlor...	7.819	9.159	29902440	384.6E6	22.437	24.730
Target Compounds							
23)	Chlordane-1	4.043	5.046	1656257	43423371	26.376	28.305
24)	Chlordane-2	4.523	5.517	2021536	48847199	27.165	34.879 #
25)	Chlordane-3	5.063	6.167	5275527	144.3E6	23.856	32.710 #
26)	Chlordane-4	5.118	6.241	5182066	168.4E6	24.433	33.114 #
27)	Chlordane-5	5.923	7.051	1200356	25097456	18.458	27.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052364.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2019 00:00
Operator : AJ\SJ
Sample : MDL-CHL-W-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-W-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:43:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

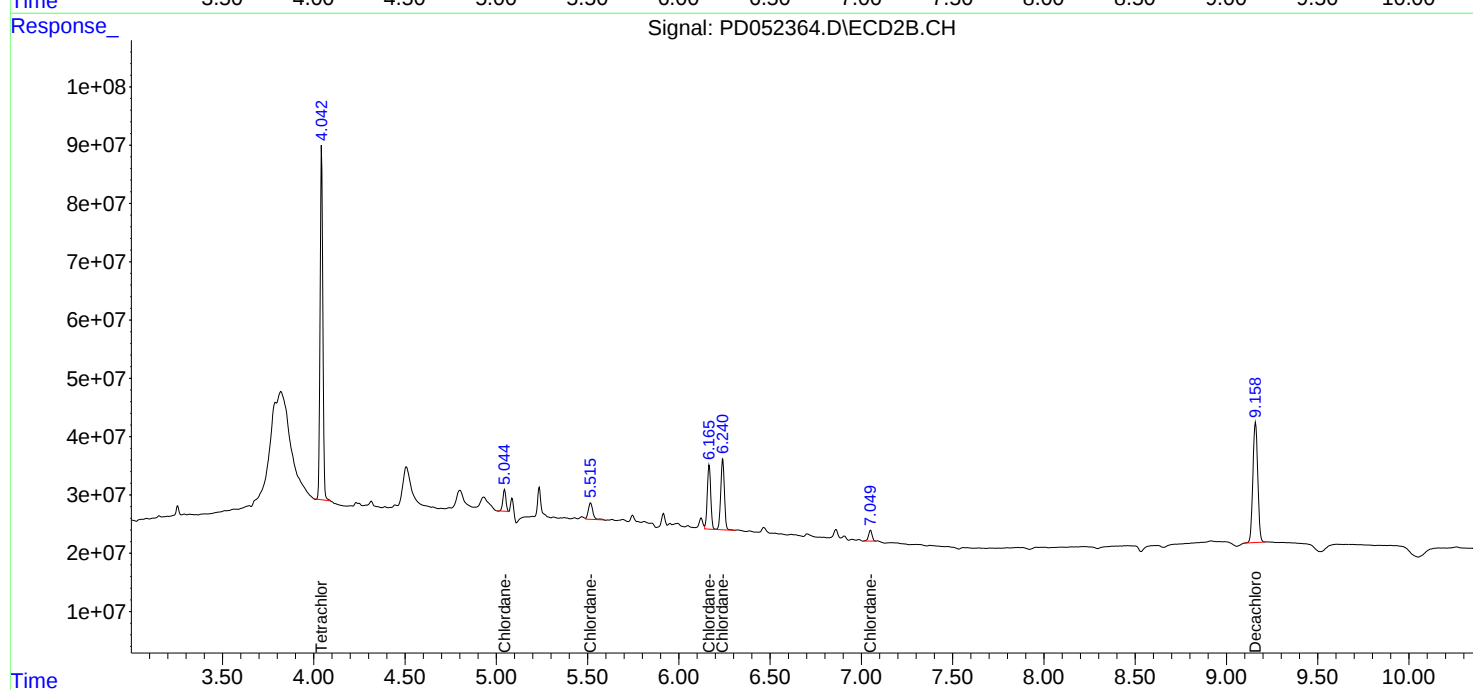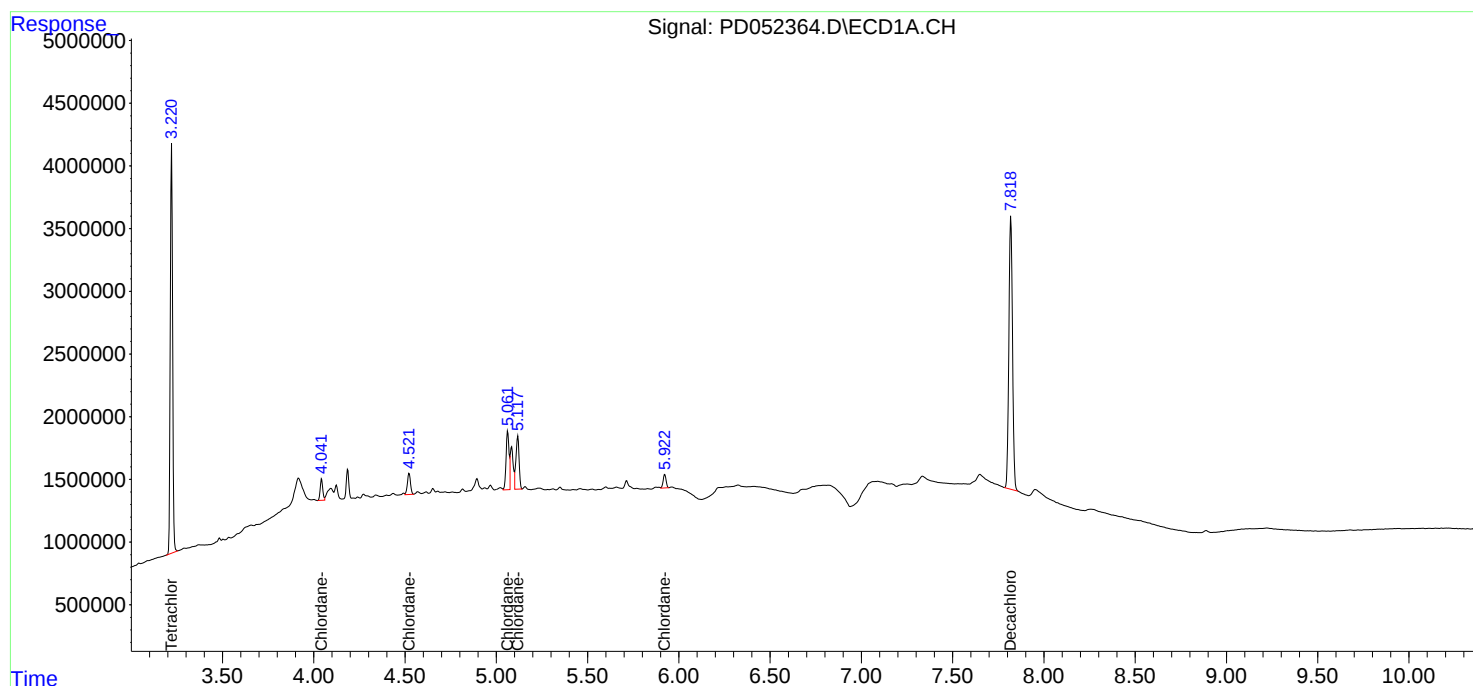


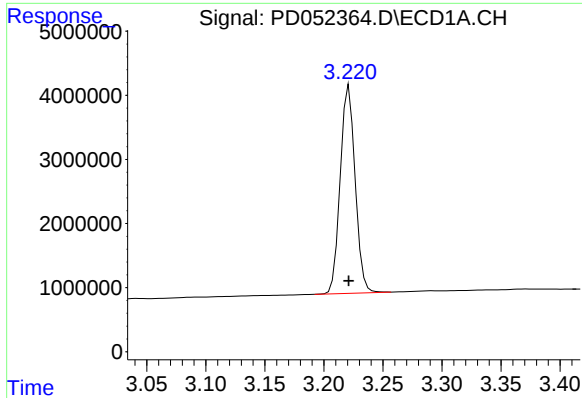

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28456168
Conc: 20.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-W-04

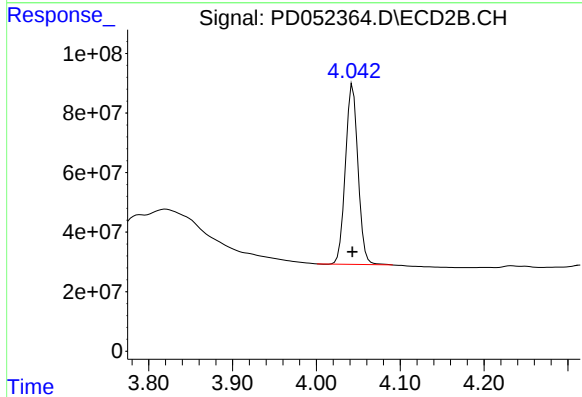


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 632451168
Conc: 21.82 ng/ml

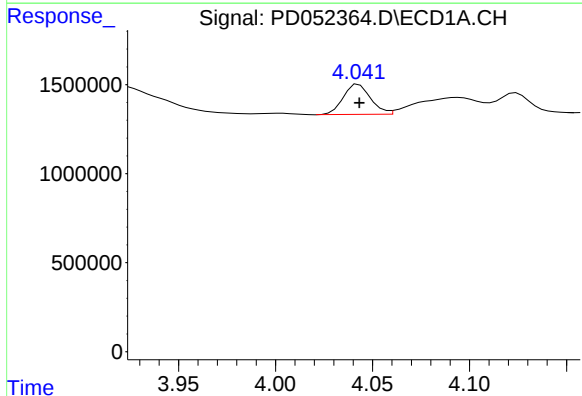


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1656257
Conc: 26.38 ng/ml

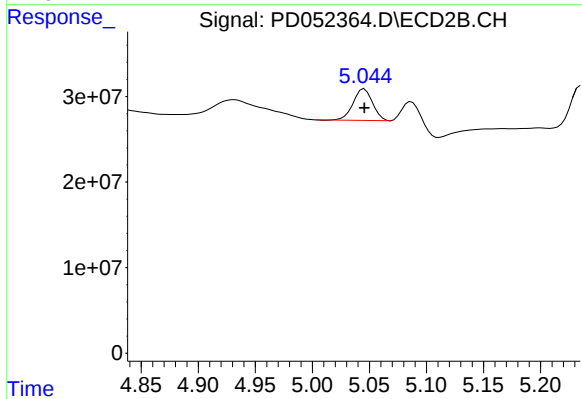

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 43423371
Conc: 28.31 ng/ml

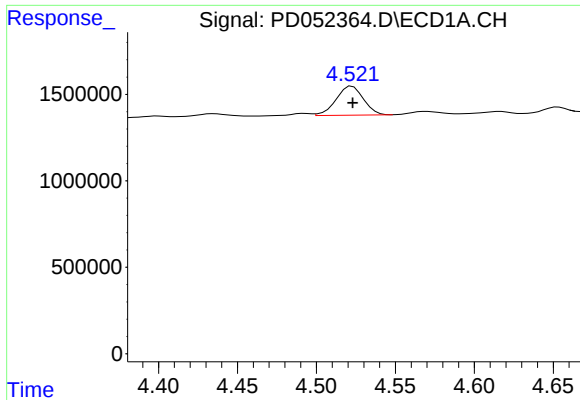

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 2021536
Conc: 27.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-W-04

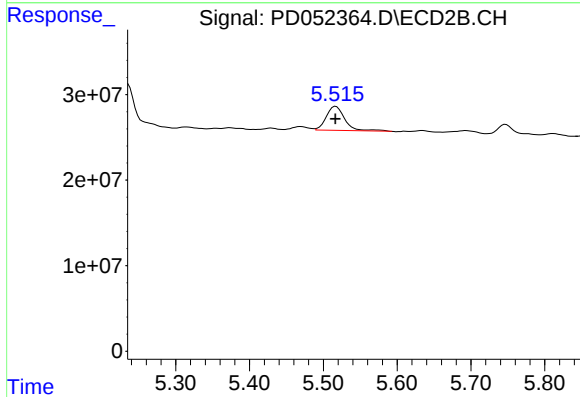


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 48847199
Conc: 34.88 ng/ml

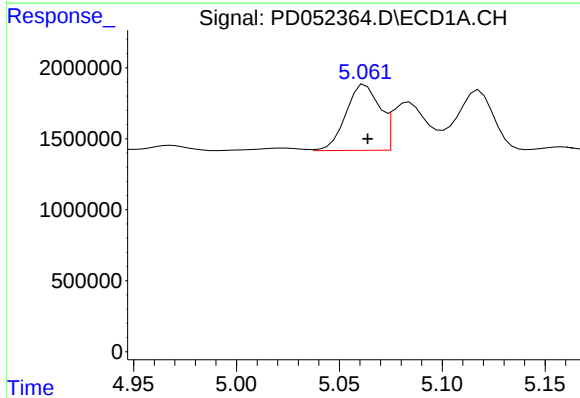


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 5275527
Conc: 23.86 ng/ml

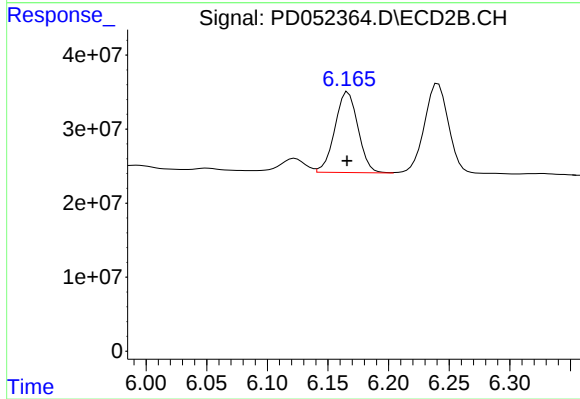

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 144340823
Conc: 32.71 ng/ml

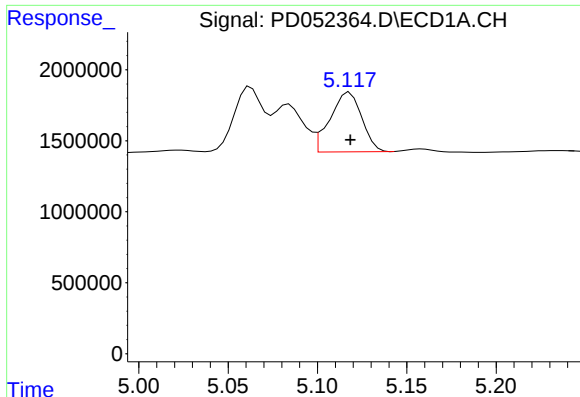

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 5182066
Conc: 24.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-W-04

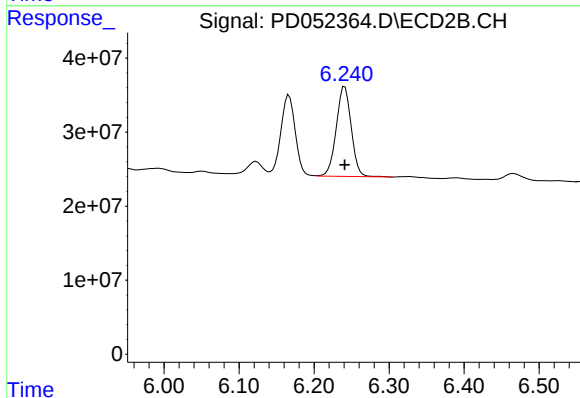


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 168387699
Conc: 33.11 ng/ml

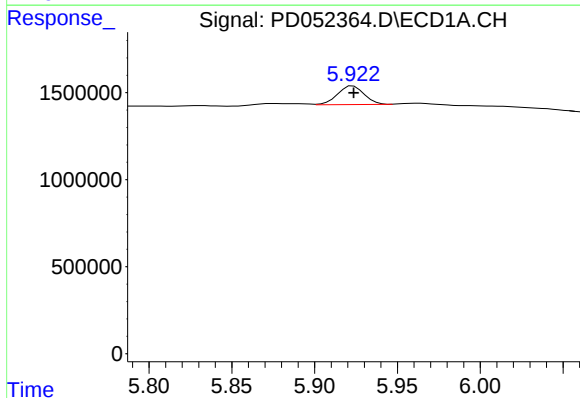


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1200356
Conc: 18.46 ng/ml

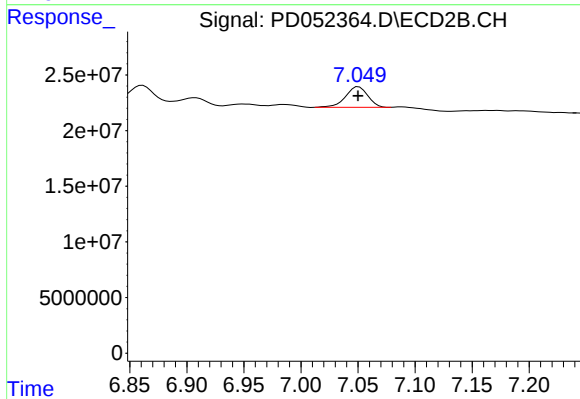

#27 Chlordane-5


R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 25097456
Conc: 27.20 ng/ml

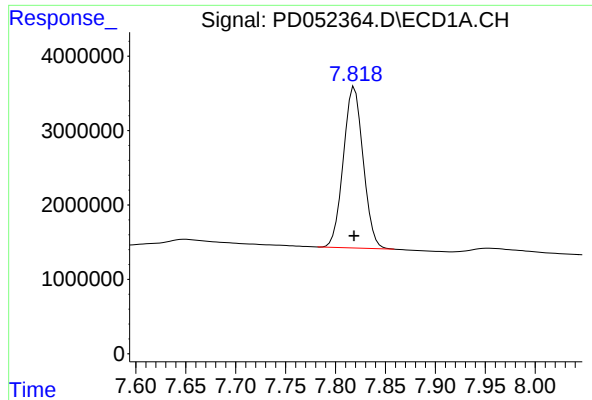

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 29902440
Conc: 22.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-W-04

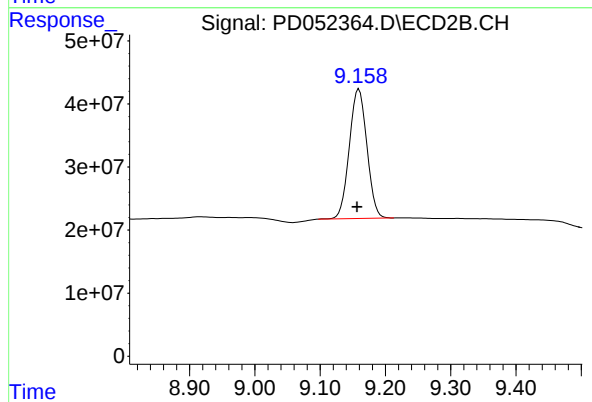

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 384585519
Conc: 24.73 ng/ml