

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052368.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2019 00:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:44:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	28545958	667.5E6	20.457	23.029
28)	SA Decachlor...	7.820	9.160	30754319	392.6E6	23.076	25.243
Target Compounds							
3)	MA gamma-BHC...	3.923	0.000	2516544	0	1.151	N.D. #
8)	B Heptachlo...	0.000	5.925	0	63158199	N.D.	1.957 #
9)	A Endosulfan I	0.000	6.284	0	11527002	N.D.	0.395 #
10)	B gamma-Chl...	0.000	6.167	0	78332025	N.D.	2.448 #
11)	B alpha-Chl...	0.000	6.263f	0	7380822	N.D.	0.235 #
25)	Chlordane-3	0.000	6.167	0	78332025	N.D.	17.751 #
26)	Chlordane-4	0.000	6.263f	0	7380822	N.D.	1.451 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052368.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2019 00:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:44:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

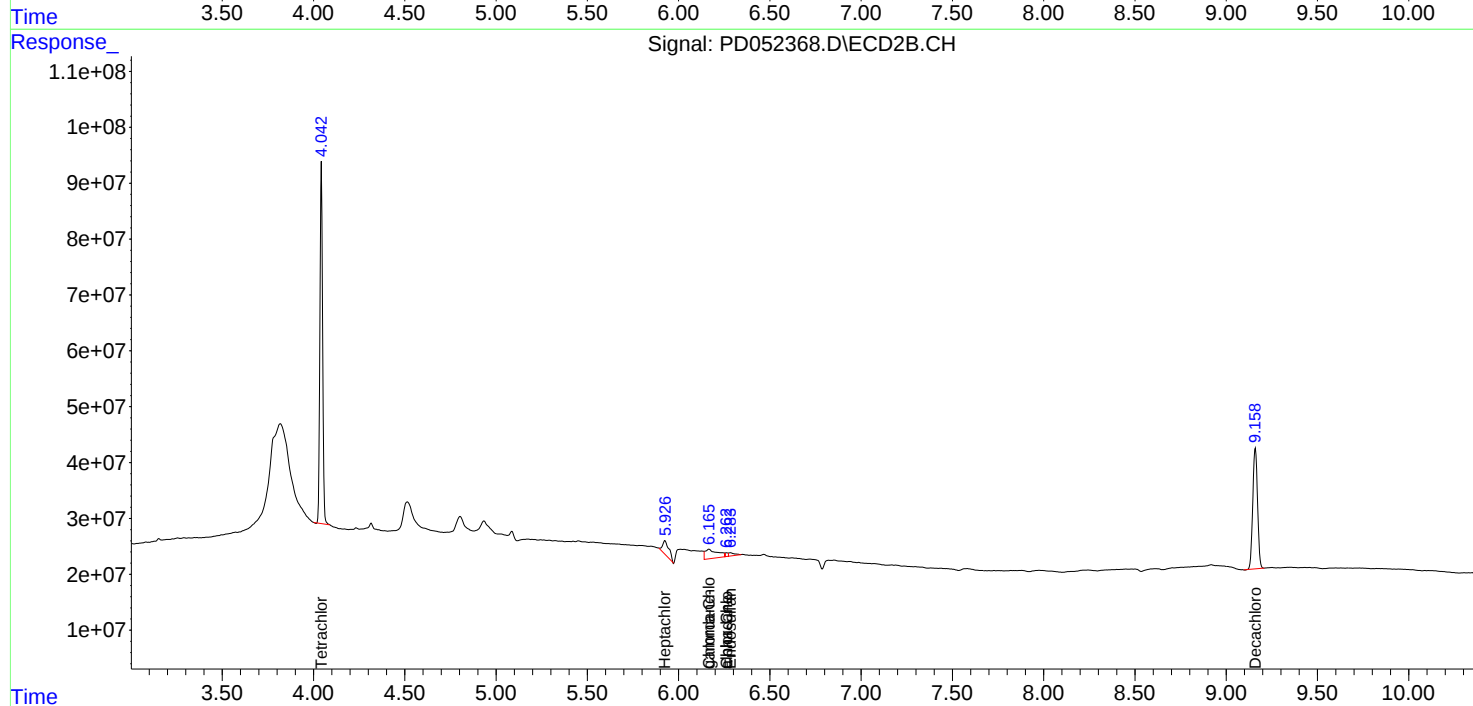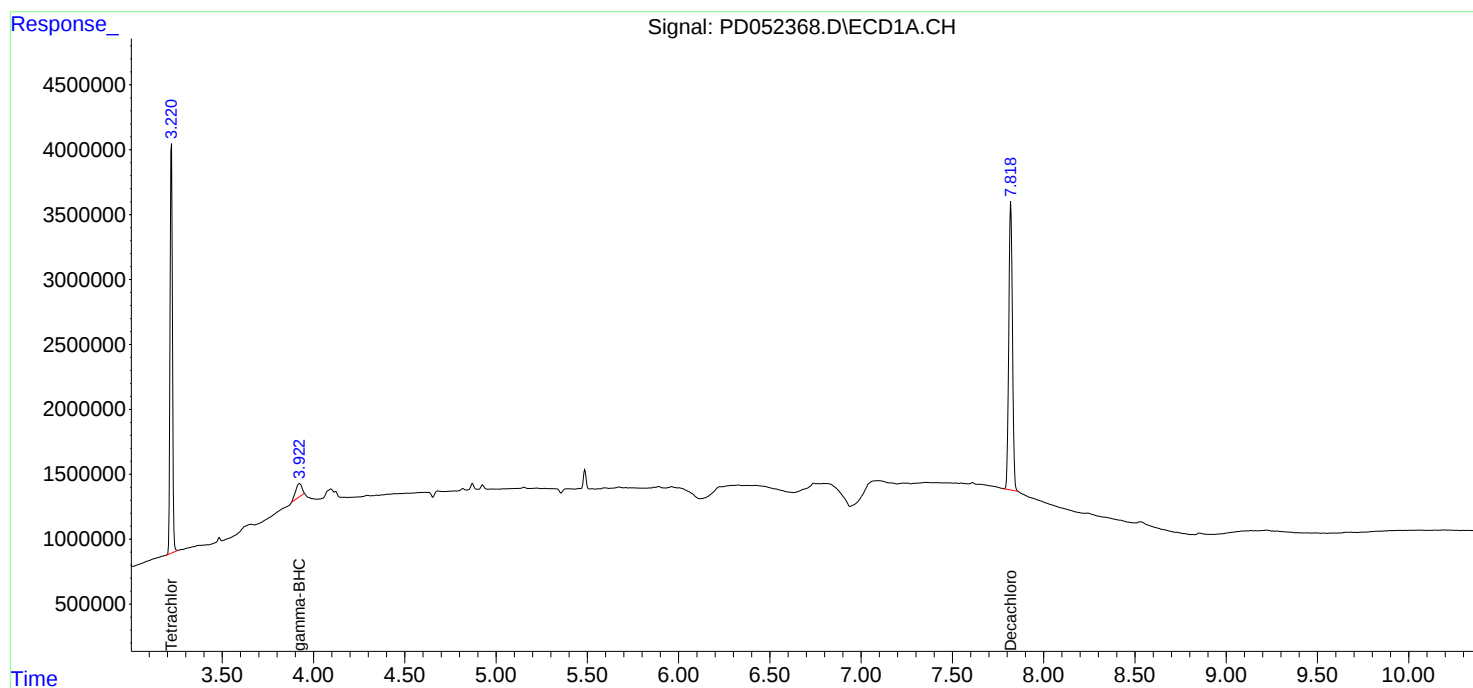


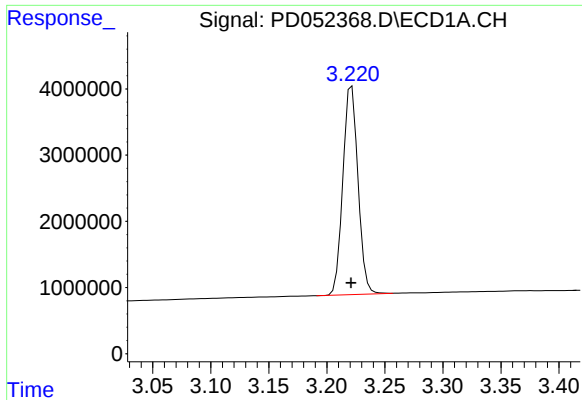

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 28545958
Conc: 20.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

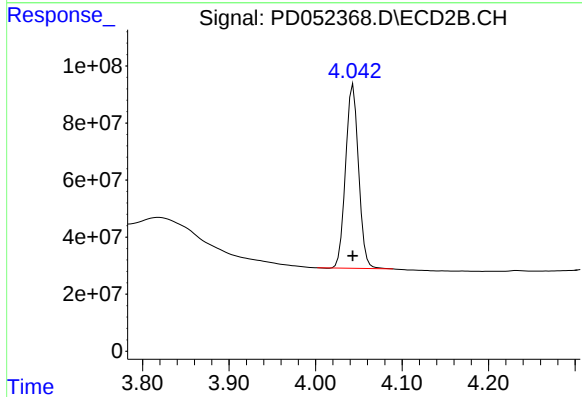


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 667472316
Conc: 23.03 ng/ml

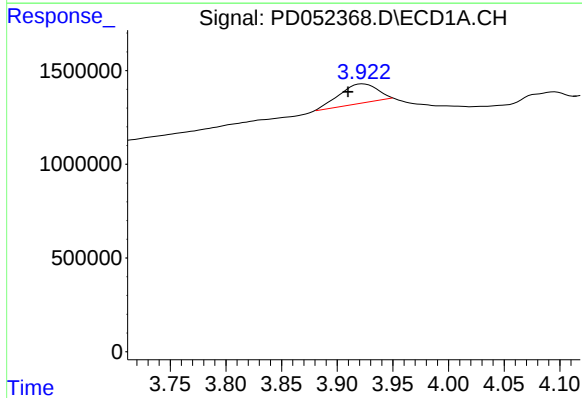


#3 gamma-BHC (Lindane)

R.T.: 3.923 min
Delta R.T.: 0.013 min
Response: 2516544
Conc: 1.15 ng/ml

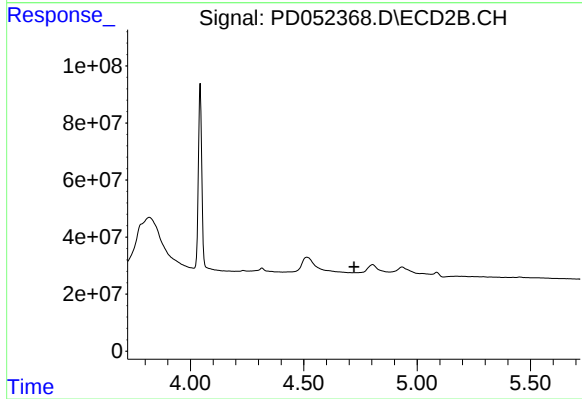

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

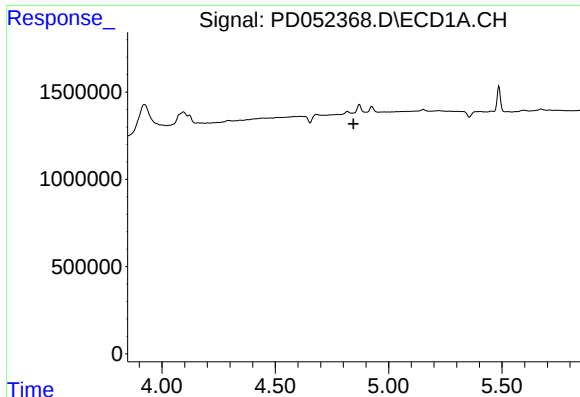

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

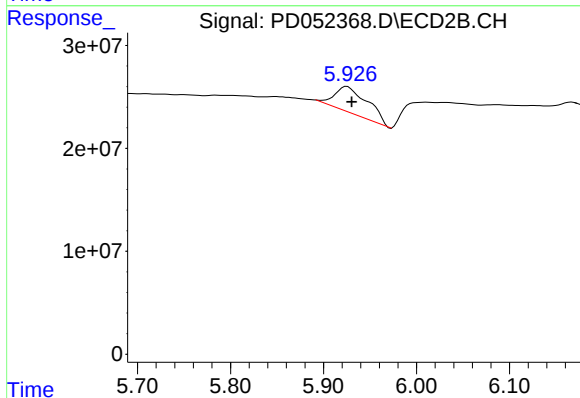


#8 Heptachlor epoxide

R.T.: 5.925 min
Delta R.T.: -0.005 min
Response: 63158199
Conc: 1.96 ng/ml

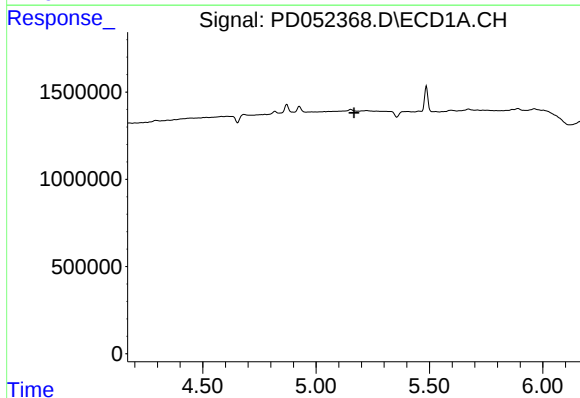


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

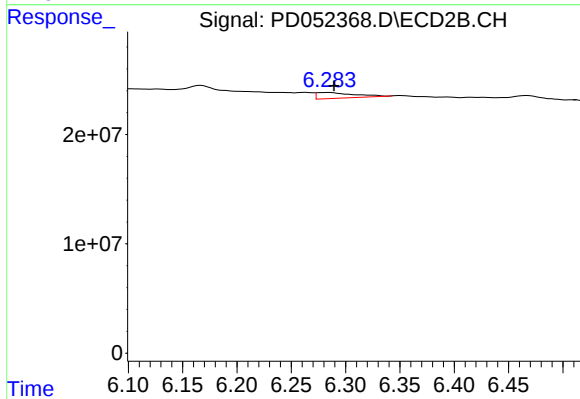

#9 Endosulfan I


R.T.: 6.284 min
Delta R.T.: -0.005 min
Response: 11527002
Conc: 0.39 ng/ml

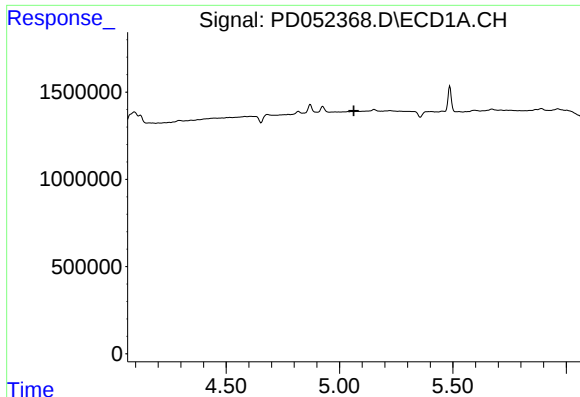

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

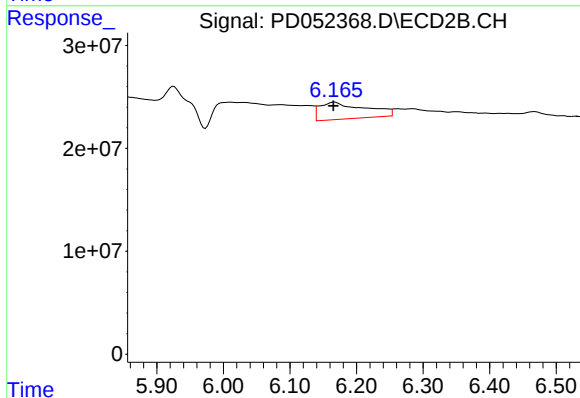


#10 gamma-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.001 min
Response: 78332025
Conc: 2.45 ng/ml

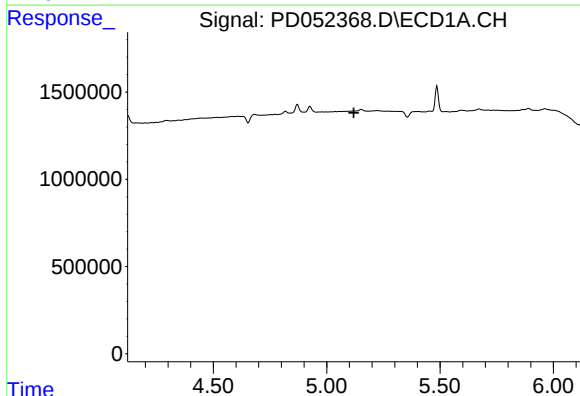


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

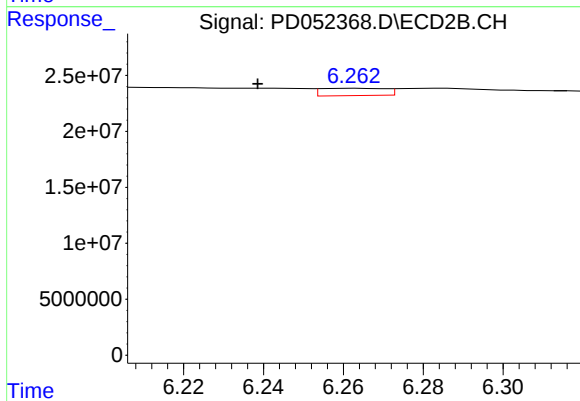

#11 alpha-Chlordane


R.T.: 6.263 min
Delta R.T.: 0.024 min
Response: 7380822
Conc: 0.24 ng/ml

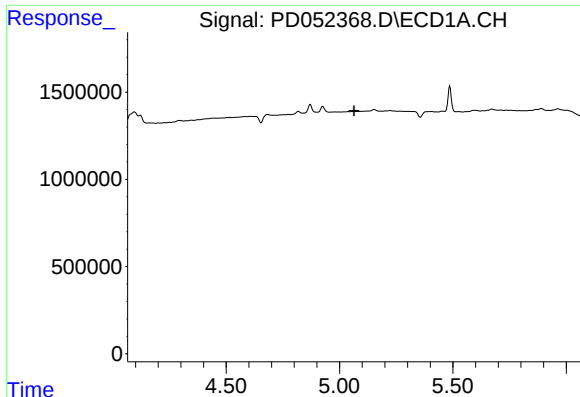

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

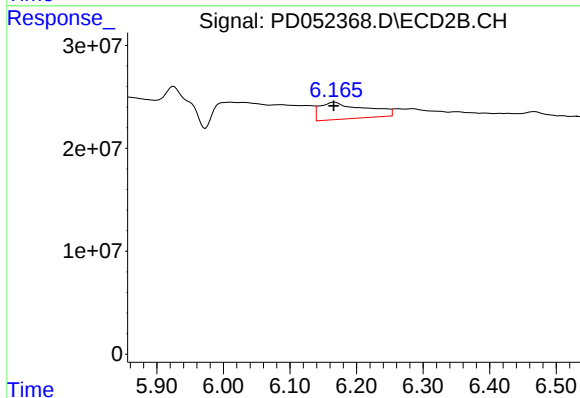


#25 Chlordane-3

R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 78332025
Conc: 17.75 ng/ml

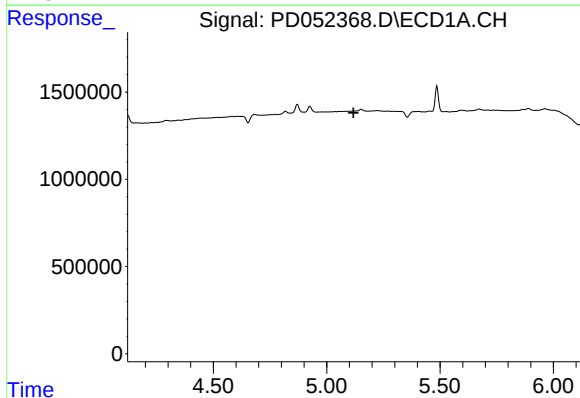


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

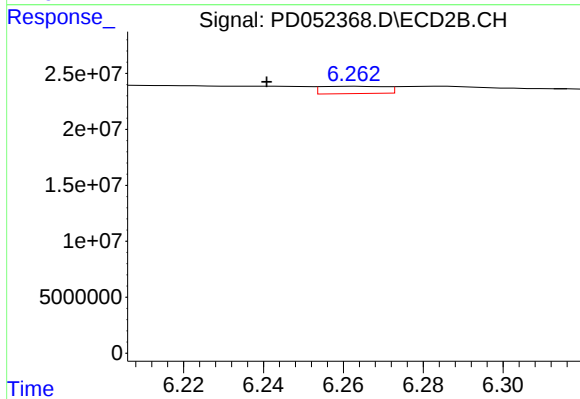

#26 Chlordane-4


R.T.: 6.263 min
Delta R.T.: 0.022 min
Response: 7380822
Conc: 1.45 ng/ml

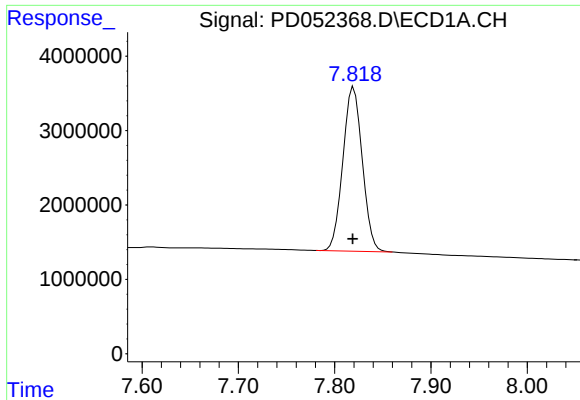

#28 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: 0.001 min
Response: 30754319
Conc: 23.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

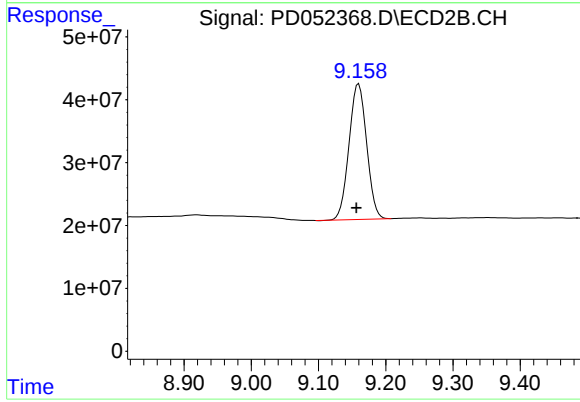

#28 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.003 min
Response: 392555810
Conc: 25.24 ng/ml