

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 1:40
 Operator : AJ\SJ
 Sample : MDL-CHL-S-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-CHL-S-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:47:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	31630182	729.1E6	22.667	25.154
28)	SA Decachlor...	7.818	9.159	32351079	440.7E6	24.274	28.341
Target Compounds							
23)	Chlordane-1	4.043	5.045	1713590	49775359	27.289	32.446
24)	Chlordane-2	4.522	5.516	2293208	53383963	30.816	38.119
25)	Chlordane-3	5.062	6.166	5681138	168.5E6	25.691	38.189 #
26)	Chlordane-4	5.118	6.240	5626680	199.8E6	26.529	39.284 #
27)	Chlordane-5	5.923	7.050	1620147	32694348	24.913	35.437 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 1:40
Operator : AJ\SJ
Sample : MDL-CHL-S-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:47:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

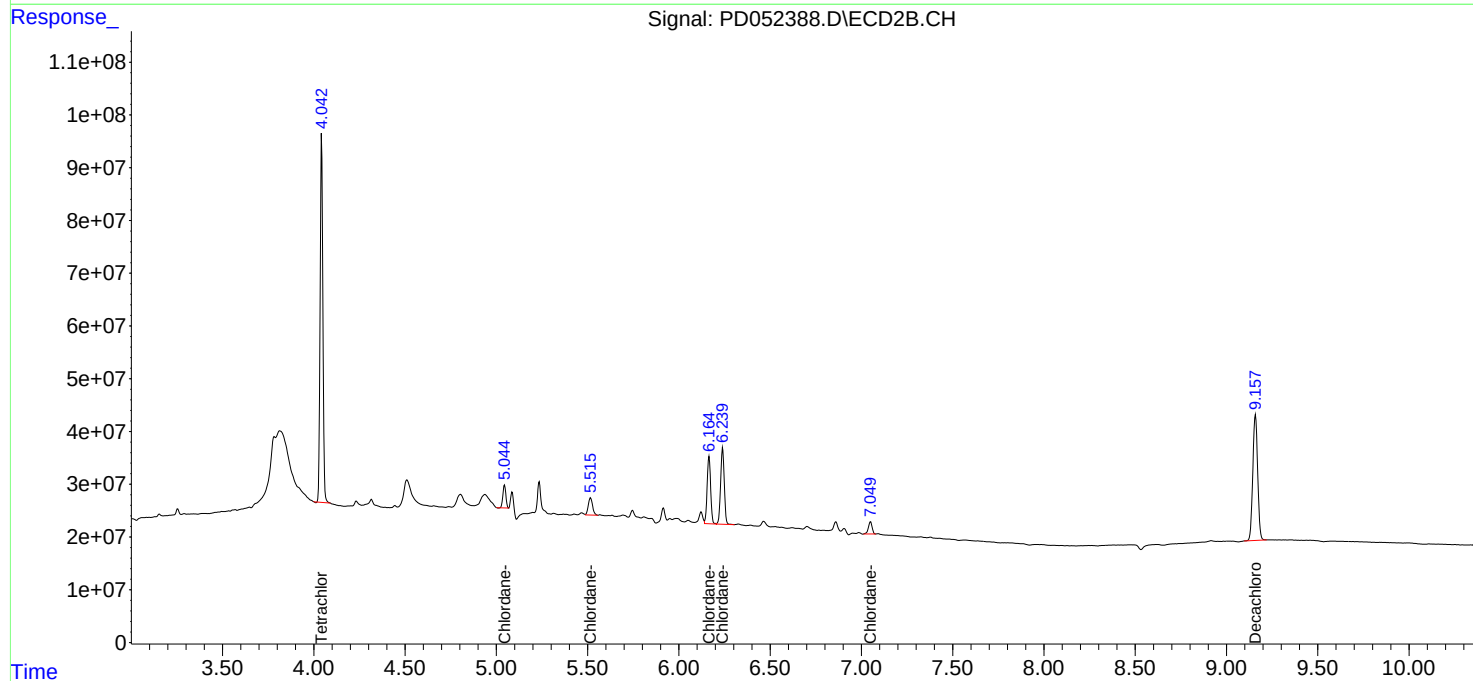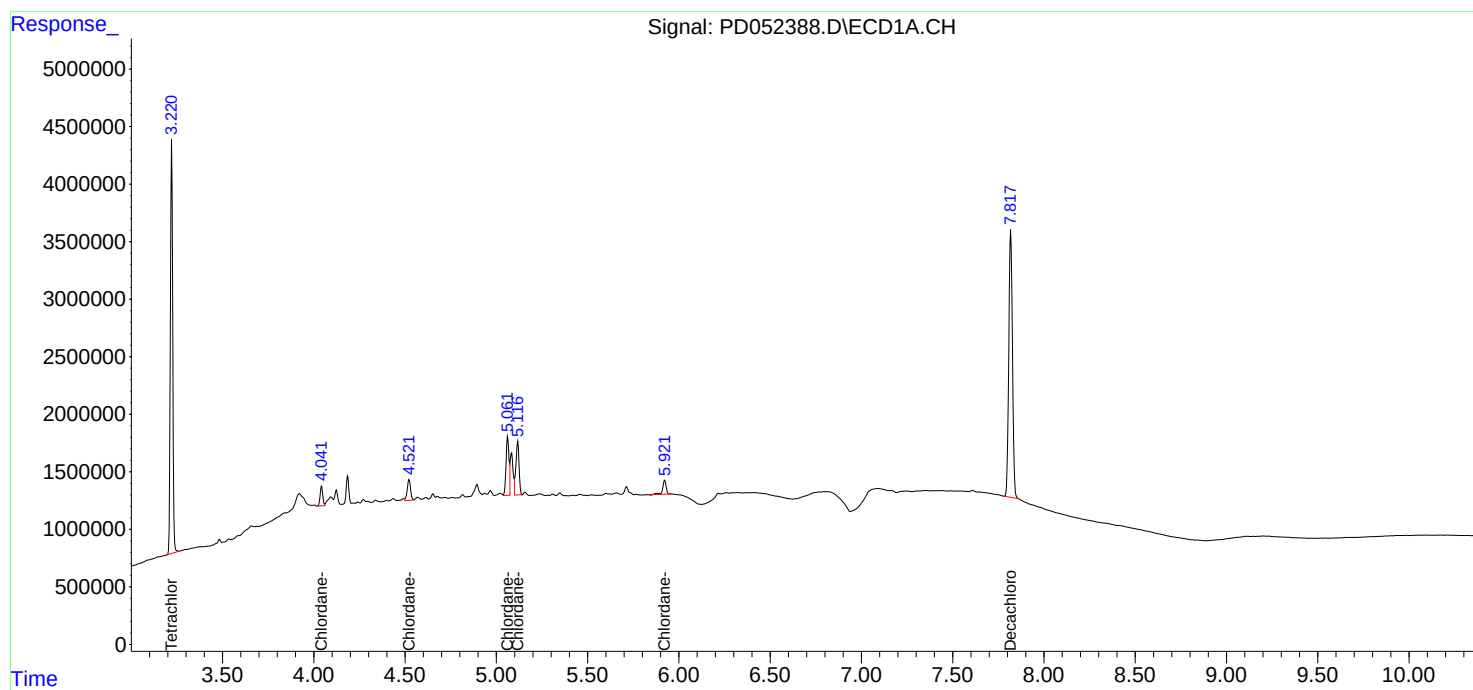


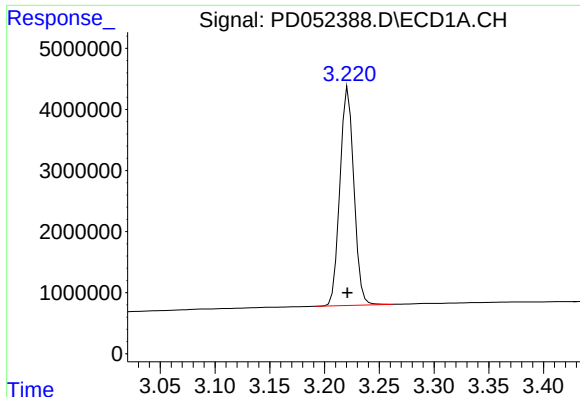

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 31630182
Conc: 22.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-07

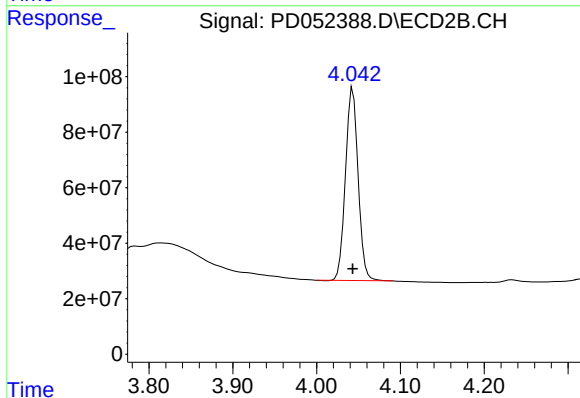


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 729068563
Conc: 25.15 ng/ml

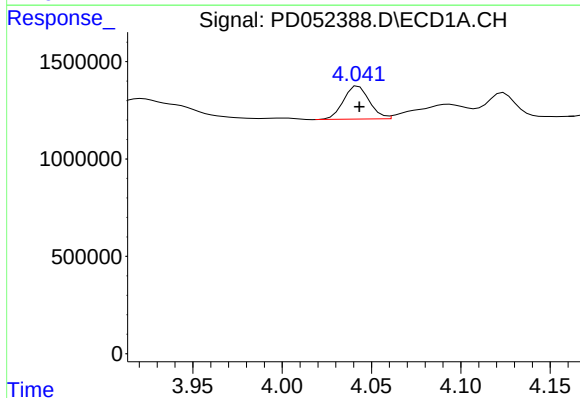


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1713590
Conc: 27.29 ng/ml

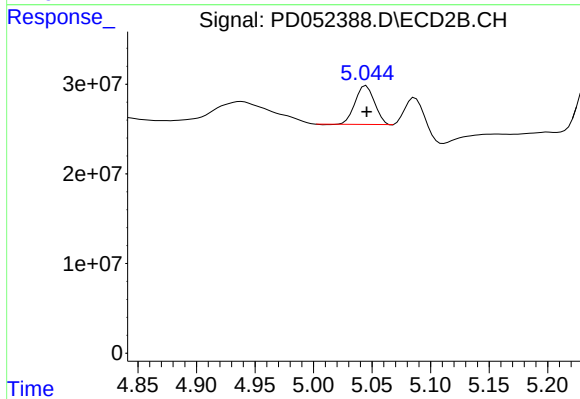

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 49775359
Conc: 32.45 ng/ml

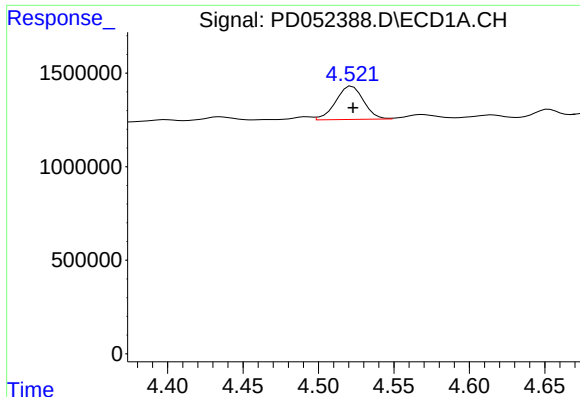

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 2293208
Conc: 30.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-07

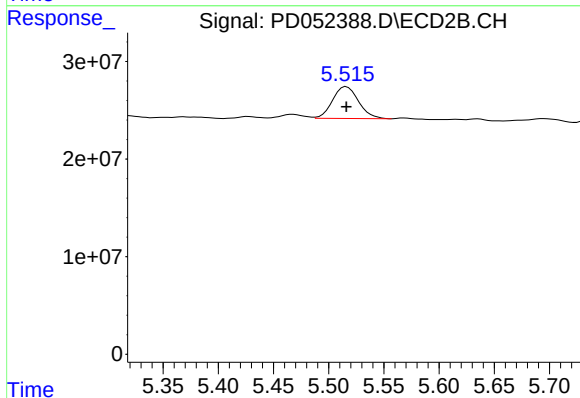


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 53383963
Conc: 38.12 ng/ml

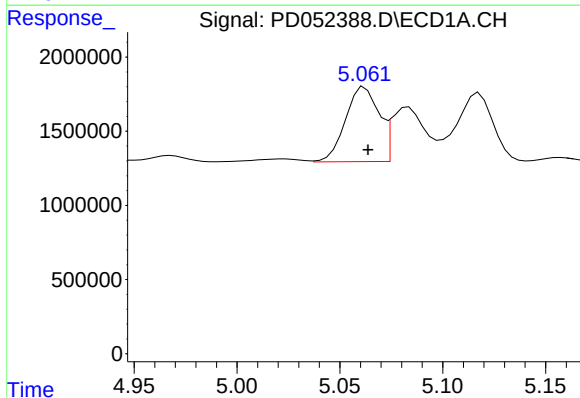


#25 Chlordane-3

R.T.: 5.062 min
Delta R.T.: -0.001 min
Response: 5681138
Conc: 25.69 ng/ml

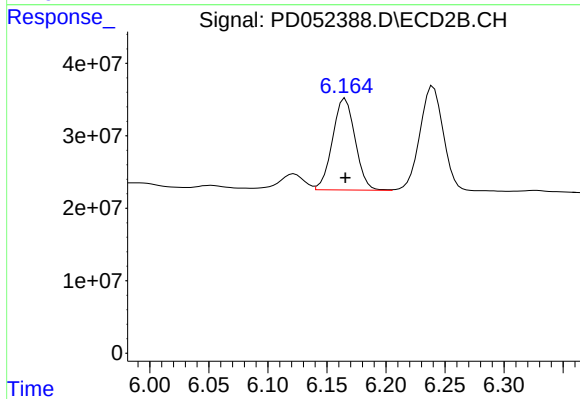

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 168520325
Conc: 38.19 ng/ml

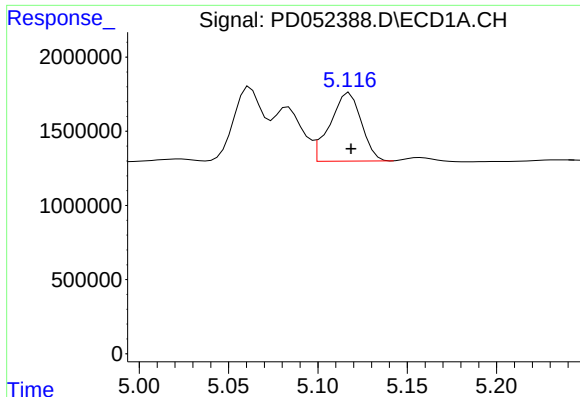

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 5626680
Conc: 26.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-07

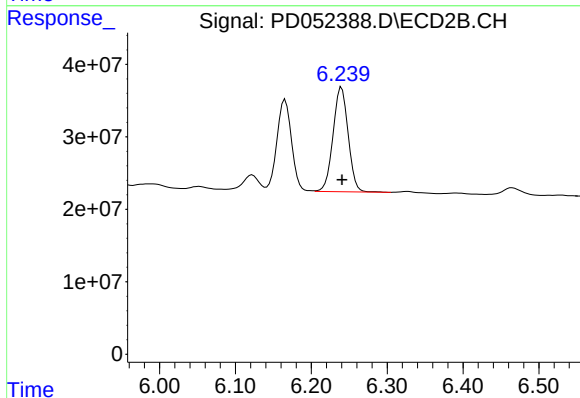


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 199762944
Conc: 39.28 ng/ml

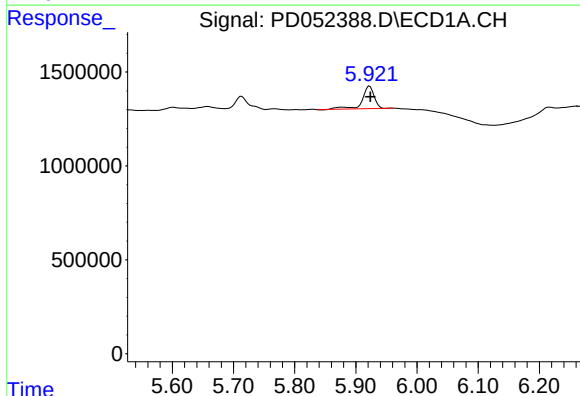


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1620147
Conc: 24.91 ng/ml

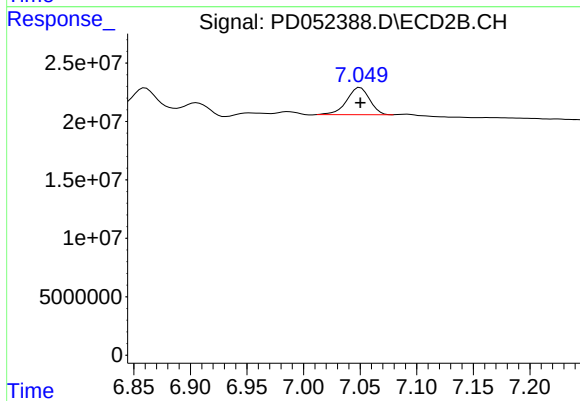

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 32694348
Conc: 35.44 ng/ml

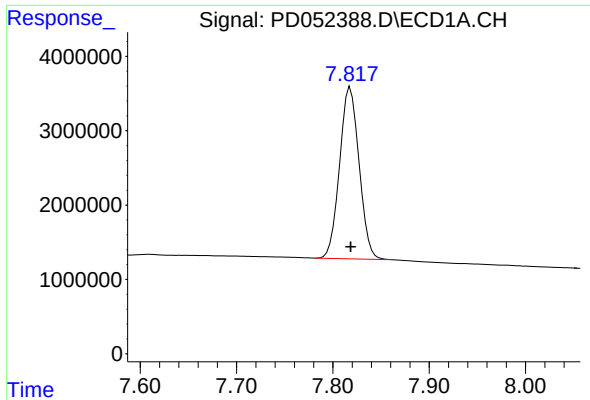

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 32351079
Conc: 24.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-07

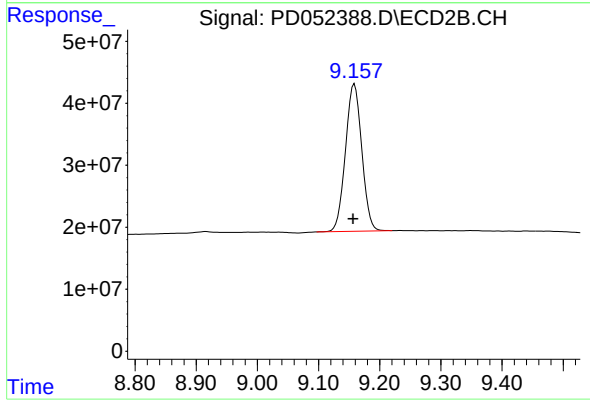

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 440740019
Conc: 28.34 ng/ml