

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033120\
 Data File : PD057676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2020 11:02
 Operator : AJ\MA
 Sample : L2059-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 06:39:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:32:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	3.926	4.525f	1253080	1109678	1.007 0.822
6) B	beta-BHC	0.000	4.700f	0	142329	N.D. 0.219
7) B	delta-BHC	0.000	4.920	0	268557	N.D. 0.197
8) B	Heptachlo...	0.000	5.789f	0	27749	N.D. <MDL
9) A	Endosulfan I	0.000	6.102	0	221736	N.D. 0.180
11) B	cis-Chlor...	0.000	6.061	0	203953	N.D. 0.150
13) MA	Dieldrin	0.000	6.367	0	127750	N.D. <MDL
15) B	Endosulfa...	0.000	6.798	0	184235	N.D. 0.160
19) B	Endosulfa...	6.280f	0.000	418453	0	0.457 N.D. #
21) B	Endrin ke...	6.826	0.000	620177	0	0.729 N.D. #
22)	Toxaphene-1	0.000	6.286	0	71366	N.D. 11.338


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033120\
Data File : PD057676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2020 11:02
Operator : AJ\MA
Sample : L2059-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 06:39:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:32:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

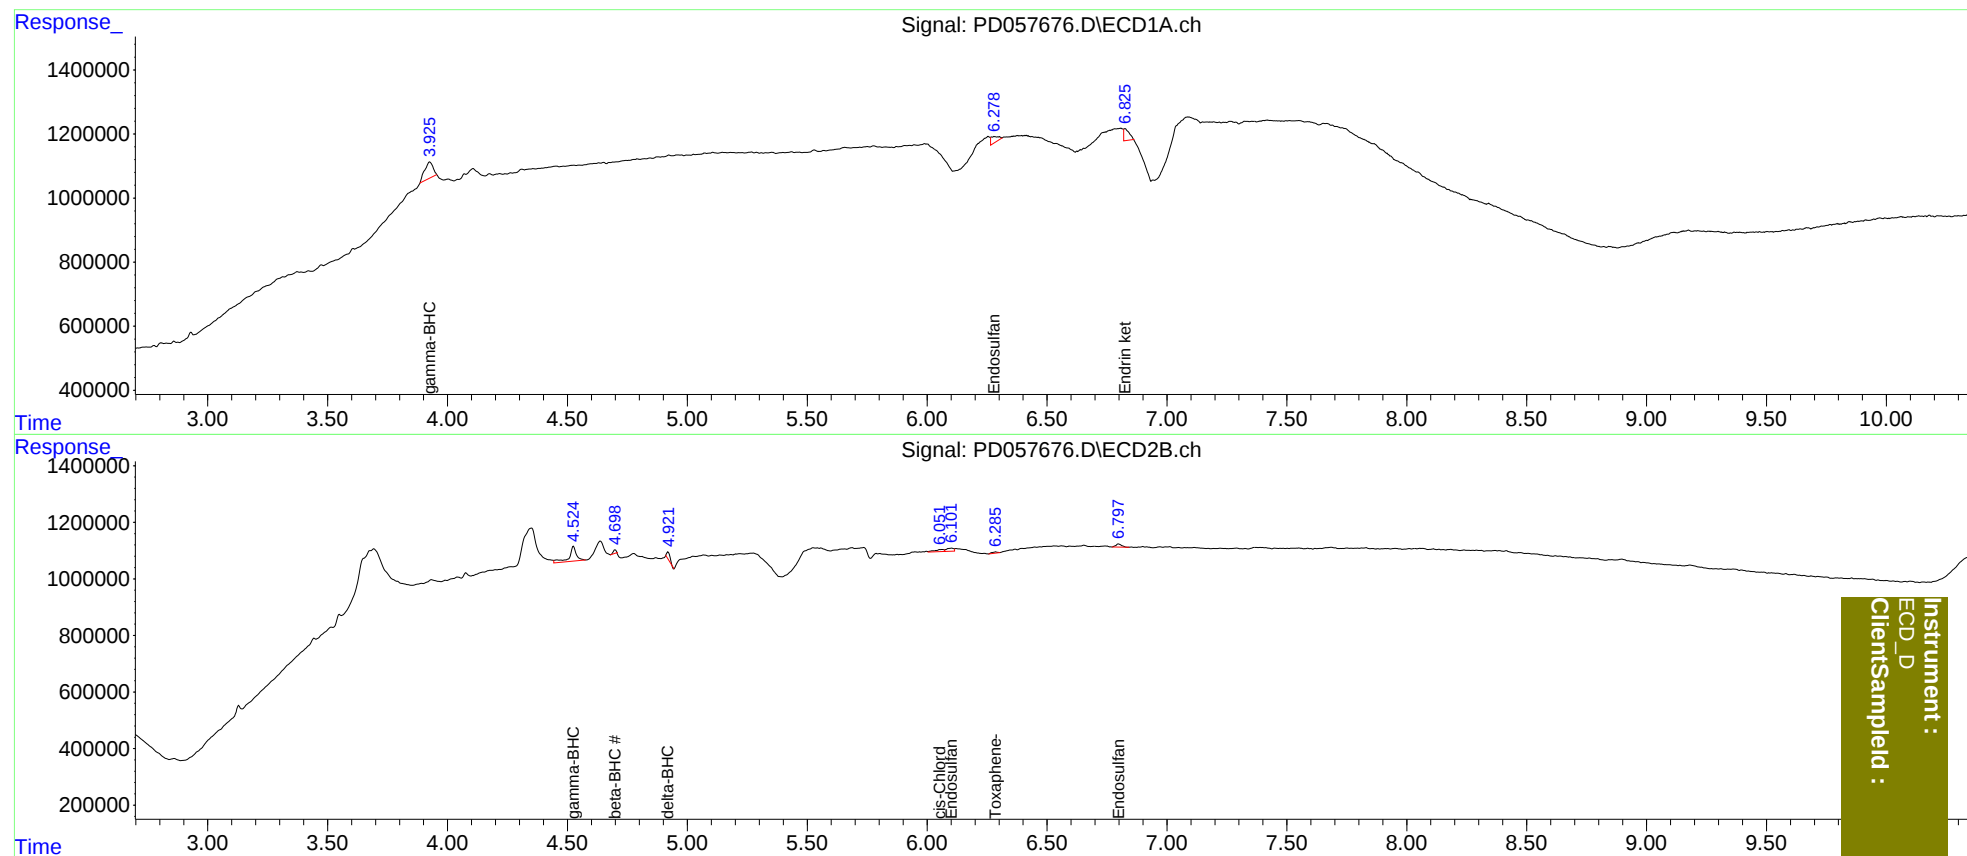


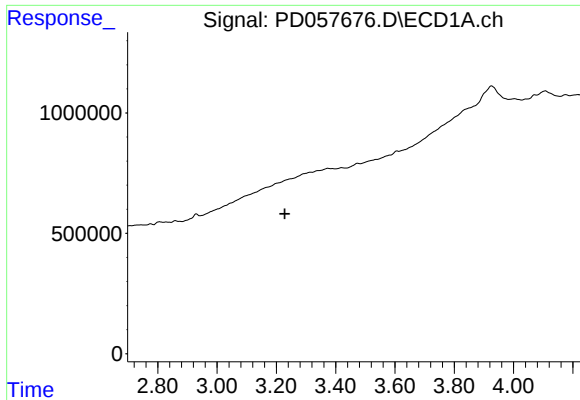

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

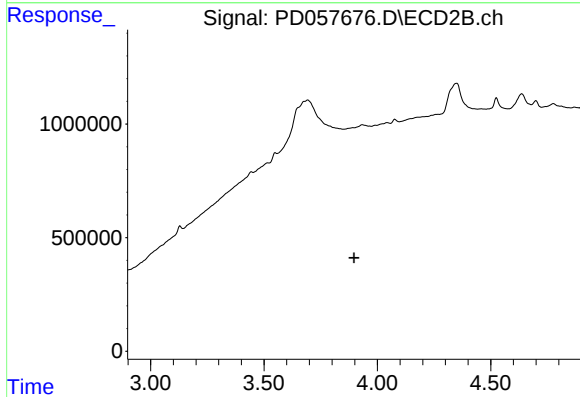


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.897 min
Response: 0
Conc: N.D.

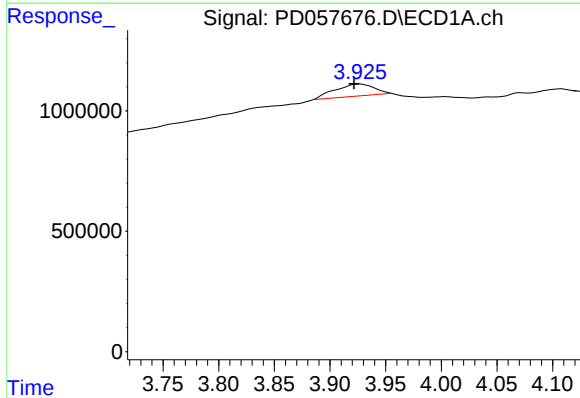


#3 gamma-BHC (Lindane)

R.T.: 3.926 min
Delta R.T.: 0.004 min
Response: 1253080
Conc: 1.01 ng/ml

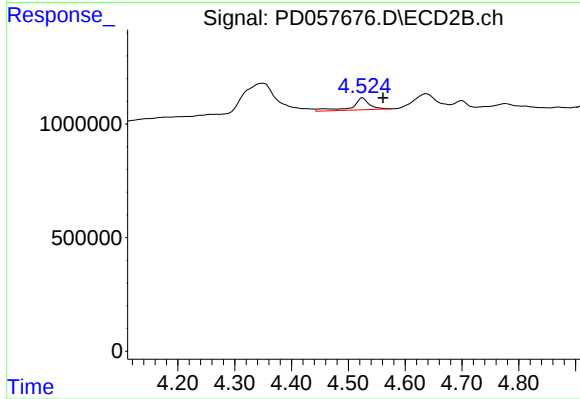

#3 gamma-BHC (Lindane)


R.T.: 4.525 min
Delta R.T.: -0.036 min
Response: 1109678
Conc: 0.82 ng/ml

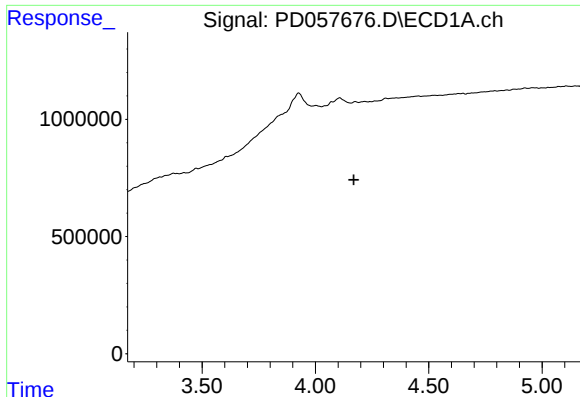

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

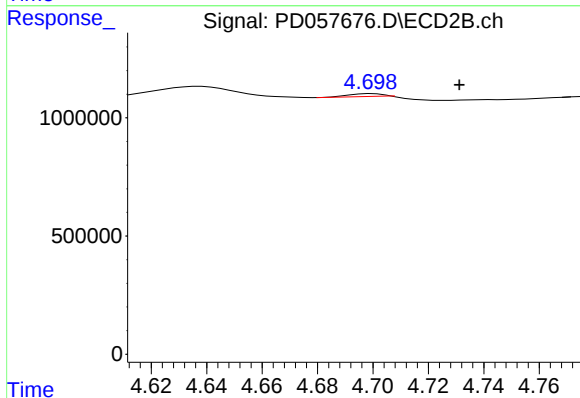


#6 beta-BHC

R.T.: 4.700 min
Delta R.T.: -0.032 min
Response: 142329
Conc: 0.22 ng/ml

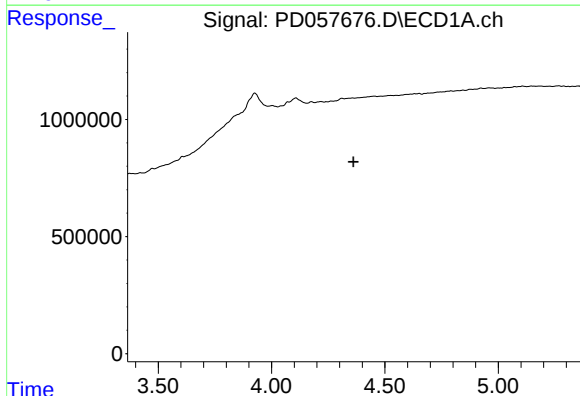


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.362 min
Response: 0
Conc: N.D.

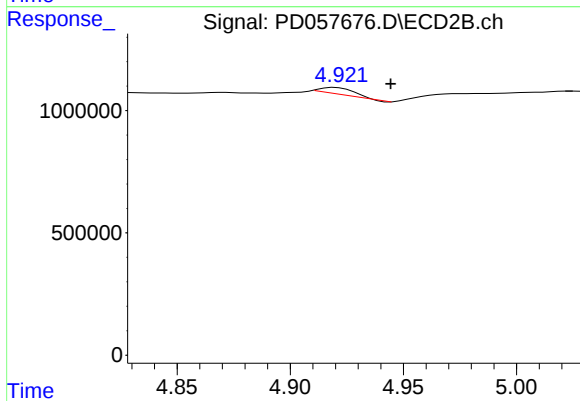

#7 delta-BHC


R.T.: 4.920 min
Delta R.T.: -0.025 min
Response: 268557
Conc: 0.20 ng/ml

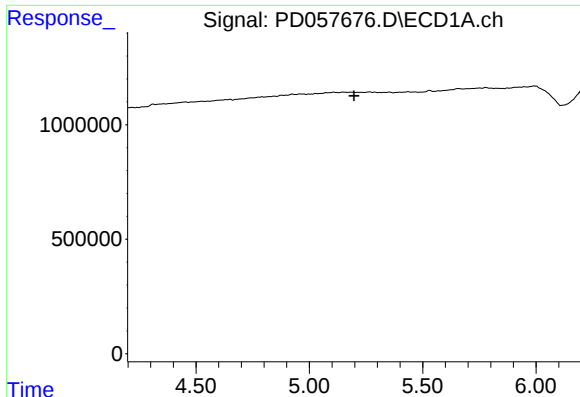

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

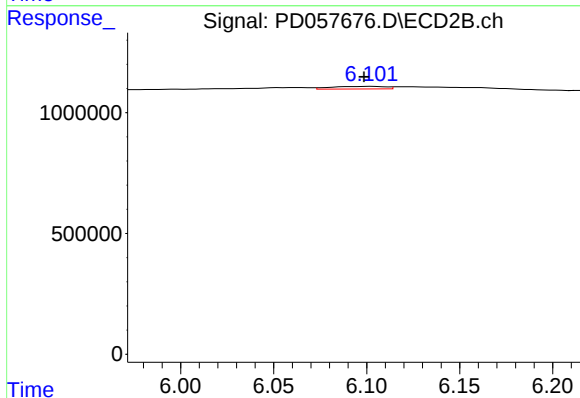


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.004 min
Response: 221736
Conc: 0.18 ng/ml

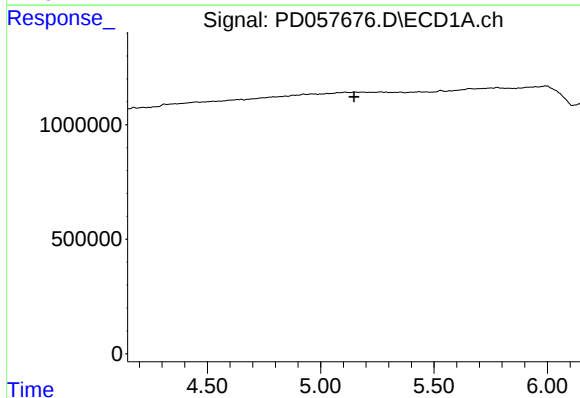


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.147 min
Response: 0
Conc: N.D.

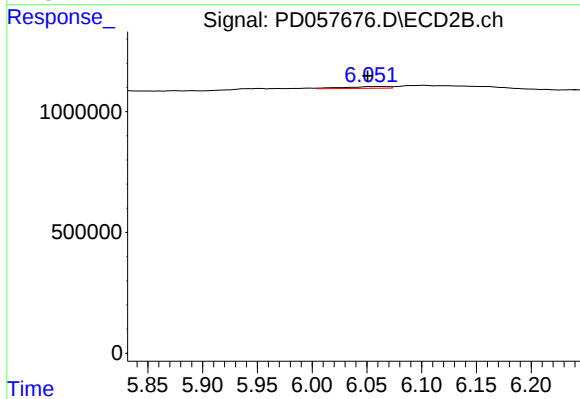

#11 cis-Chlordane


R.T.: 6.061 min
Delta R.T.: 0.010 min
Response: 203953
Conc: 0.15 ng/ml

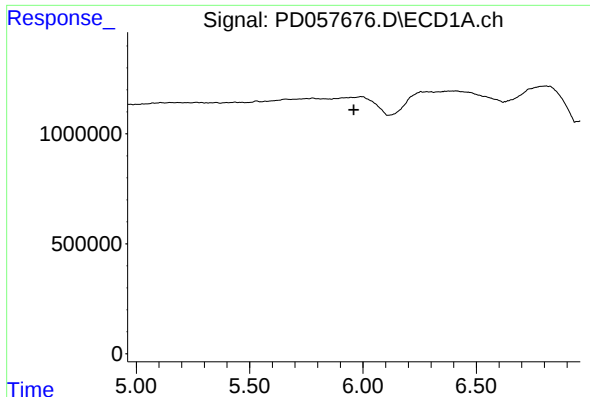

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

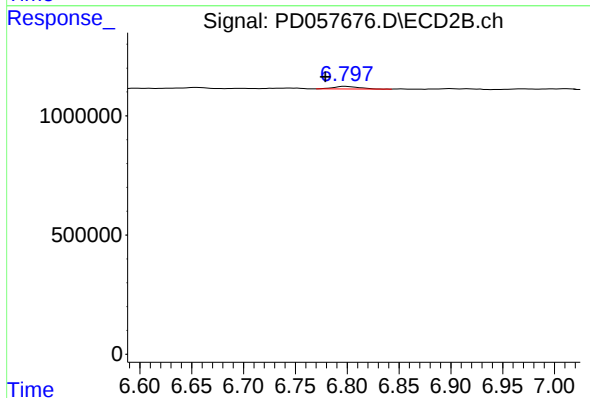


#15 Endosulfan II

R.T.: 6.798 min
Delta R.T.: 0.020 min
Response: 184235
Conc: 0.16 ng/ml

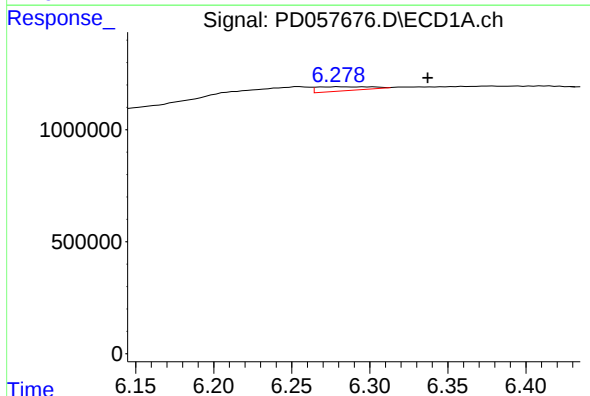


#19 Endosulfan Sulfate

R.T.: 6.280 min
Delta R.T.: -0.057 min
Response: 418453
Conc: 0.46 ng/ml

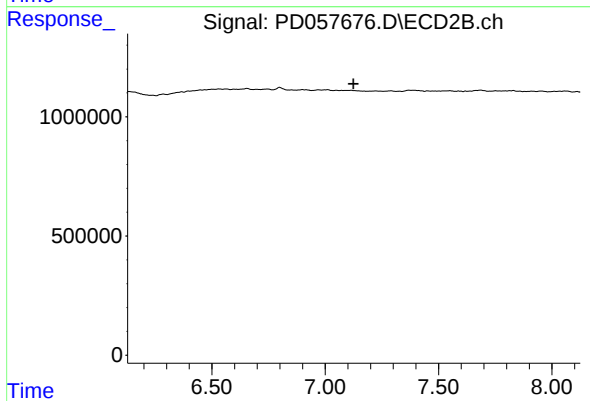

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.125 min
Response: 0
Conc: N.D.

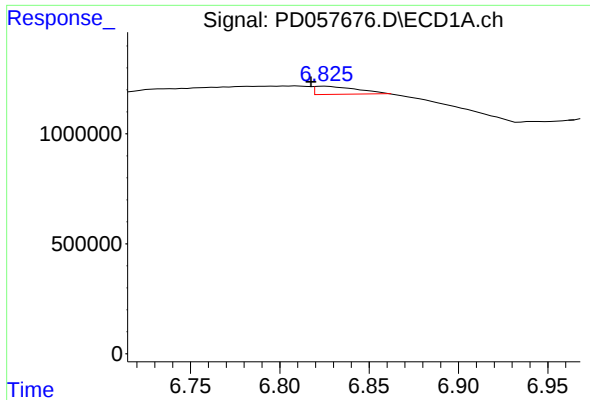

#21 Endrin ketone


R.T.: 6.826 min
Delta R.T.: 0.008 min
Response: 620177
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

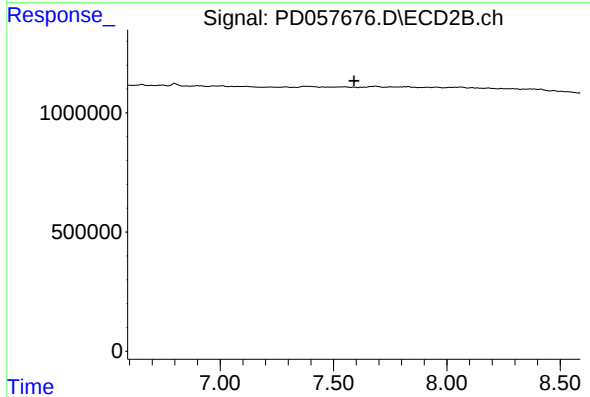


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.591 min
Response: 0
Conc: N.D.

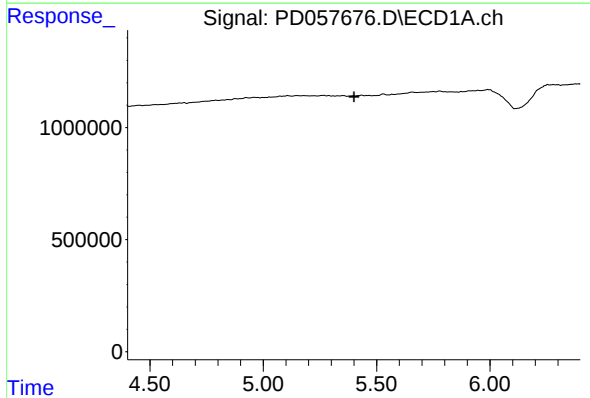


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

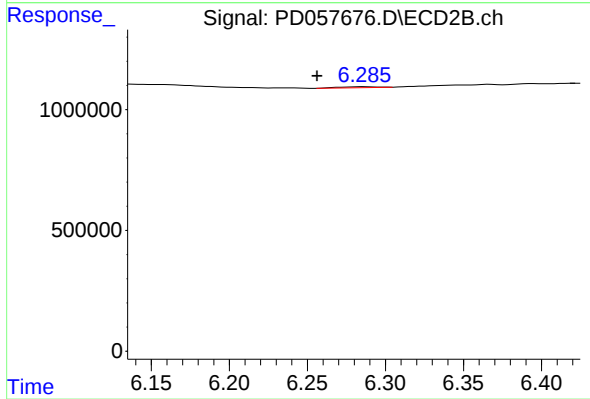

#22 Toxaphene-1


R.T.: 6.286 min
Delta R.T.: 0.030 min
Response: 71366
Conc: 11.34 ng/ml

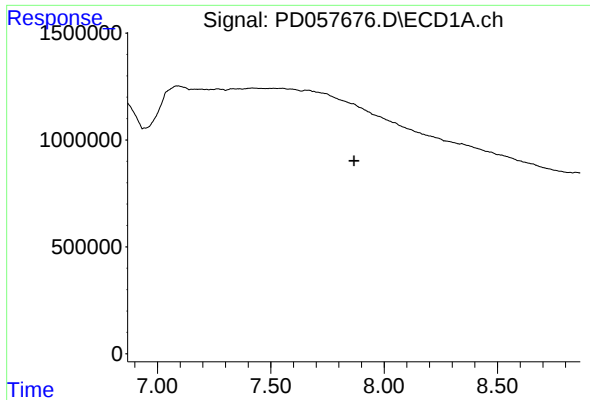

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

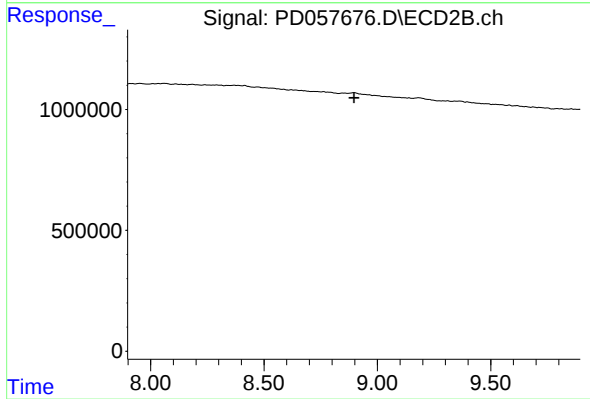

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.897 min
Response: 0
Conc: N.D.