

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033120\
 Data File : PD057677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2020 11:16
 Operator : AJ\MA
 Sample : L2059-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 06:39:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 12 06:32:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	3.854f	0	42959	N.D.	<MDL
Target Compounds						
3) MA gamma-BHC...	3.930	4.526f	1170440	806759	0.940	0.597 #
4) MA Heptachlor	0.000	5.073	0	52710	N.D.	<MDL
6) B beta-BHC	0.000	4.699f	0	153717	N.D.	0.237
7) B delta-BHC	0.000	4.921	0	342938	N.D.	0.251
8) B Heptachlo...	0.000	5.796f	0	102482	N.D.	<MDL
9) A Endosulfan I	0.000	6.089	0	748885	N.D.	0.608
11) B cis-Chlor...	0.000	6.089f	0	748885	N.D.	0.550
13) MA Dieldrin	0.000	6.351	0	63357	N.D.	<MDL
14) MA Endrin	0.000	6.508f	0	41140	N.D.	<MDL
15) B Endosulfa...	0.000	6.799	0	193434	N.D.	0.168
21) B Endrin ke...	6.805	0.000	2944790	0	3.459	N.D. #
23) Toxaphene-2	0.000	6.508	0	41140	N.D.	4.957


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033120\
Data File : PD057677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2020 11:16
Operator : AJ\MA
Sample : L2059-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 06:39:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031120CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 12 06:32:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

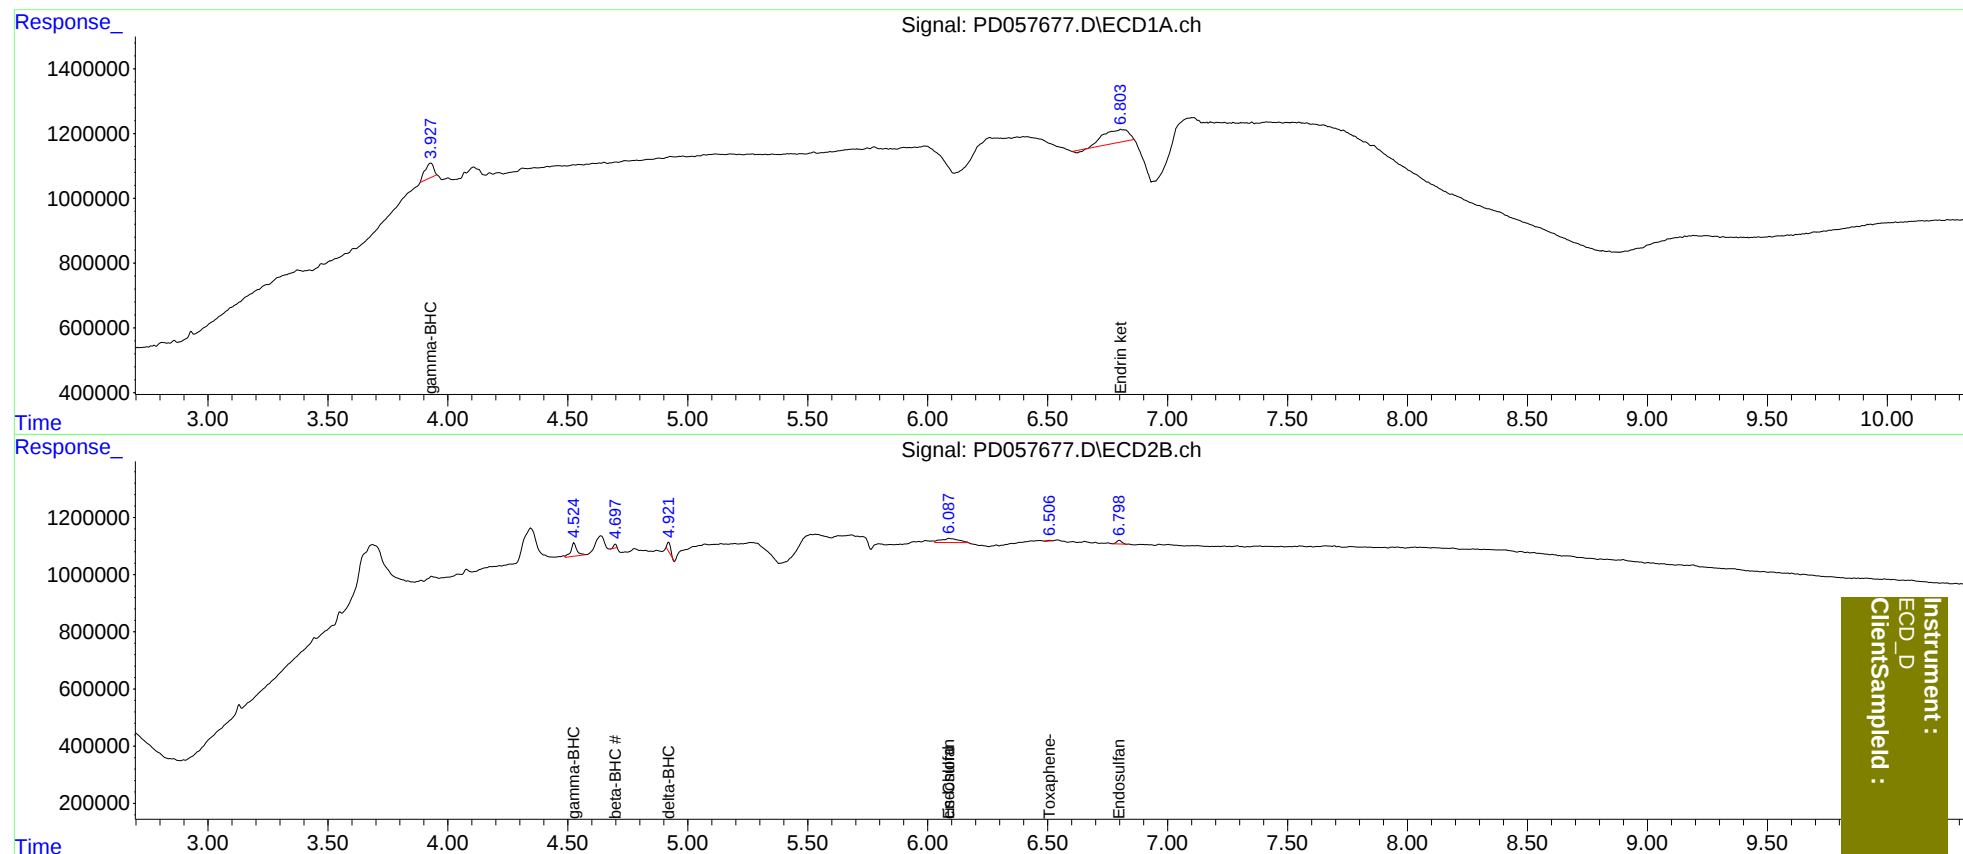


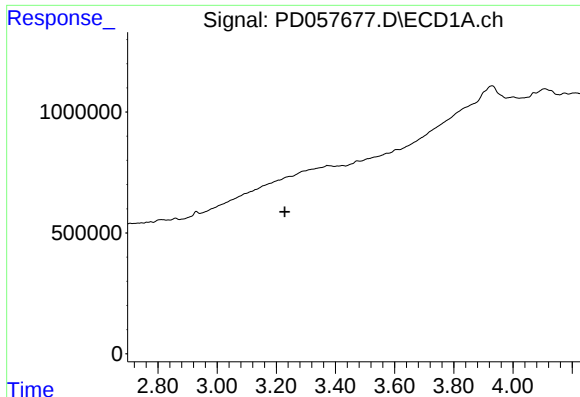

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

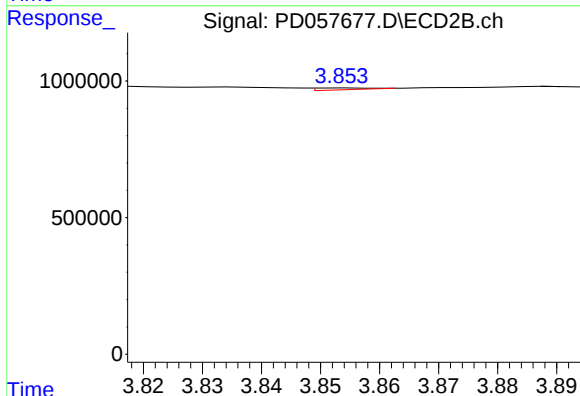


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.043 min
Response: 42959
Conc: N.D.

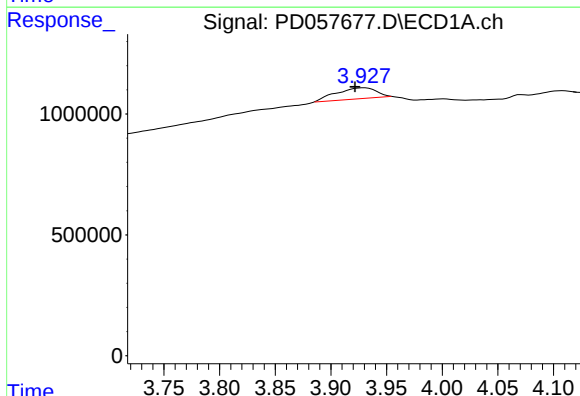


#3 gamma-BHC (Lindane)

R.T.: 3.930 min
Delta R.T.: 0.008 min
Response: 1170440
Conc: 0.94 ng/ml

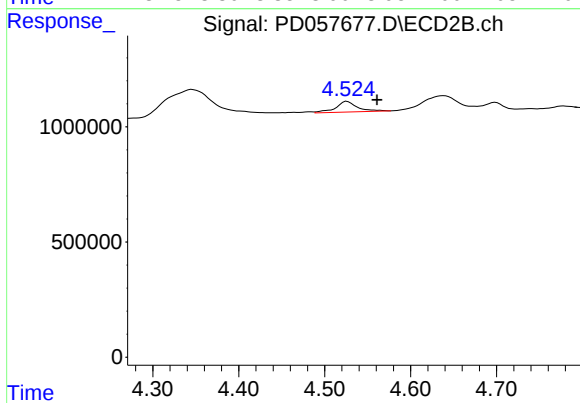

#3 gamma-BHC (Lindane)


R.T.: 4.526 min
Delta R.T.: -0.035 min
Response: 806759
Conc: 0.60 ng/ml

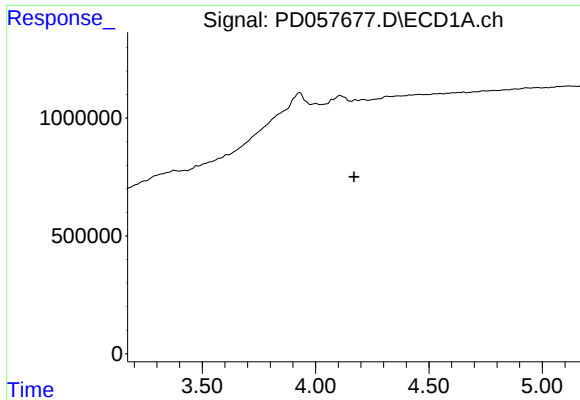

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

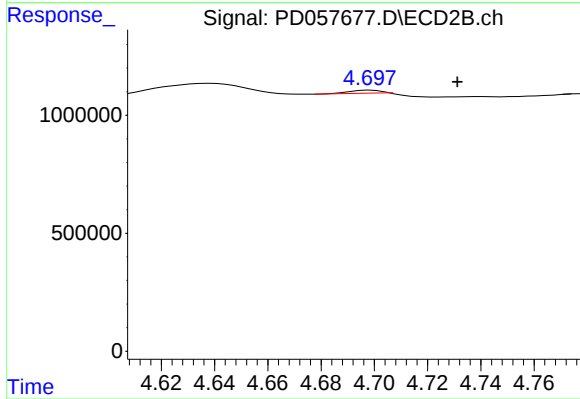


#6 beta-BHC

R.T.: 4.699 min
Delta R.T.: -0.032 min
Response: 153717
Conc: 0.24 ng/ml

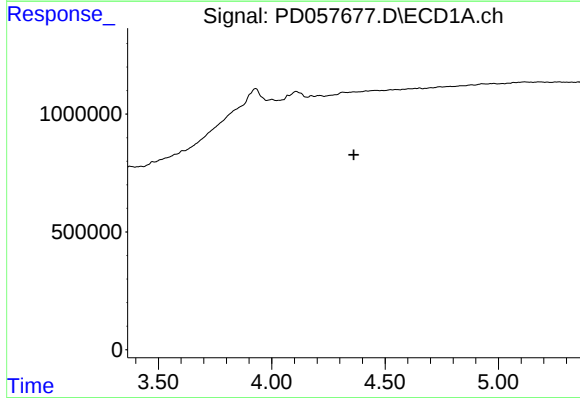


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.362 min
Response: 0
Conc: N.D.

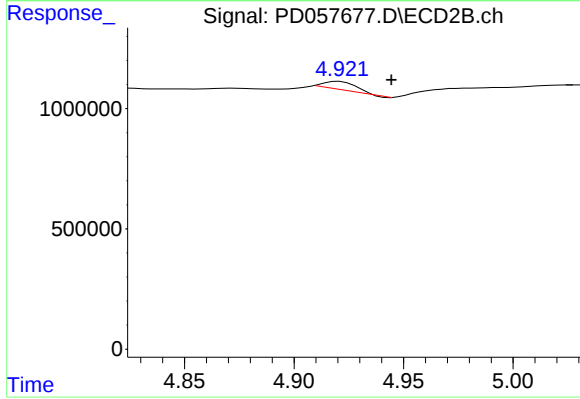

#7 delta-BHC


R.T.: 4.921 min
Delta R.T.: -0.024 min
Response: 342938
Conc: 0.25 ng/ml

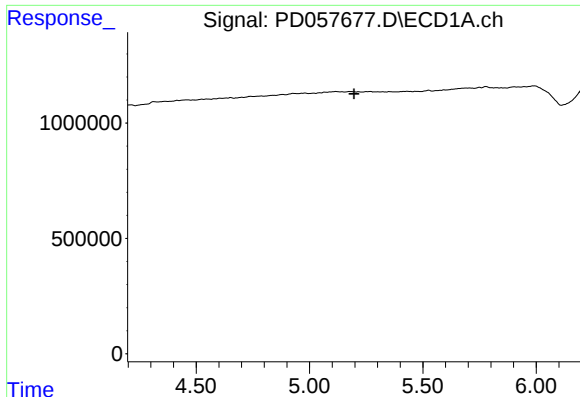

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

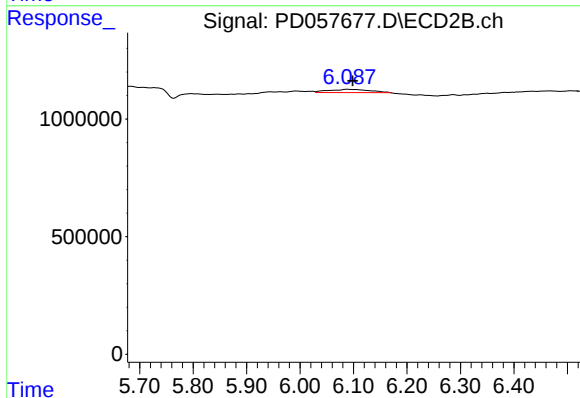


#9 Endosulfan I

R.T.: 6.089 min
Delta R.T.: -0.010 min
Response: 748885
Conc: 0.61 ng/ml

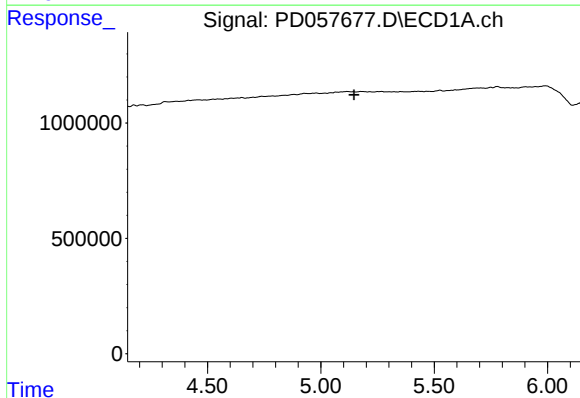


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.147 min
Response: 0
Conc: N.D.

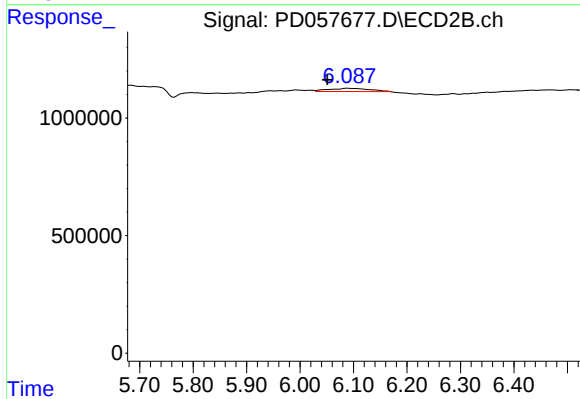

#11 cis-Chlordane


R.T.: 6.089 min
Delta R.T.: 0.038 min
Response: 748885
Conc: 0.55 ng/ml

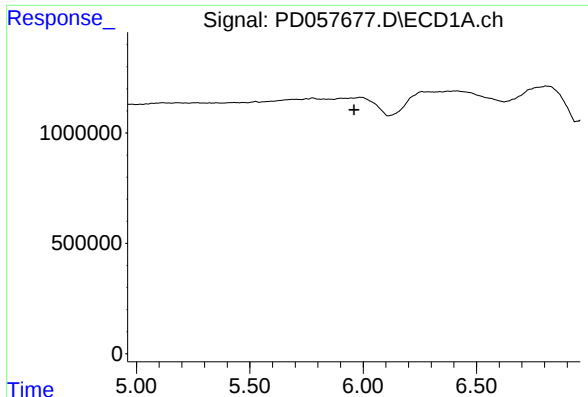

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

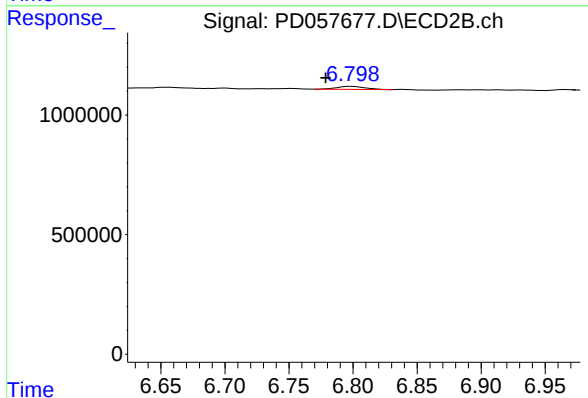


#15 Endosulfan II

R.T.: 6.799 min
Delta R.T.: 0.020 min
Response: 193434
Conc: 0.17 ng/ml

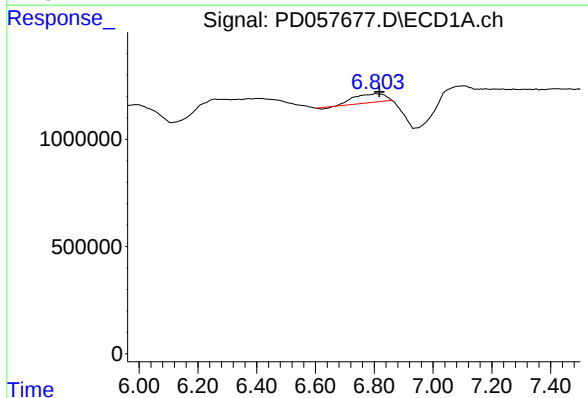


#21 Endrin ketone

R.T.: 6.805 min
Delta R.T.: -0.013 min
Response: 2944790
Conc: 3.46 ng/ml

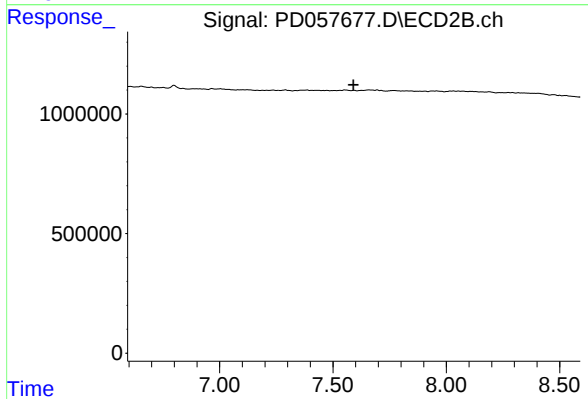

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.591 min
Response: 0
Conc: N.D.

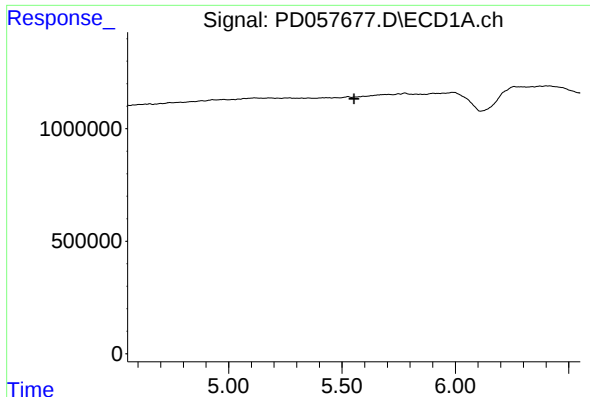

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 5.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

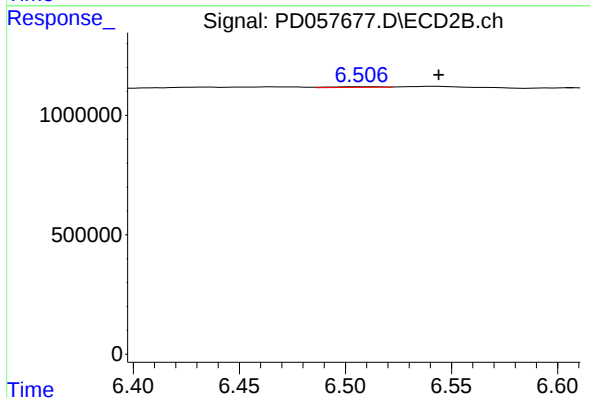


#23 Toxaphene-2

R.T.: 6.508 min
Delta R.T.: -0.036 min
Response: 41140
Conc: 4.96 ng/ml

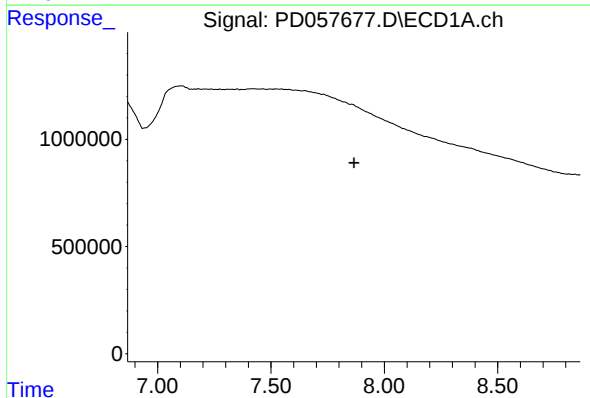

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.867 min
Response: 0
Conc: N.D.

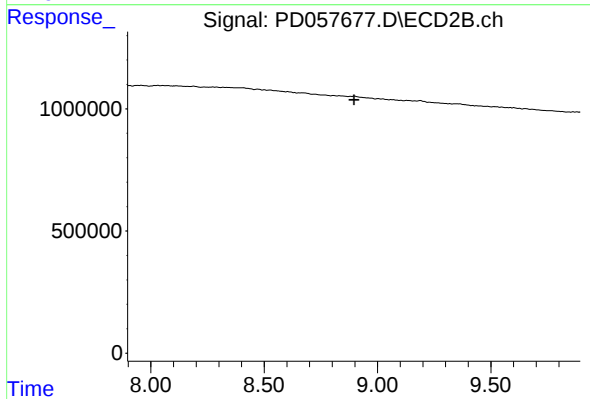

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.897 min
Response: 0
Conc: N.D.