

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
 Data File : PD061913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 09:12
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 14:25:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	0.000	5.465	0	3145292	N.D.	0.253 #
7) B delta-BHC	0.000	5.027	0	61907155	N.D.	4.680 #
8) B Heptachlo...	0.000	5.848	0	103.9E6	N.D.	8.773 #
10) B gamma-Chl...	0.000	6.095	0	11882438	N.D.	1.002 #
11) B alpha-Chl...	0.000	6.161	0	3216051	N.D.	0.282 #
17) MA 4,4'-DDT	0.000	7.077f	0	25581653	N.D.	2.678 #
18) B Endrin al...	6.490	6.988f	3523876	11458662	4.125	1.457 #
21) B Endrin ke...	0.000	7.734f	0	4017800	N.D.	0.396 #
24) Chlordane-2	0.000	5.465f	0	3145292	N.D.	8.197 #
25) Chlordane-3	0.000	6.095	0	11882438	N.D.	7.168 #
26) Chlordane-4	0.000	6.161	0	3216051	N.D.	1.676 #
27) Chlordane-5	0.000	6.962	0	10862199	N.D.	30.139 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
Data File : PD061913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 09:12
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 14:25:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

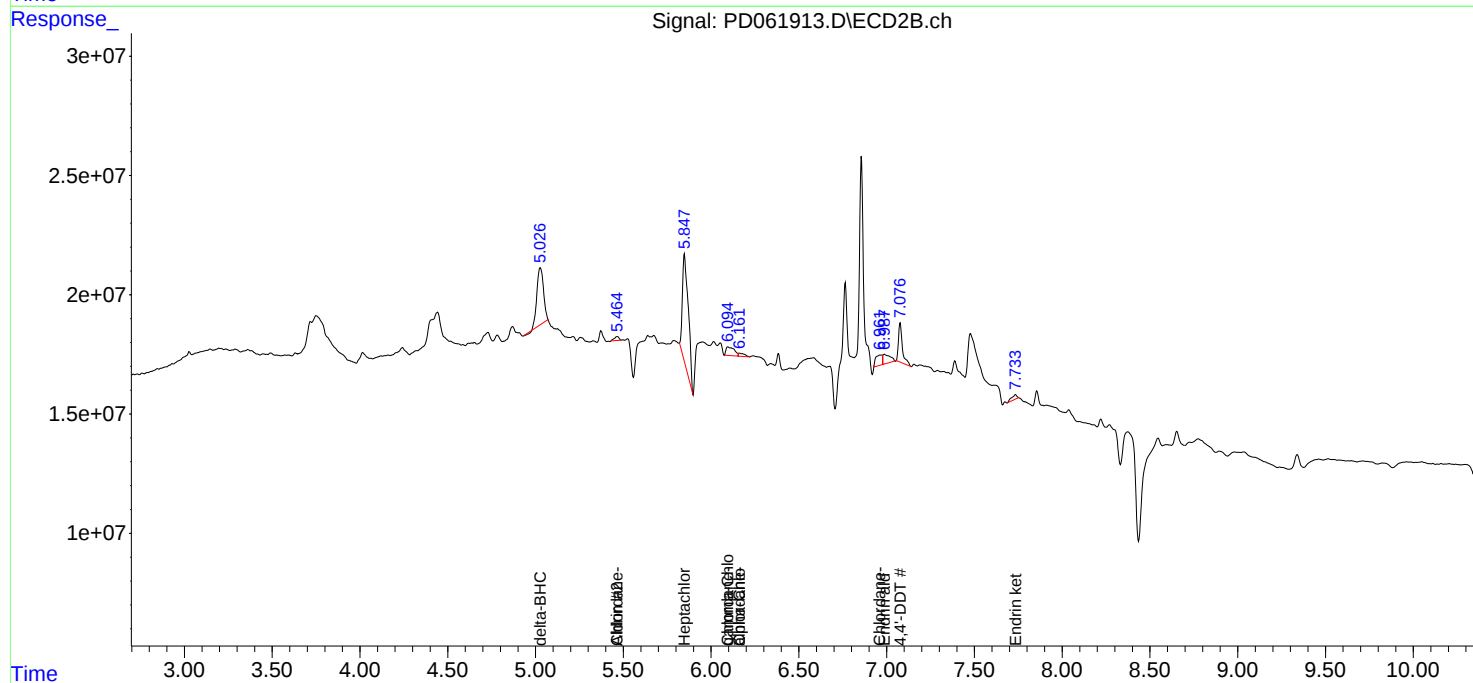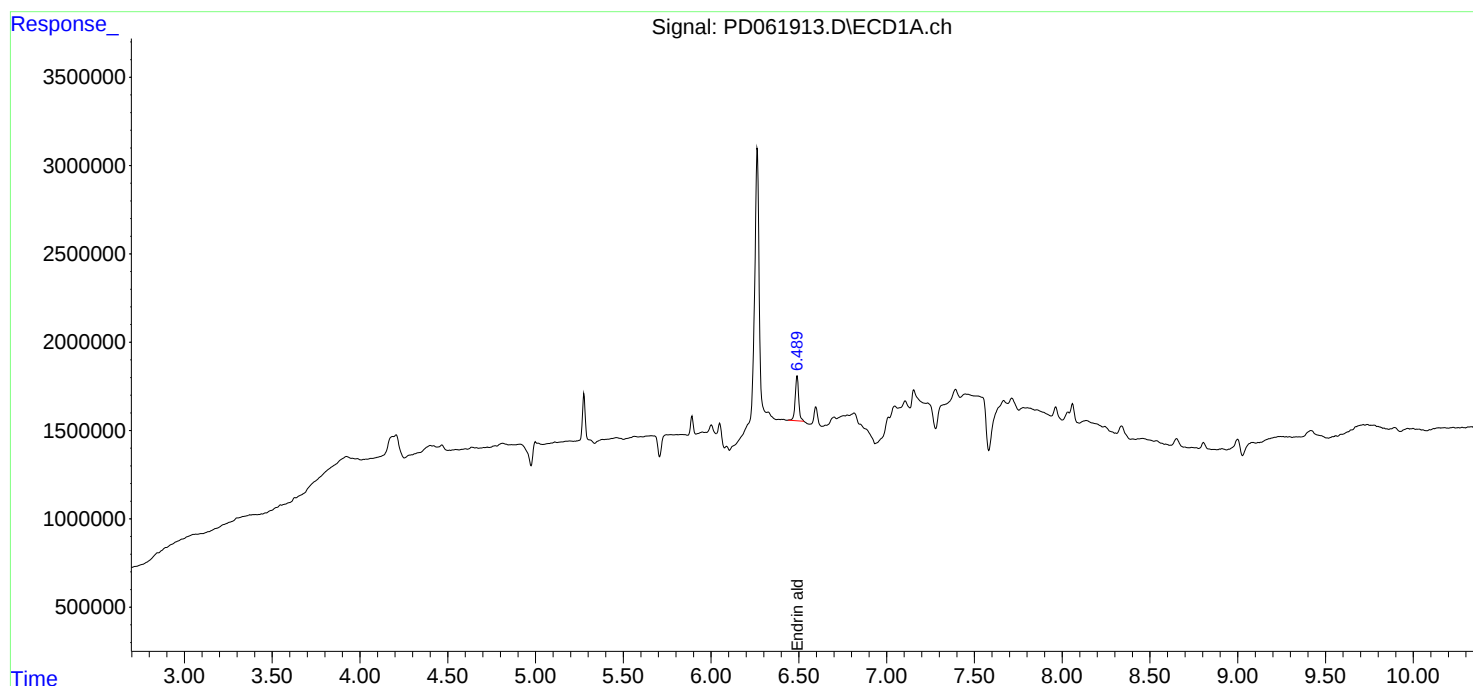


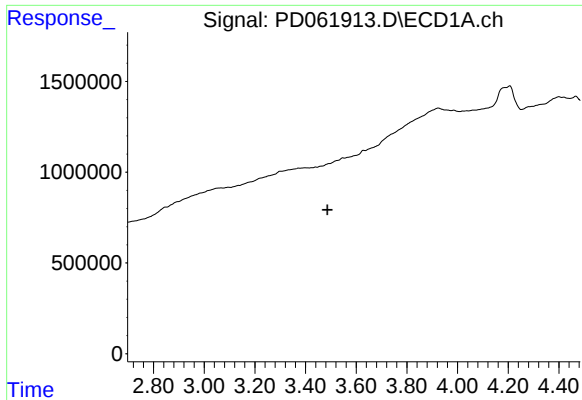

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

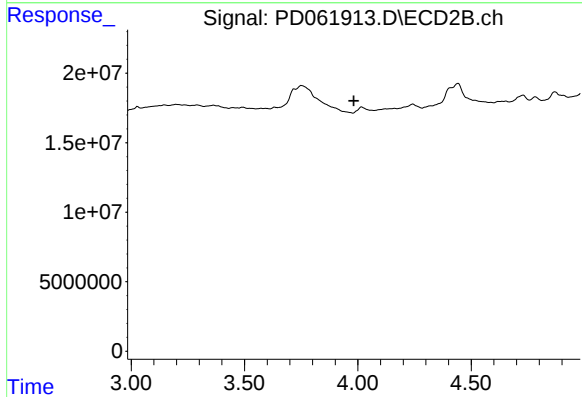


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.982 min
Response: 0
Conc: N.D.

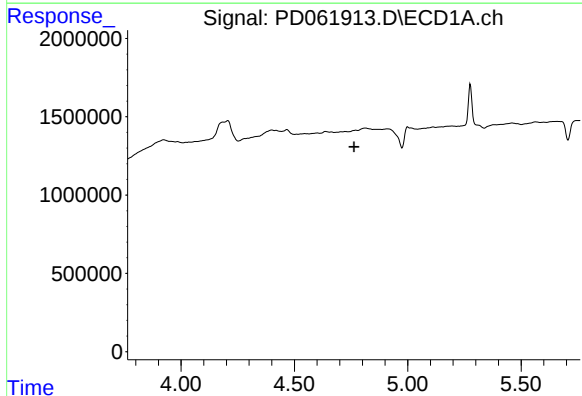


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

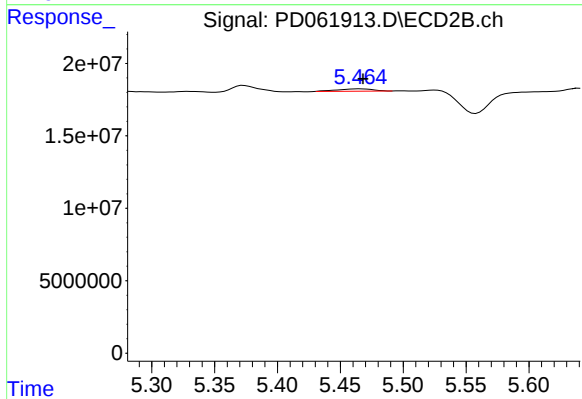

#5 Aldrin


R.T.: 5.465 min
Delta R.T.: -0.003 min
Response: 3145292
Conc: 0.25 ng/ml

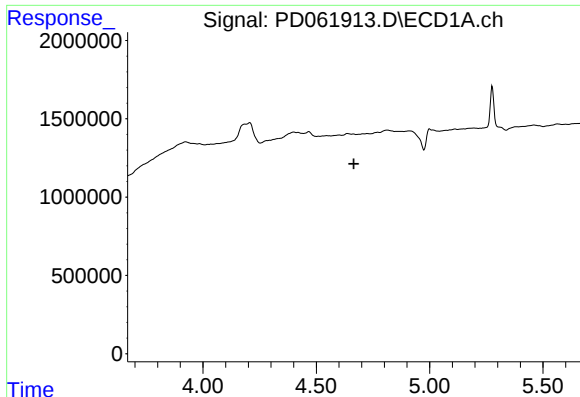

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

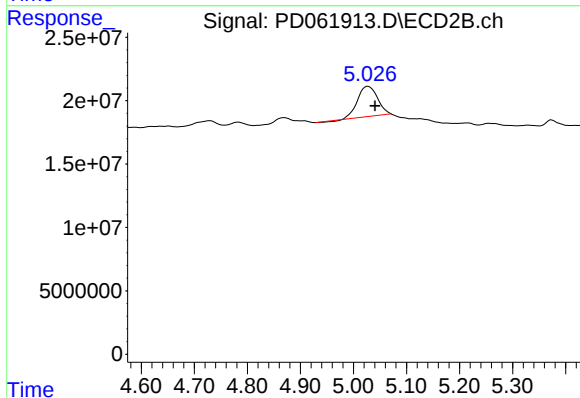


#7 delta-BHC

R.T.: 5.027 min
Delta R.T.: -0.014 min
Response: 61907155
Conc: 4.68 ng/ml

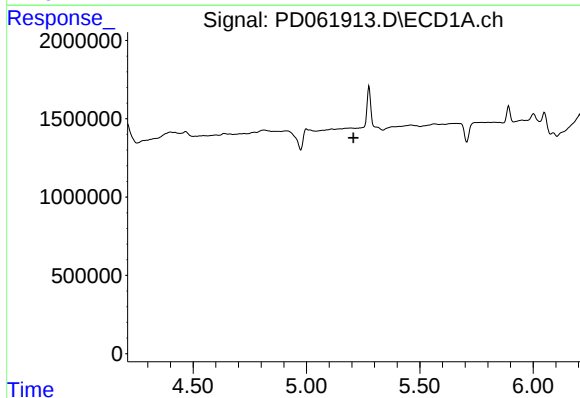


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

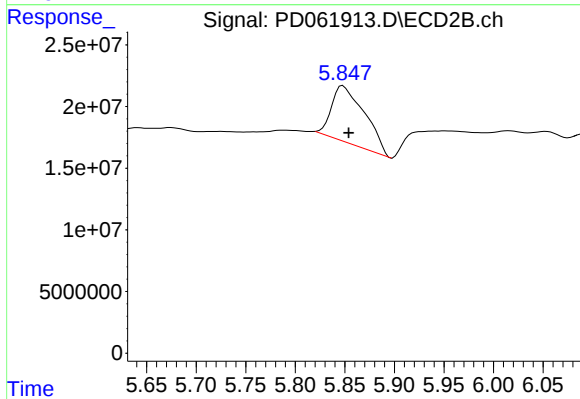

#8 Heptachlor epoxide


R.T.: 5.848 min
Delta R.T.: -0.006 min
Response: 103885614
Conc: 8.77 ng/ml

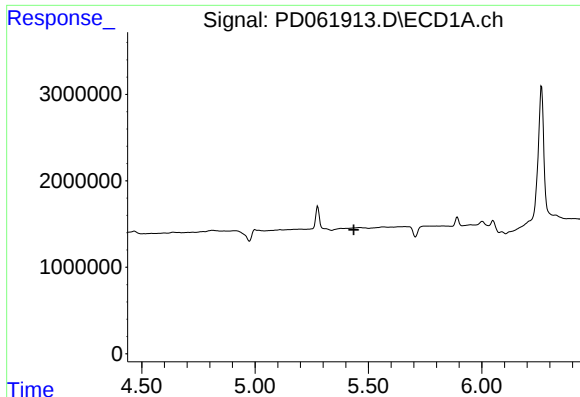

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

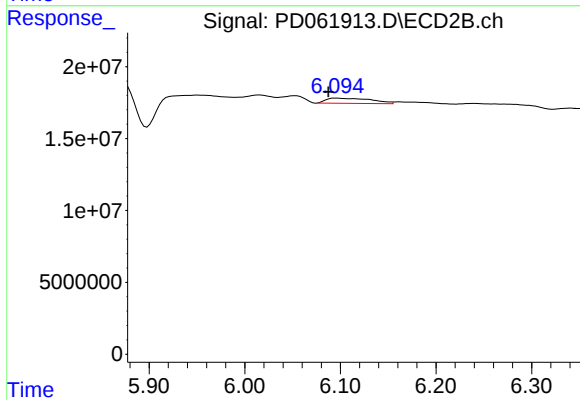


#10 gamma-Chlordane

R.T.: 6.095 min
Delta R.T.: 0.008 min
Response: 11882438
Conc: 1.00 ng/ml

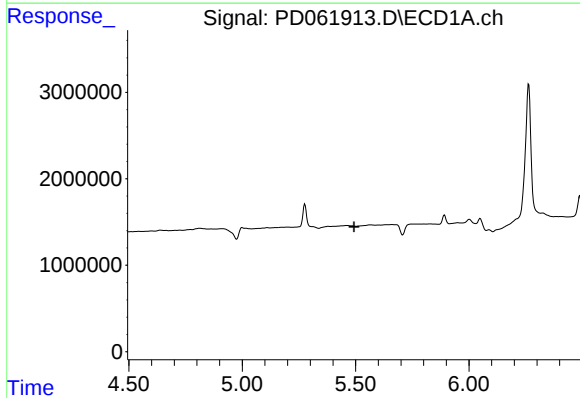


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.494 min
Response: 0
Conc: N.D.

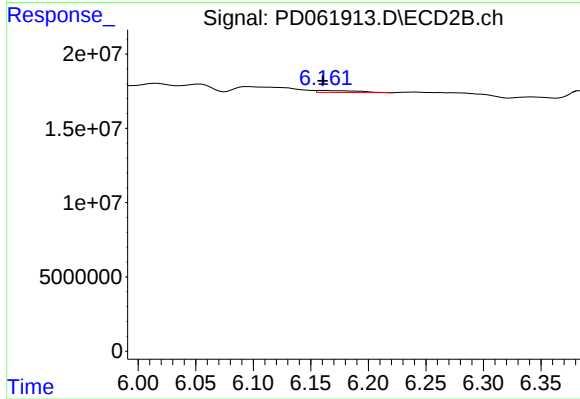

#11 alpha-Chlordane


R.T.: 6.161 min
Delta R.T.: 0.001 min
Response: 3216051
Conc: 0.28 ng/ml

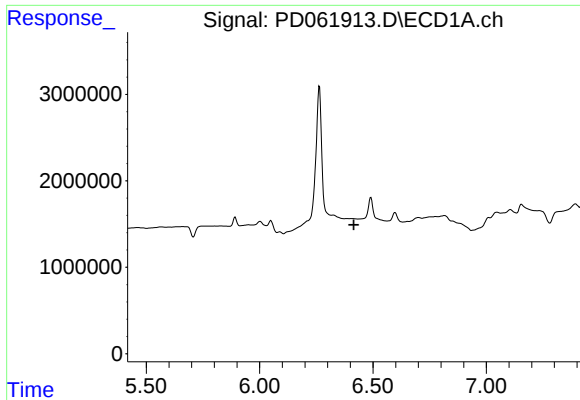

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

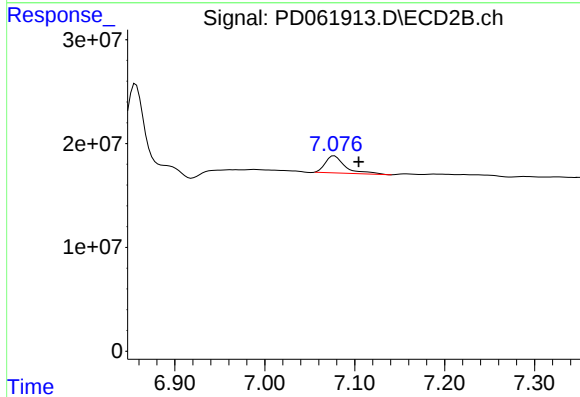


#17 4,4'-DDT

R.T.: 7.077 min
Delta R.T.: -0.027 min
Response: 25581653
Conc: 2.68 ng/ml

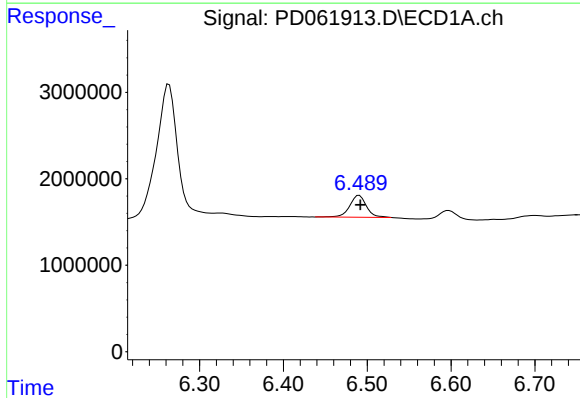


#18 Endrin aldehyde

R.T.: 6.490 min
Delta R.T.: -0.001 min
Response: 3523876
Conc: 4.12 ng/ml

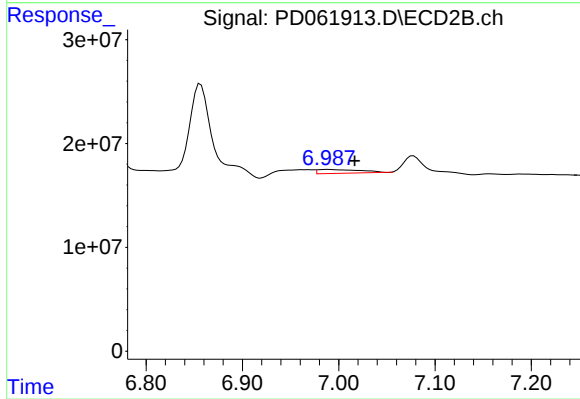

#18 Endrin aldehyde


R.T.: 6.988 min
Delta R.T.: -0.028 min
Response: 11458662
Conc: 1.46 ng/ml

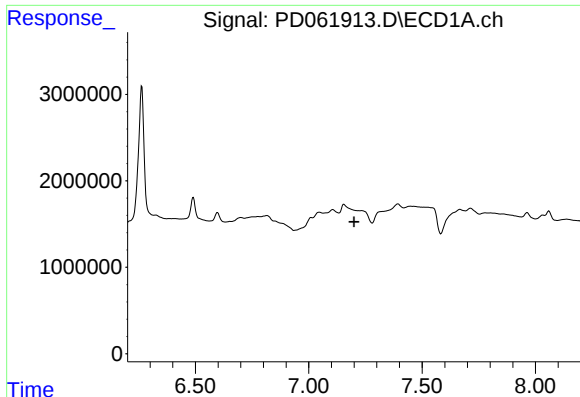

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

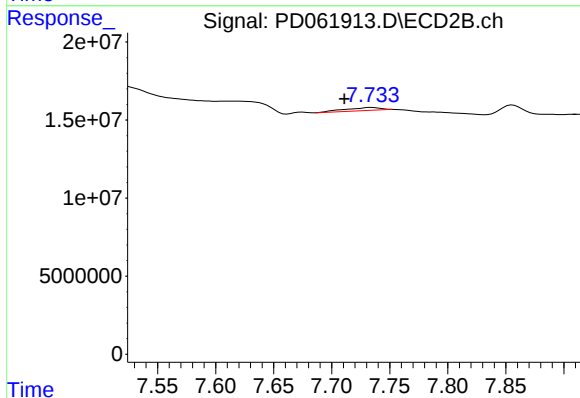


#21 Endrin ketone

R.T.: 7.734 min
Delta R.T.: 0.023 min
Response: 4017800
Conc: 0.40 ng/ml

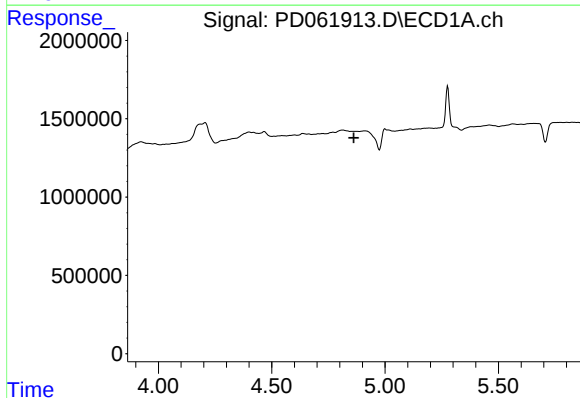


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

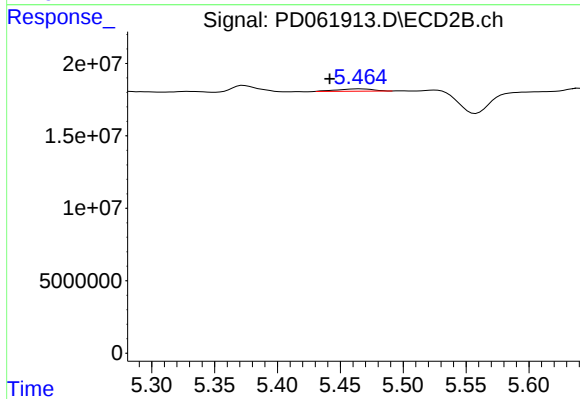

#24 Chlordane-2


R.T.: 5.465 min
Delta R.T.: 0.024 min
Response: 3145292
Conc: 8.20 ng/ml

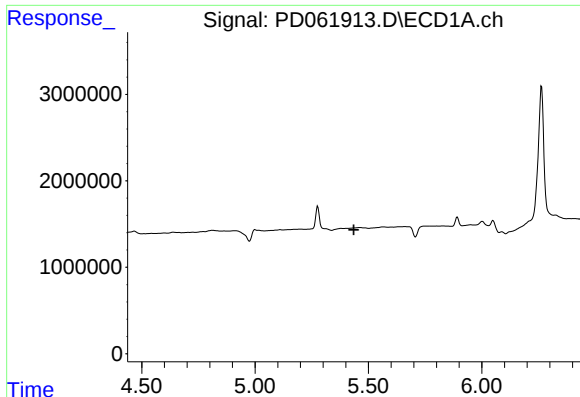

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

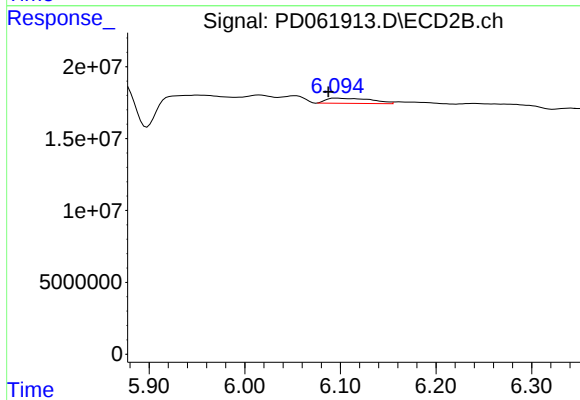


#25 Chlordane-3

R.T.: 6.095 min
Delta R.T.: 0.008 min
Response: 11882438
Conc: 7.17 ng/ml

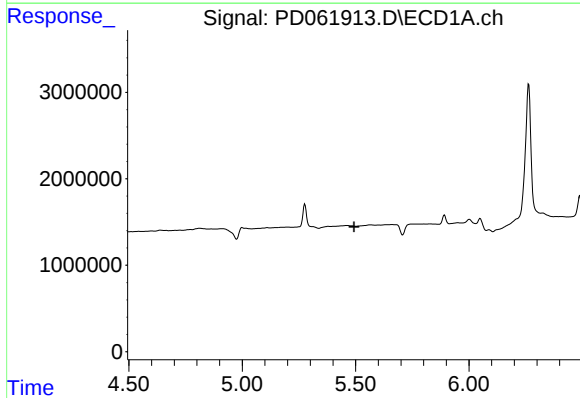


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

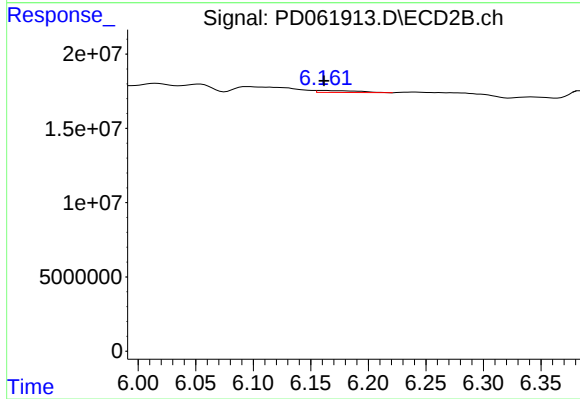

#26 Chlordane-4


R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 3216051
Conc: 1.68 ng/ml

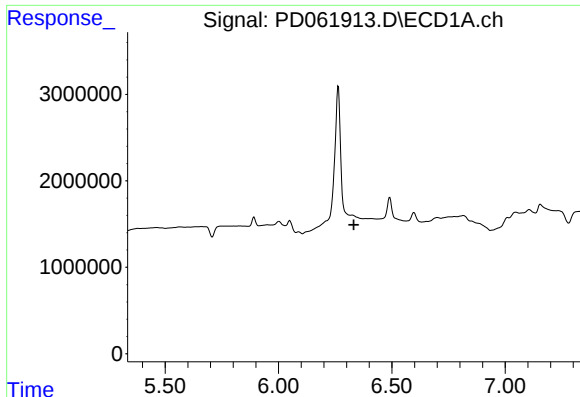

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

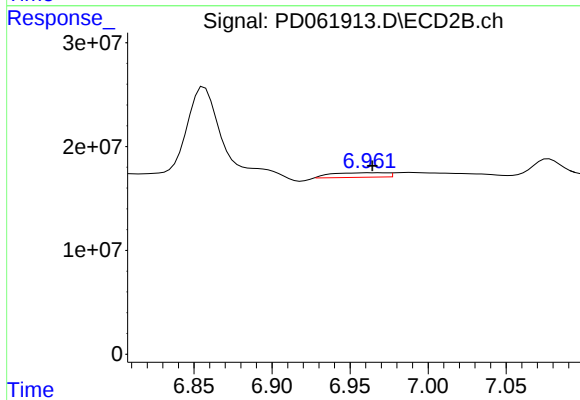


#27 Chlordane-5

R.T.: 6.962 min
Delta R.T.: -0.002 min
Response: 10862199
Conc: 30.14 ng/ml

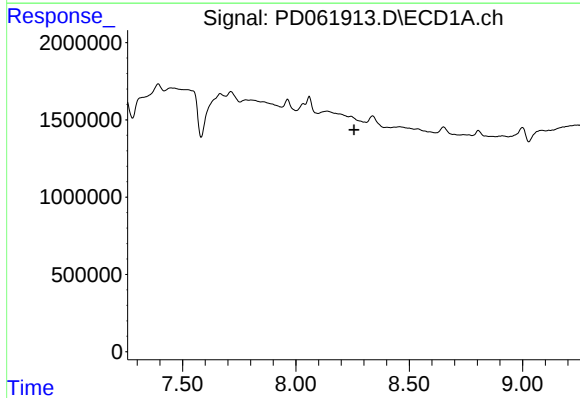

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.257 min
Response: 0
Conc: N.D.

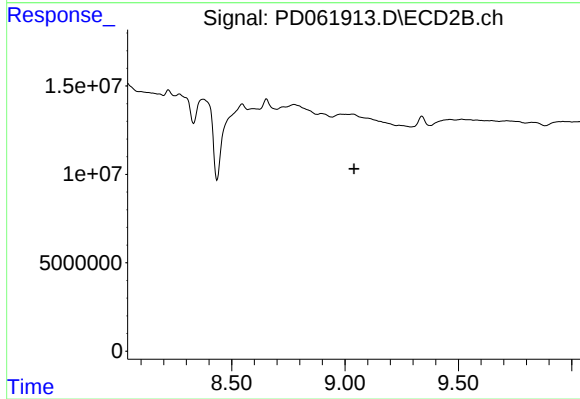

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.040 min
Response: 0
Conc: N.D.