

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
 Data File : PD061917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 10:26
 Operator : AR\AJ
 Sample : M1823-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MK-3-29-B1

Manual Integrations
 APPROVED

Ankita
 4/1/2021 1:47:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 14:25:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.488	3.980	11458699	118.4E6	13.685	13.624m
28)	SA Decachlor...	8.261	9.041	15087290	107.6E6	12.262	11.398

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
Data File : PD061917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 10:26
Operator : AR\AJ
Sample : M1823-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
MK-3-29-B1


Manual Integrations
APPROVED

Ankita
4/1/2021 1:47:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 14:25:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

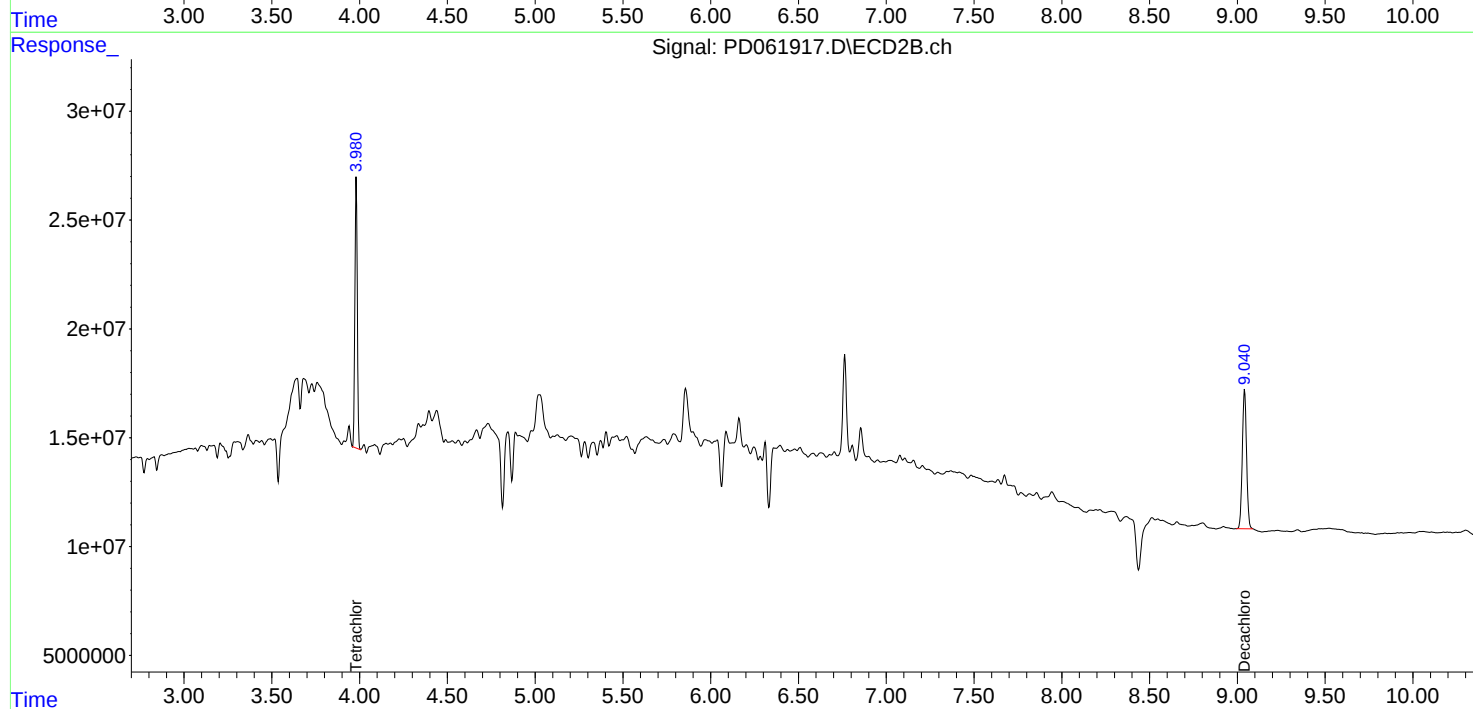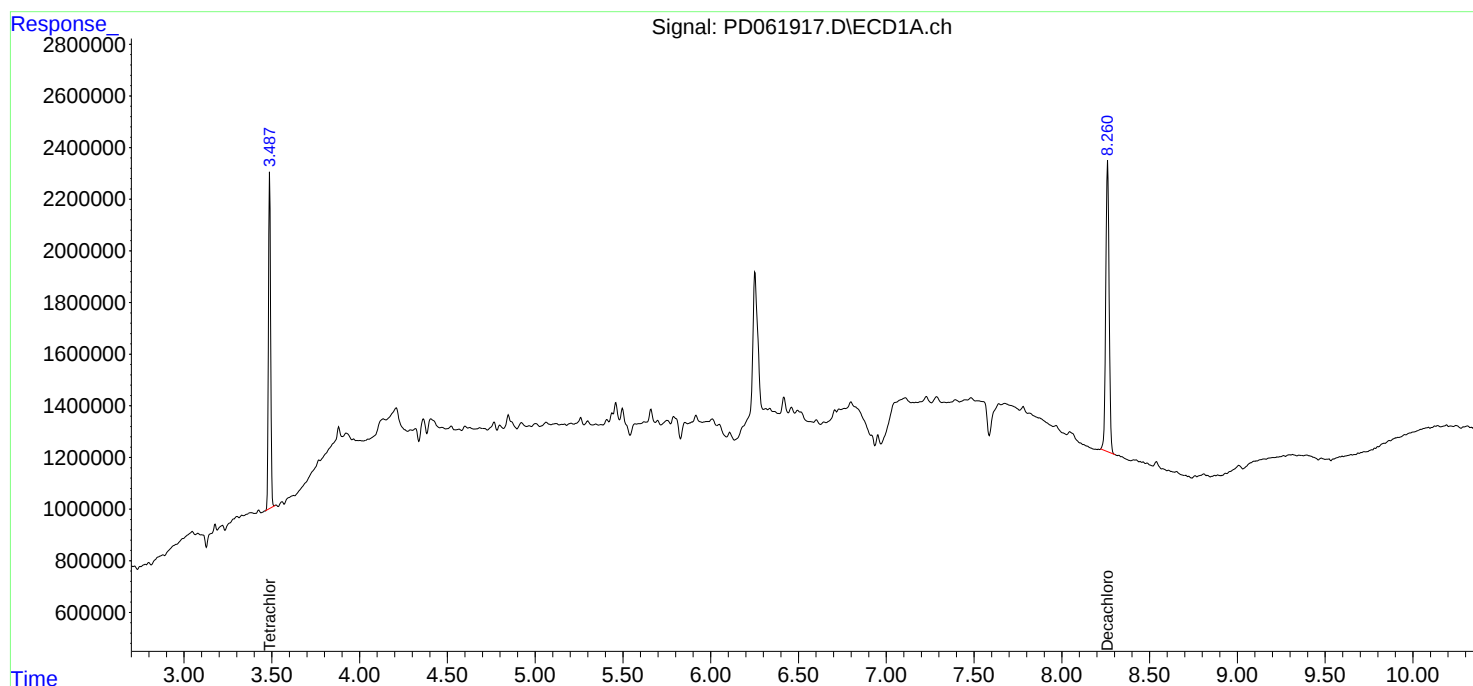

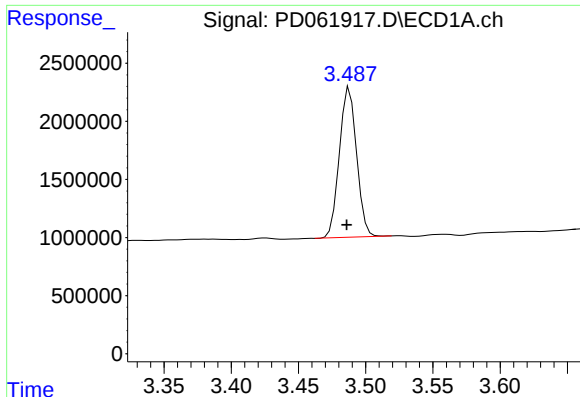


#1 Tetrachloro-m-xylene

R.T.: 3.488 min
Delta R.T.: 0.002 min
Response: 11458699
Conc: 13.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
MK-3-29-B1


Manual Integrations
APPROVED

Ankita
4/1/2021 1:47:03 PM

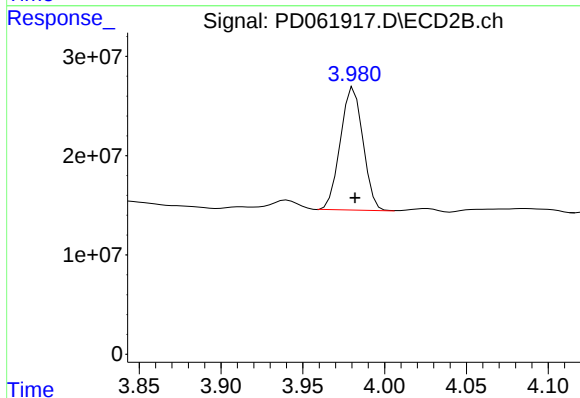


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 118373289
Conc: 13.62 ng/ml m

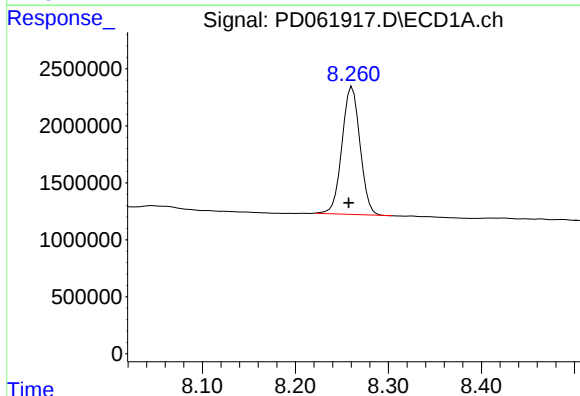

#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: 0.004 min
Response: 15087290
Conc: 12.26 ng/ml

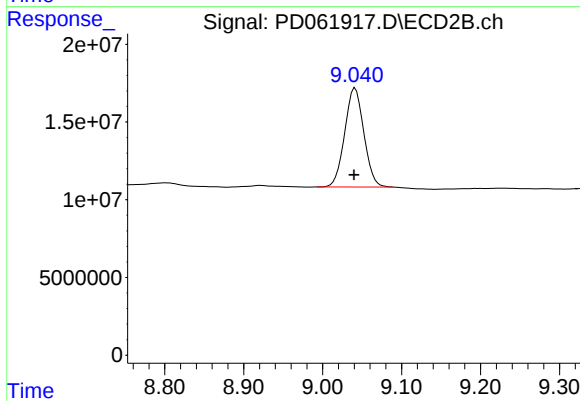

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 107607550
Conc: 11.40 ng/ml