

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
 Data File : PD061928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 13:50
 Operator : AR\AJ
 Sample : M1832-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 IG003

Manual Integrations
 APPROVED

Ankita
 4/2/2021 10:15:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 09:35:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.982	18050919	185.6E6	21.559m	21.359
28)	SA Decachlor...	8.264	9.043	21758514	156.0E6	17.684	16.526
Target Compounds							
17)	MA 4,4'-DDT	6.420	7.104	1733296	10907787	1.924m	1.142m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033121\
Data File : PD061928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 13:50
Operator : AR\AJ
Sample : M1832-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
IG003


Manual Integrations
APPROVED

Ankita
4/2/2021 10:15:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 09:35:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

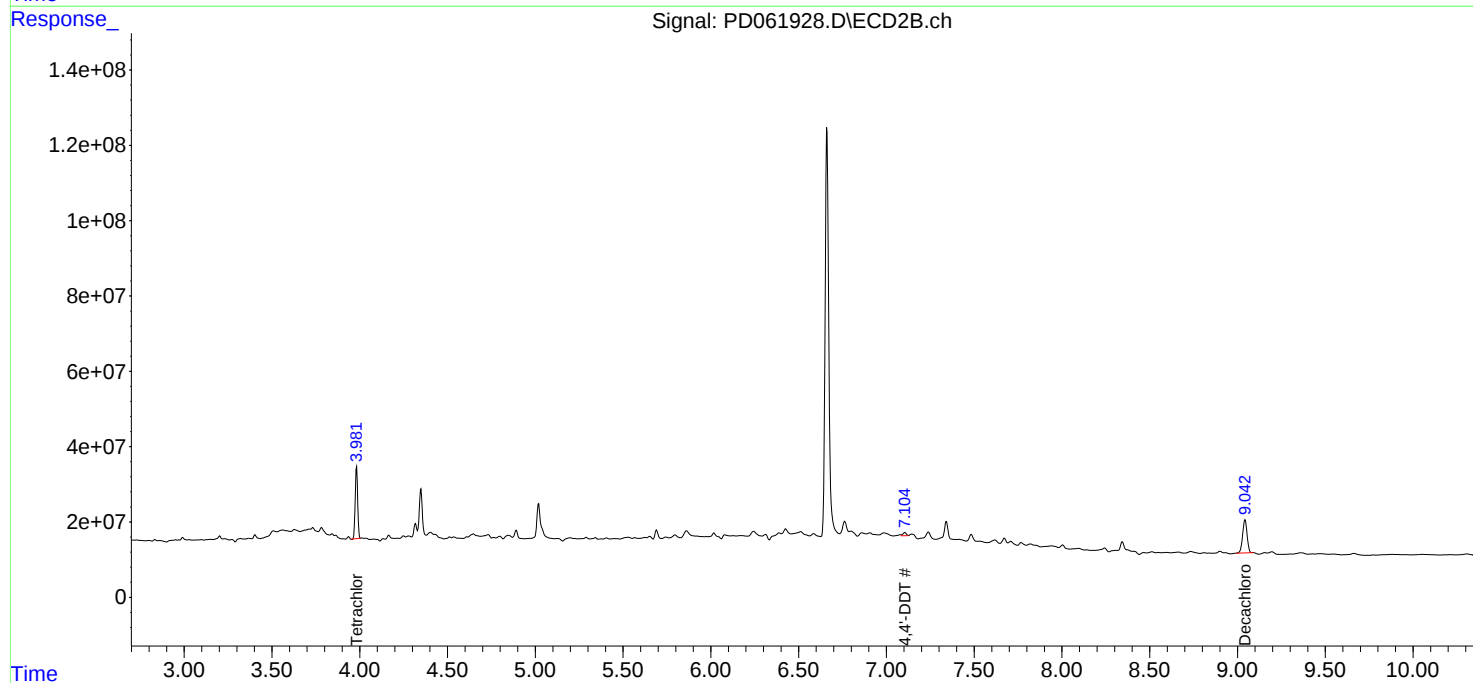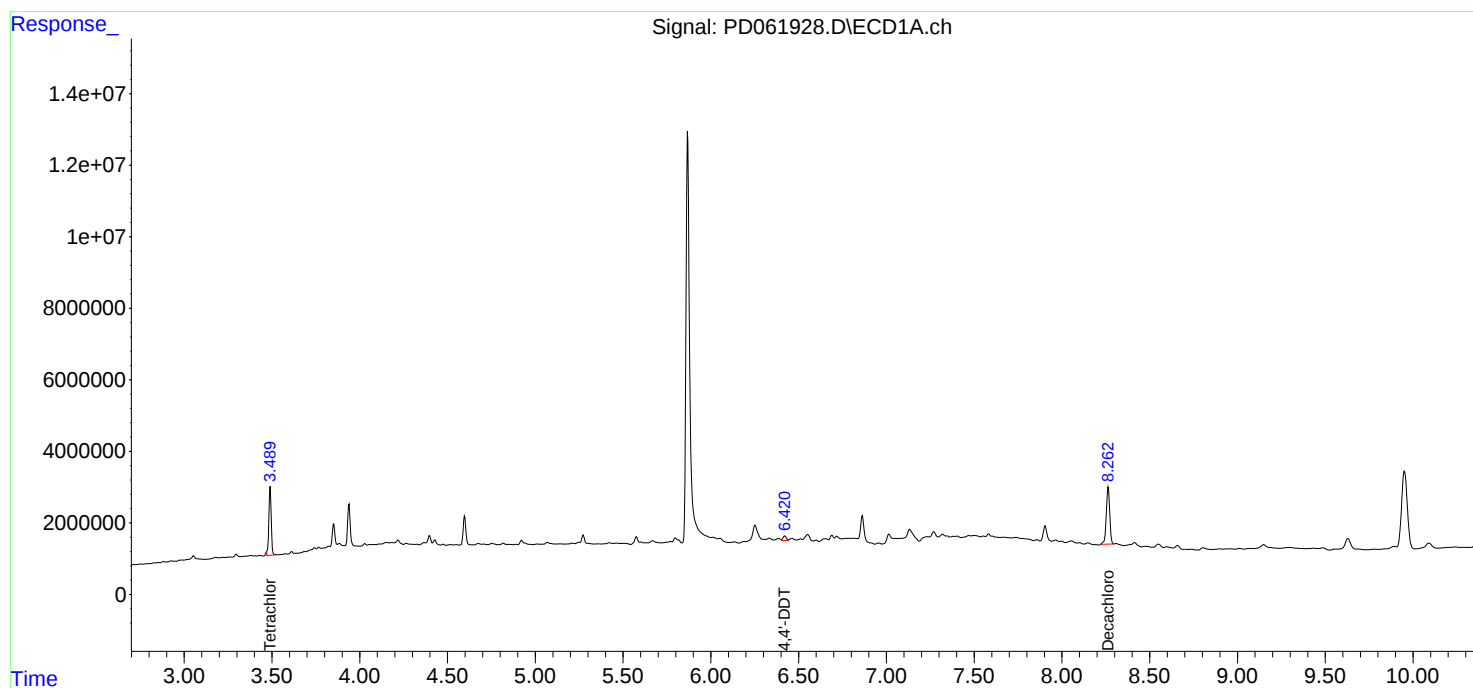

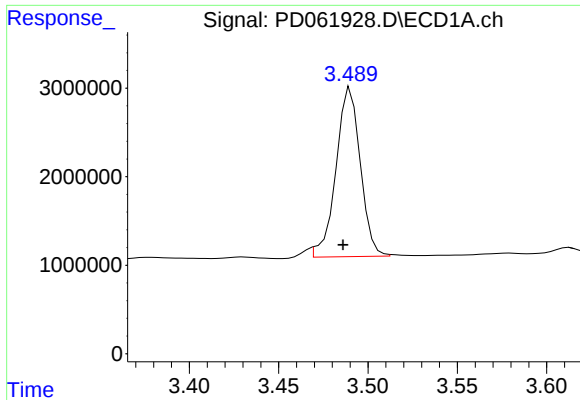


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: 0.003 min
Response: 18050919
Conc: 21.56 ng/ml m

Instrument :
ECD_D
ClientSampleId :
IG003


Manual Integrations
APPROVED

Ankita
4/2/2021 10:15:37 AM

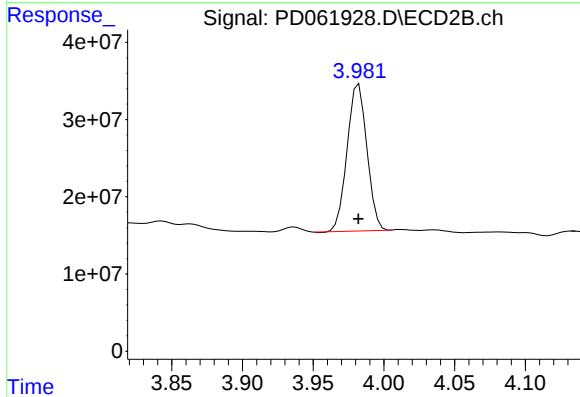


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 185582426
Conc: 21.36 ng/ml

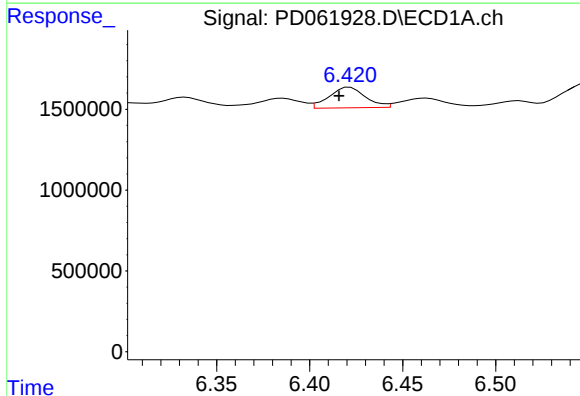


#17 4,4'-DDT

R.T.: 6.420 min
Delta R.T.: 0.004 min
Response: 1733296
Conc: 1.92 ng/ml m

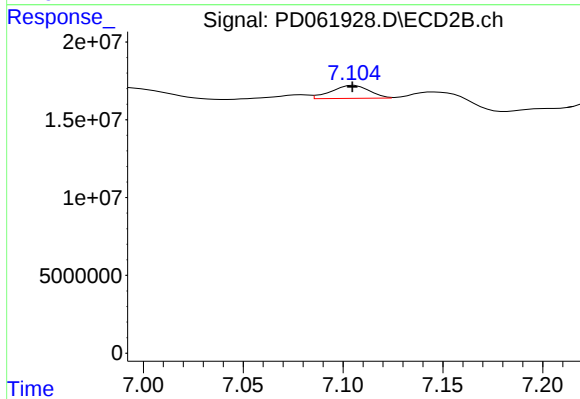

#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 10907787
Conc: 1.14 ng/ml m

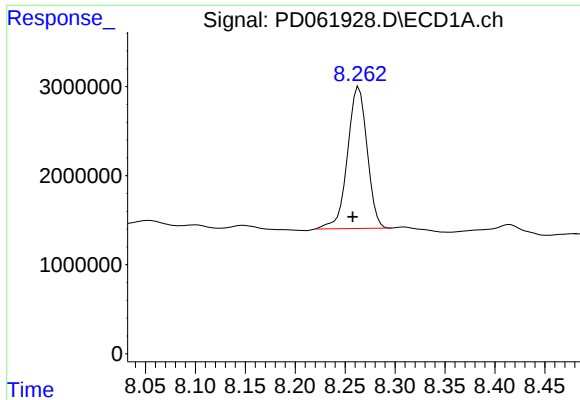


#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: 0.006 min
Response: 21758514
Conc: 17.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
IG003

Manual Integrations
APPROVED

Ankita
4/2/2021 10:15:37 AM

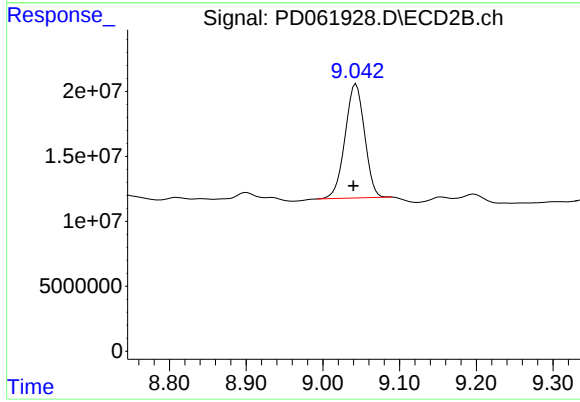

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.003 min
Response: 156010595
Conc: 16.53 ng/ml