

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033122\
 Data File : PD068833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 16:51
 Operator : AR\AJ
 Sample : PB143717BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:49:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.172	22841512	199.9E6	18.812	20.905
28)	SA Decachlor...	8.206	9.368	26163650	129.8E6	20.709	22.911
Target Compounds							
2)	A alpha-BHC	0.000	4.551f	0	160242	N.D.	0.012 #
5)	MB Aldrin	0.000	5.691	0	230026	N.D.	0.020 #
6)	B beta-BHC	0.000	5.027	0	41343	N.D.	0.008 #
7)	B delta-BHC	0.000	5.228f	0	2238500	N.D.	0.186 #
19)	B Endosulfa...	6.672	0.000	99538	0	0.078	N.D. #
21)	B Endrin ke...	0.000	7.966	0	1021260	N.D.	0.132 #
23)	Chlordane-1	4.344f	0.000	190954	0	4.500	N.D. #
24)	Chlordane-2	0.000	5.691f	0	230026	N.D.	0.602 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033122\
Data File : PD068833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 16:51
Operator : AR\AJ
Sample : PB143717BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:49:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

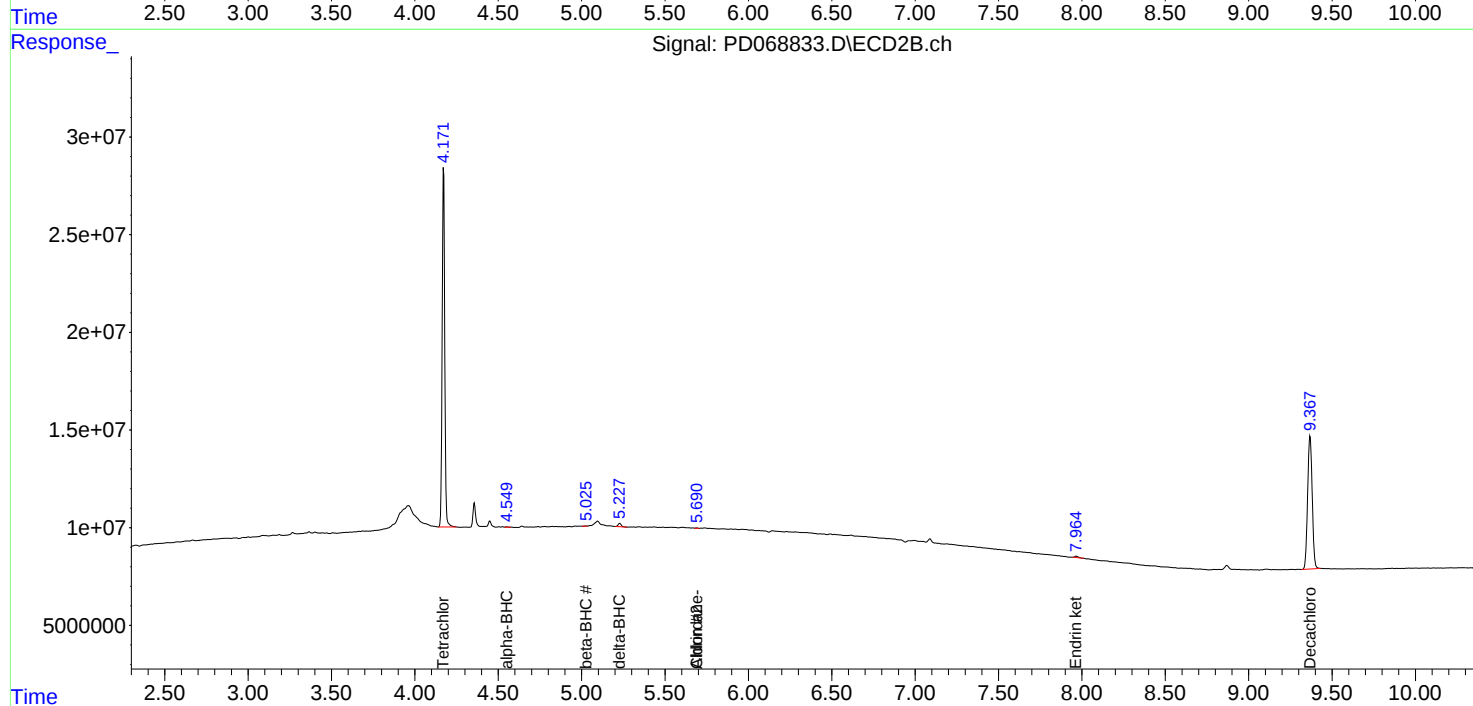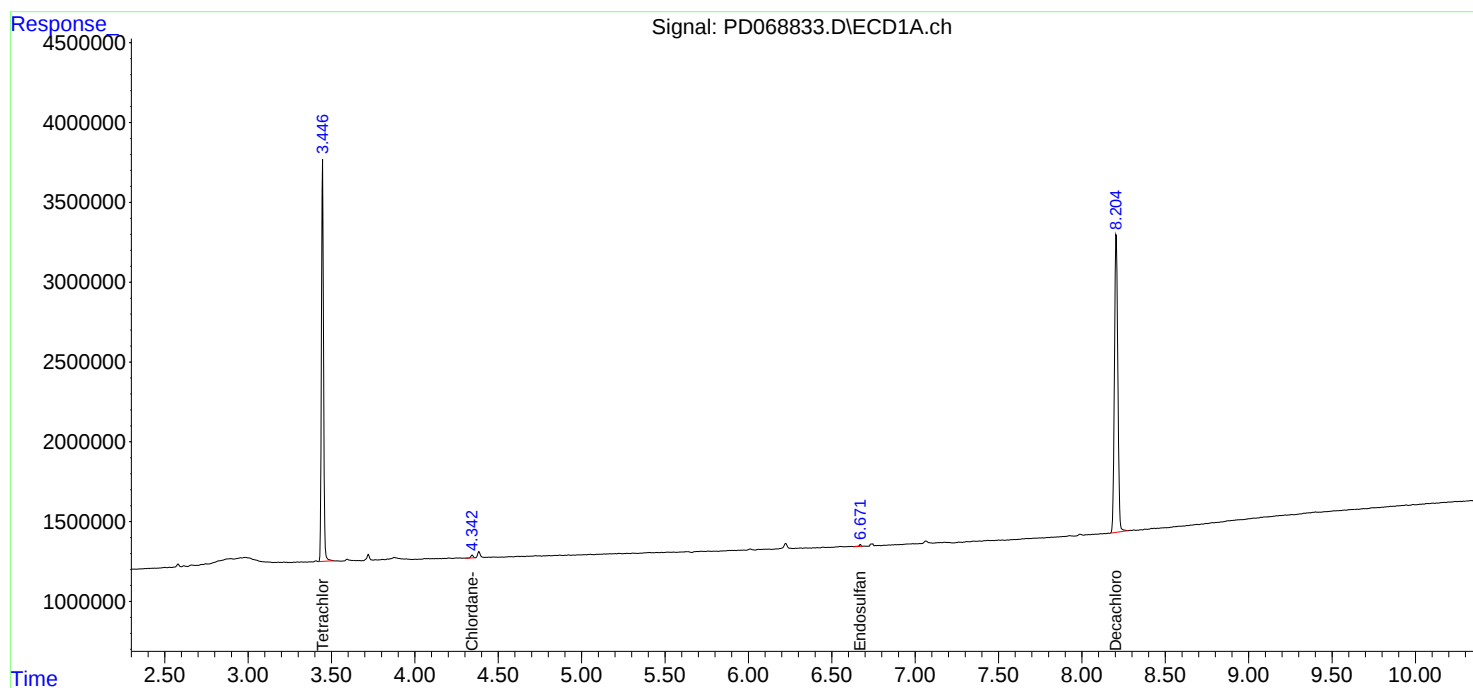


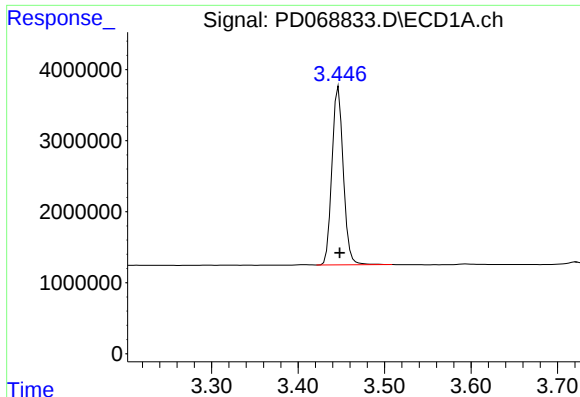

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: -0.001 min
Response: 22841512
Conc: 18.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

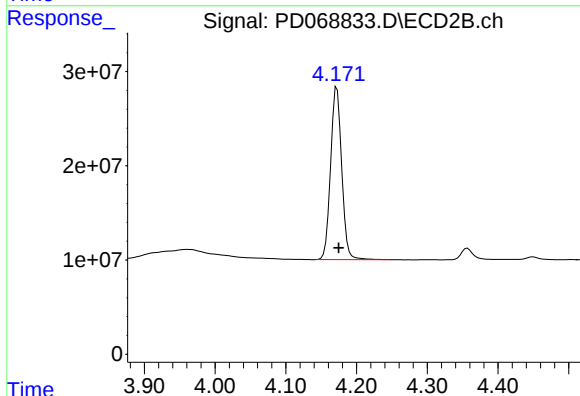


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.002 min
Response: 199867683
Conc: 20.91 ng/ml

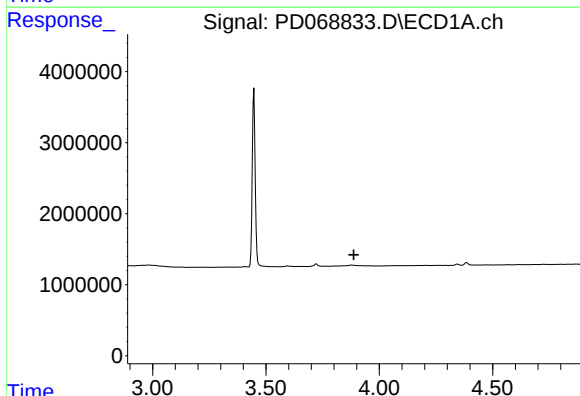


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

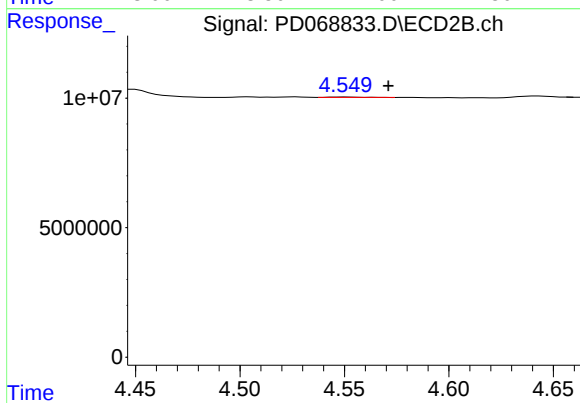

#2 alpha-BHC


R.T.: 4.551 min
Delta R.T.: -0.020 min
Response: 160242
Conc: 0.01 ng/ml

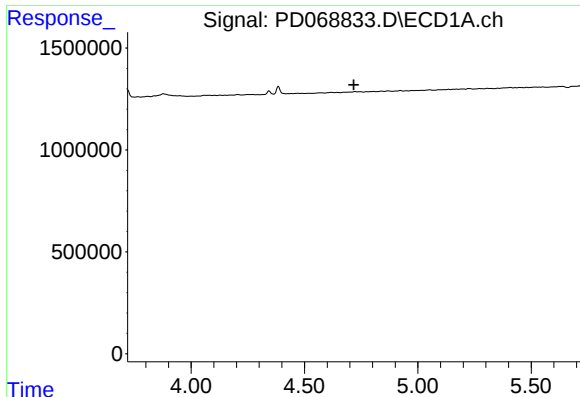

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.718 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

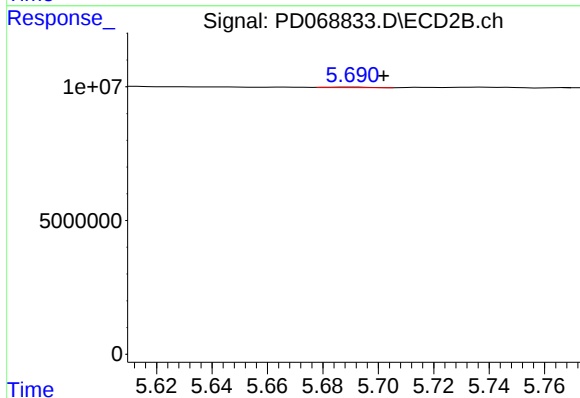


#5 Aldrin

R.T.: 5.691 min
Delta R.T.: -0.011 min
Response: 230026
Conc: 0.02 ng/ml

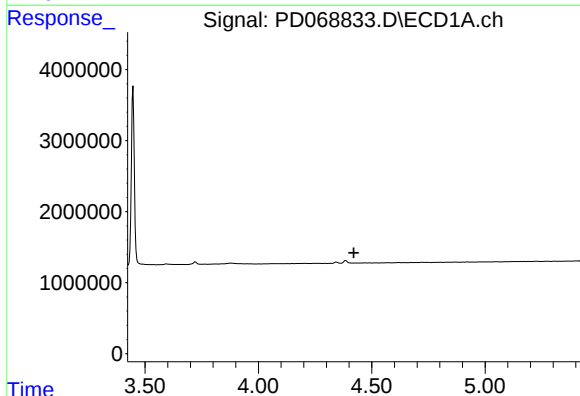


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.421 min
Response: 0
Conc: N.D.

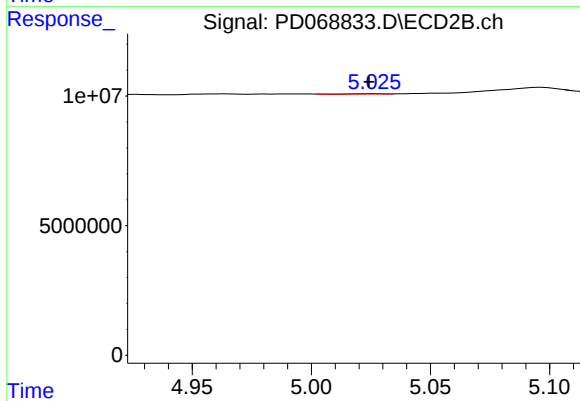

#6 beta-BHC


R.T.: 5.027 min
Delta R.T.: 0.002 min
Response: 41343
Conc: 0.01 ng/ml

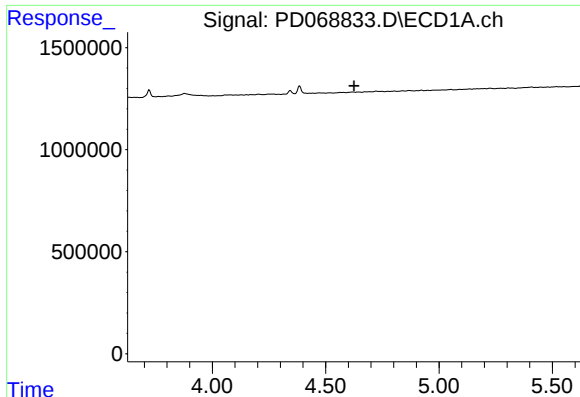

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

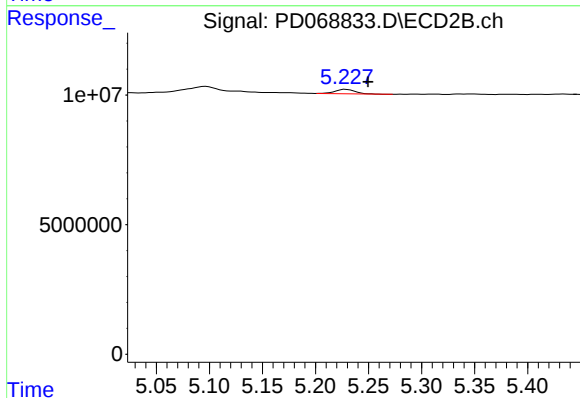


#7 delta-BHC

R.T.: 5.228 min
Delta R.T.: -0.021 min
Response: 2238500
Conc: 0.19 ng/ml

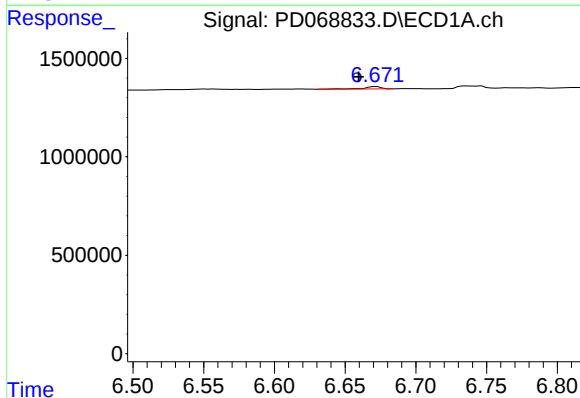


#19 Endosulfan Sulfate

R.T.: 6.672 min
Delta R.T.: 0.012 min
Response: 99538
Conc: 0.08 ng/ml

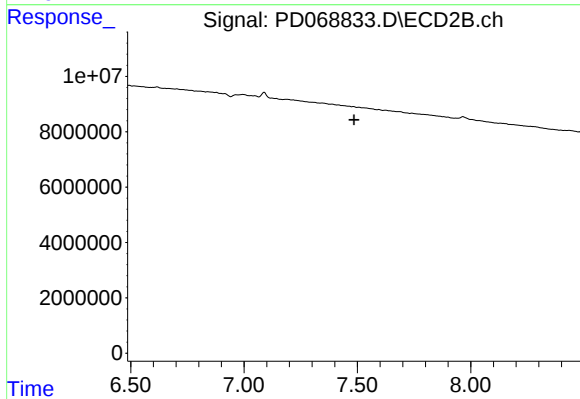

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

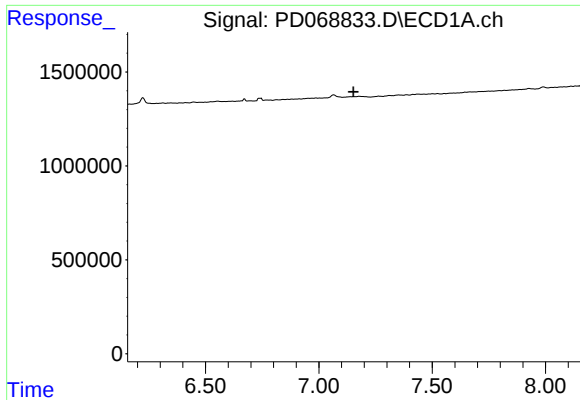

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

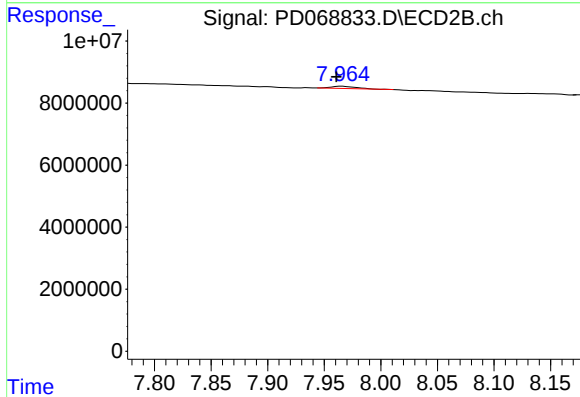


#21 Endrin ketone

R.T.: 7.966 min
Delta R.T.: 0.005 min
Response: 1021260
Conc: 0.13 ng/ml

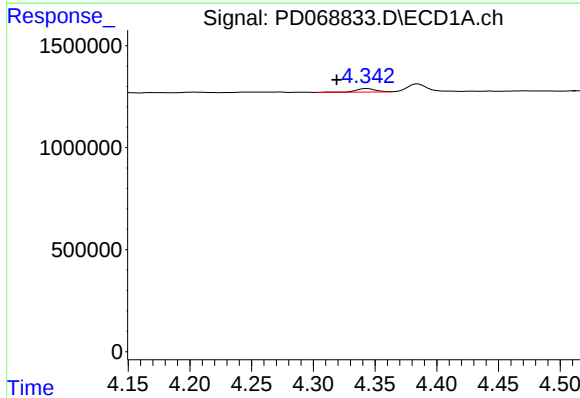


#23 Chlordane-1

R.T.: 4.344 min
Delta R.T.: 0.025 min
Response: 190954
Conc: 4.50 ng/ml

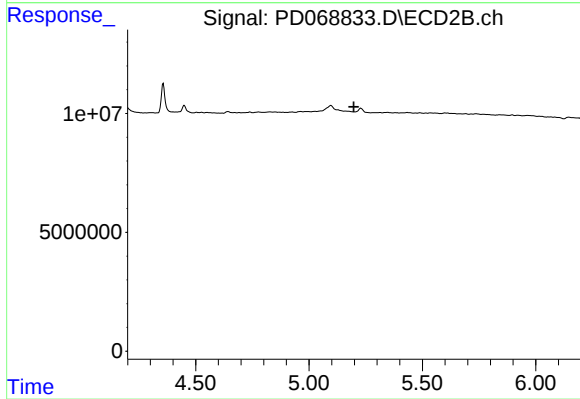

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.198 min
Response: 0
Conc: N.D.

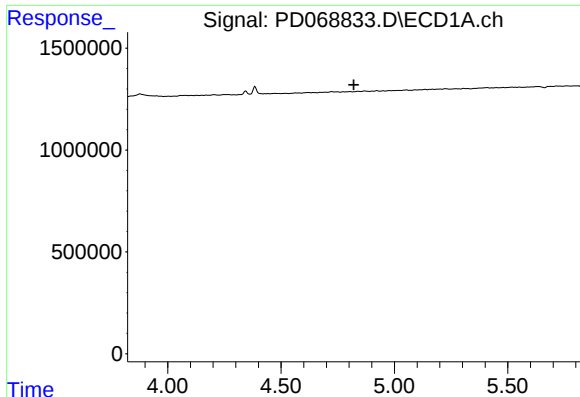

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

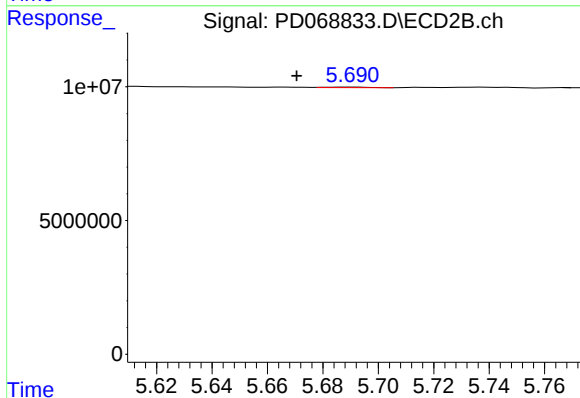


#24 Chlordane-2

R.T.: 5.691 min
Delta R.T.: 0.020 min
Response: 230026
Conc: 0.60 ng/ml

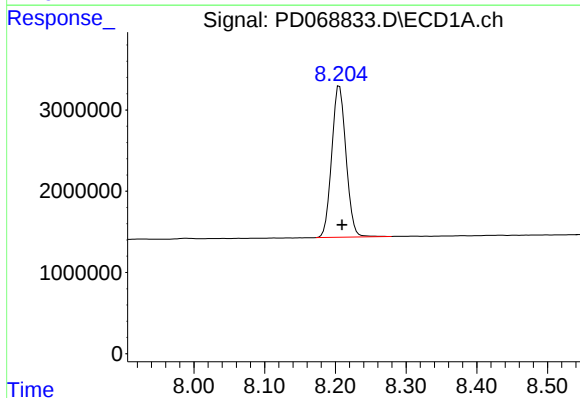

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 26163650
Conc: 20.71 ng/ml

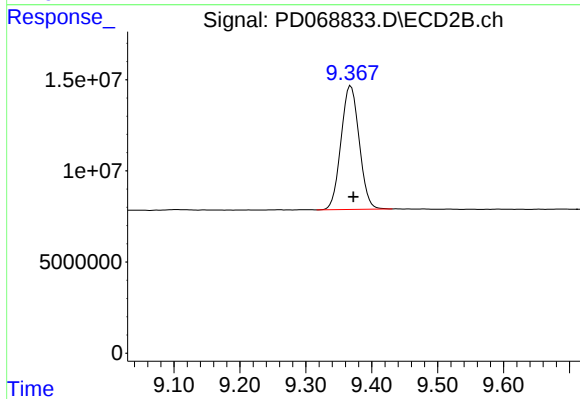

#28 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: -0.004 min
Response: 129828806
Conc: 22.91 ng/ml