

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033122\
 Data File : PD068837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 17:47
 Operator : AR\AJ
 Sample : N2140-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:51:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.173	24956380	207.9E6	20.554	21.744
28)	SA Decachlor...	8.204	9.366	28621756	143.8E6	22.655	25.379
Target Compounds							
2)	A alpha-BHC	0.000	4.580	0	465544	N.D.	0.034 #
7)	B delta-BHC	0.000	5.229f	0	9890251	N.D.	0.822 #
8)	B Heptachlo...	0.000	6.066f	0	1334130	N.D.	0.128 #
10)	B gamma-Chl...	5.410f	6.337	214196	632580	0.141	0.061 #
15)	B Endosulfa...	0.000	7.133	0	501780	N.D.	0.066 #
17)	MA 4,4'-DDT	0.000	7.357	0	415428	N.D.	0.057 #
21)	B Endrin ke...	0.000	7.967	0	1787888	N.D.	0.231 #
23)	Chlordane-1	4.344f	0.000	282967	0	6.668	N.D. #
25)	Chlordane-3	5.410f	6.337	214196	632580	1.536	0.471 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD03122\
Data File : PD068837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 17:47
Operator : AR\AJ
Sample : N2140-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:51:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

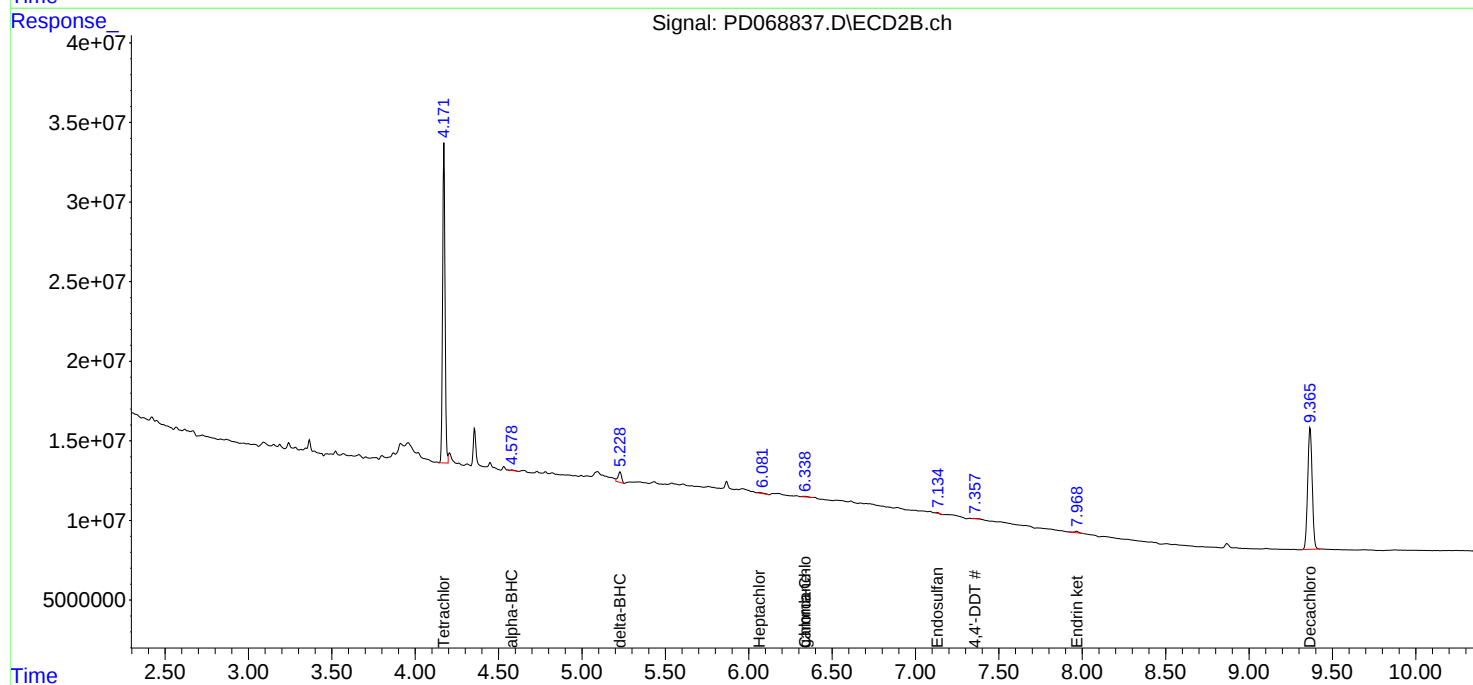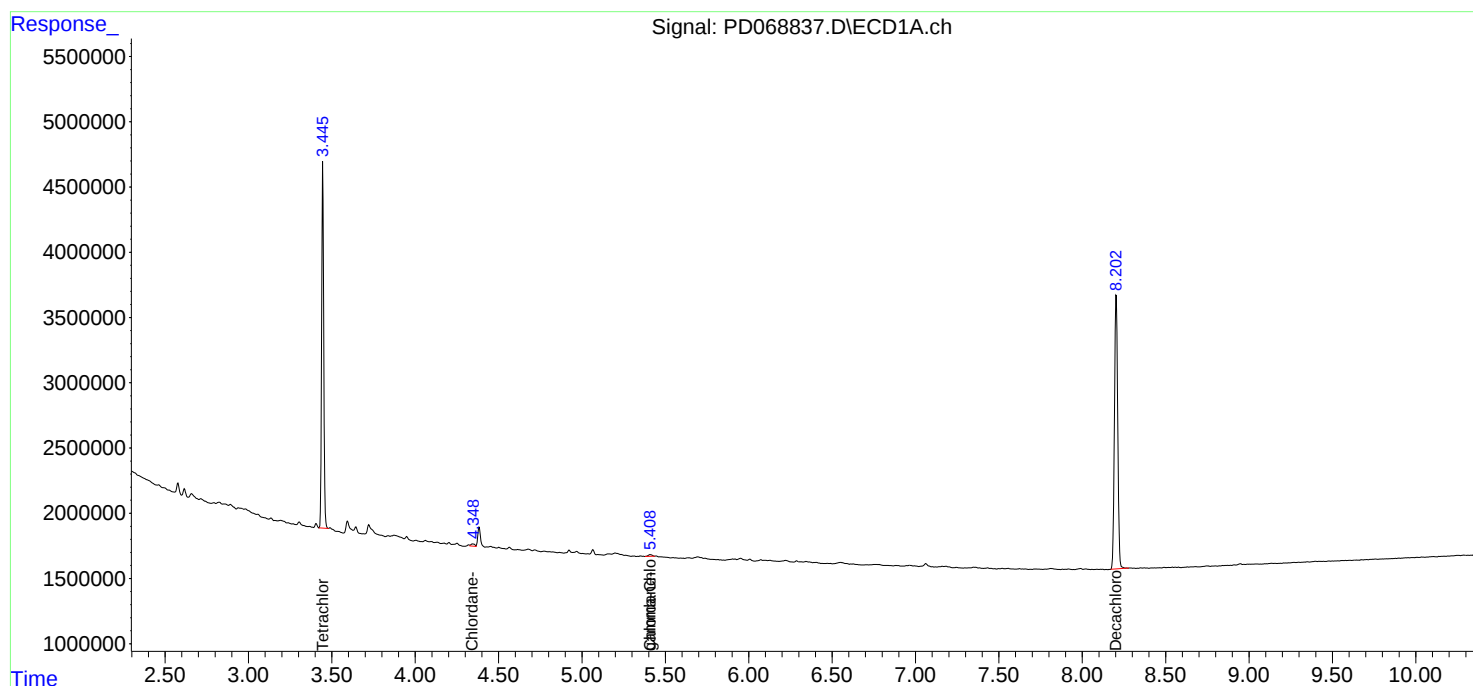


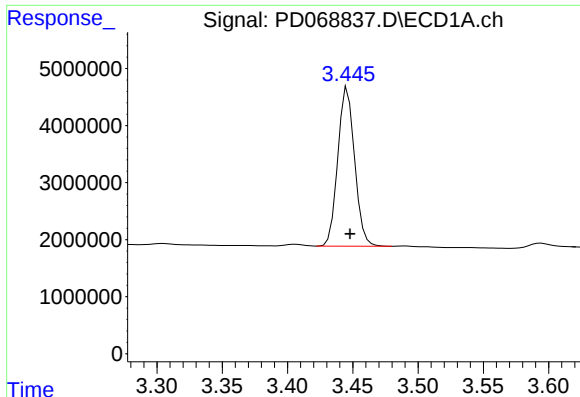

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 24956380
Conc: 20.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

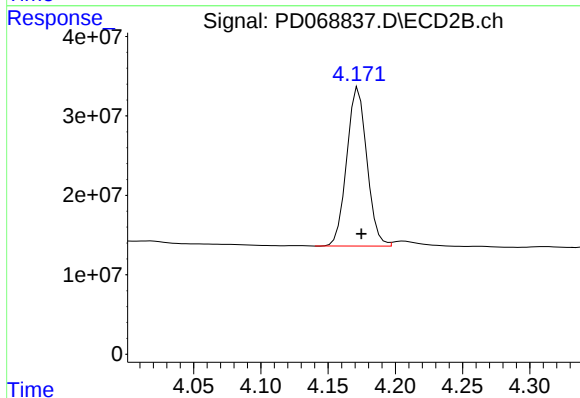


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.002 min
Response: 207891180
Conc: 21.74 ng/ml

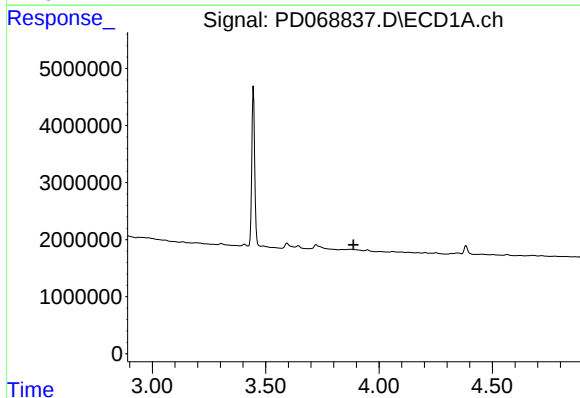


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

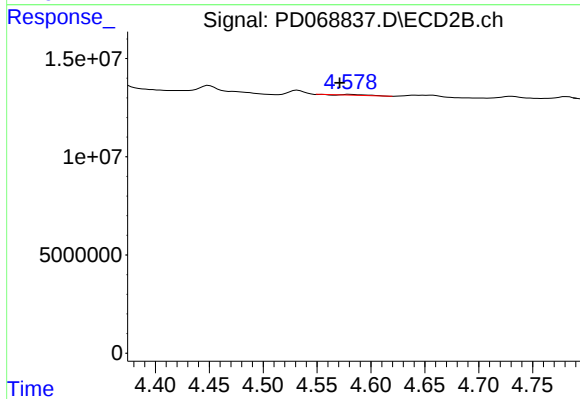

#2 alpha-BHC


R.T.: 4.580 min
Delta R.T.: 0.009 min
Response: 465544
Conc: 0.03 ng/ml

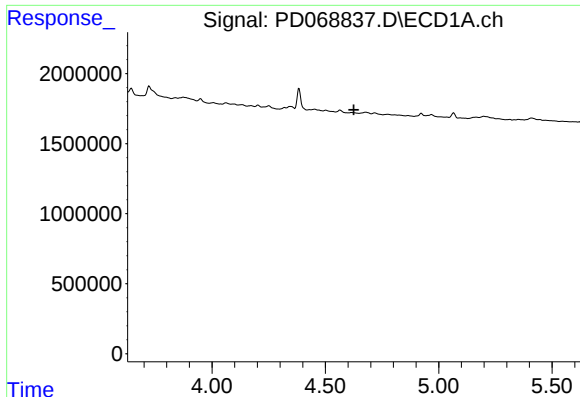

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

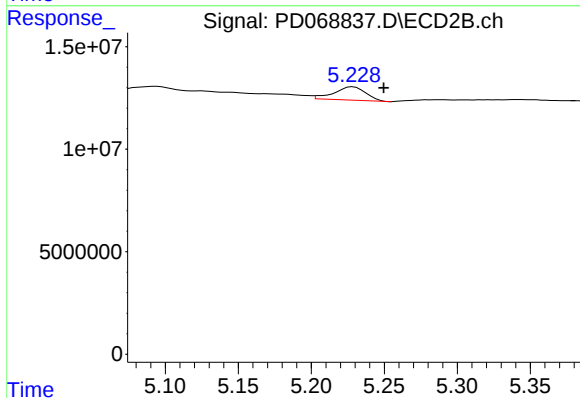


#7 delta-BHC

R.T.: 5.229 min
Delta R.T.: -0.021 min
Response: 9890251
Conc: 0.82 ng/ml

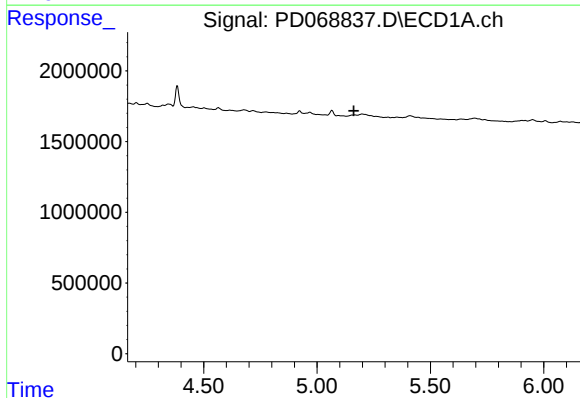


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

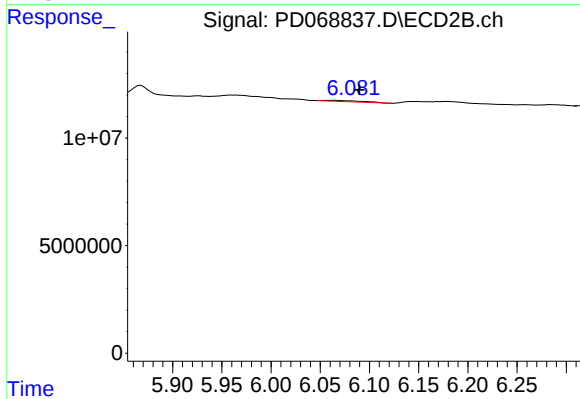

#8 Heptachlor epoxide


R.T.: 6.066 min
Delta R.T.: -0.024 min
Response: 1334130
Conc: 0.13 ng/ml

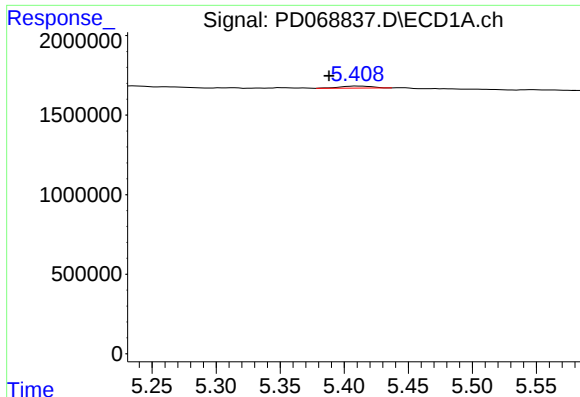

#10 gamma-Chlordane


R.T.: 5.410 min
Delta R.T.: 0.022 min
Response: 214196
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

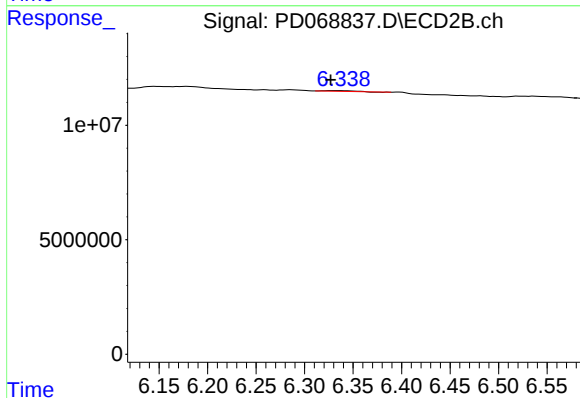


#10 gamma-Chlordane

R.T.: 6.337 min
Delta R.T.: 0.010 min
Response: 632580
Conc: 0.06 ng/ml

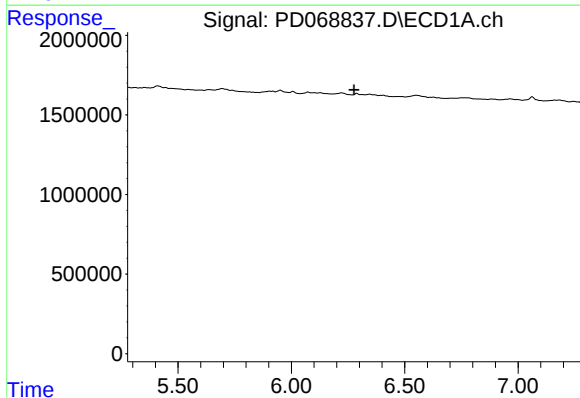


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.277 min
Response: 0
Conc: N.D.

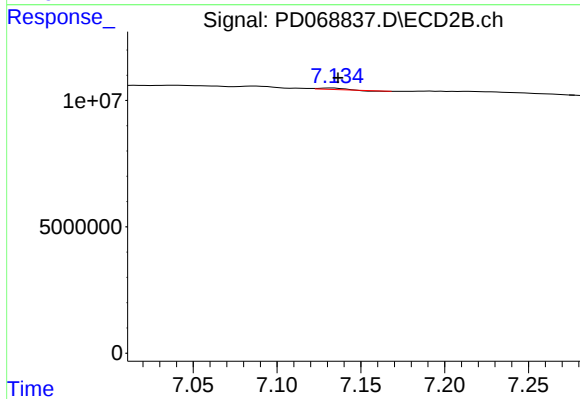

#15 Endosulfan II


R.T.: 7.133 min
Delta R.T.: -0.003 min
Response: 501780
Conc: 0.07 ng/ml

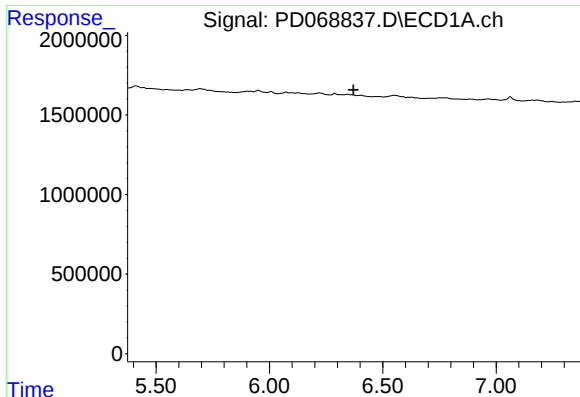

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

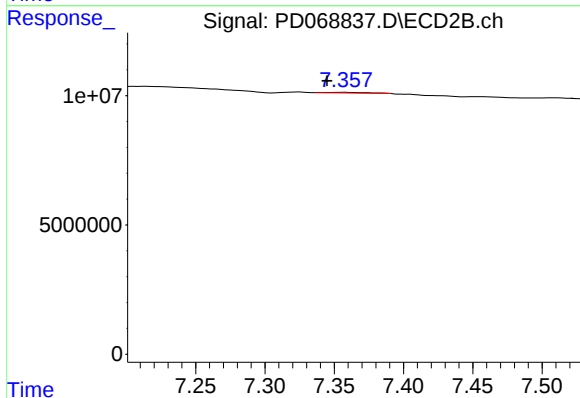


#17 4,4'-DDT

R.T.: 7.357 min
Delta R.T.: 0.012 min
Response: 415428
Conc: 0.06 ng/ml

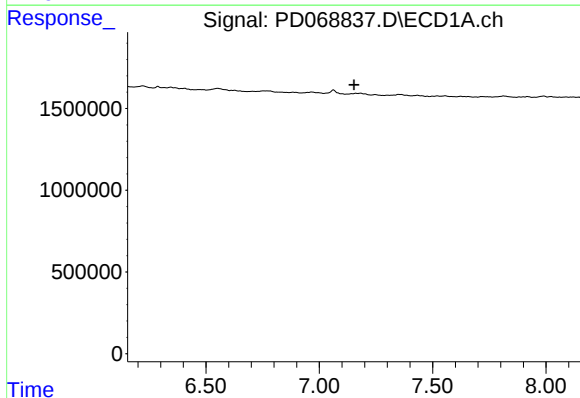


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

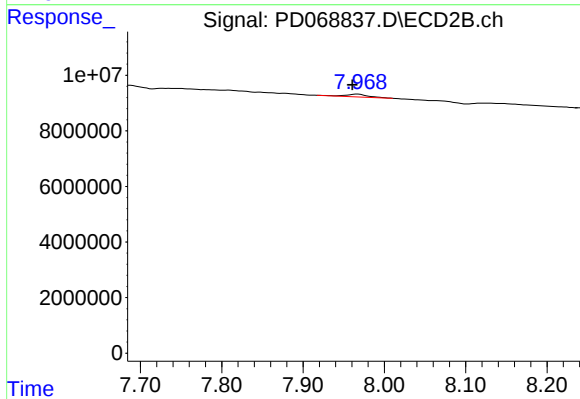

#21 Endrin ketone


R.T.: 7.967 min
Delta R.T.: 0.007 min
Response: 1787888
Conc: 0.23 ng/ml

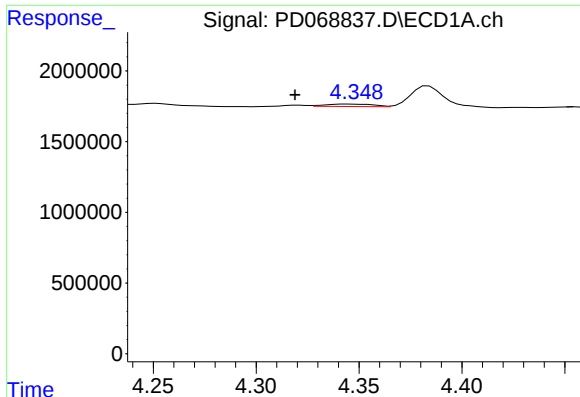

#23 Chlordane-1


R.T.: 4.344 min
Delta R.T.: 0.025 min
Response: 282967
Conc: 6.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

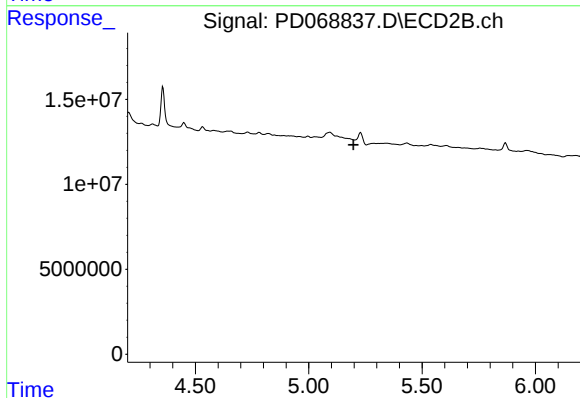


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.198 min
Response: 0
Conc: N.D.

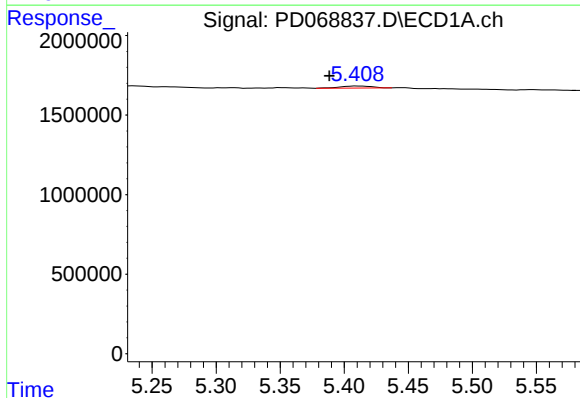


#25 Chlordane-3

R.T.: 5.410 min
Delta R.T.: 0.021 min
Response: 214196
Conc: 1.54 ng/ml

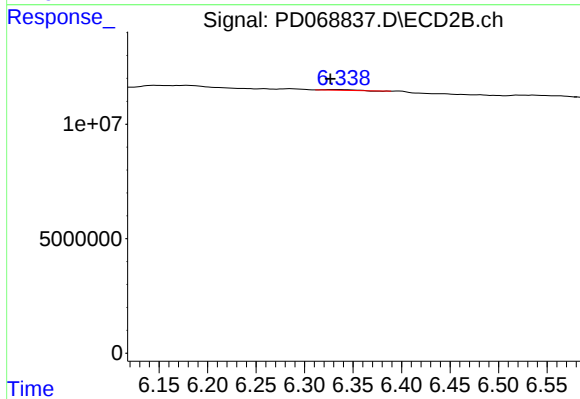

#25 Chlordane-3


R.T.: 6.337 min
Delta R.T.: 0.010 min
Response: 632580
Conc: 0.47 ng/ml

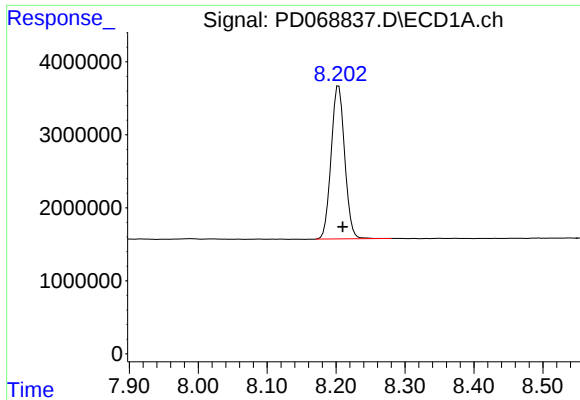

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.006 min
Response: 28621756
Conc: 22.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

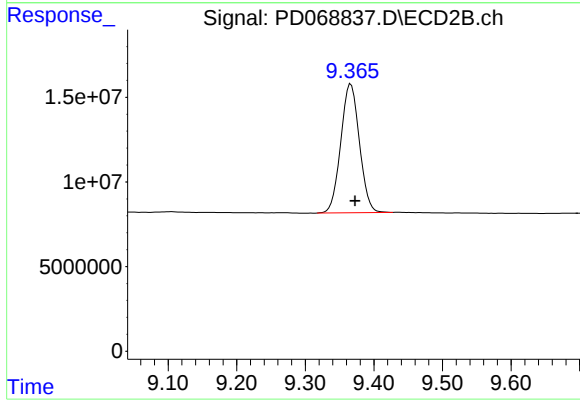

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.006 min
Response: 143818111
Conc: 25.38 ng/ml