

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033122\
 Data File : PD068840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 18:29
 Operator : AR\AJ
 Sample : N2157-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:52:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.172	24053655	199.8E6	19.811	20.898
28)	SA Decachlor...	8.203	9.367	25252774	125.3E6	19.988	22.118
Target Compounds							
4)	MA Heptachlor	0.000	5.377	0	54104	N.D.	0.005 #
5)	MB Aldrin	0.000	5.705	0	269061	N.D.	0.023 #
7)	B delta-BHC	0.000	5.229f	0	5375131	N.D.	0.447 #
8)	B Heptachlo...	0.000	6.068f	0	1550933	N.D.	0.149 #
9)	A Endosulfan I	0.000	6.463	0	551087	N.D.	0.059 #
10)	B gamma-Chl...	0.000	6.327	0	1142328	N.D.	0.111 #
21)	B Endrin ke...	0.000	7.966	0	1323215	N.D.	0.171 #
23)	Chlordane-1	4.319	5.177f	172008	1104428	4.053	2.799 #
25)	Chlordane-3	0.000	6.327	0	1142328	N.D.	0.850 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033122\
Data File : PD068840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 18:29
Operator : AR\AJ
Sample : N2157-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:52:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

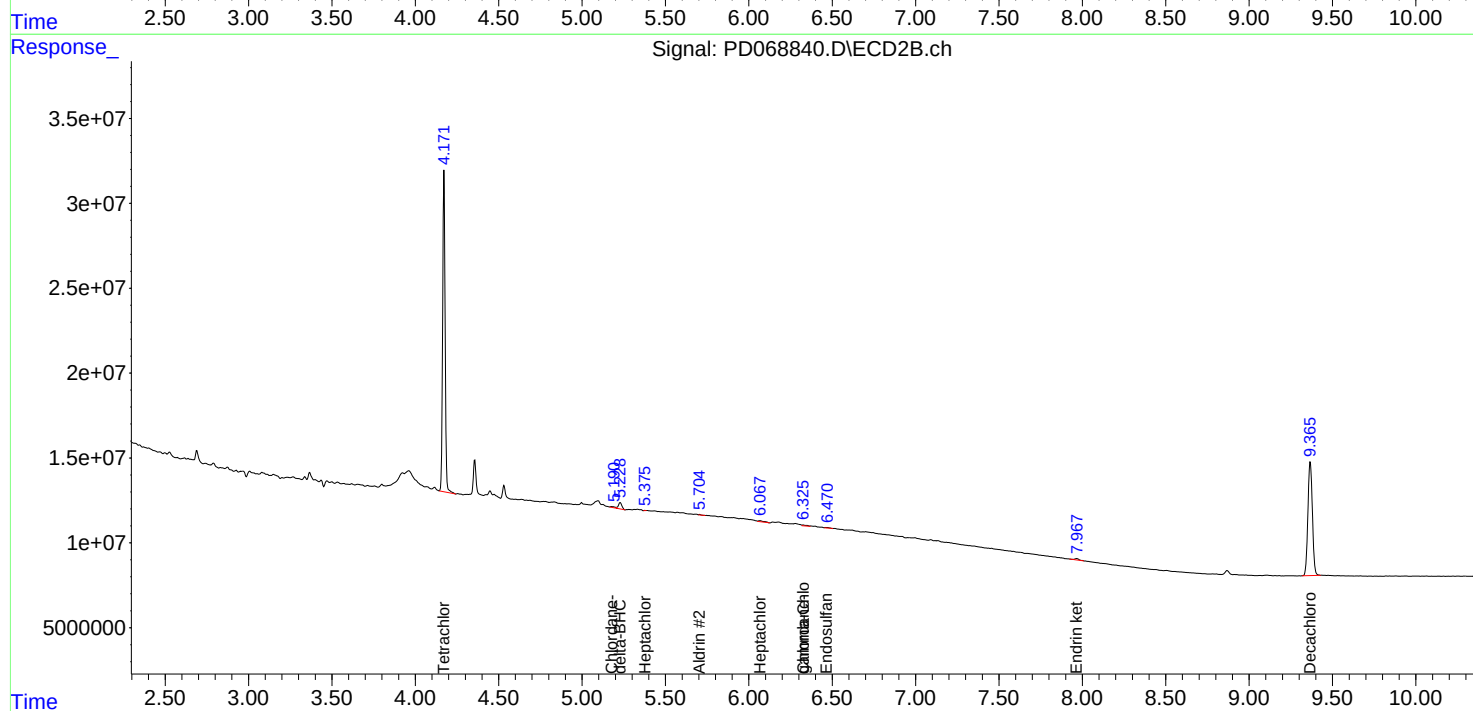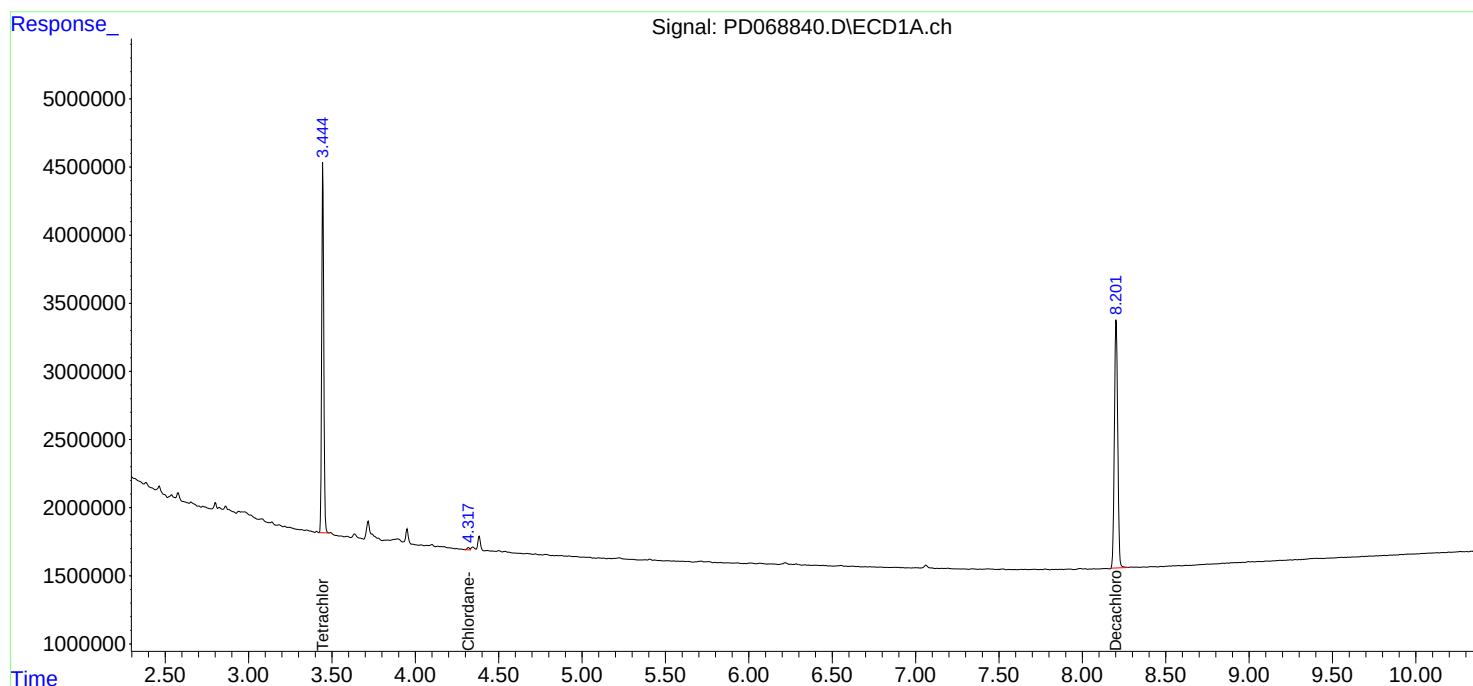


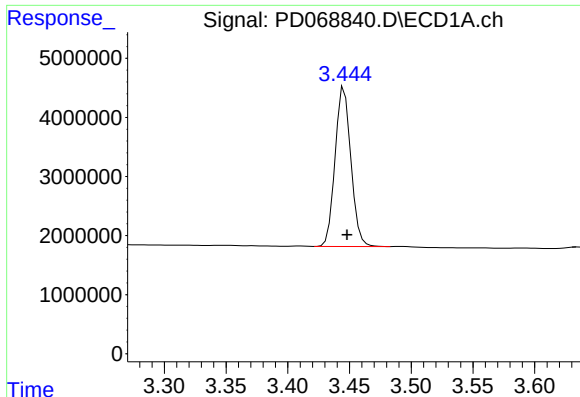

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 24053655
Conc: 19.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

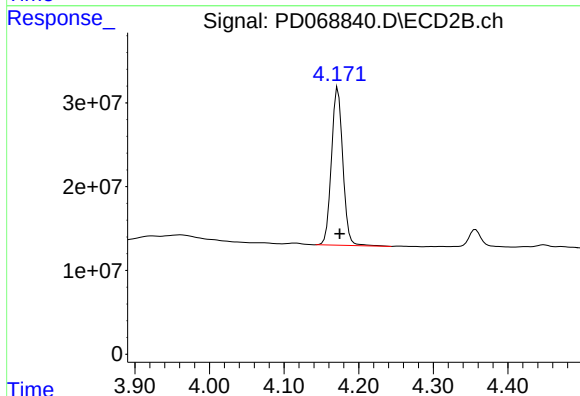


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.002 min
Response: 199796278
Conc: 20.90 ng/ml

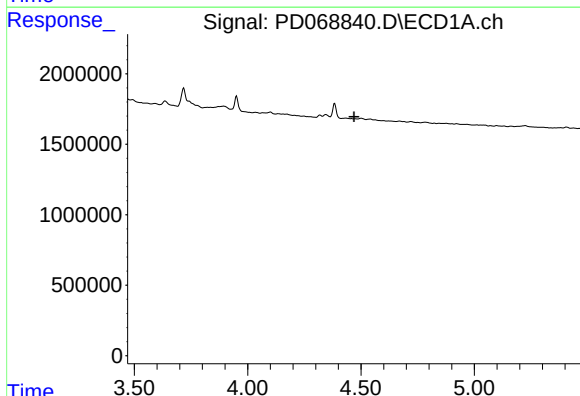


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

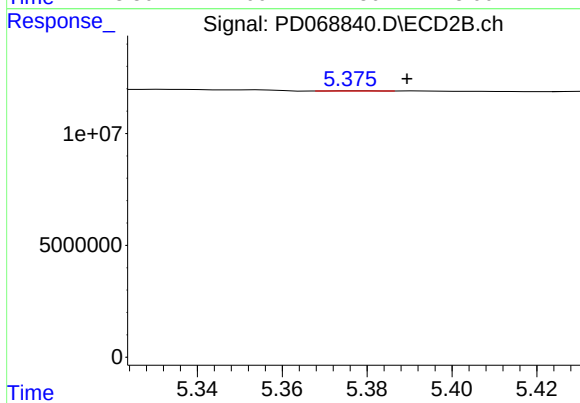

#4 Heptachlor


R.T.: 5.377 min
Delta R.T.: -0.012 min
Response: 54104
Conc: 0.00 ng/ml

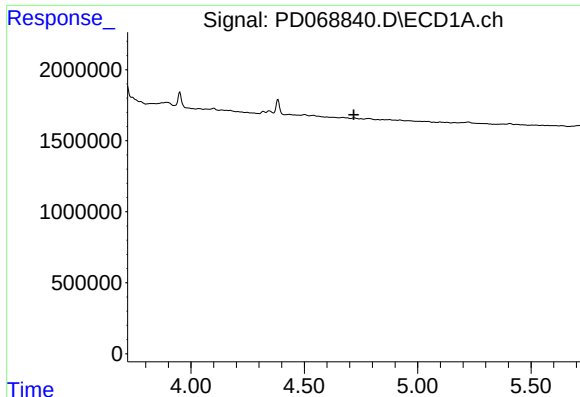

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.718 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

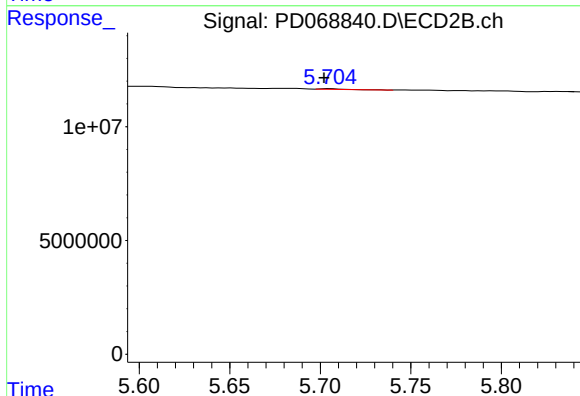


#5 Aldrin

R.T.: 5.705 min
Delta R.T.: 0.003 min
Response: 269061
Conc: 0.02 ng/ml

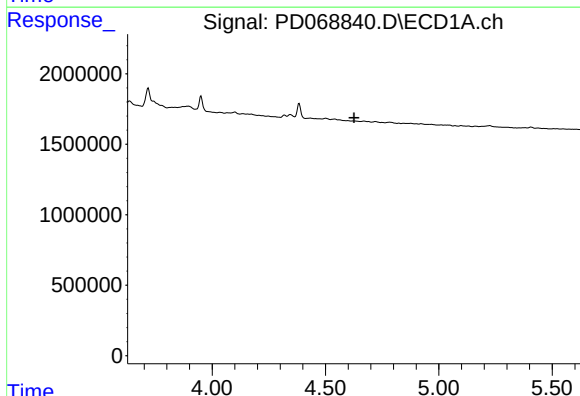


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

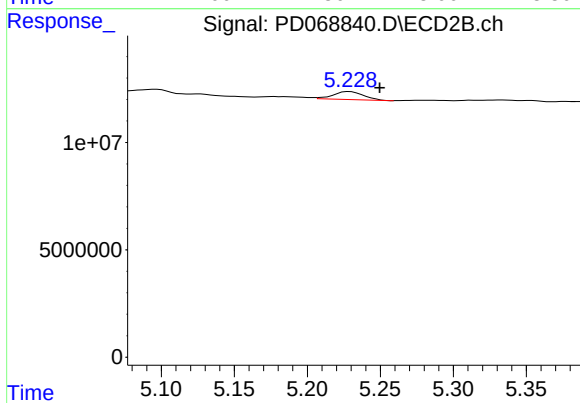

#7 delta-BHC


R.T.: 5.229 min
Delta R.T.: -0.021 min
Response: 5375131
Conc: 0.45 ng/ml

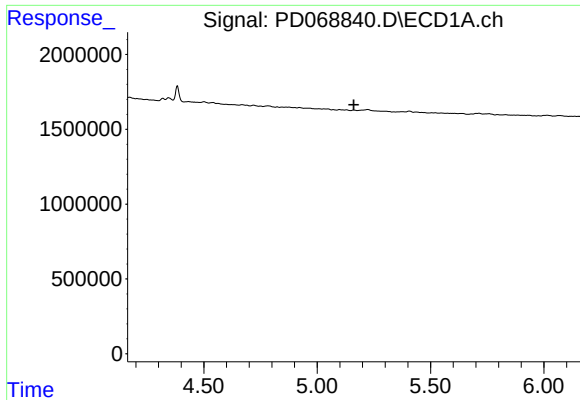

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

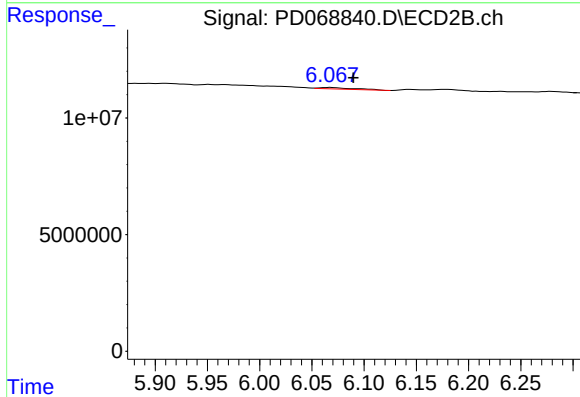


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.022 min
Response: 1550933
Conc: 0.15 ng/ml

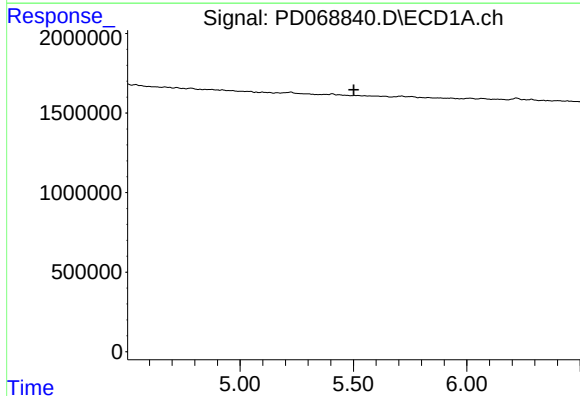


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

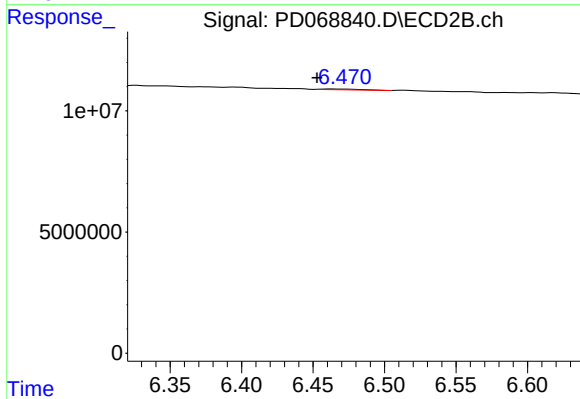

#9 Endosulfan I


R.T.: 6.463 min
Delta R.T.: 0.010 min
Response: 551087
Conc: 0.06 ng/ml

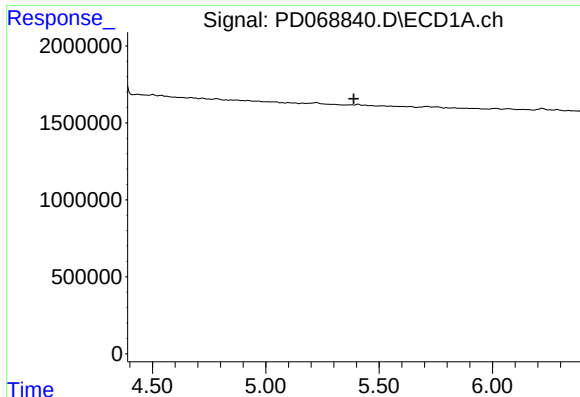

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

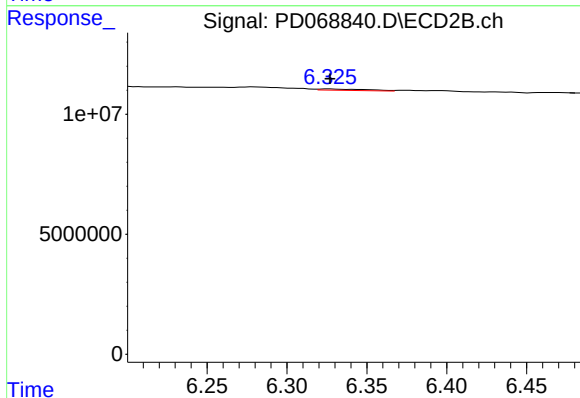


#10 gamma-Chlordane

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 1142328
Conc: 0.11 ng/ml

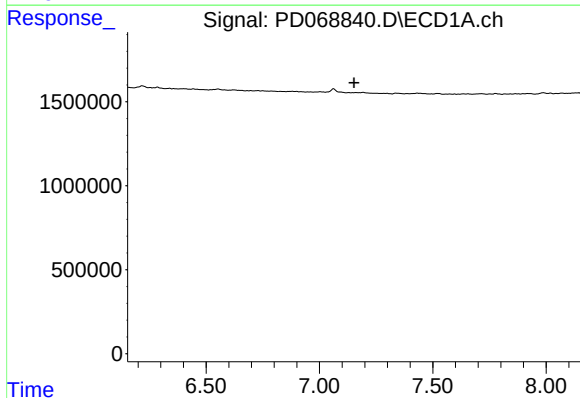


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

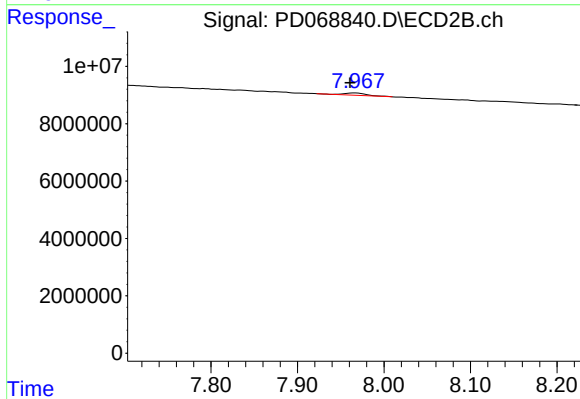

#21 Endrin ketone


R.T.: 7.966 min
Delta R.T.: 0.005 min
Response: 1323215
Conc: 0.17 ng/ml

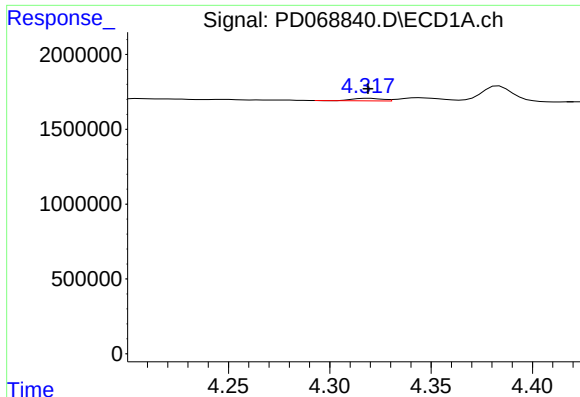

#23 Chlordane-1


R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 172008
Conc: 4.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

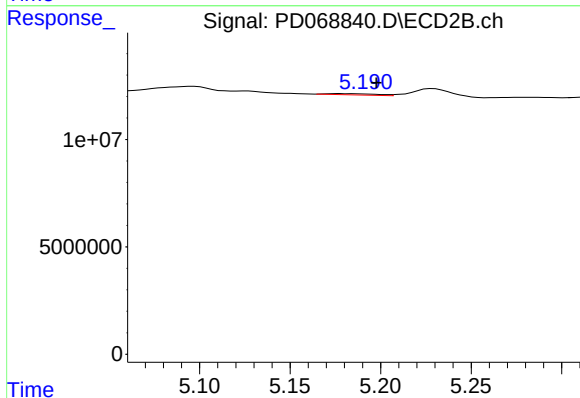


#23 Chlordane-1

R.T.: 5.177 min
Delta R.T.: -0.021 min
Response: 1104428
Conc: 2.80 ng/ml

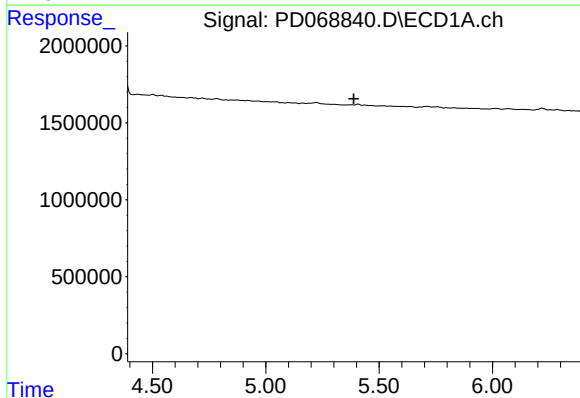


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

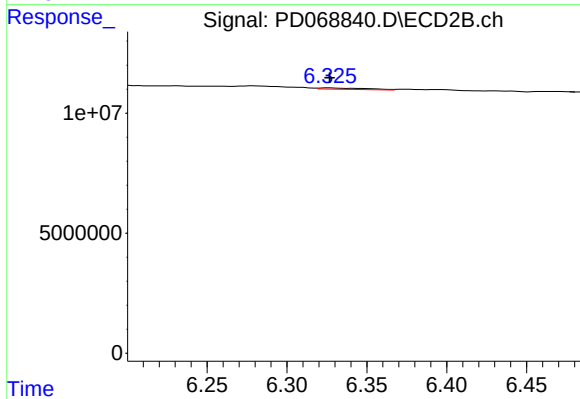

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 1142328
Conc: 0.85 ng/ml

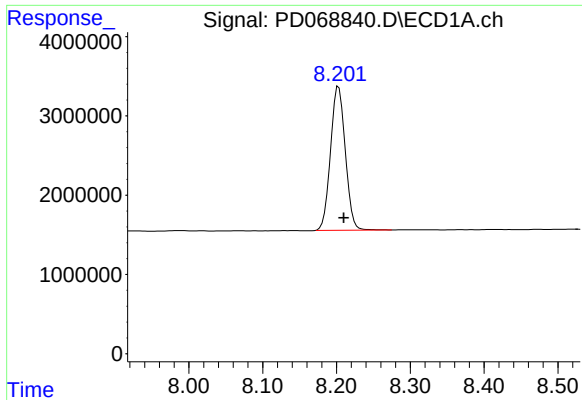

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.007 min
Response: 25252774
Conc: 19.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

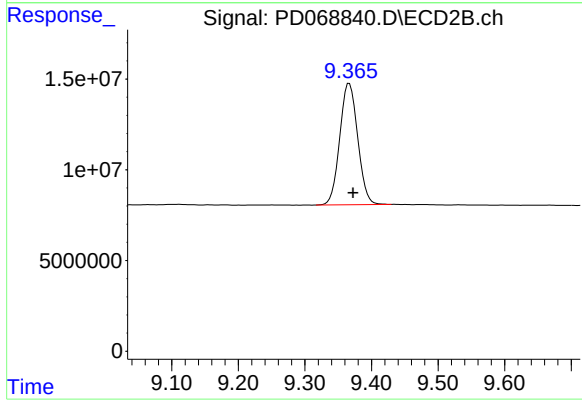

#28 Decachlorobiphenyl

R.T.: 9.367 min
Delta R.T.: -0.006 min
Response: 125334961
Conc: 22.12 ng/ml