

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040122\
 Data File : PD068846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 09:24
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 02:45:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.172	25397810	224.1E6	20.918	23.440
28)	SA Decachlor...	8.203	9.365	27698358	138.1E6	21.924	24.379
Target Compounds							
2)	A alpha-BHC	3.885	4.568	17700192	165.1E6	9.776	11.996
3)	MA gamma-BHC...	4.168	4.859	16392646	150.1E6	9.817	12.008
4)	MA Heptachlor	0.000	5.388	0	126645	N.D.	0.011 #
5)	MB Aldrin	4.713	0.000	136652	0	0.086	N.D. #
6)	B beta-BHC	4.419	5.021	8557721	70273244	11.494	12.801
7)	B delta-BHC	4.622	5.244	163512	1758291	0.100	0.146 #
8)	B Heptachlo...	0.000	6.061f	0	23717060	N.D.	2.271 #
9)	A Endosulfan I	0.000	6.464	0	177074	N.D.	0.019 #
10)	B gamma-Chl...	5.383	6.316	421015	3151463	0.278	0.306
11)	B alpha-Chl...	0.000	6.403	0	2534370	N.D.	0.255 #
12)	B 4,4'-DDE	5.609	6.547	1331465	8182310	0.973	0.883
13)	MA Dieldrin	0.000	6.707	0	7209462	N.D.	0.742 #
14)	MA Endrin	5.999	6.927	65585713	404.8E6	49.787	52.320
15)	B Endosulfa...	6.276	7.132	1350294	11991421	1.083	1.586 #
16)	A 4,4'-DDD	6.126	7.038	5375022	43651310	4.558	5.911 #
17)	MA 4,4'-DDT	6.367	7.341	117.3E6	702.1E6	97.570	95.562
18)	B Endrin al...	6.442	7.256	2514047	18134400	2.532	2.997
19)	B Endosulfa...	0.000	7.478	0	200673	N.D.	0.027 #
20)	A Methoxychlor	6.917	7.794	149.6E6	793.0E6	215.832	217.536
21)	B Endrin ke...	7.148	7.956	5006518	30953374	3.401	3.995
23)	Chlordane-1	0.000	5.227f	0	1553061	N.D.	3.936 #
24)	Chlordane-2	0.000	5.651f	0	358727	N.D.	0.938 #
25)	Chlordane-3	5.383	6.316	421015	3151463	3.019	2.346
26)	Chlordane-4	0.000	6.403	0	2534370	N.D.	1.630 #
27)	Chlordane-5	6.276	0.000	1350294	0	27.028	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040122\
 Data File : PD068846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 09:24
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 02:45:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

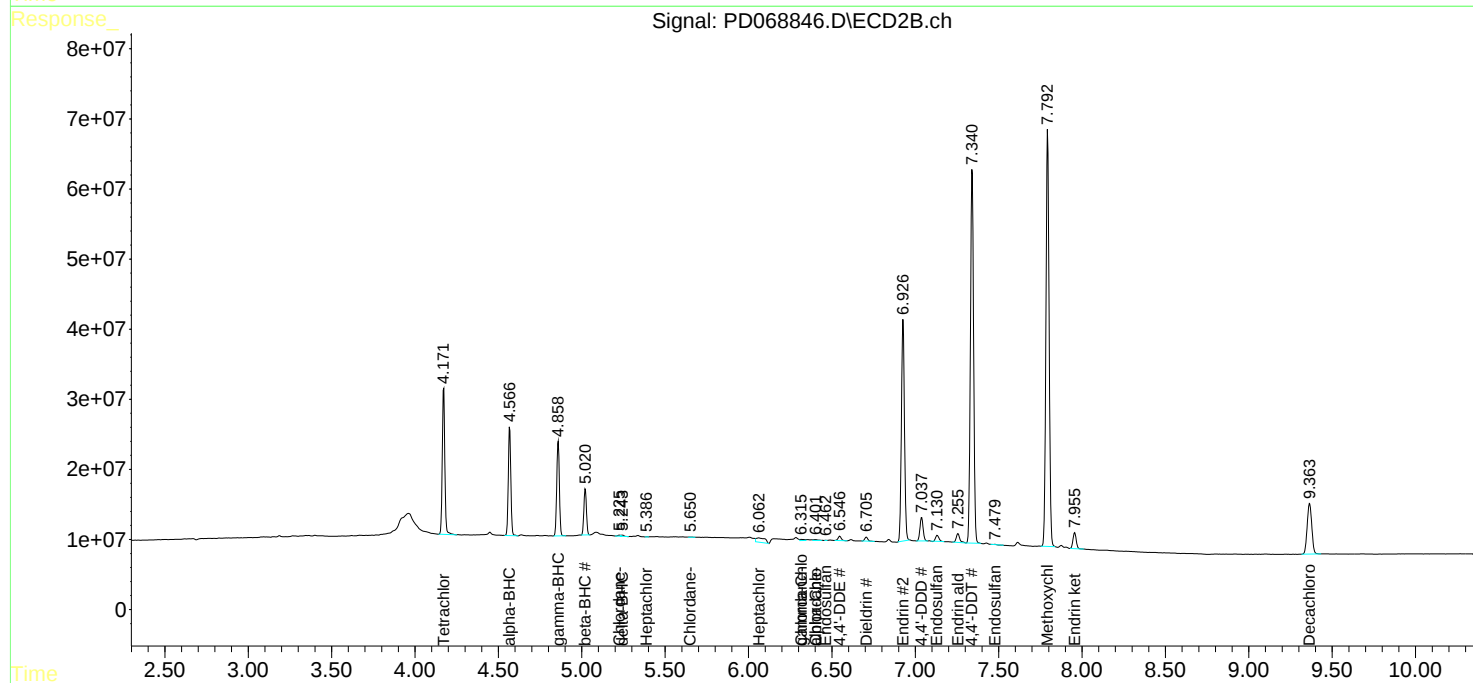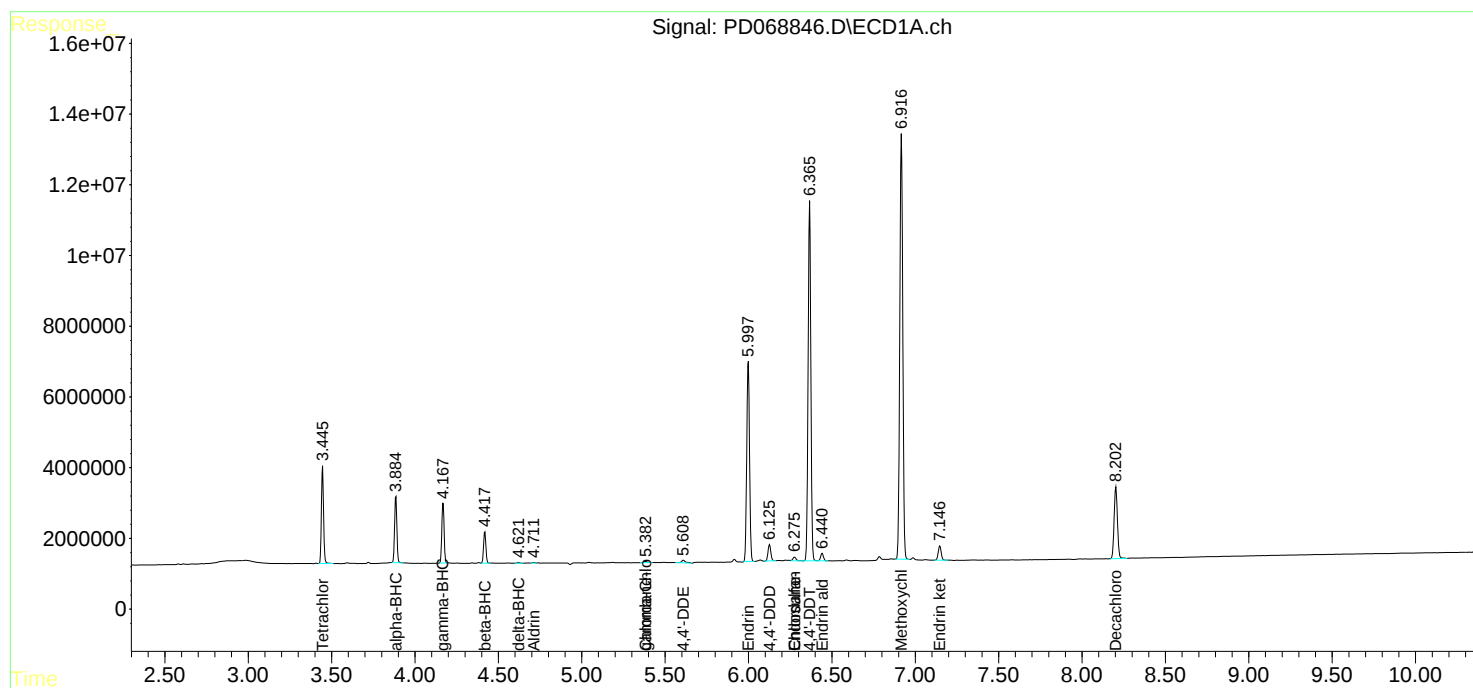


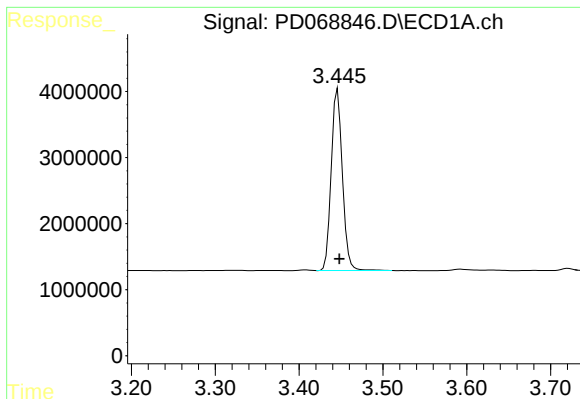

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 25397810
Conc: 20.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

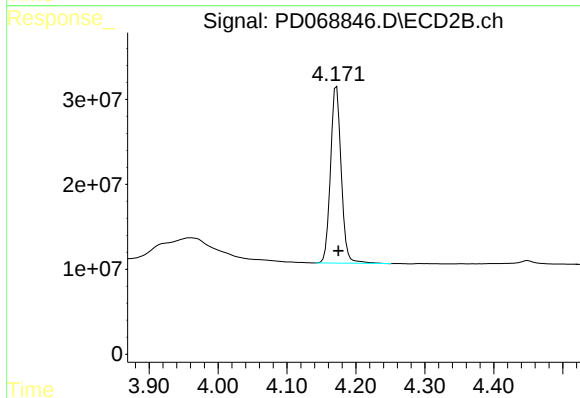


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.003 min
Response: 224105123
Conc: 23.44 ng/ml

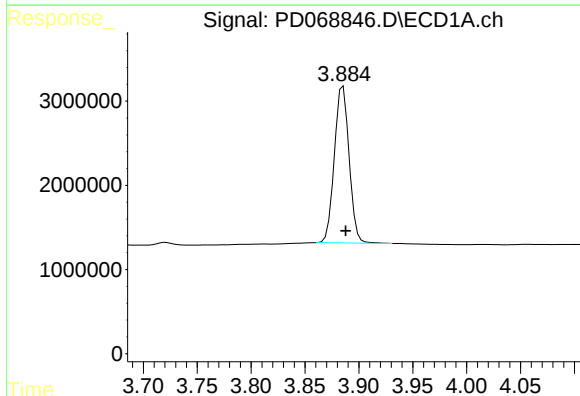


#2 alpha-BHC

R.T.: 3.885 min
Delta R.T.: -0.002 min
Response: 17700192
Conc: 9.78 ng/ml

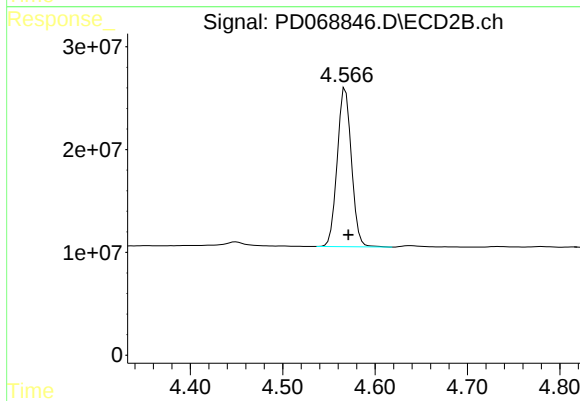

#2 alpha-BHC


R.T.: 4.568 min
Delta R.T.: -0.003 min
Response: 165100494
Conc: 12.00 ng/ml

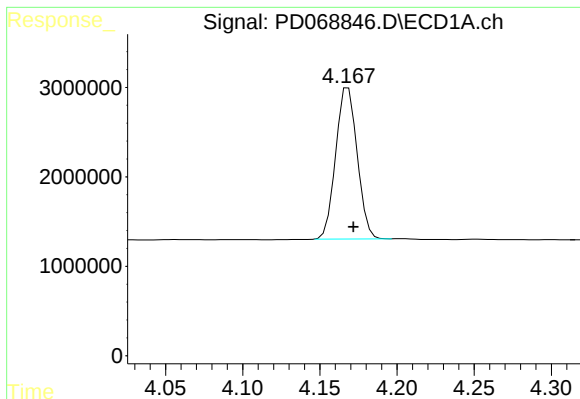

#3 gamma-BHC (Lindane)


R.T.: 4.168 min
Delta R.T.: -0.003 min
Response: 16392646
Conc: 9.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

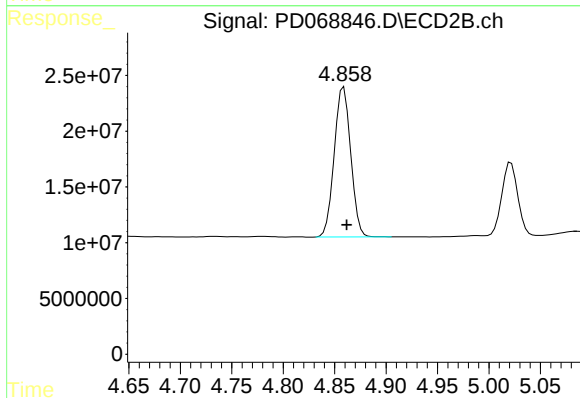


#3 gamma-BHC (Lindane)

R.T.: 4.859 min
Delta R.T.: -0.003 min
Response: 150134907
Conc: 12.01 ng/ml

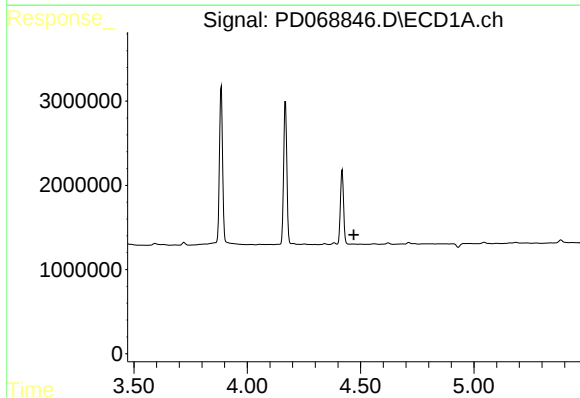


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

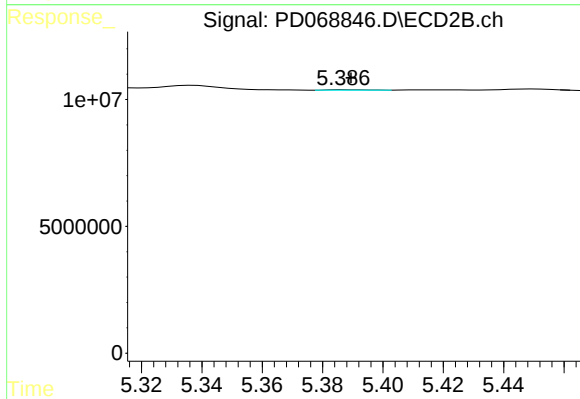

#4 Heptachlor


R.T.: 5.388 min
Delta R.T.: -0.001 min
Response: 126645
Conc: 0.01 ng/ml

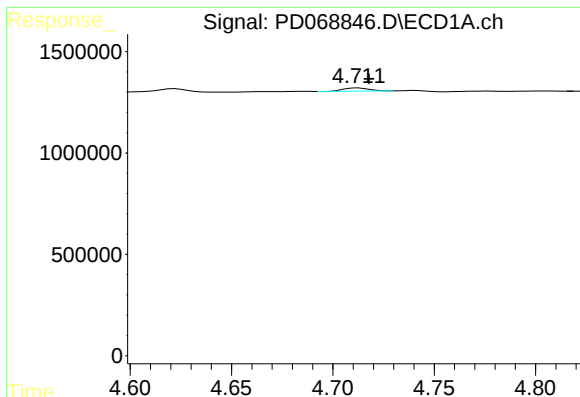

#5 Aldrin


R.T.: 4.713 min
Delta R.T.: -0.005 min
Response: 136652
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

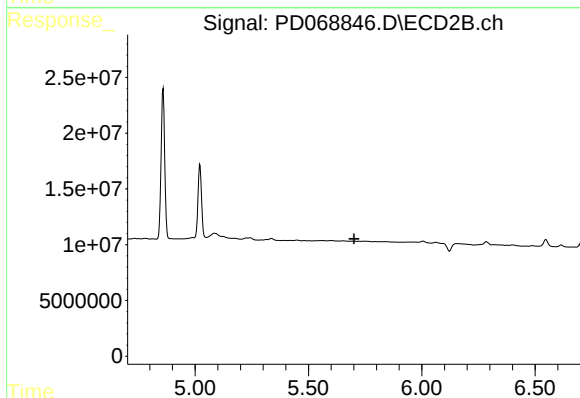


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.702 min
Response: 0
Conc: N.D.

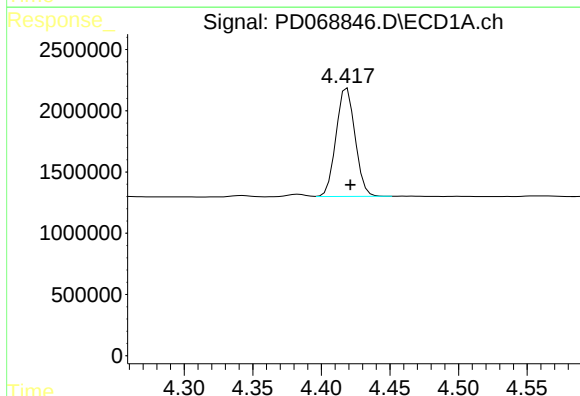


#6 beta-BHC

R.T.: 4.419 min
Delta R.T.: -0.002 min
Response: 8557721
Conc: 11.49 ng/ml

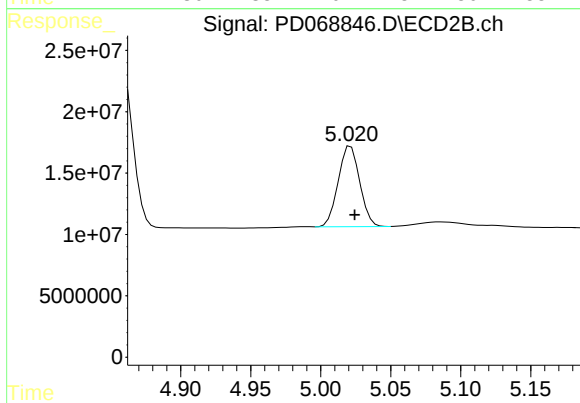

#6 beta-BHC


R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 70273244
Conc: 12.80 ng/ml

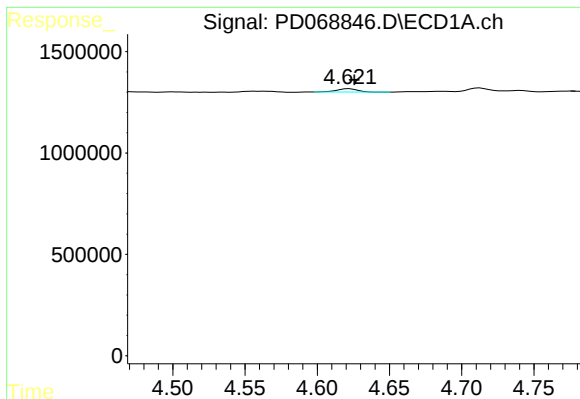

#7 delta-BHC


R.T.: 4.622 min
Delta R.T.: -0.004 min
Response: 163512
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

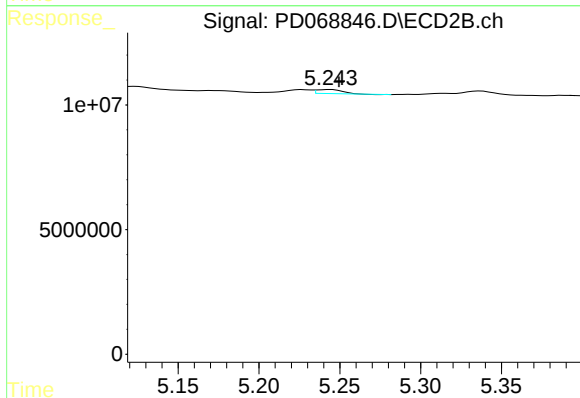


#7 delta-BHC

R.T.: 5.244 min
Delta R.T.: -0.005 min
Response: 1758291
Conc: 0.15 ng/ml

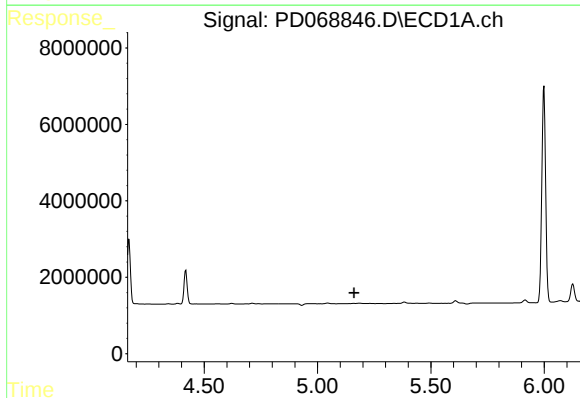


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

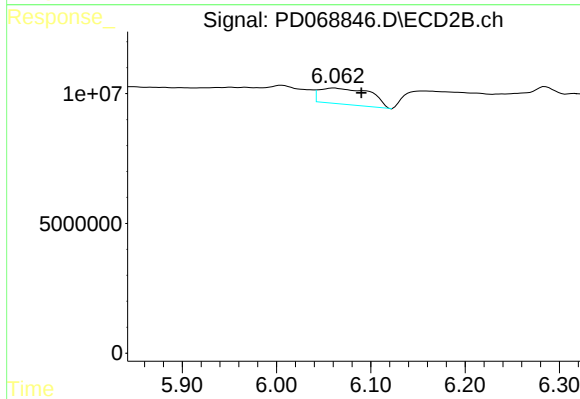

#8 Heptachlor epoxide


R.T.: 6.061 min
Delta R.T.: -0.029 min
Response: 23717060
Conc: 2.27 ng/ml

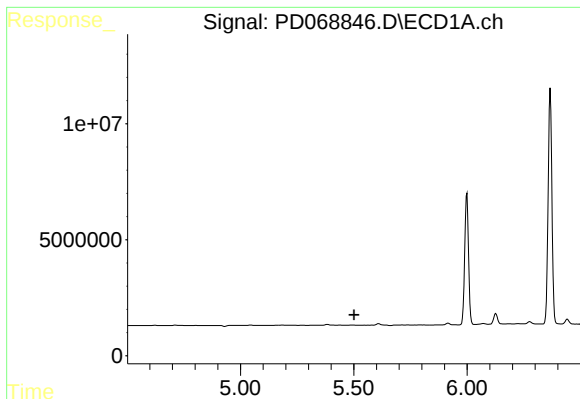

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

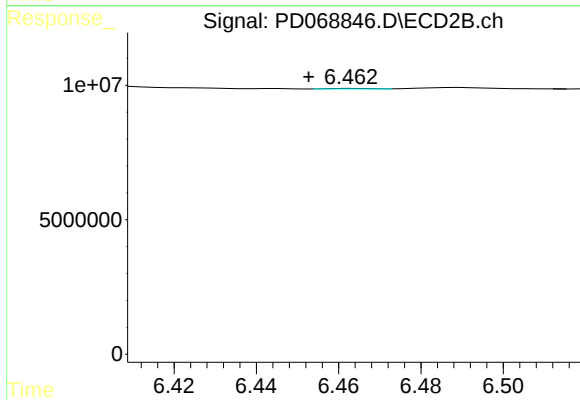


#9 Endosulfan I

R.T.: 6.464 min
Delta R.T.: 0.011 min
Response: 177074
Conc: 0.02 ng/ml

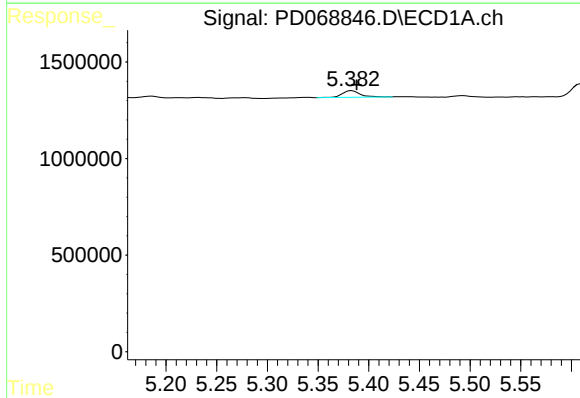


#10 gamma-Chlordane

R.T.: 5.383 min
Delta R.T.: -0.005 min
Response: 421015
Conc: 0.28 ng/ml

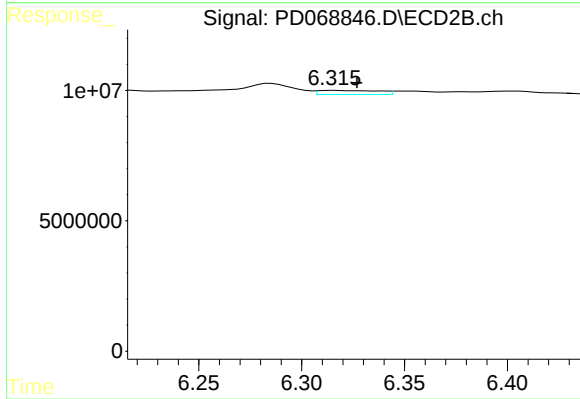

#10 gamma-Chlordane


R.T.: 6.316 min
Delta R.T.: -0.011 min
Response: 3151463
Conc: 0.31 ng/ml

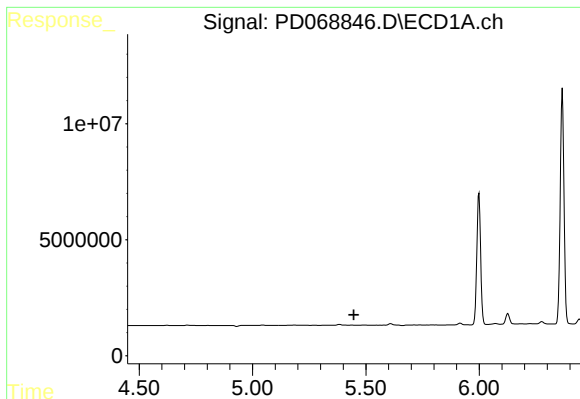

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

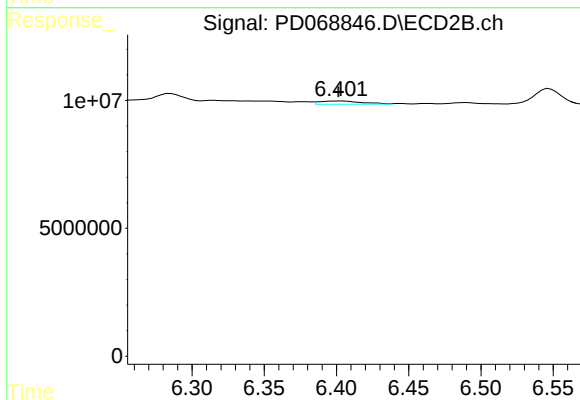


#11 alpha-Chlordane

R.T.: 6.403 min
Delta R.T.: 0.001 min
Response: 2534370
Conc: 0.25 ng/ml

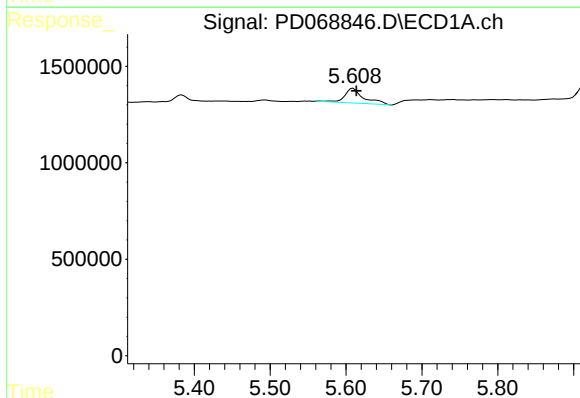


#12 4,4'-DDE

R.T.: 5.609 min
Delta R.T.: -0.004 min
Response: 1331465
Conc: 0.97 ng/ml

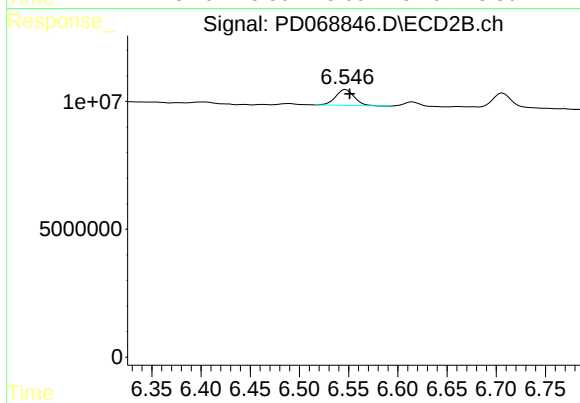

#12 4,4'-DDE


R.T.: 6.547 min
Delta R.T.: -0.004 min
Response: 8182310
Conc: 0.88 ng/ml

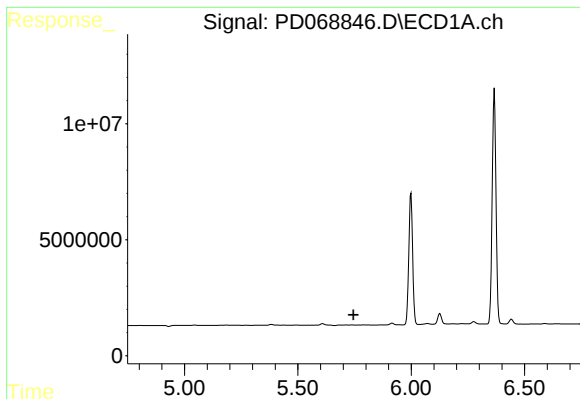

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

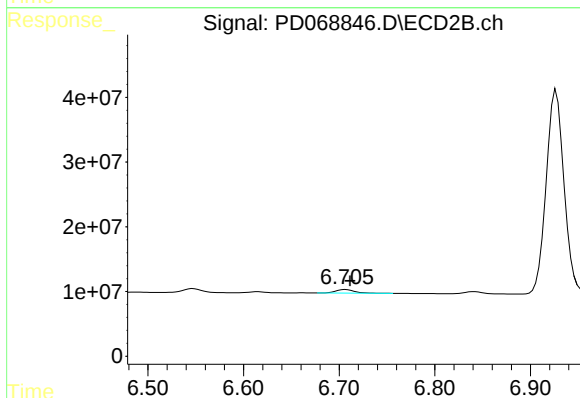


#13 Dieldrin

R.T.: 6.707 min
Delta R.T.: -0.005 min
Response: 7209462
Conc: 0.74 ng/ml

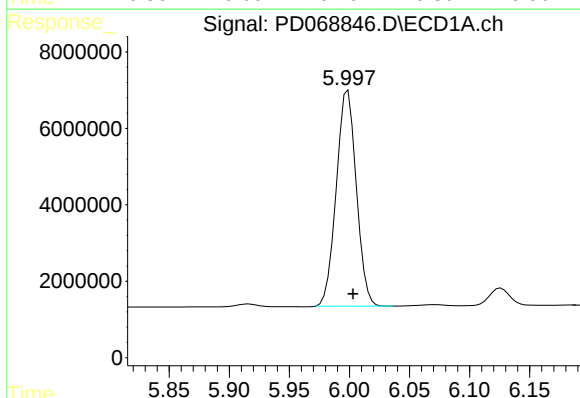


#14 Endrin

R.T.: 5.999 min
Delta R.T.: -0.004 min
Response: 65585713
Conc: 49.79 ng/ml

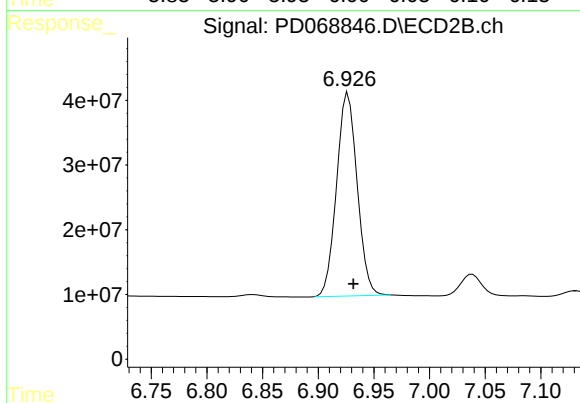

#14 Endrin


R.T.: 6.927 min
Delta R.T.: -0.005 min
Response: 404829816
Conc: 52.32 ng/ml

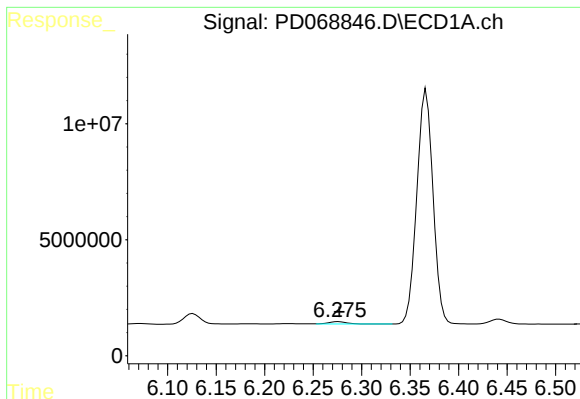

#15 Endosulfan II


R.T.: 6.276 min
Delta R.T.: -0.001 min
Response: 1350294
Conc: 1.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

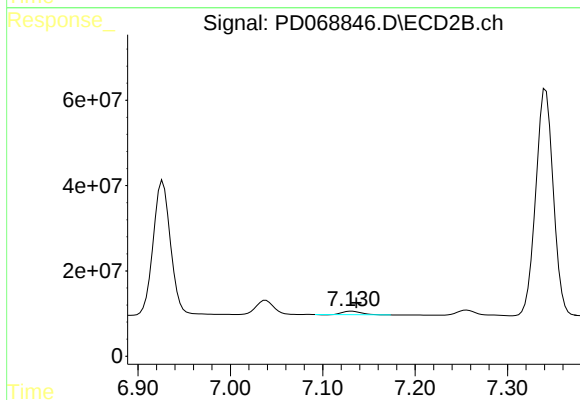


#15 Endosulfan II

R.T.: 7.132 min
Delta R.T.: -0.005 min
Response: 11991421
Conc: 1.59 ng/ml

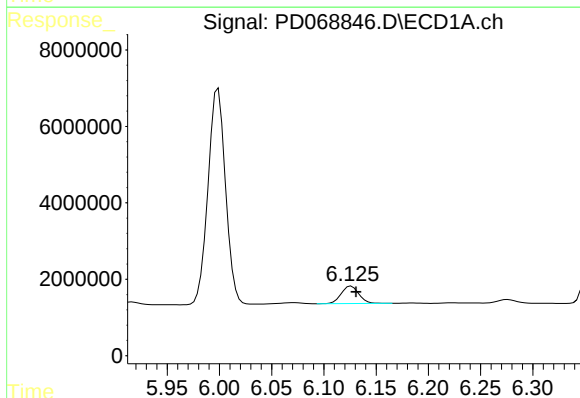


#16 4,4'-DDD

R.T.: 6.126 min
Delta R.T.: -0.005 min
Response: 5375022
Conc: 4.56 ng/ml

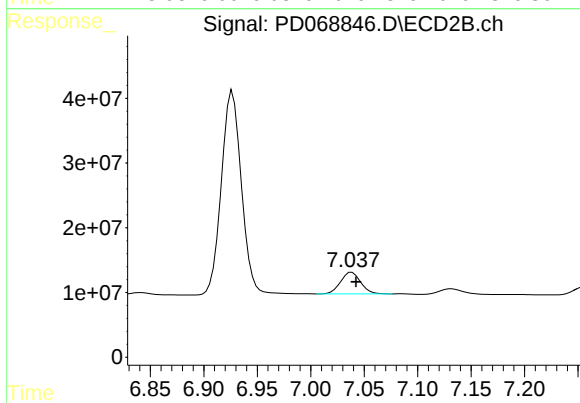

#16 4,4'-DDD


R.T.: 7.038 min
Delta R.T.: -0.004 min
Response: 43651310
Conc: 5.91 ng/ml

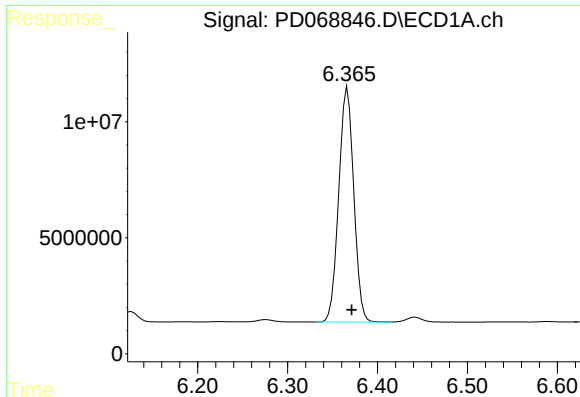

#17 4,4'-DDT


R.T.: 6.367 min
Delta R.T.: -0.004 min
Response: 117276386
Conc: 97.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

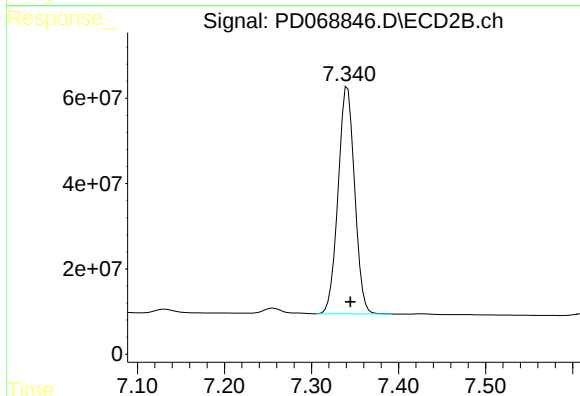


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: -0.003 min
Response: 702071517
Conc: 95.56 ng/ml

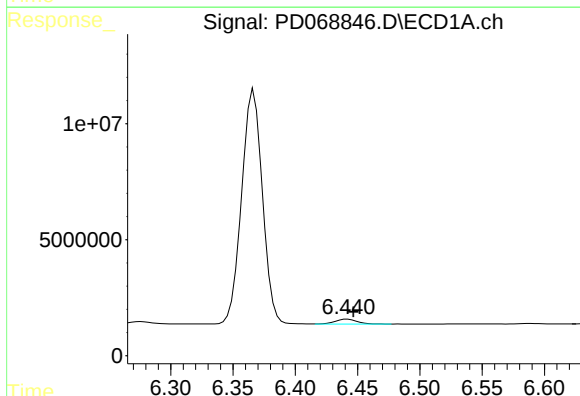


#18 Endrin aldehyde

R.T.: 6.442 min
Delta R.T.: -0.005 min
Response: 2514047
Conc: 2.53 ng/ml

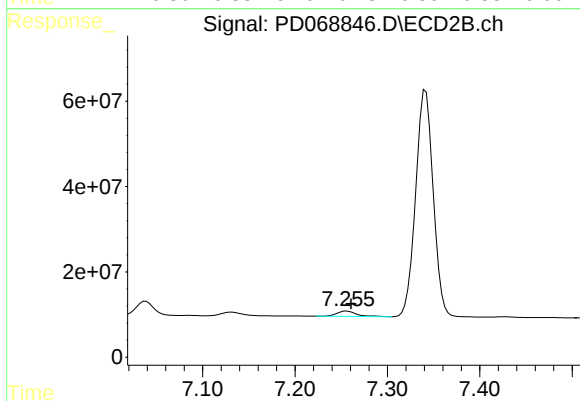

#18 Endrin aldehyde


R.T.: 7.256 min
Delta R.T.: -0.005 min
Response: 18134400
Conc: 3.00 ng/ml

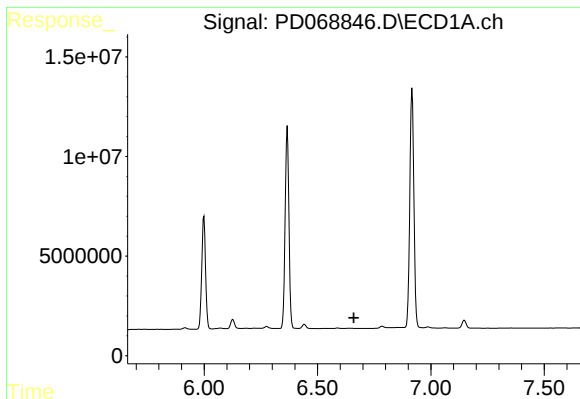

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

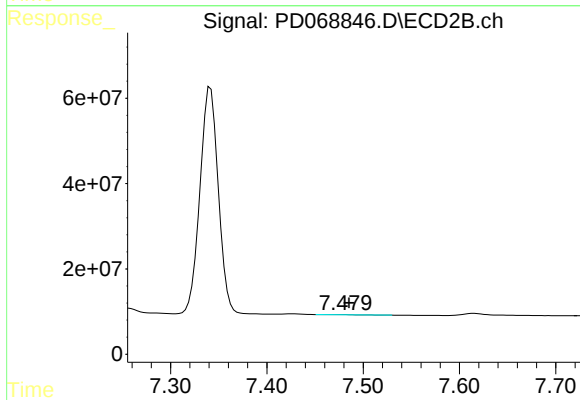


#19 Endosulfan Sulfate

R.T.: 7.478 min
Delta R.T.: -0.008 min
Response: 200673
Conc: 0.03 ng/ml

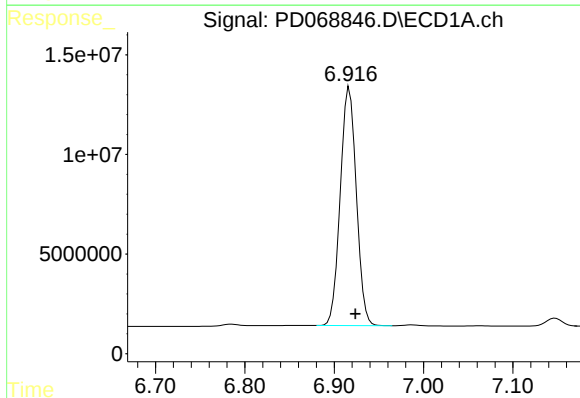


#20 Methoxychlor

R.T.: 6.917 min
Delta R.T.: -0.007 min
Response: 149577745
Conc: 215.83 ng/ml

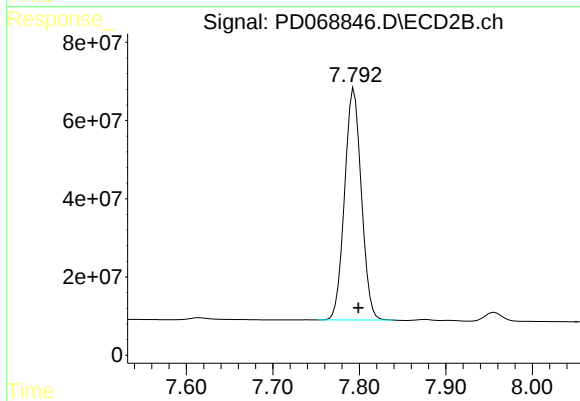

#20 Methoxychlor


R.T.: 7.794 min
Delta R.T.: -0.005 min
Response: 792980996
Conc: 217.54 ng/ml

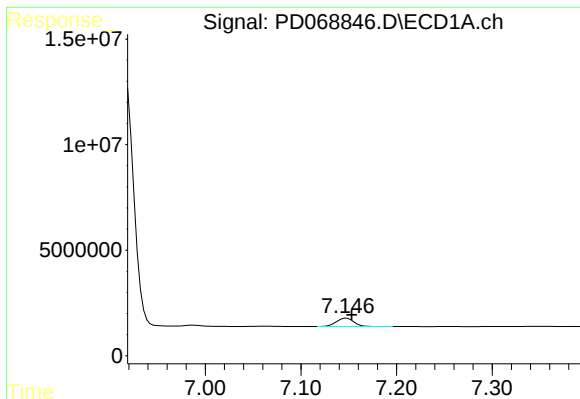

#21 Endrin ketone


R.T.: 7.148 min
Delta R.T.: -0.005 min
Response: 5006518
Conc: 3.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

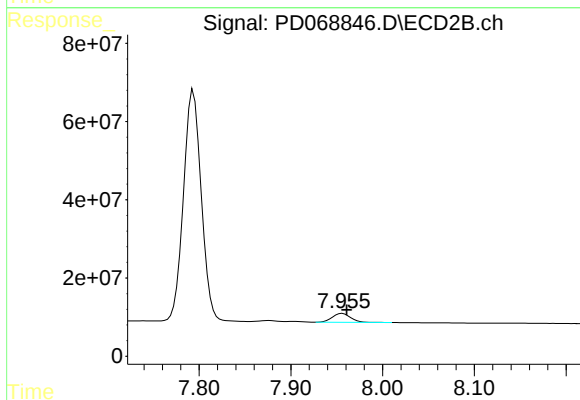


#21 Endrin ketone

R.T.: 7.956 min
Delta R.T.: -0.005 min
Response: 30953374
Conc: 3.99 ng/ml

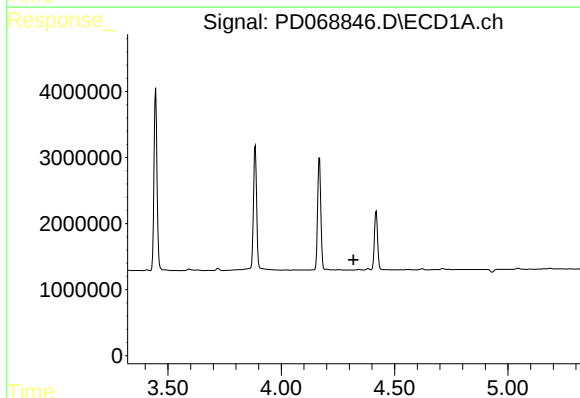


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

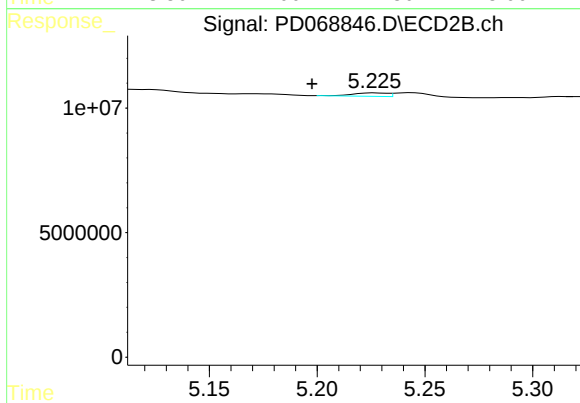

#23 Chlordane-1


R.T.: 5.227 min
Delta R.T.: 0.029 min
Response: 1553061
Conc: 3.94 ng/ml

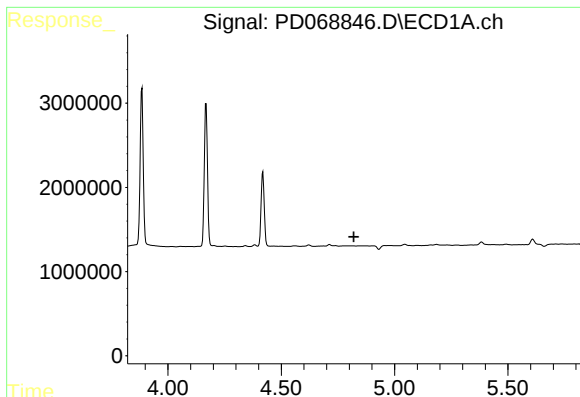

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

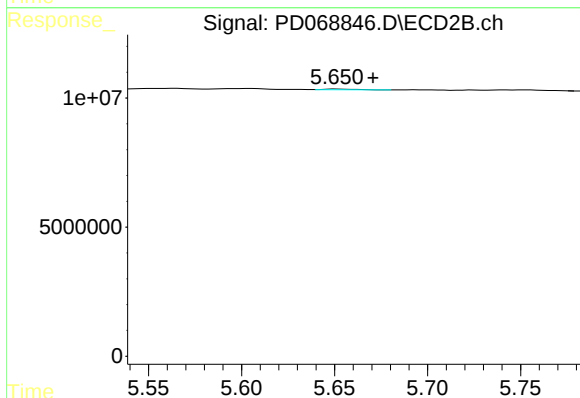


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: -0.020 min
Response: 358727
Conc: 0.94 ng/ml

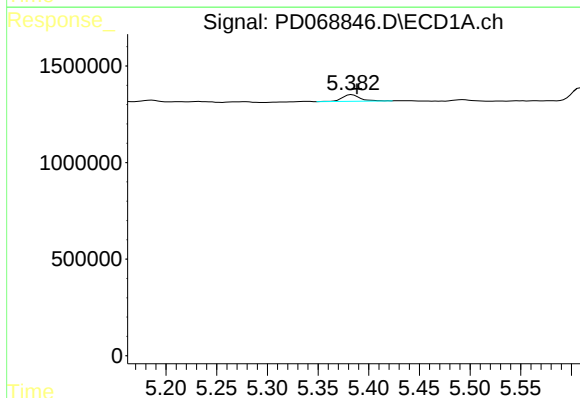


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: -0.005 min
Response: 421015
Conc: 3.02 ng/ml

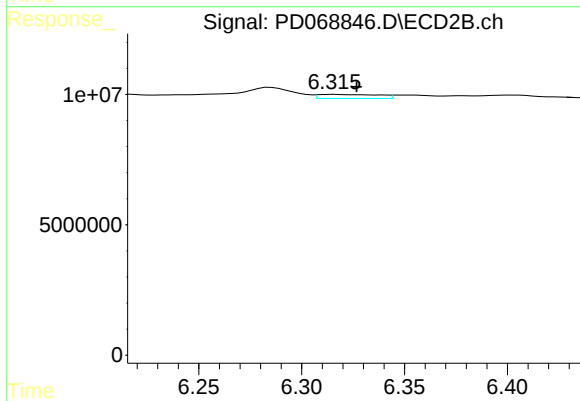

#25 Chlordane-3


R.T.: 6.316 min
Delta R.T.: -0.011 min
Response: 3151463
Conc: 2.35 ng/ml

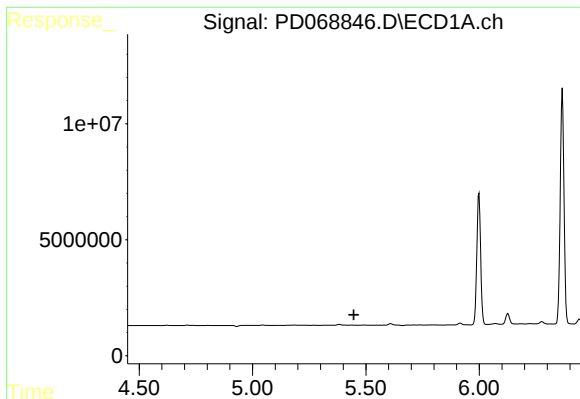

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

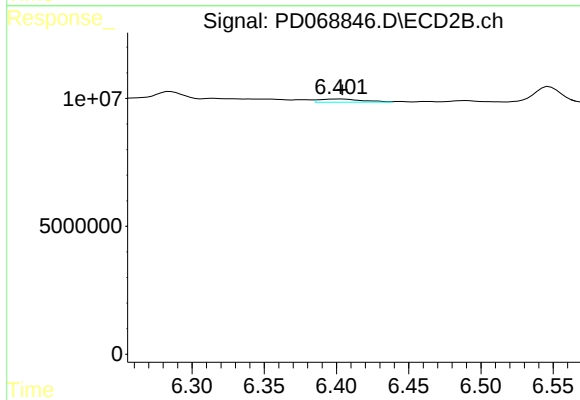


#26 Chlordane-4

R.T.: 6.403 min
Delta R.T.: -0.001 min
Response: 2534370
Conc: 1.63 ng/ml

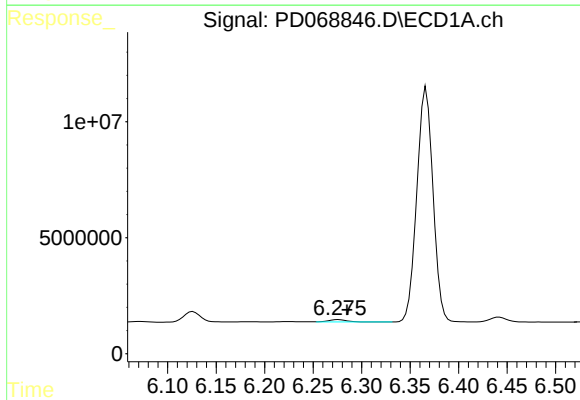


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: -0.009 min
Response: 1350294
Conc: 27.03 ng/ml

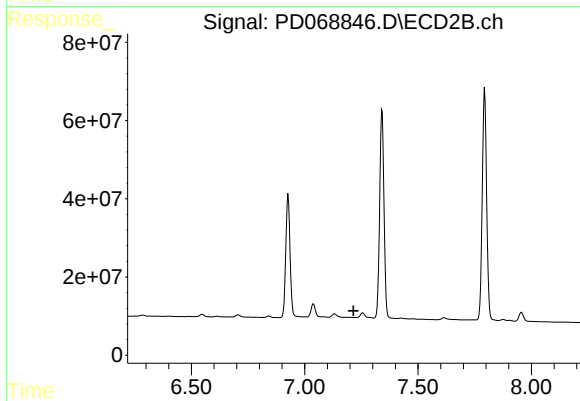

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.215 min
Response: 0
Conc: N.D.

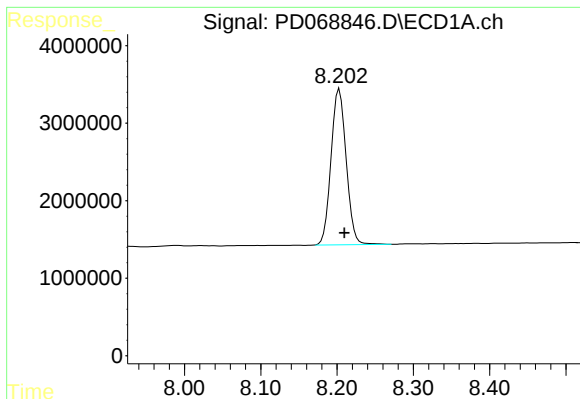

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.007 min
Response: 27698358
Conc: 21.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

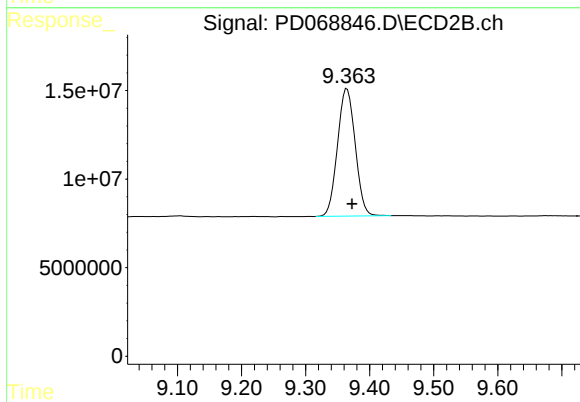

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.008 min
Response: 138148467
Conc: 24.38 ng/ml