

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
 Data File : PD052423.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 12:59
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:32:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


2) A	alpha-BHC	0.000	4.459	0 71921085	N.D.	1.493
6) B	beta-BHC	0.000	4.931f	0 39574045	N.D.	1.908
13) MA	Dieldrin	0.000	6.544	0 37123309	N.D.	1.075

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
Data File : PD052423.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 12:59
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:32:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

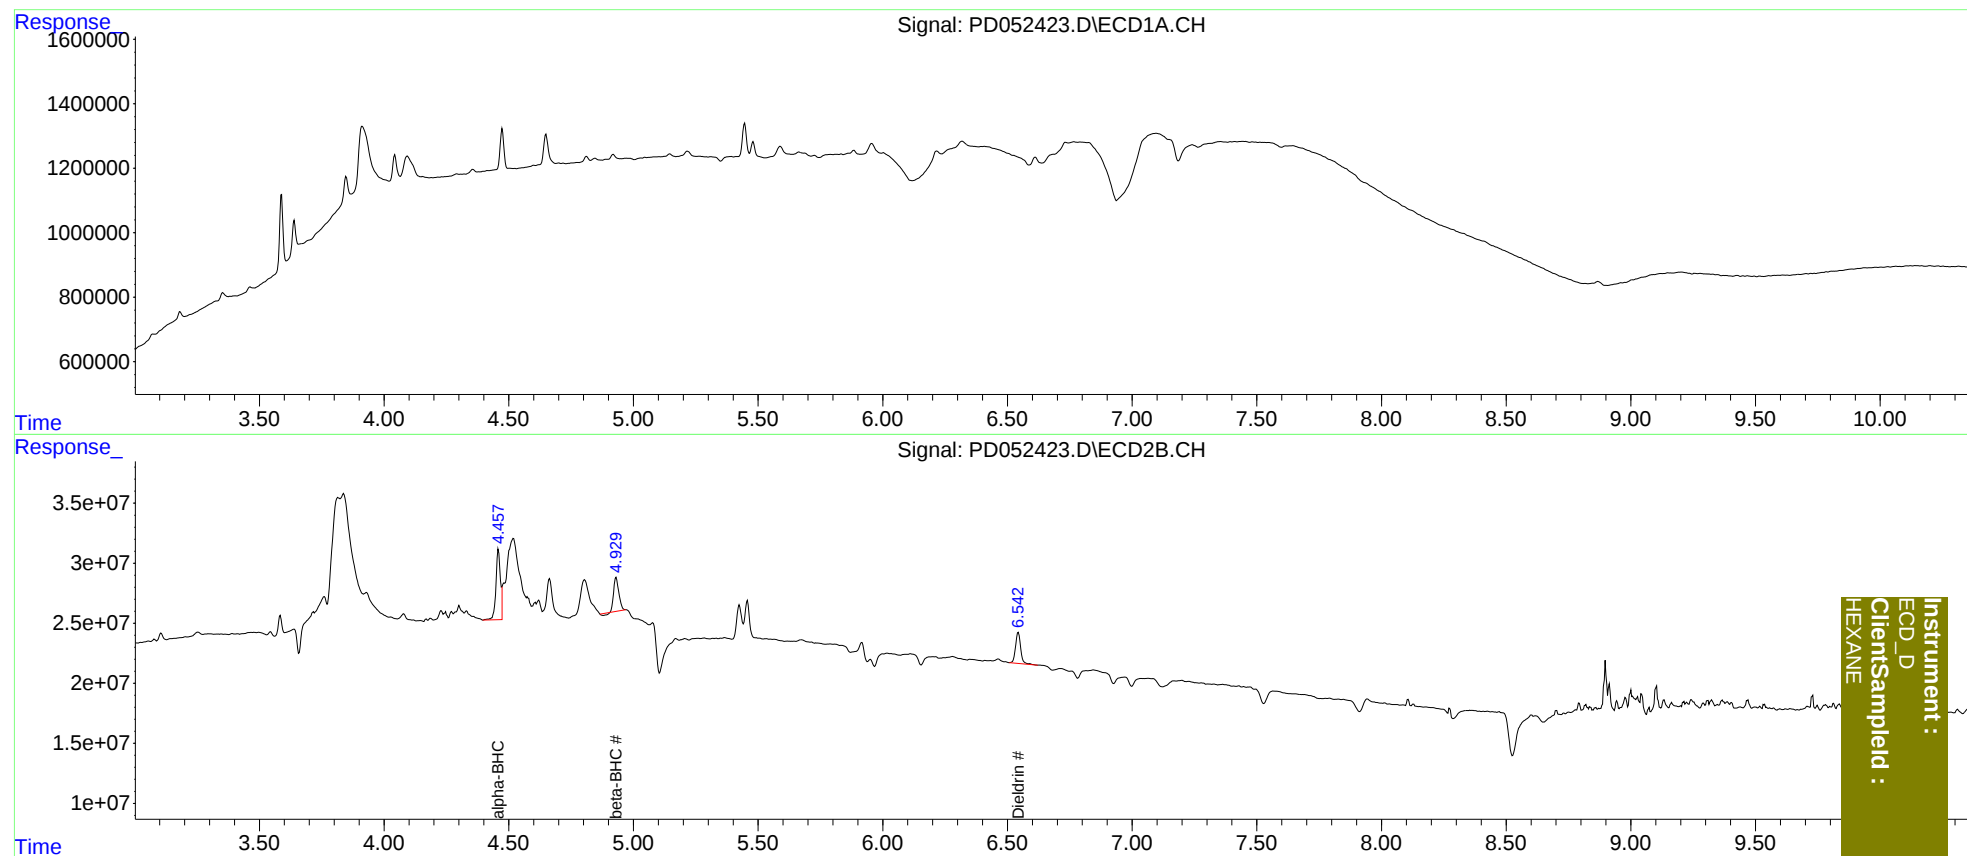


Instrument :
ECD_D
ClientSampleId :
HEXANE

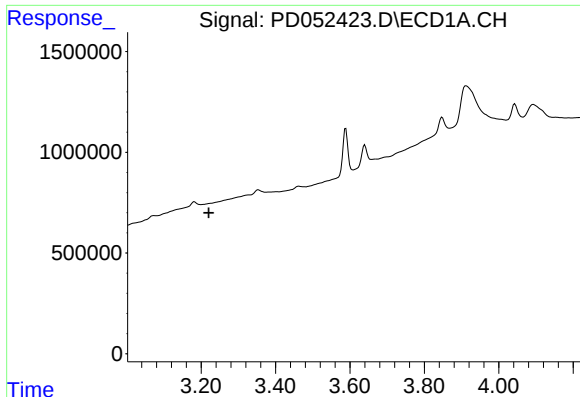

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

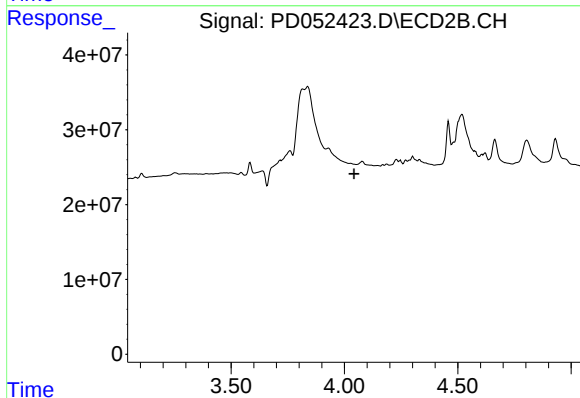


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.042 min
Response: 0
Conc: N.D.

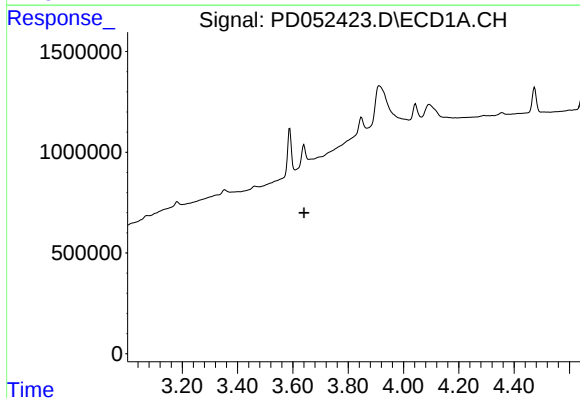


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

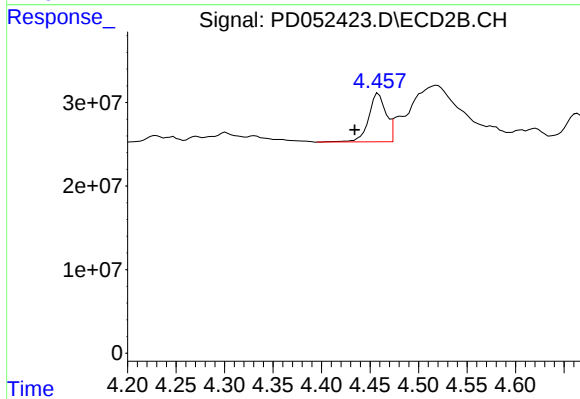

#2 alpha-BHC


R.T.: 4.459 min
Delta R.T.: 0.024 min
Response: 71921085
Conc: 1.49 ng/ml

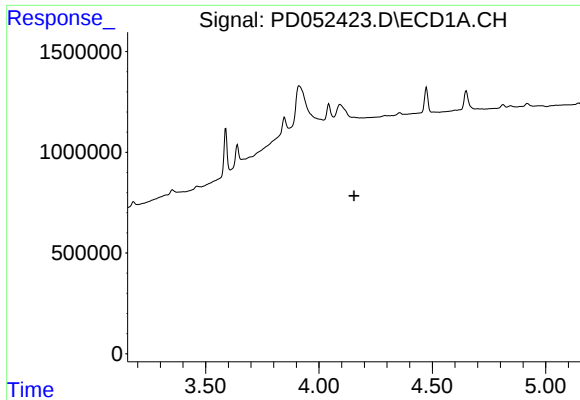

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

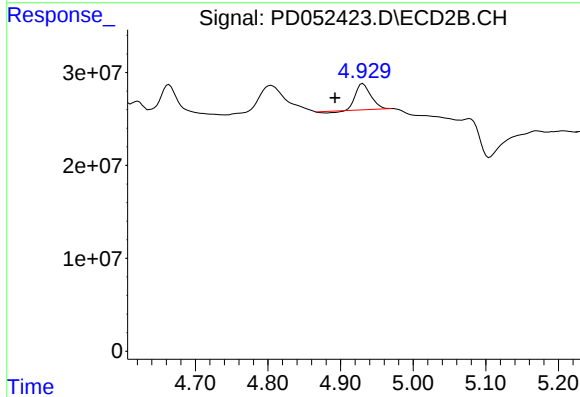


#6 beta-BHC

R.T.: 4.931 min
Delta R.T.: 0.039 min
Response: 39574045
Conc: 1.91 ng/ml

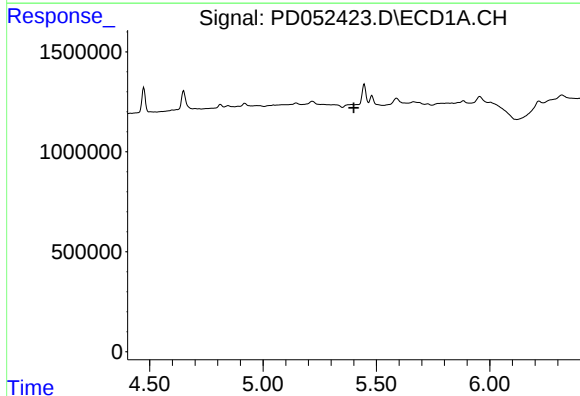


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

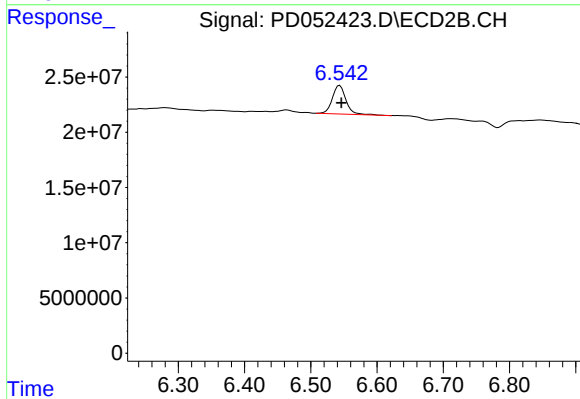

#13 Dieldrin


R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 37123309
Conc: 1.07 ng/ml

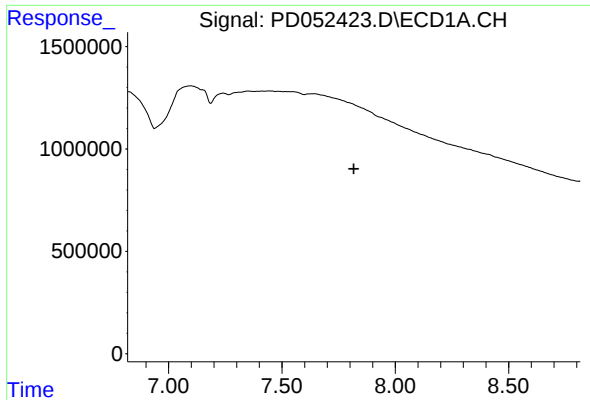

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

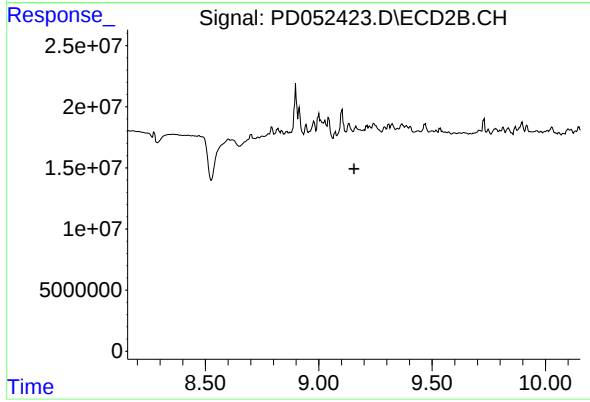

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.157 min
Response: 0
Conc: N.D.