

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
 Data File : PD052424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 13:13
 Operator : AJ\SJ
 Sample : PIBLK10
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:33:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.041	32699914	745.7E6	23.053	23.334
27)	SA Decachlor...	7.816	9.156	63886659	874.4E6	42.526	44.980
Target Compounds							
6)	B beta-BHC	0.000	4.933f	0	48468676	N.D.	2.337

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
Data File : PD052424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 13:13
Operator : AJ\SJ
Sample : PIBLK10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:33:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

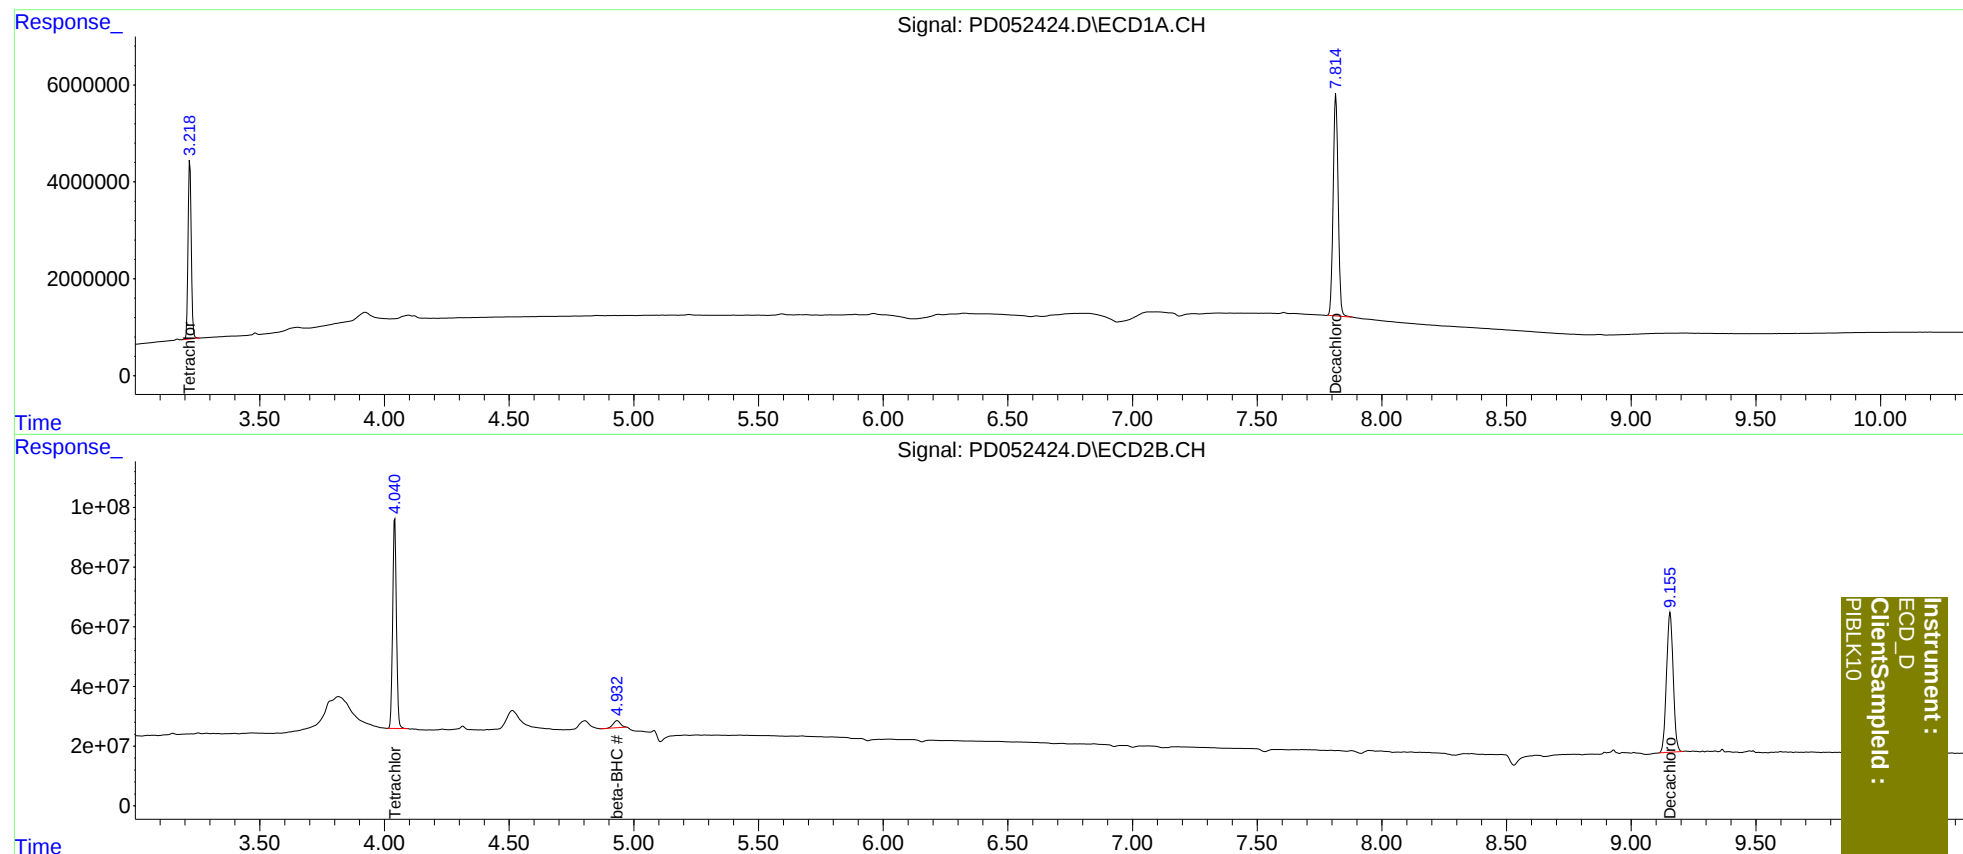


Instrument :
ECD_D
ClientSampleId :
PIBLK10

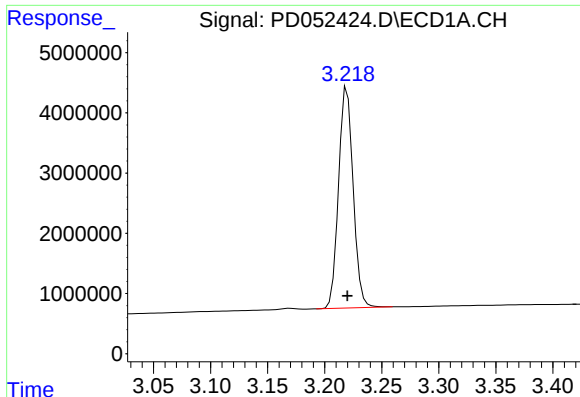

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 32699914
Conc: 23.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK10

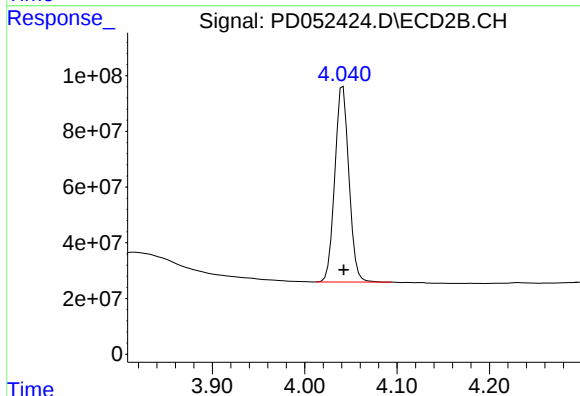


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.000 min
Response: 745683816
Conc: 23.33 ng/ml

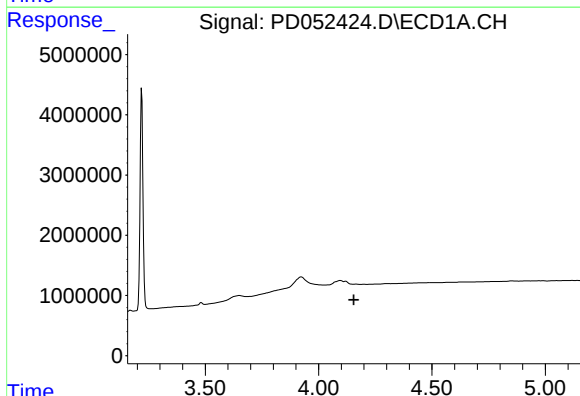


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

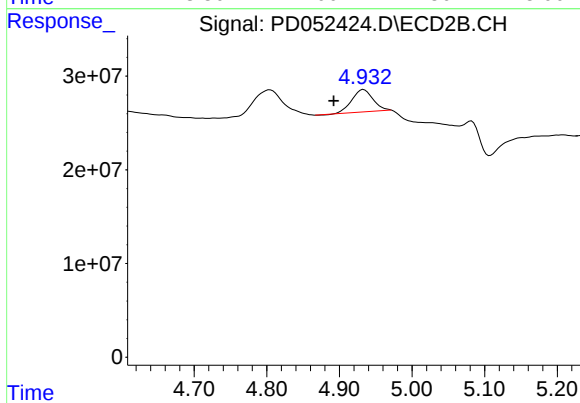

#6 beta-BHC


R.T.: 4.933 min
Delta R.T.: 0.041 min
Response: 48468676
Conc: 2.34 ng/ml

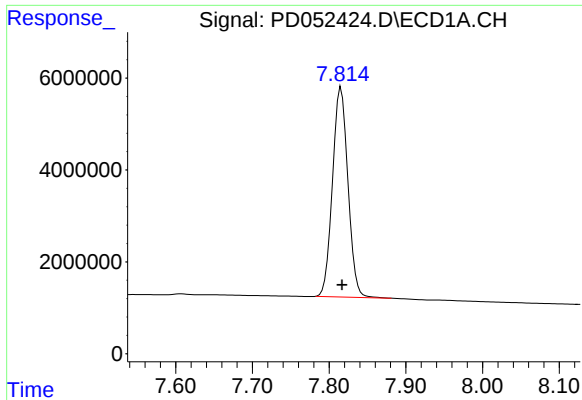

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.001 min
Response: 63886659
Conc: 42.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK10

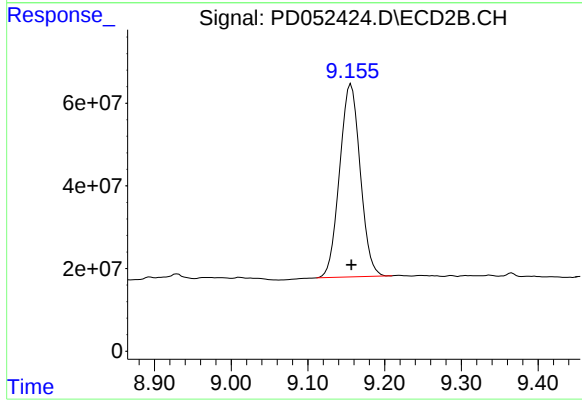

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 874439513
Conc: 44.98 ng/ml