

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
 Data File : PD052476.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 2:40
 Operator : AJ\SJ
 Sample : K2119-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5A9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 07:53:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.042	22487692	492.7E6	15.854	15.419
27)	SA Decachlor...	7.814	9.155	34517195	441.9E6	22.976	22.728
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0	12428064	N.D.	0.258
3)	MA gamma-BHC...	3.920	0.000	5521449	0	2.496	N.D. #
6)	B beta-BHC	0.000	4.939f	0	7965460	N.D.	0.384
8)	B Heptachlo...	0.000	5.911	0	44359569	N.D.	1.164
9)	A Endosulfan I	0.000	6.238f	0	26287372	N.D.	0.760
10)	B trans-Chl...	0.000	6.164	0	13437441	N.D.	0.355
11)	B cis-Chlor...	0.000	6.238	0	26287372	N.D.	0.728
15)	B Endosulfa...	0.000	6.952	0	10030788	N.D.	0.352
16)	A 4,4'-DDD	0.000	6.952f	0	10030788	N.D.	0.377


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
Data File : PD052476.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 2:40
Operator : AJ\SJ
Sample : K2119-14
Misc :
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 07:53:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

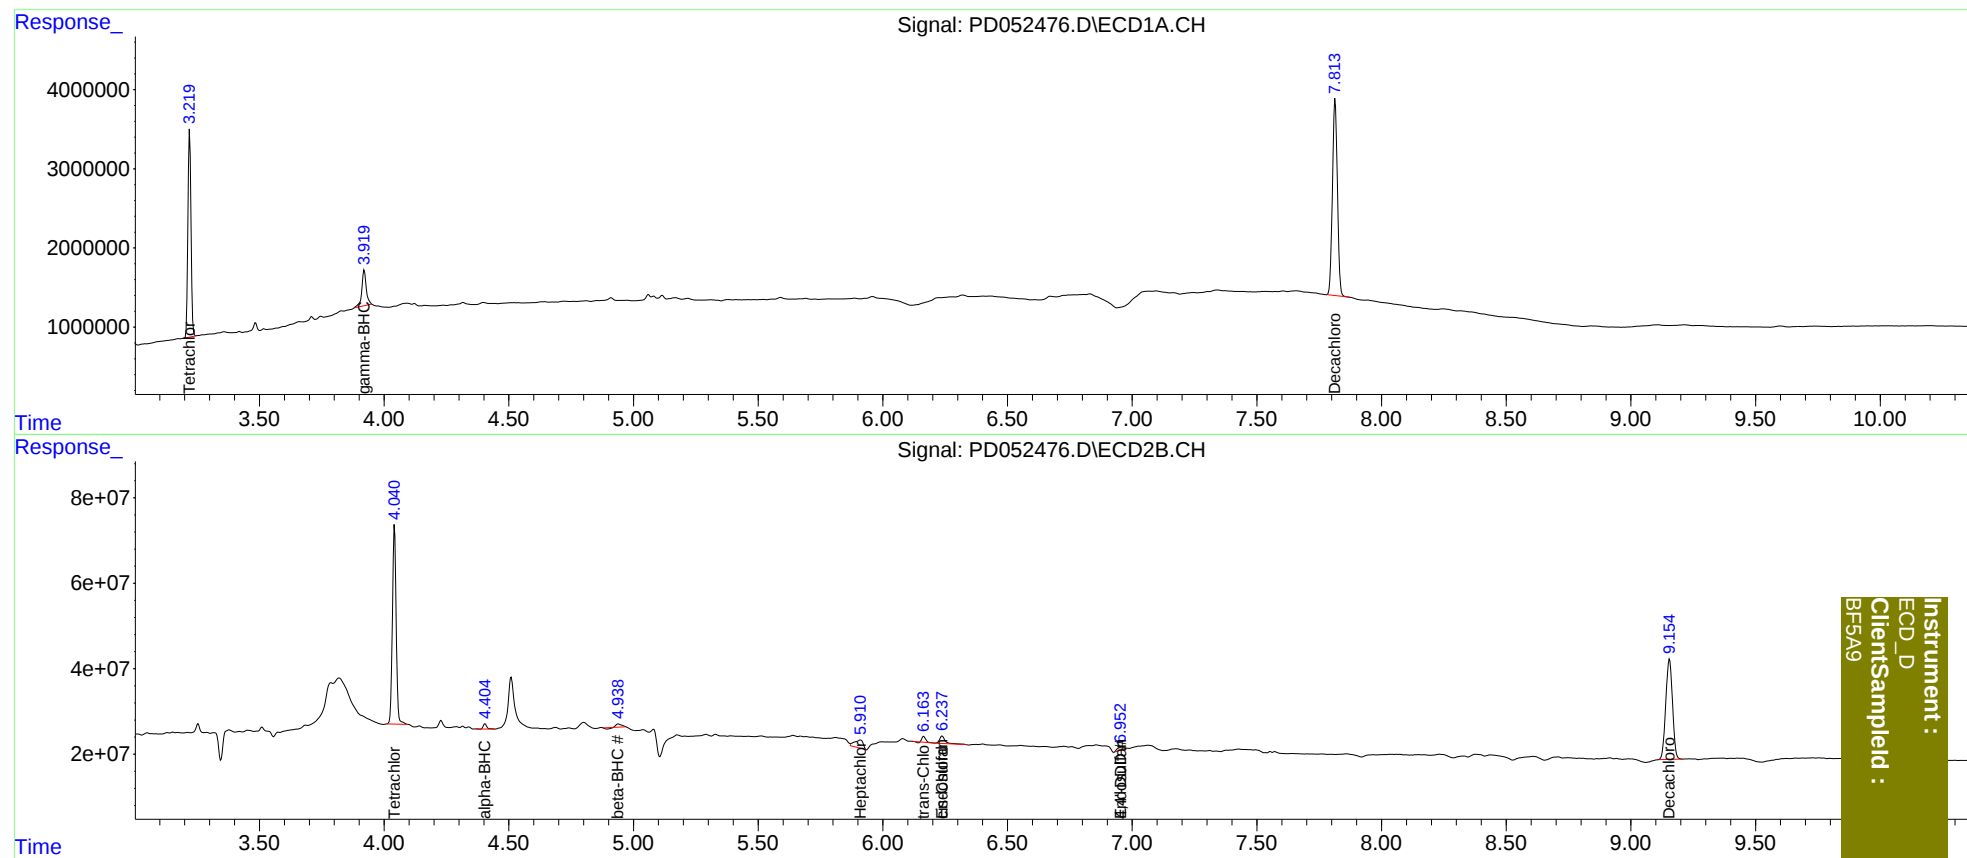


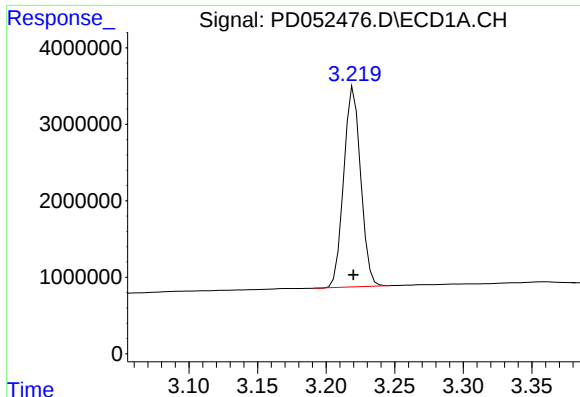

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 22487692
Conc: 15.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5A9

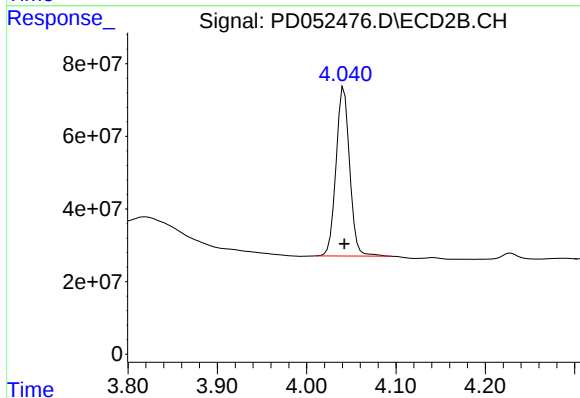


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 492729582
Conc: 15.42 ng/ml

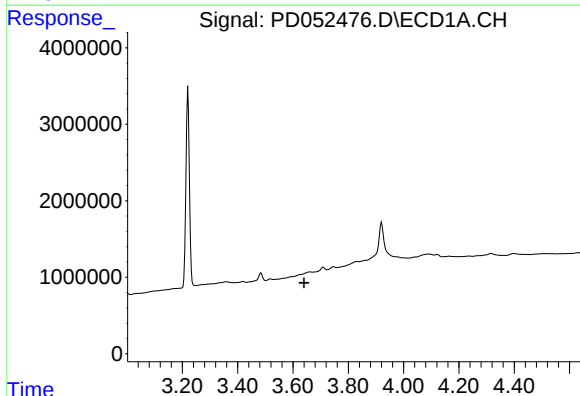


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

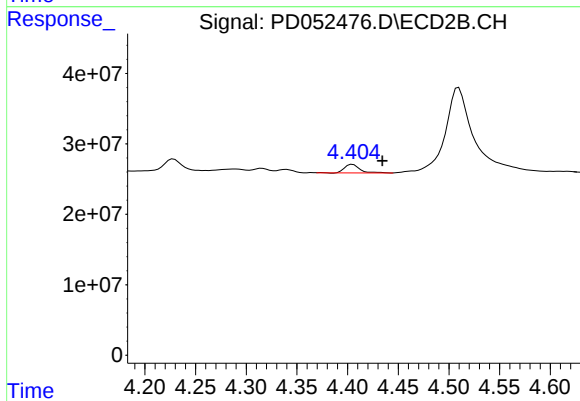

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.029 min
Response: 12428064
Conc: 0.26 ng/ml

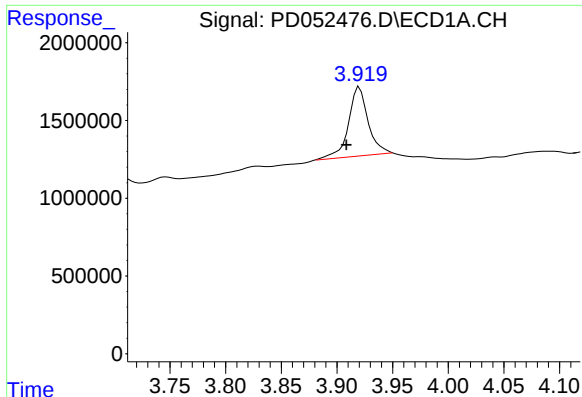

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.012 min
Response: 5521449
Conc: 2.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5A9

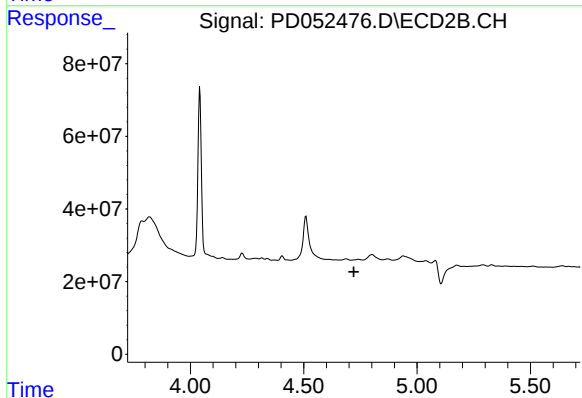


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

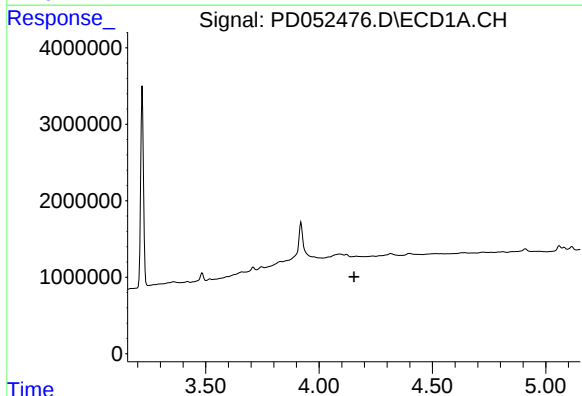


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

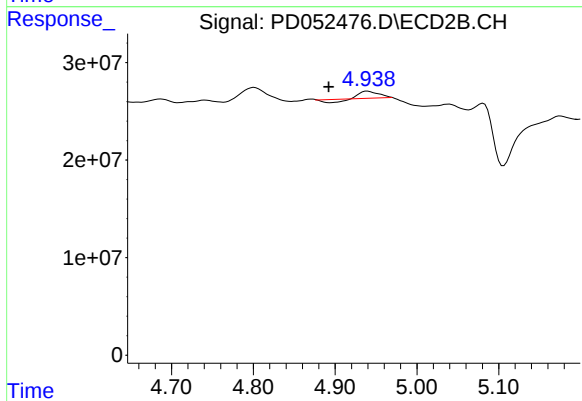

#6 beta-BHC


R.T.: 4.939 min
Delta R.T.: 0.047 min
Response: 7965460
Conc: 0.38 ng/ml

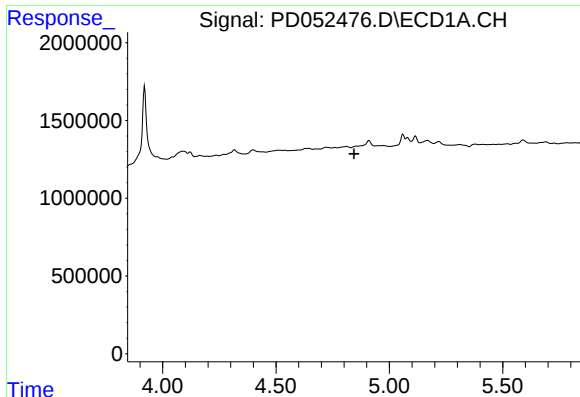

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5A9

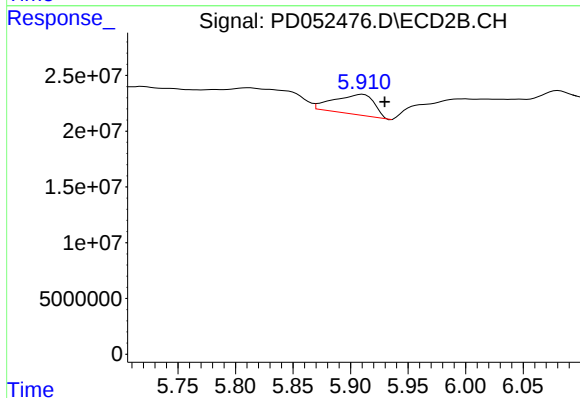


#8 Heptachlor epoxide

R.T.: 5.911 min
Delta R.T.: -0.019 min
Response: 44359569
Conc: 1.16 ng/ml

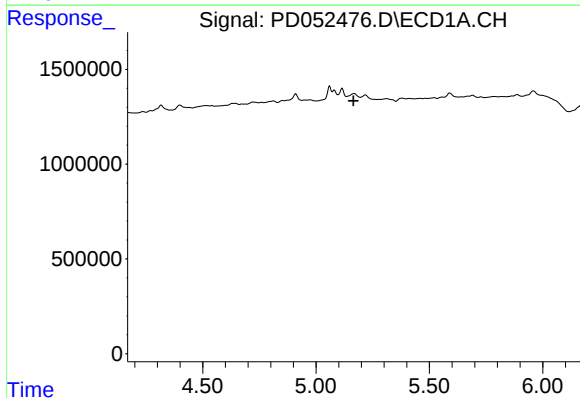


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

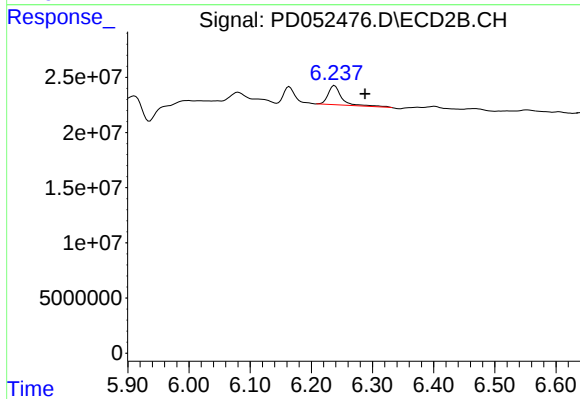

#9 Endosulfan I


R.T.: 6.238 min
Delta R.T.: -0.050 min
Response: 26287372
Conc: 0.76 ng/ml

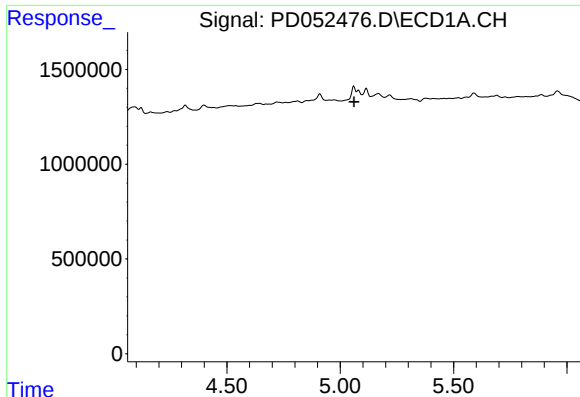

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5A9

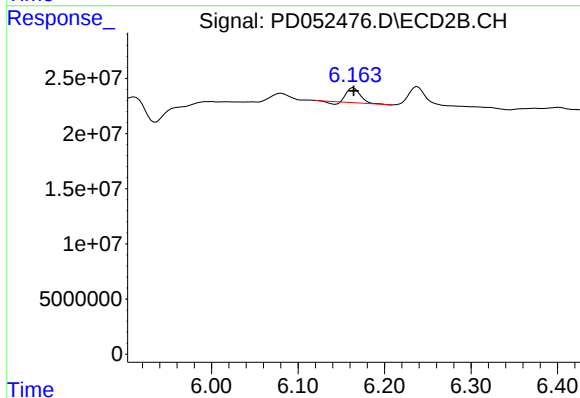


#10 trans-Chlordane

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 13437441
Conc: 0.36 ng/ml

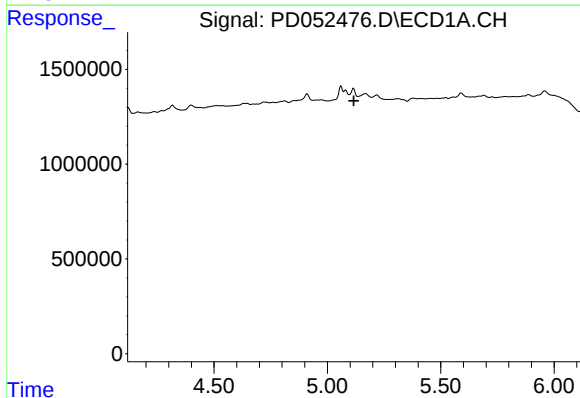


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.117 min
Response: 0
Conc: N.D.

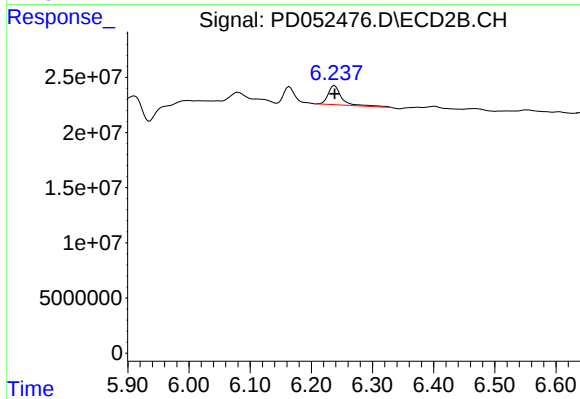

#11 cis-Chlordane


R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 26287372
Conc: 0.73 ng/ml

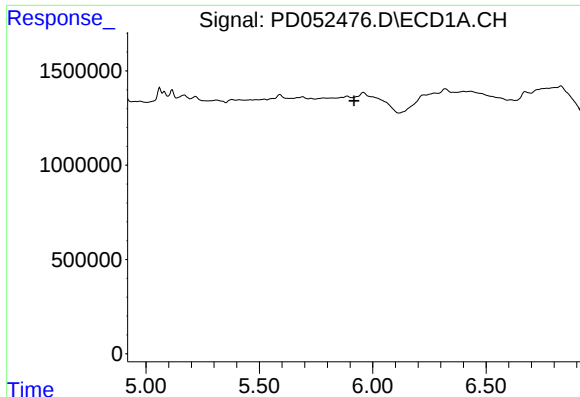

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5A9

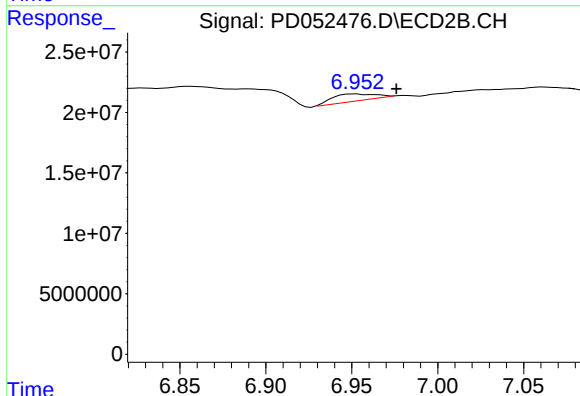


#15 Endosulfan II

R.T.: 6.952 min
Delta R.T.: -0.024 min
Response: 10030788
Conc: 0.35 ng/ml

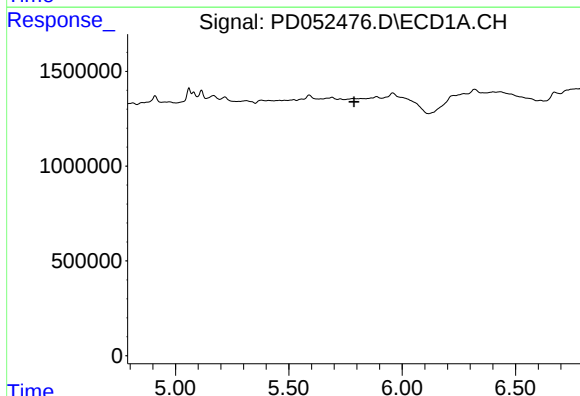


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.788 min
Response: 0
Conc: N.D.

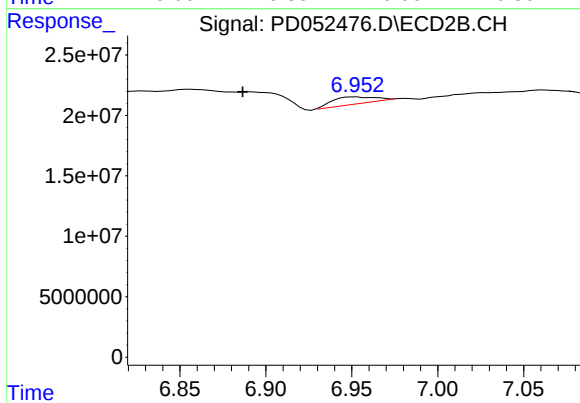

#16 4,4'-DDD


R.T.: 6.952 min
Delta R.T.: 0.066 min
Response: 10030788
Conc: 0.38 ng/ml

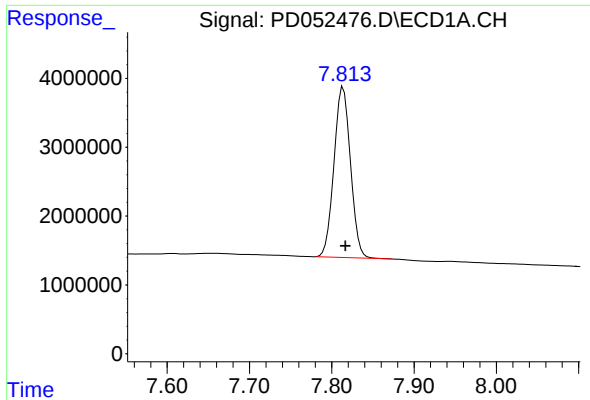

#27 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: -0.003 min
Response: 34517195
Conc: 22.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5A9

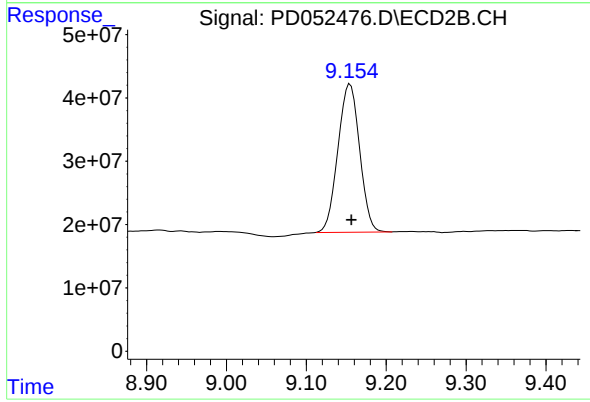

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 441853395
Conc: 22.73 ng/ml