

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
 Data File : PD052467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 00:33
 Operator : AJ\SJ
 Sample : K2119-04
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5A1

Manual Integrations
 APPROVED

Sohil
 4/3/2019 9:08:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 06:04:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.041	21271930	465.4E6	14.997	14.563
27)	SA Decachlor...	7.815	9.155	38794685	519.1E6	25.823	26.703
Target Compounds							
4)	MA Heptachlor	4.183	5.233	824606	21950753	0.372m	0.494 #
10)	B trans-Chl...	5.059	6.163	2780009	55624129	1.351m	1.471
11)	B cis-Chlor...	5.114	6.238	499567	20981393	0.249m	0.581m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040219\
Data File : PD052467.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 00:33
Operator : AJ\SJ
Sample : K2119-04
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 06:04:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

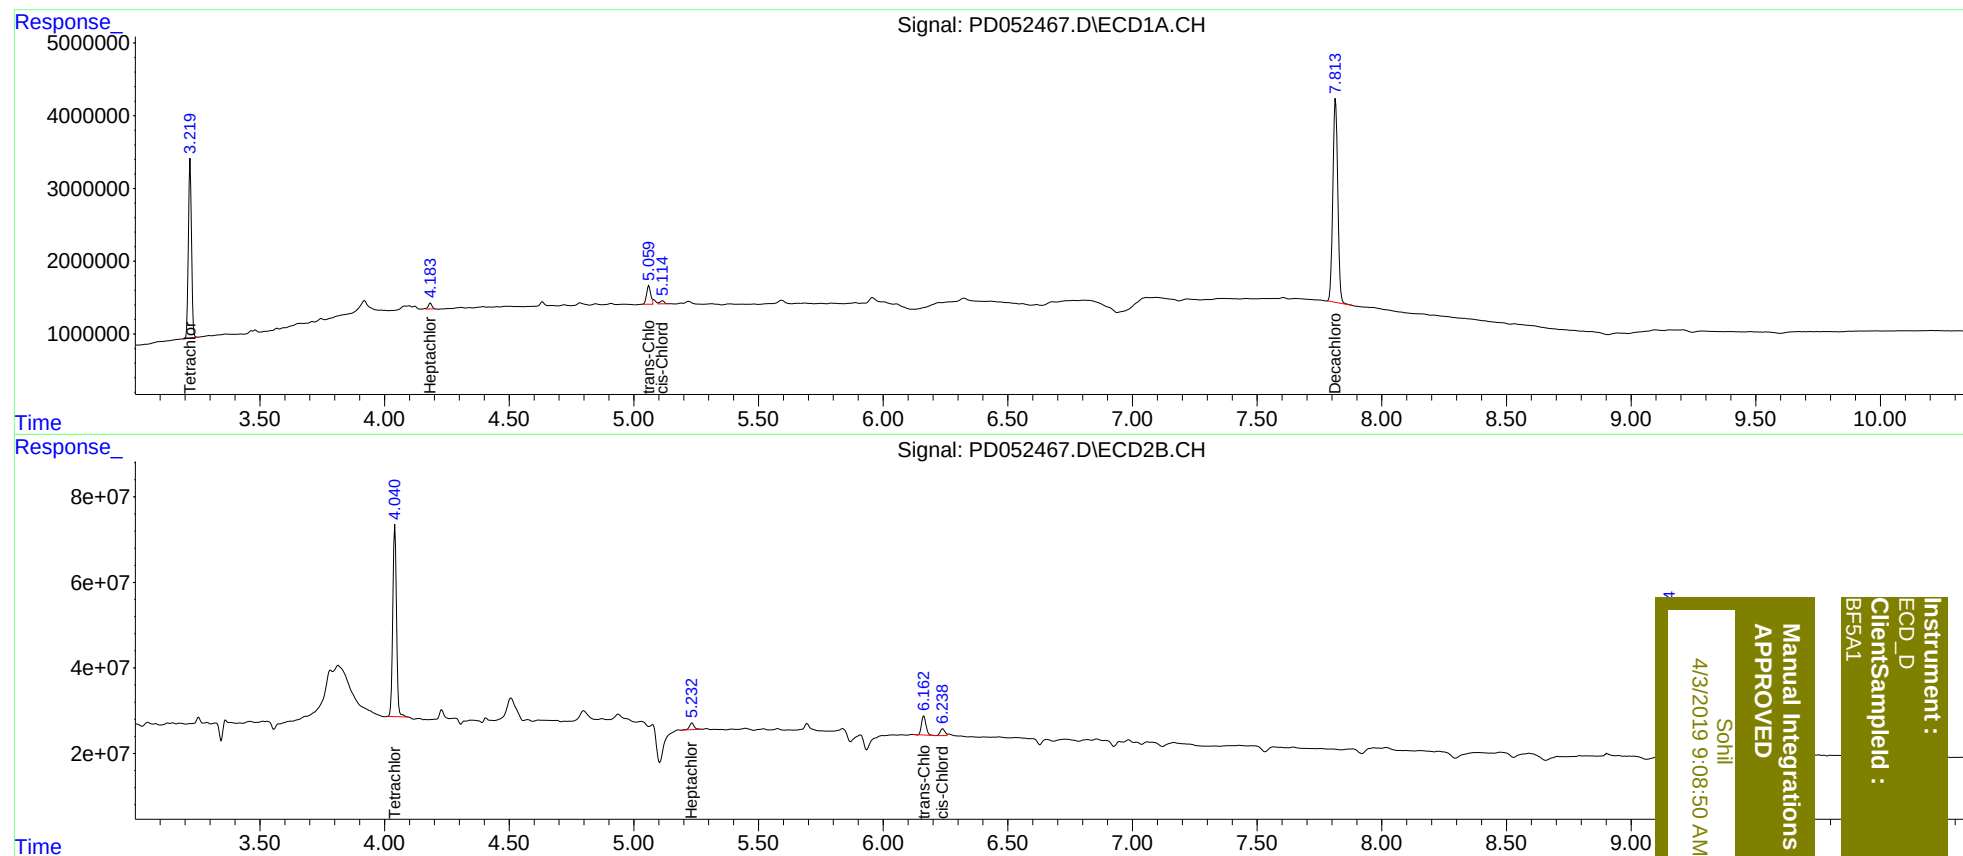

4/3/2019 9:08:50 AM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampleId :
BF5A1