

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 10:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:50:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.895	17256066	21355071	24.169	27.220
28)	SA Decachlor...	7.870	8.900	18059858	21621029	23.720	24.582
Target Compounds							
3)	MA gamma-BHC...	3.935f	0.000	1274798	0	1.184	N.D. #
7)	B delta-BHC	4.375	0.000	276975	0	0.268	N.D. #
9)	A Endosulfan I	5.173f	0.000	100308	0	0.121	N.D. #
11)	B alpha-Chl...	5.154	0.000	787802	0	0.860	N.D. #
18)	B Endrin al...	6.125	0.000	63599	0	0.103	N.D. #
25)	Chlordane-3	5.154f	0.000	787802	0	8.975	N.D. #
26)	Chlordane-4	5.154	0.000	787802	0	9.742	N.D. #
27)	Chlordane-5	5.989f	0.000	338438	0	12.696	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 10:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:50:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

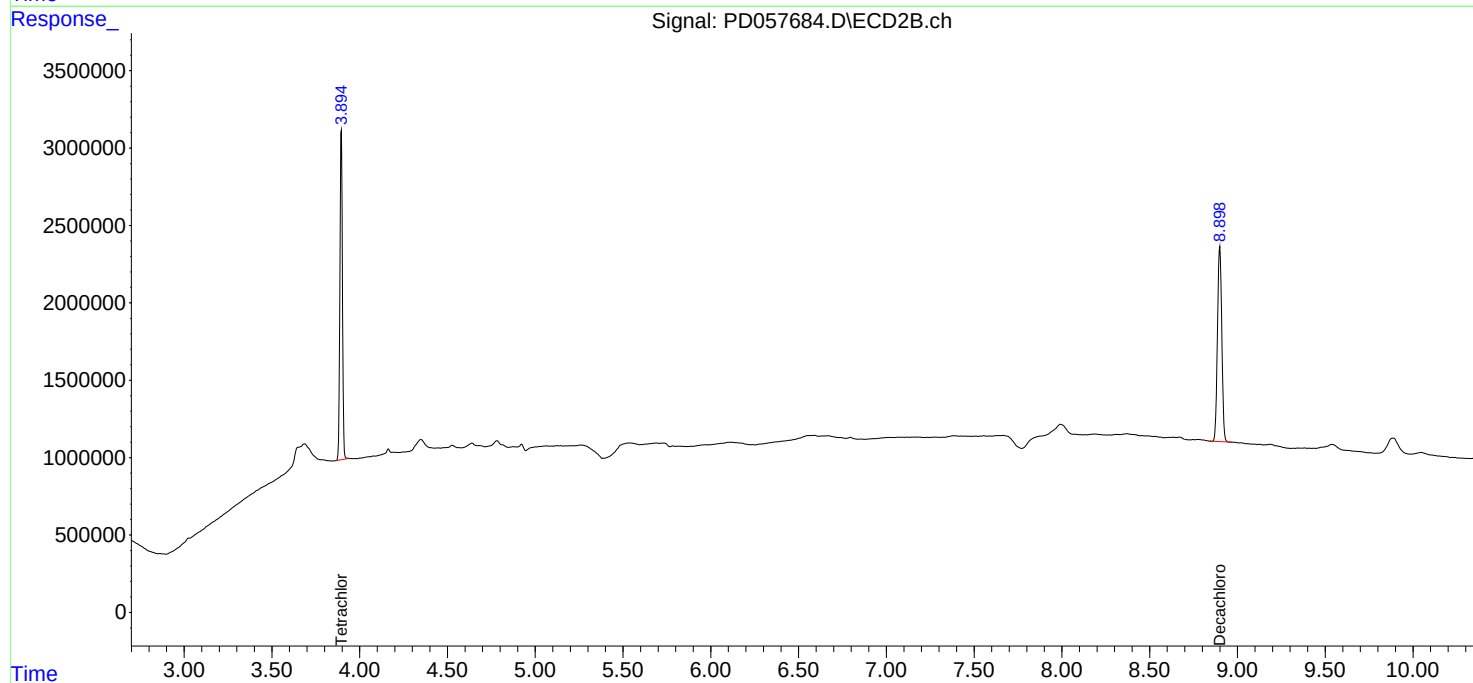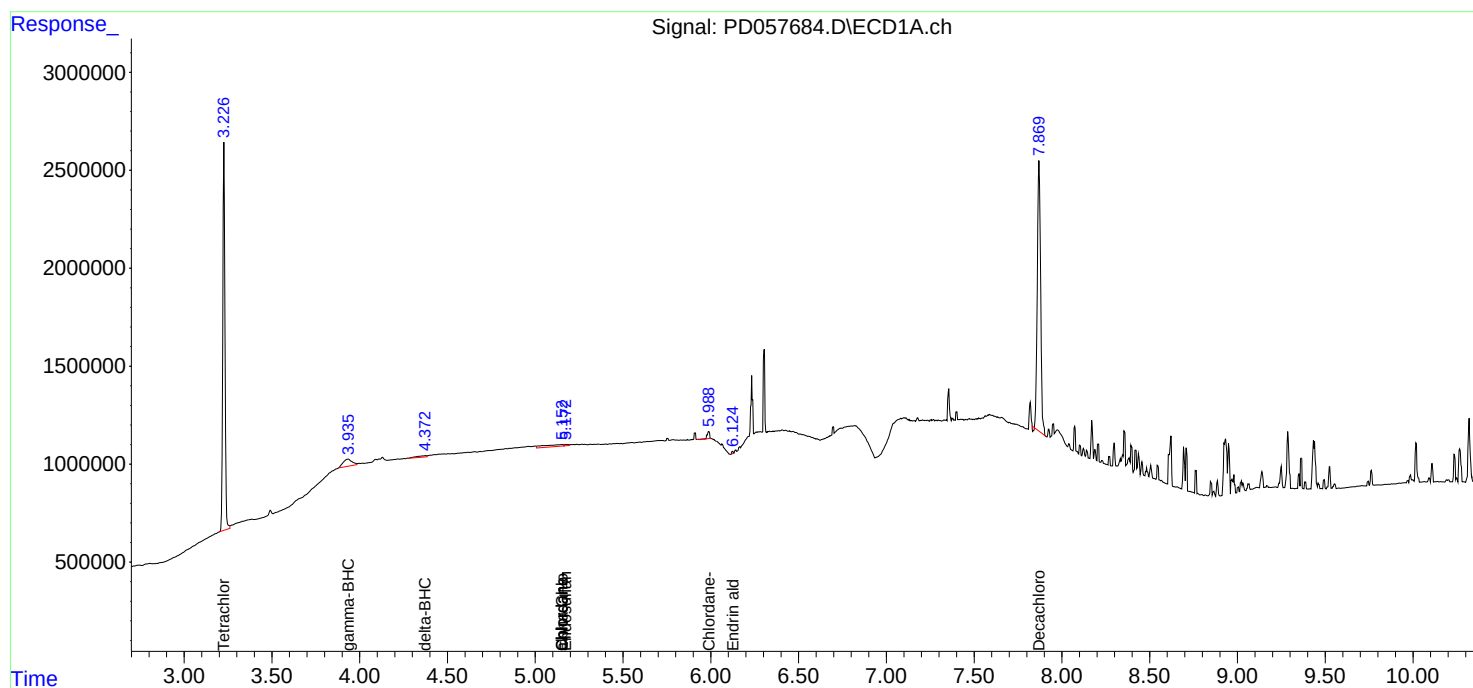


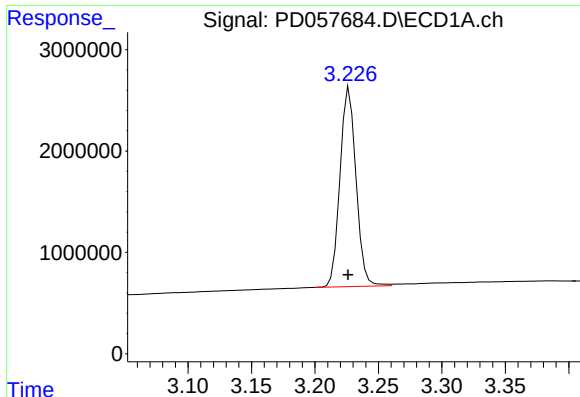

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 17256066
Conc: 24.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

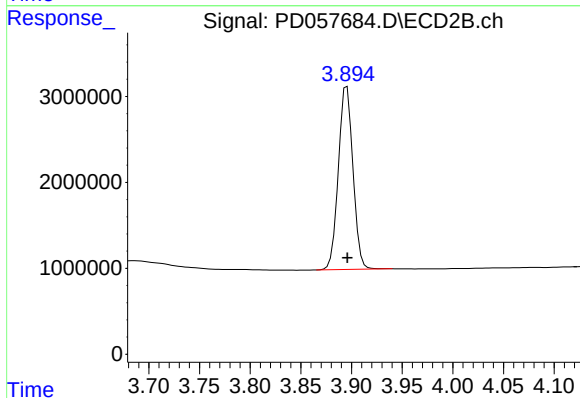


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 21355071
Conc: 27.22 ng/ml

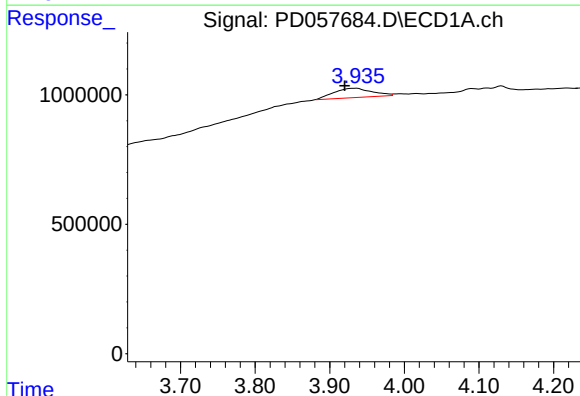


#3 gamma-BHC (Lindane)

R.T.: 3.935 min
Delta R.T.: 0.015 min
Response: 1274798
Conc: 1.18 ng/ml

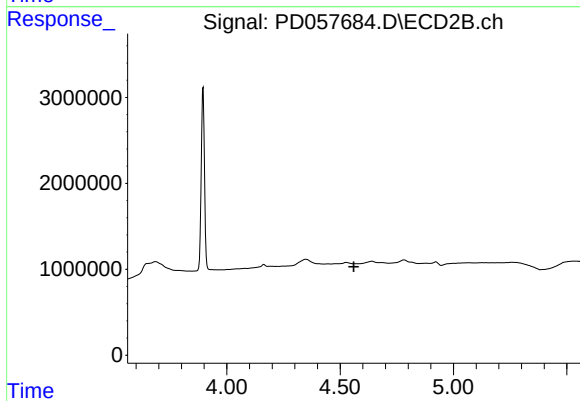

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

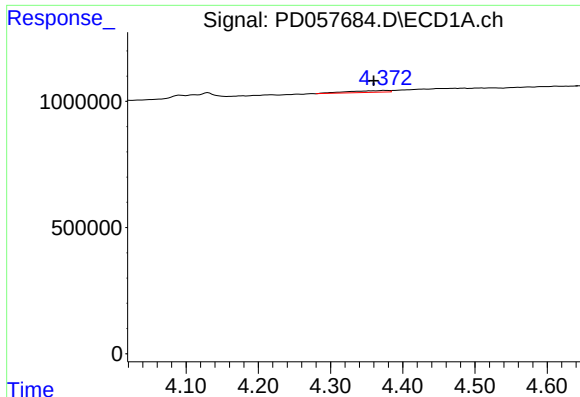

#7 delta-BHC


R.T.: 4.375 min
Delta R.T.: 0.015 min
Response: 276975
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

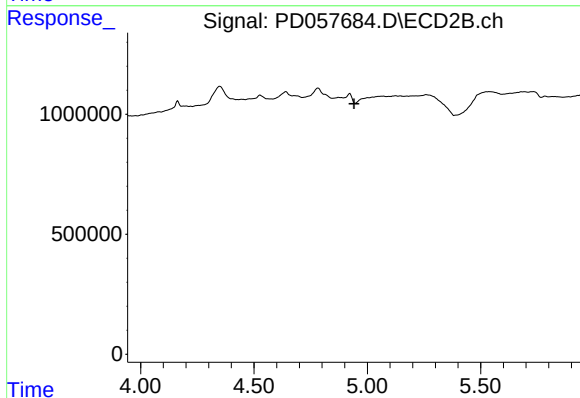


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

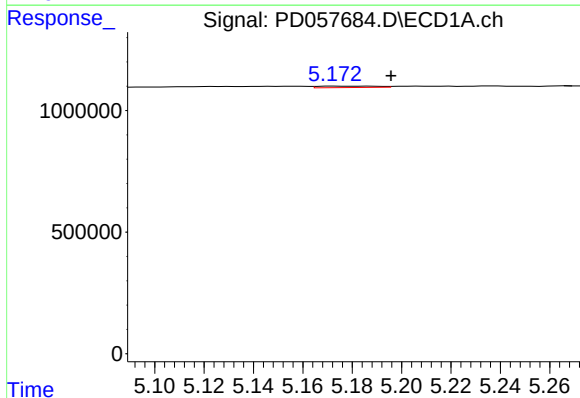


#9 Endosulfan I

R.T.: 5.173 min
Delta R.T.: -0.022 min
Response: 100308
Conc: 0.12 ng/ml

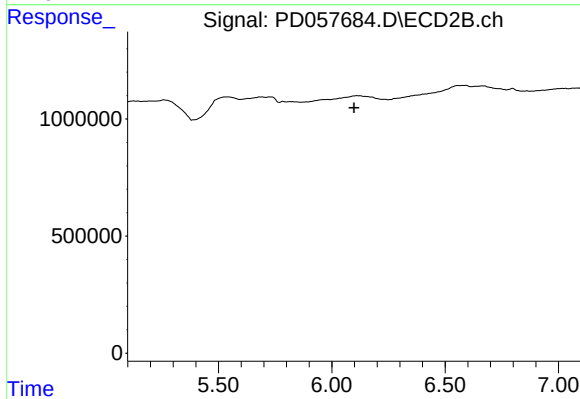

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

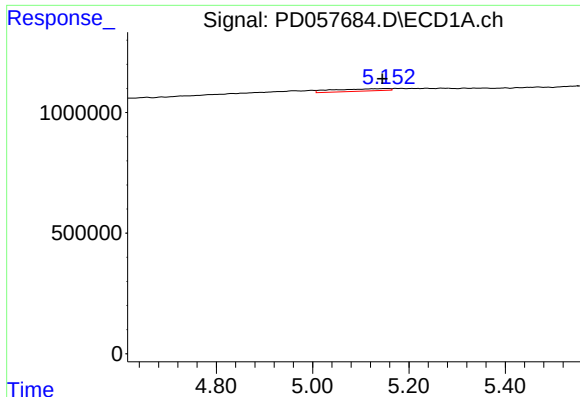

#11 alpha-Chlordane

R.T.: 5.154 min
Delta R.T.: 0.009 min
Response: 787802
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

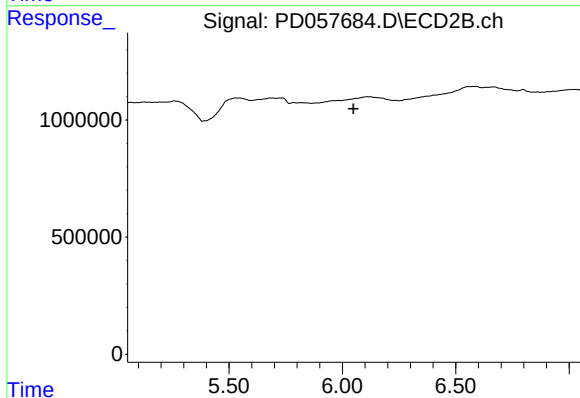


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.


#18 Endrin aldehyde

R.T.: 6.125 min
Delta R.T.: -0.001 min
Response: 63599
Conc: 0.10 ng/ml

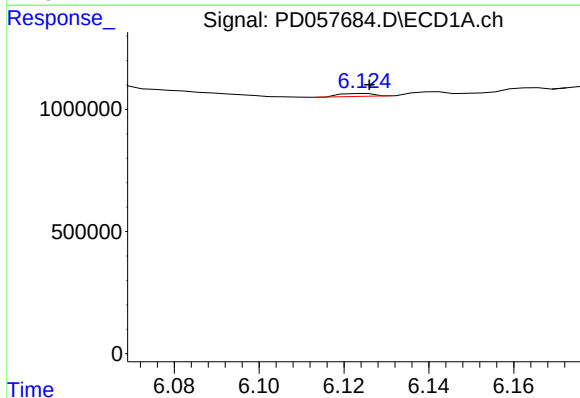

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

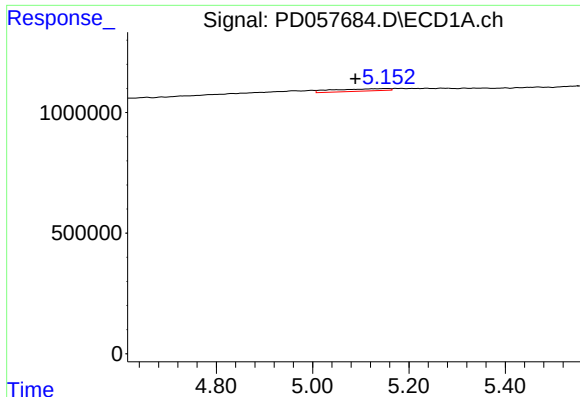

#25 Chlordane-3


R.T.: 5.154 min
Delta R.T.: 0.065 min
Response: 787802
Conc: 8.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

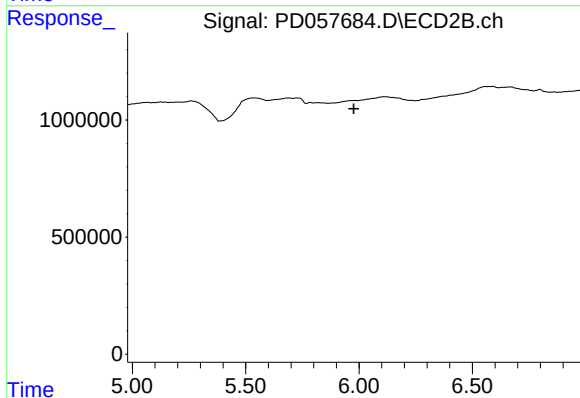


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

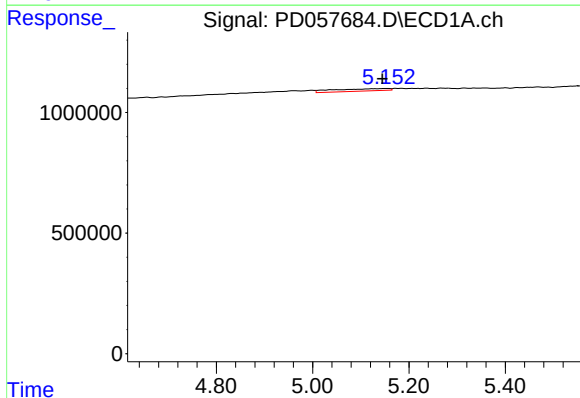


#26 Chlordane-4

R.T.: 5.154 min
Delta R.T.: 0.009 min
Response: 787802
Conc: 9.74 ng/ml

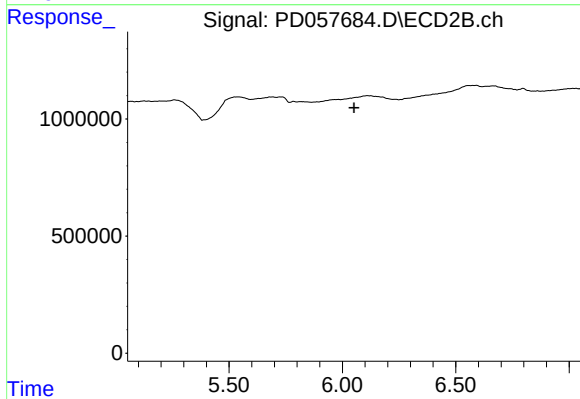

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

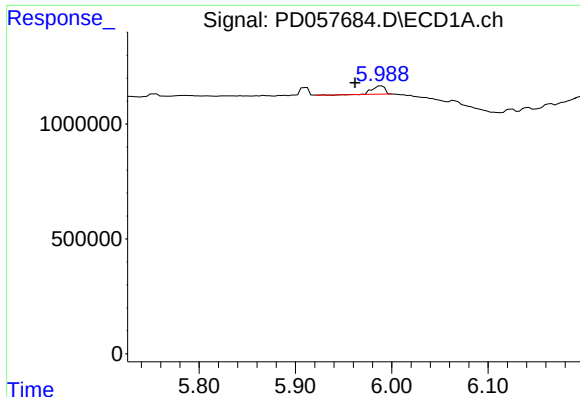

#27 Chlordane-5


R.T.: 5.989 min
Delta R.T.: 0.027 min
Response: 338438
Conc: 12.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

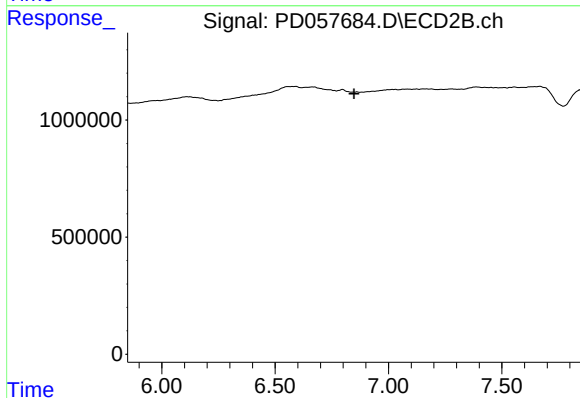


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.849 min
Response: 0
Conc: N.D.

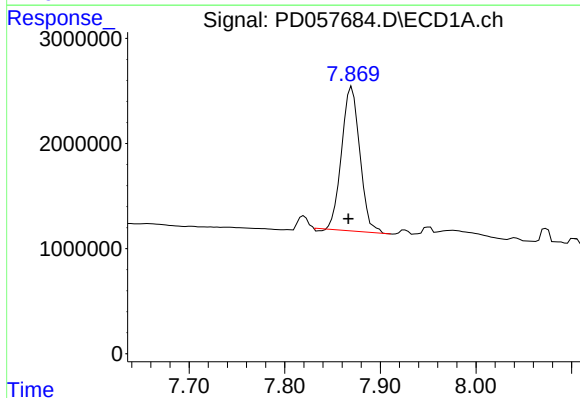

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.004 min
Response: 18059858
Conc: 23.72 ng/ml

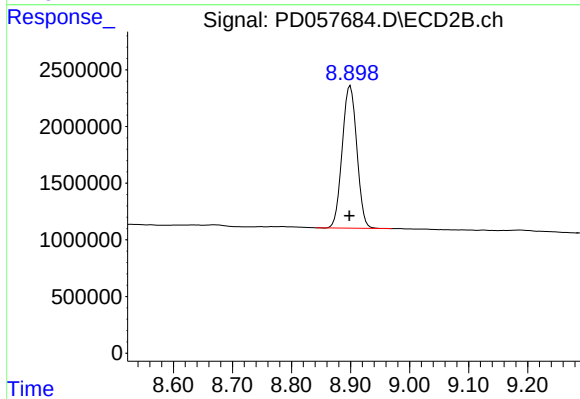

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.001 min
Response: 21621029
Conc: 24.58 ng/ml