

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 14:54
 Operator : AJ\MA
 Sample : PB127964BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB127963BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:52:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	16361961	20370572	22.916	25.965
28)	SA Decachlor...	7.871	8.900	17853377	21482825	23.449	24.425
Target Compounds							
3)	MA gamma-BHC...	3.933	0.000	884874	0	0.822	N.D. #
5)	MB Aldrin	4.435	0.000	101721	0	0.104	N.D. #
7)	B delta-BHC	4.365	0.000	170792	0	0.165	N.D. #
8)	B Heptachlo...	4.867	0.000	148818	0	0.176	N.D. #
10)	B gamma-Chl...	5.085	0.000	61511	0	0.067	N.D. #
11)	B alpha-Chl...	5.143	0.000	54522	0	0.060	N.D. #
14)	MA Endrin	5.711f	0.000	378718	0	0.521	N.D. #
16)	A 4,4'-DDD	5.793f	0.000	96952	0	0.170	N.D. #
18)	B Endrin al...	6.126	0.000	77767	0	0.126	N.D. #
25)	Chlordane-3	5.085	0.000	61511	0	0.701	N.D. #
26)	Chlordane-4	5.143	0.000	54522	0	0.674	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 14:54
Operator : AJ\MA
Sample : PB127964BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB127963BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:52:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

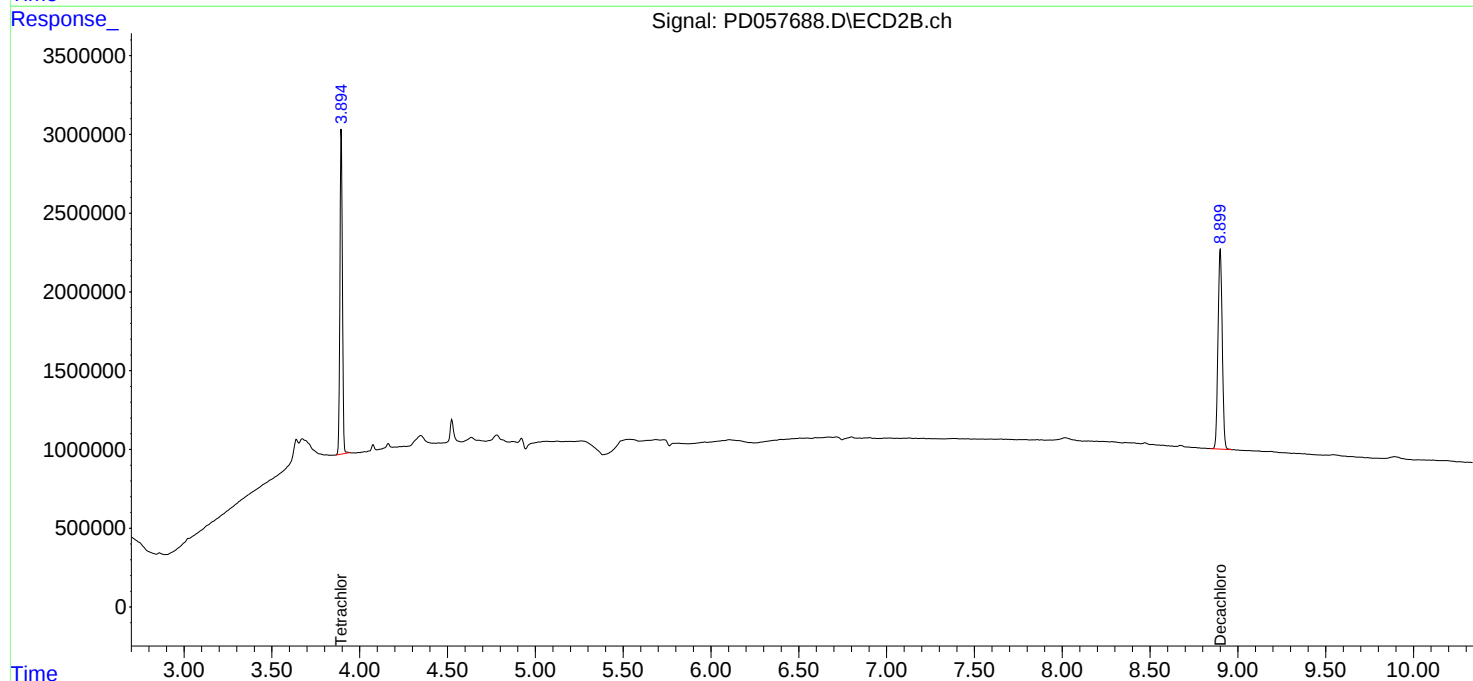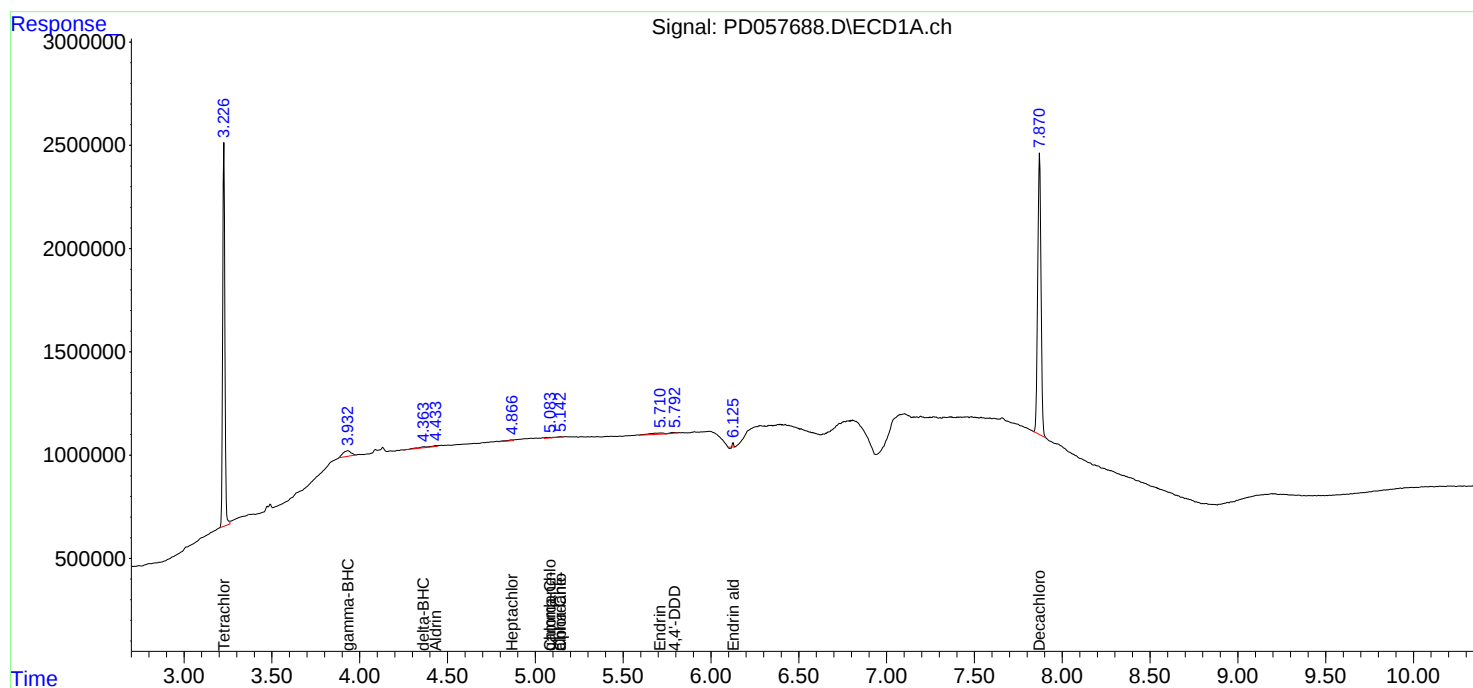


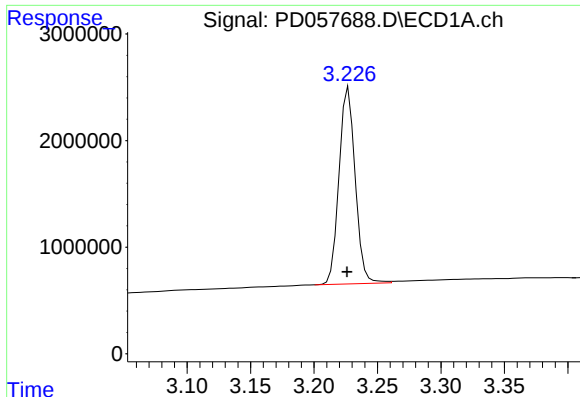

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 16361961
Conc: 22.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

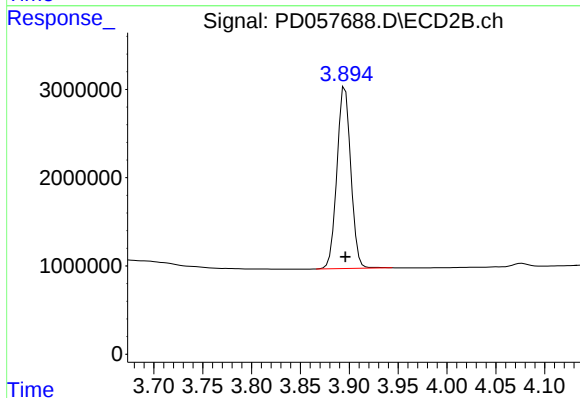


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 20370572
Conc: 25.96 ng/ml

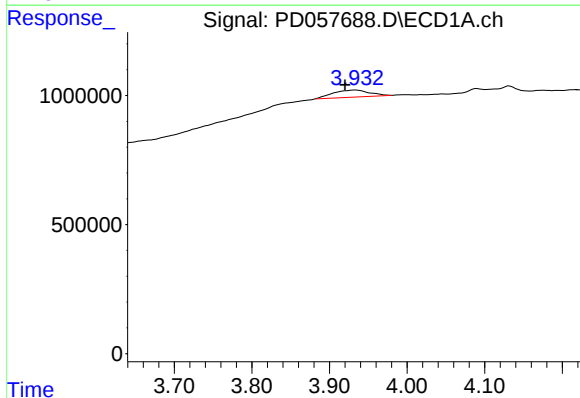


#3 gamma-BHC (Lindane)

R.T.: 3.933 min
Delta R.T.: 0.013 min
Response: 884874
Conc: 0.82 ng/ml

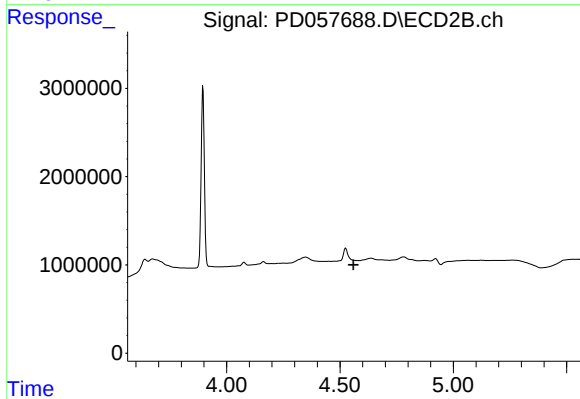

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

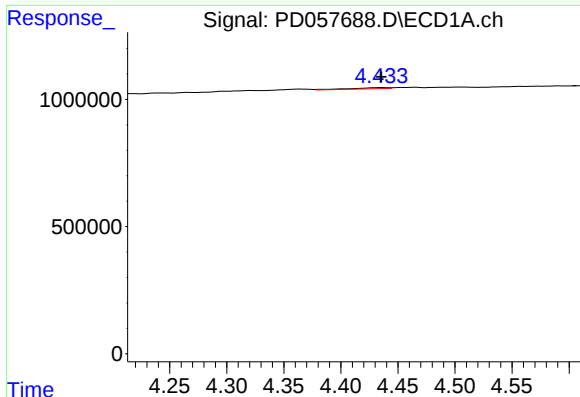

#5 Aldrin


R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 101721
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

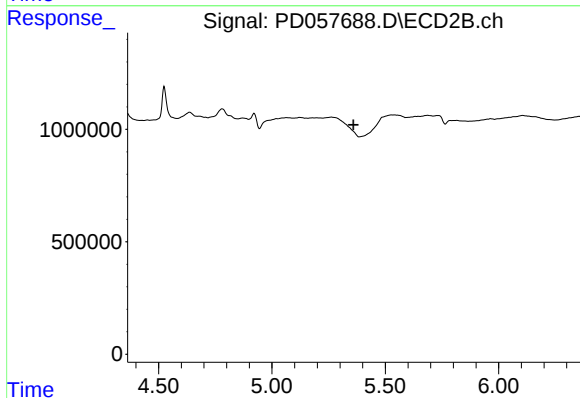


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.360 min
Response: 0
Conc: N.D.

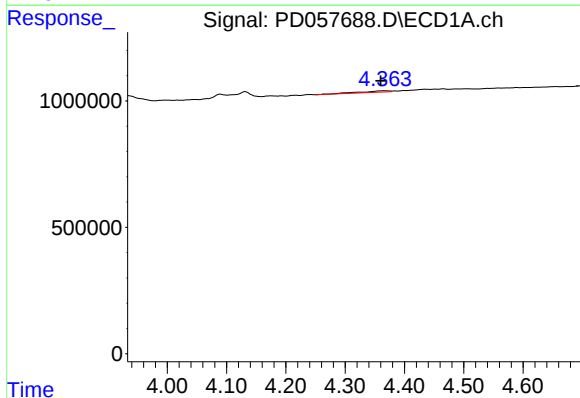


#7 delta-BHC

R.T.: 4.365 min
Delta R.T.: 0.005 min
Response: 170792
Conc: 0.17 ng/ml

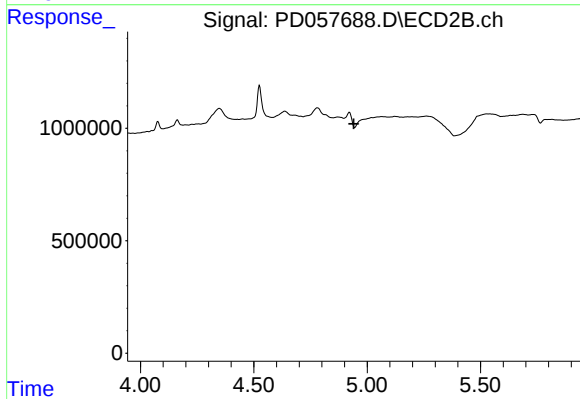

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

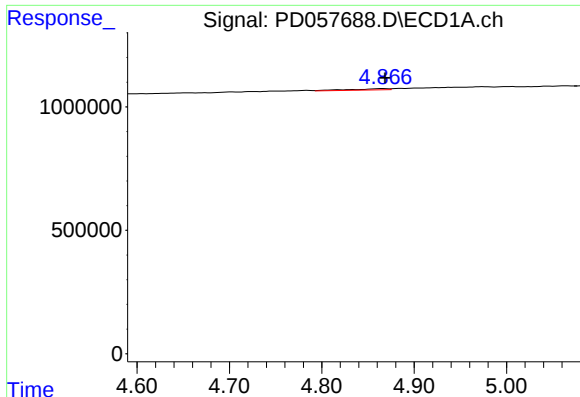

#8 Heptachlor epoxide


R.T.: 4.867 min
Delta R.T.: -0.001 min
Response: 148818
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

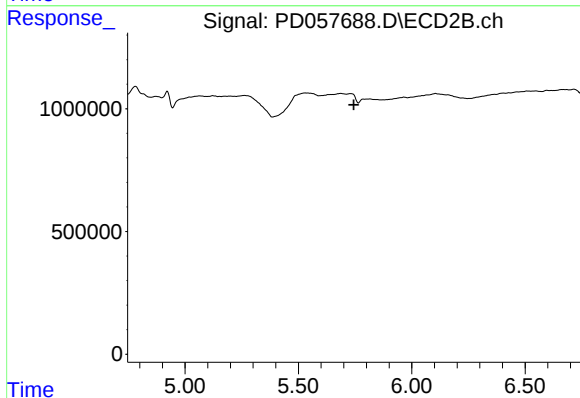


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

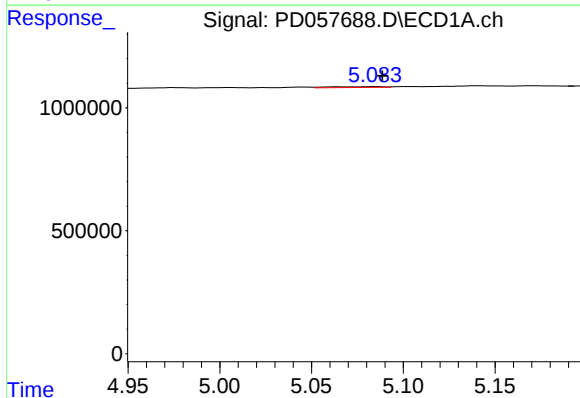


#10 gamma-Chlordane

R.T.: 5.085 min
Delta R.T.: -0.003 min
Response: 61511
Conc: 0.07 ng/ml

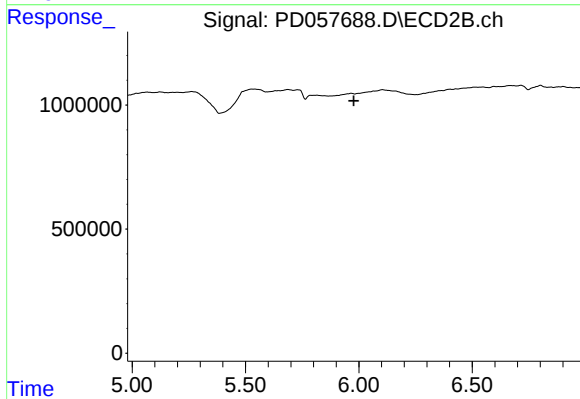

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

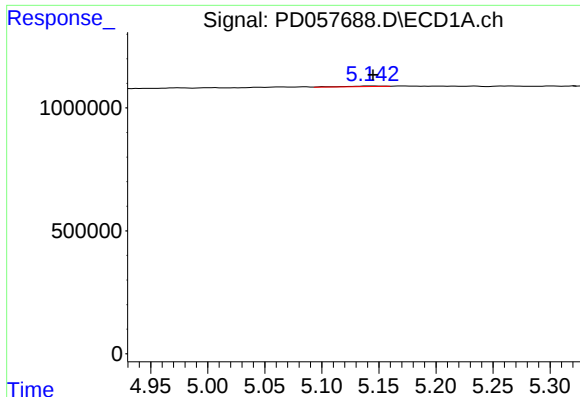

#11 alpha-Chlordane


R.T.: 5.143 min
Delta R.T.: -0.002 min
Response: 54522
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

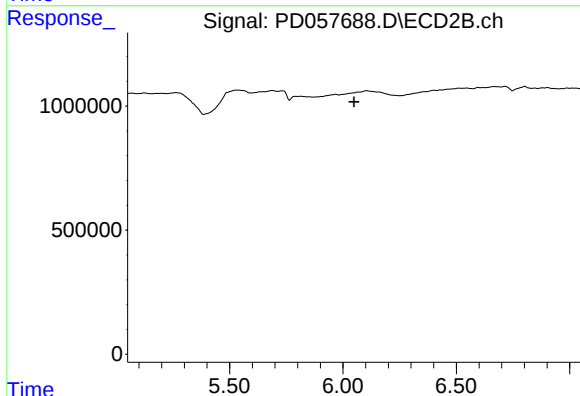


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

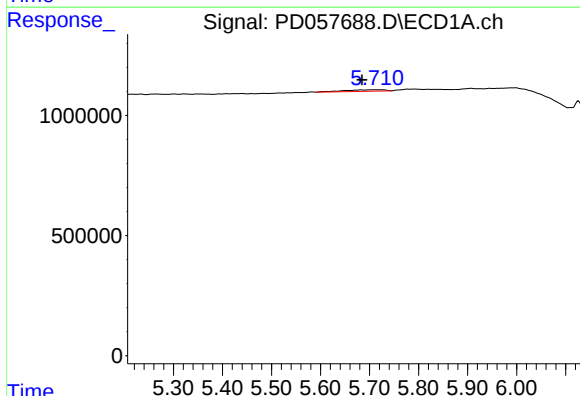


#14 Endrin

R.T.: 5.711 min
Delta R.T.: 0.026 min
Response: 378718
Conc: 0.52 ng/ml

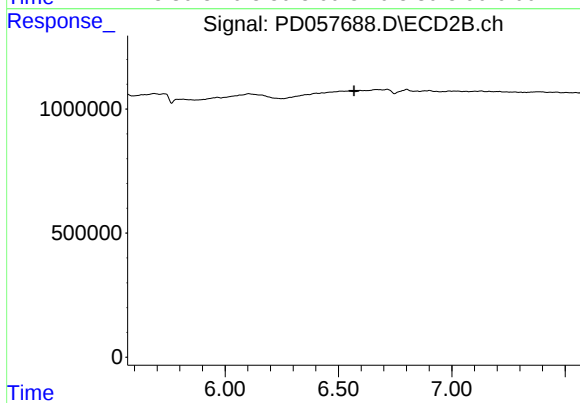

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

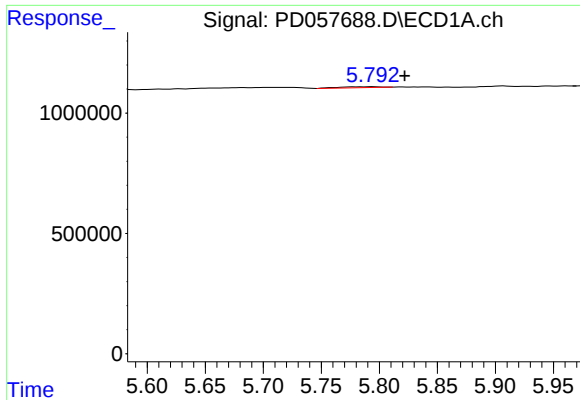

#16 4,4'-DDD


R.T.: 5.793 min
Delta R.T.: -0.028 min
Response: 96952
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

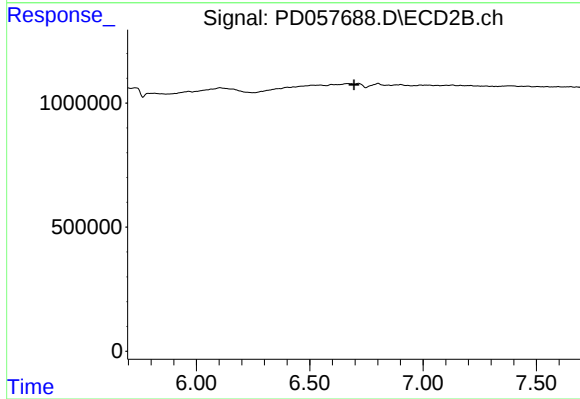


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

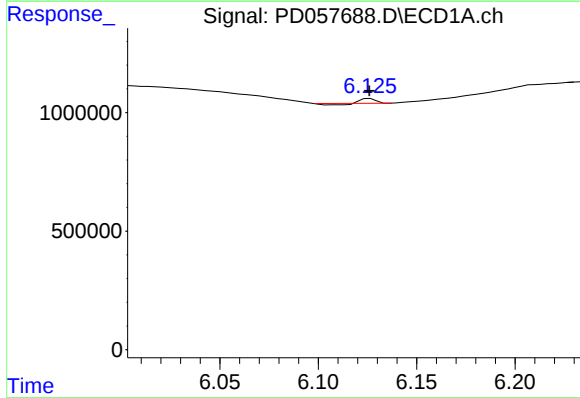


#18 Endrin aldehyde

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 77767
Conc: 0.13 ng/ml

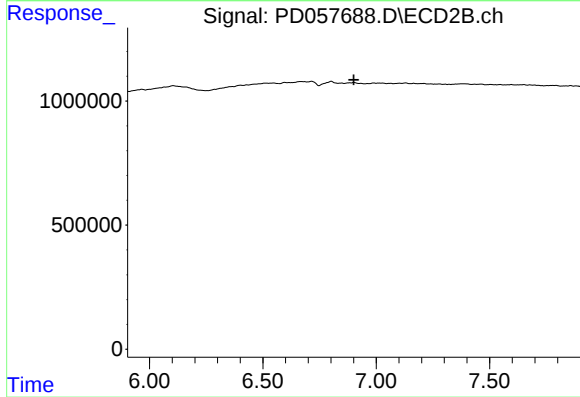

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

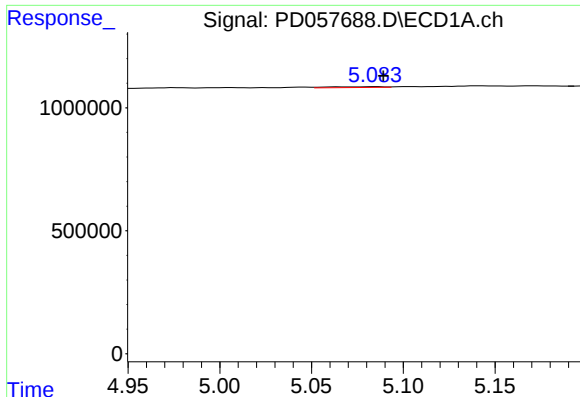

#25 Chlordane-3


R.T.: 5.085 min
Delta R.T.: -0.004 min
Response: 61511
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

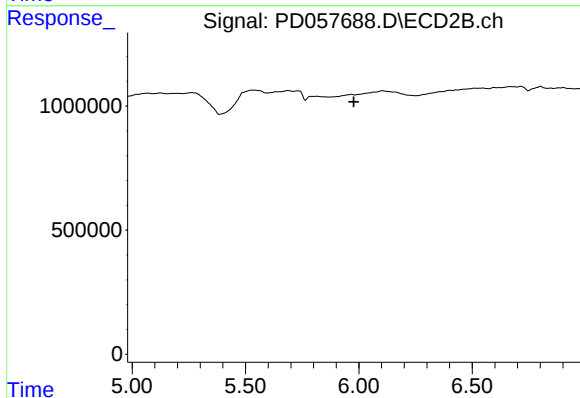


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

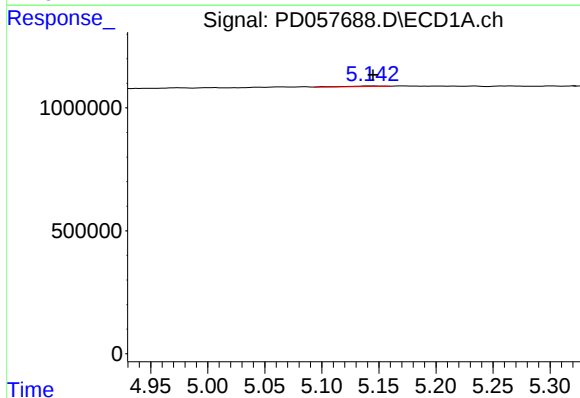


#26 Chlordane-4

R.T.: 5.143 min
Delta R.T.: -0.002 min
Response: 54522
Conc: 0.67 ng/ml

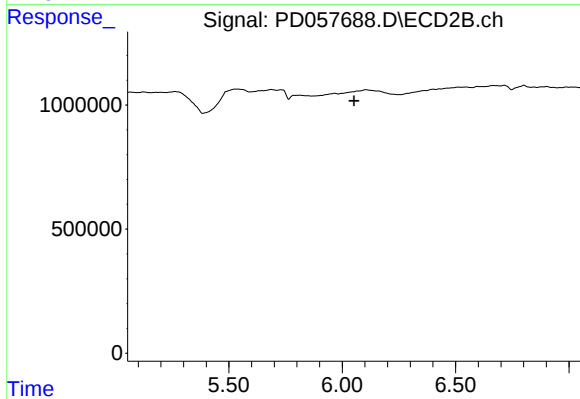

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

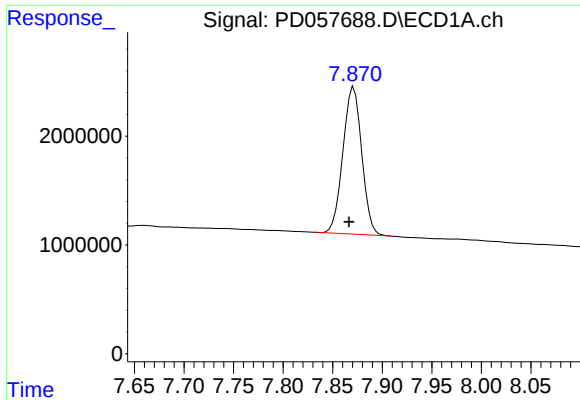

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.005 min
Response: 17853377
Conc: 23.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127963BL

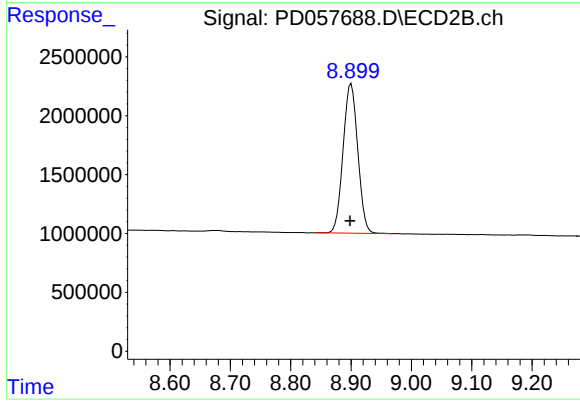

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.002 min
Response: 21482825
Conc: 24.43 ng/ml