

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 15:21
 Operator : AJ\MA
 Sample : L2096-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RO-1-2-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:52:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.232	3.896	17547512	21708577	24.577	27.670
28)	SA Decachlor...	7.877	8.904	16858677	20671017	22.142	23.502
Target Compounds							
5)	MB Aldrin	4.441	0.000	346189	0	0.353	N.D. #
8)	B Heptachlo...	4.878	0.000	183748	0	0.217	N.D. #
10)	B gamma-Chl...	5.098	0.000	801989	0	0.873	N.D. #
11)	B alpha-Chl...	5.154	0.000	821007	0	0.896	N.D. #
12)	B 4,4'-DDE	5.324	0.000	177082	0	0.202	N.D. #
13)	MA Dieldrin	5.444	0.000	585047	0	0.750	N.D. #
14)	MA Endrin	5.702f	0.000	1369202	0	1.884	N.D. #
24)	Chlordane-2	4.552	0.000	337253	0	11.764	N.D. #
25)	Chlordane-3	5.098	0.000	801989	0	9.136	N.D. #
26)	Chlordane-4	5.154	0.000	821007	0	10.152	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 15:21
Operator : AJ\MA
Sample : L2096-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:52:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

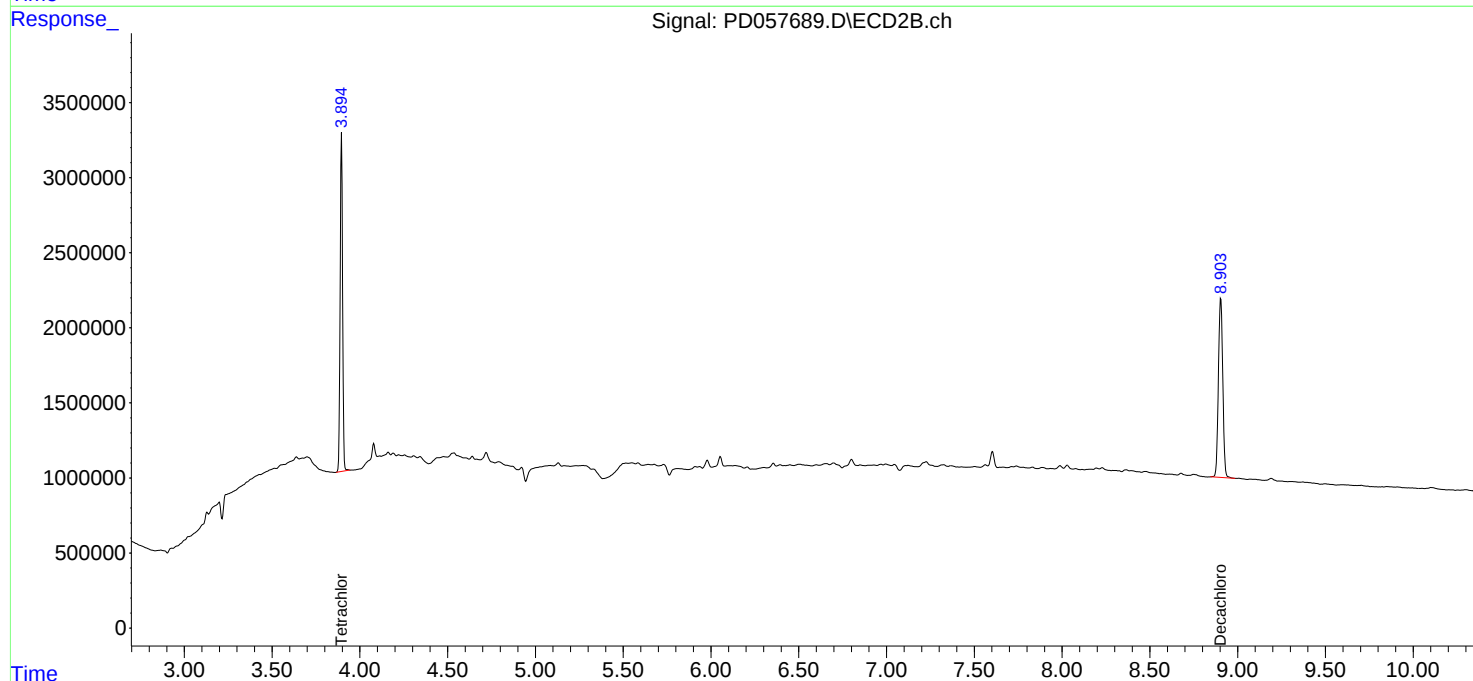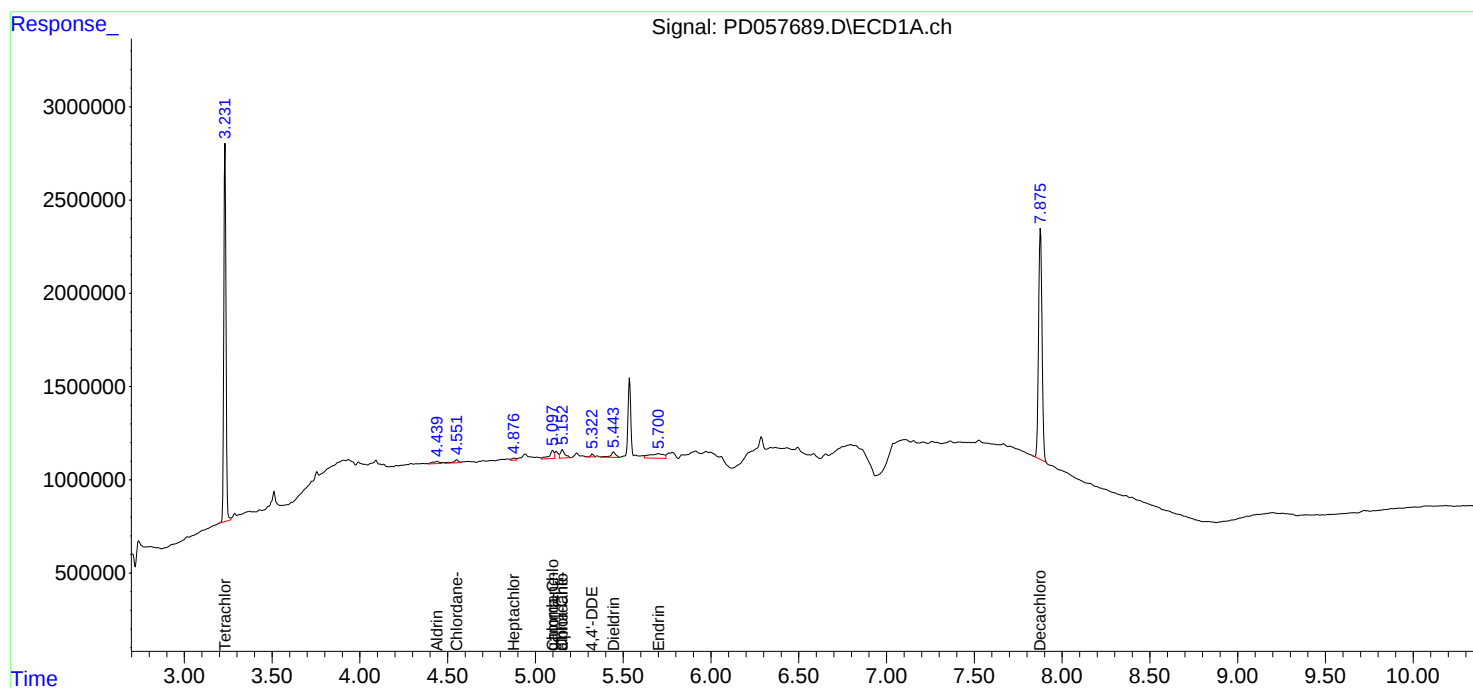


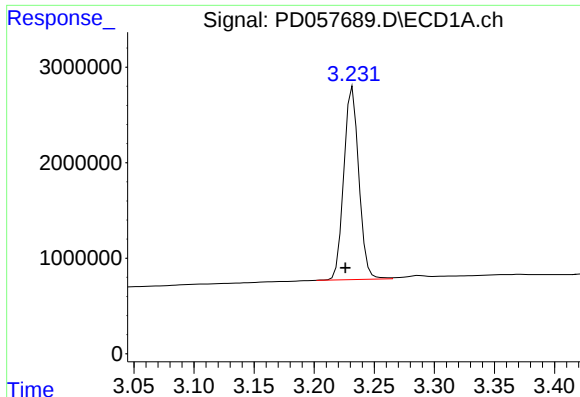

#1 Tetrachloro-m-xylene


R.T.: 3.232 min
Delta R.T.: 0.006 min
Response: 17547512
Conc: 24.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

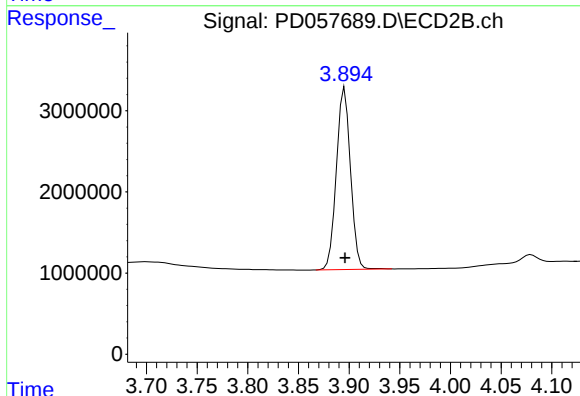


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 21708577
Conc: 27.67 ng/ml

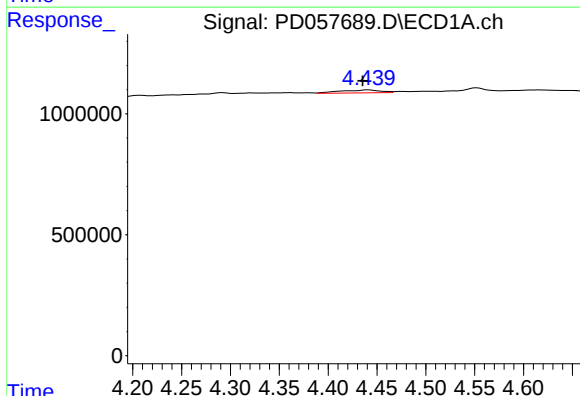


#5 Aldrin

R.T.: 4.441 min
Delta R.T.: 0.005 min
Response: 346189
Conc: 0.35 ng/ml

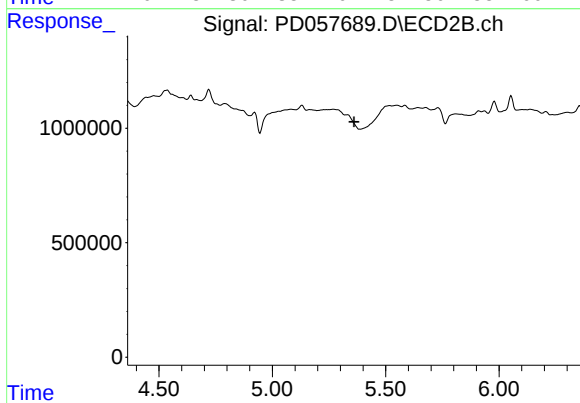

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.360 min
Response: 0
Conc: N.D.

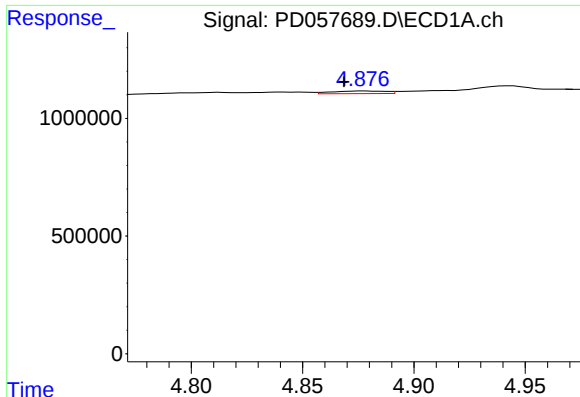

#8 Heptachlor epoxide


R.T.: 4.878 min
Delta R.T.: 0.009 min
Response: 183748
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

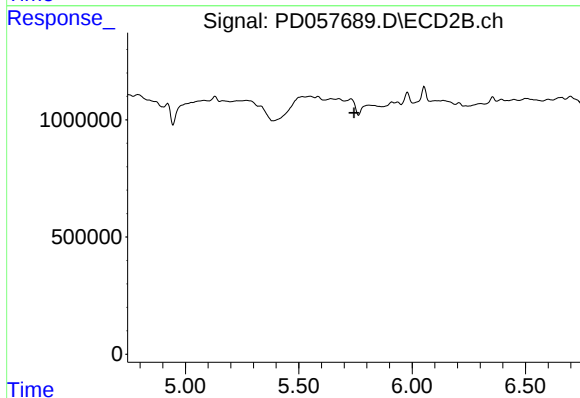


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

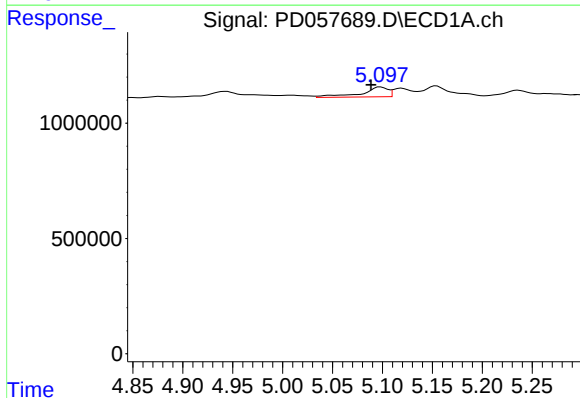


#10 gamma-Chlordane

R.T.: 5.098 min
Delta R.T.: 0.010 min
Response: 801989
Conc: 0.87 ng/ml

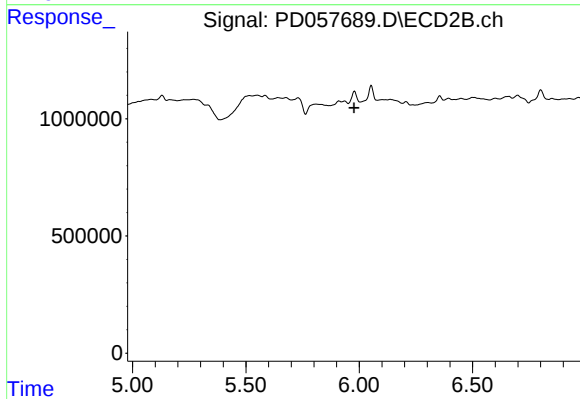

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

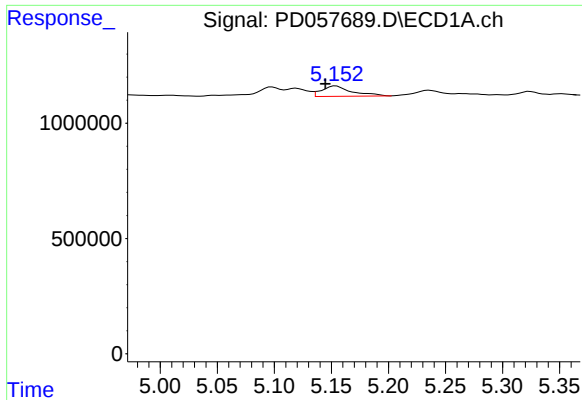

#11 alpha-Chlordane


R.T.: 5.154 min
Delta R.T.: 0.009 min
Response: 821007
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

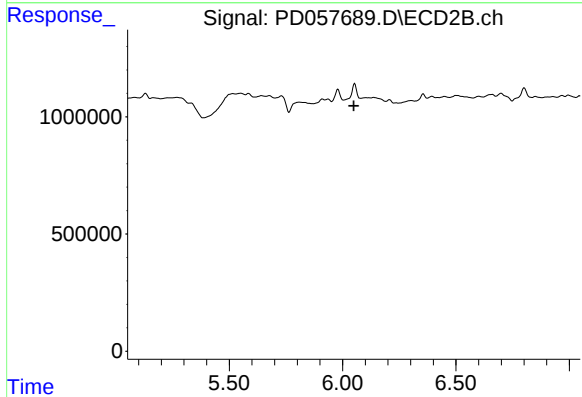


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

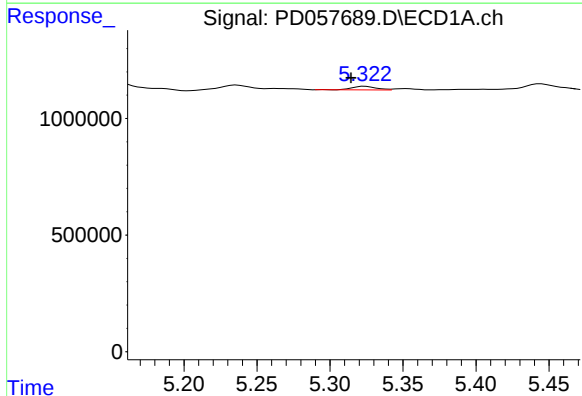


#12 4,4'-DDE

R.T.: 5.324 min
Delta R.T.: 0.009 min
Response: 177082
Conc: 0.20 ng/ml

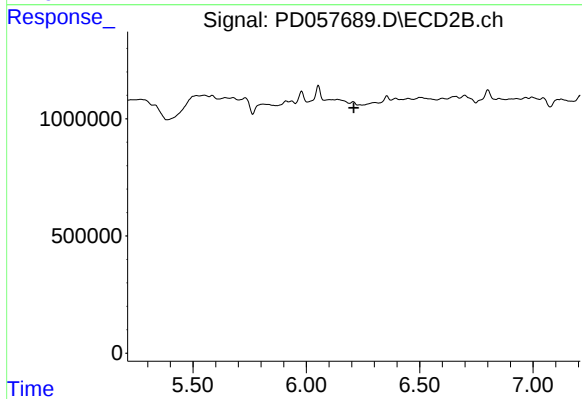

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

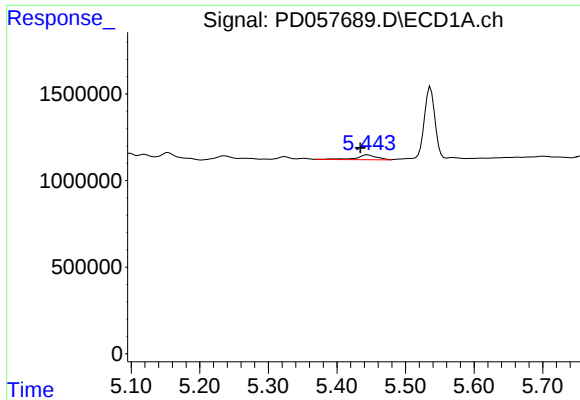

#13 Dieldrin


R.T.: 5.444 min
Delta R.T.: 0.011 min
Response: 585047
Conc: 0.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

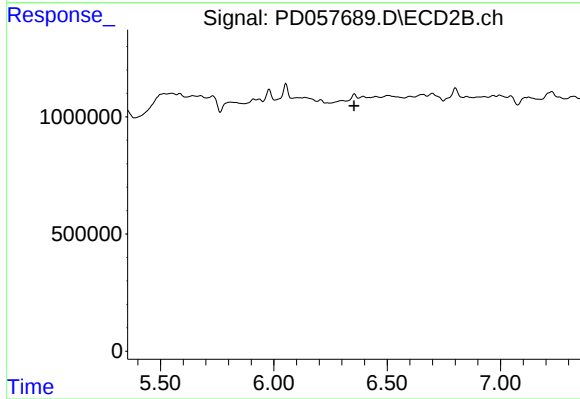


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

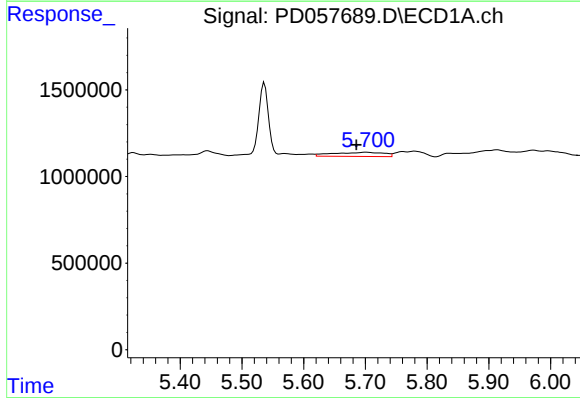


#14 Endrin

R.T.: 5.702 min
Delta R.T.: 0.017 min
Response: 1369202
Conc: 1.88 ng/ml

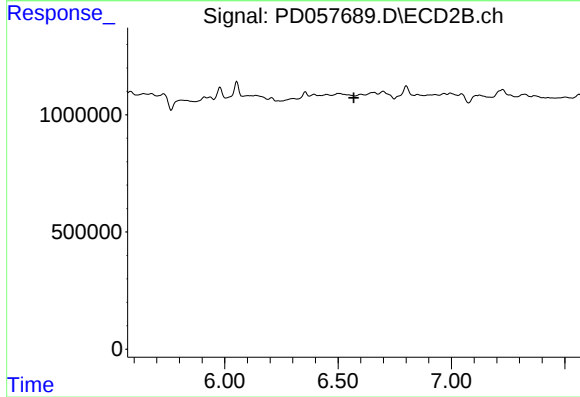

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

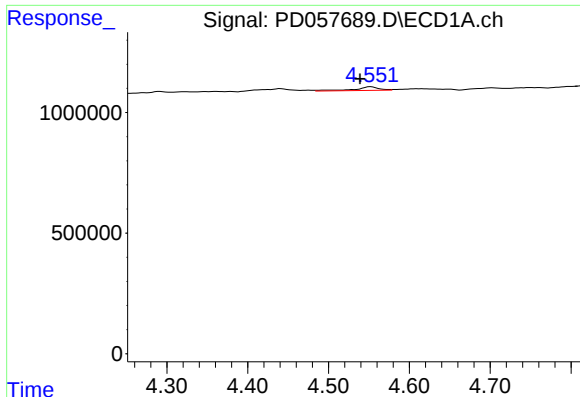

#24 Chlordane-2


R.T.: 4.552 min
Delta R.T.: 0.013 min
Response: 337253
Conc: 11.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

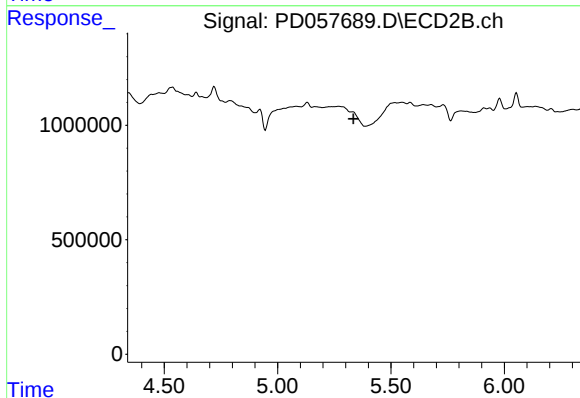


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

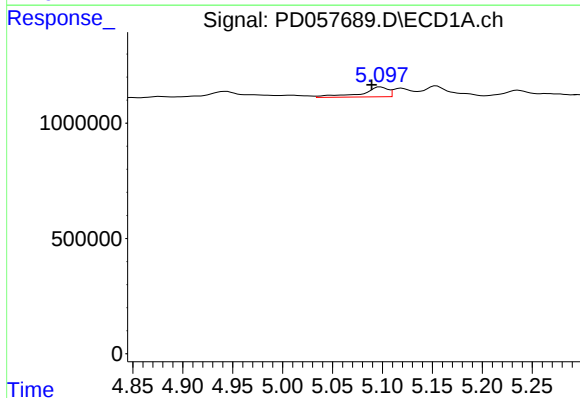


#25 Chlordane-3

R.T.: 5.098 min
Delta R.T.: 0.009 min
Response: 801989
Conc: 9.14 ng/ml

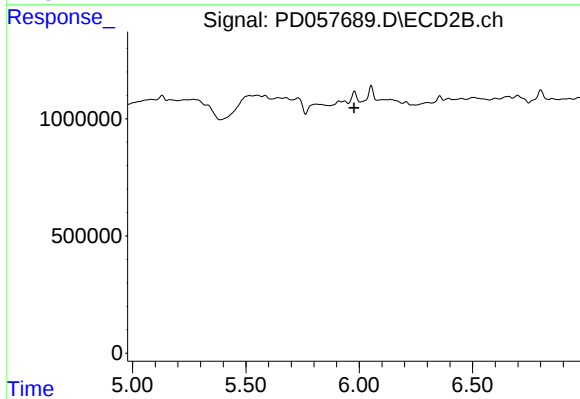

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

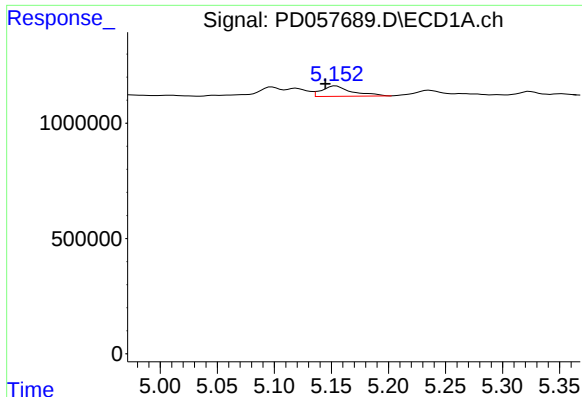

#26 Chlordane-4


R.T.: 5.154 min
Delta R.T.: 0.009 min
Response: 821007
Conc: 10.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
RO-1-2-TP

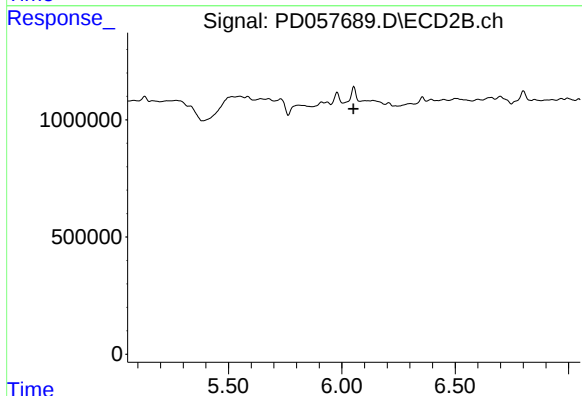


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

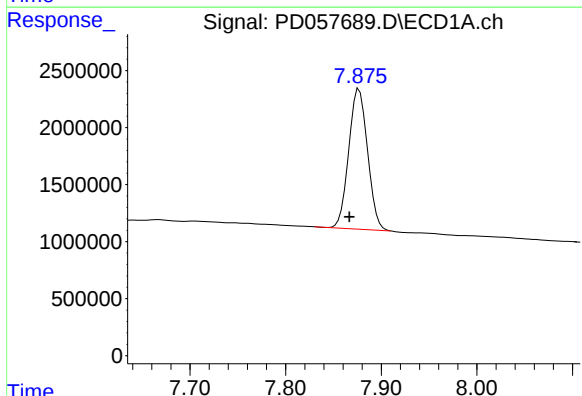

#28 Decachlorobiphenyl

R.T.: 7.877 min
Delta R.T.: 0.010 min
Response: 16858677
Conc: 22.14 ng/ml

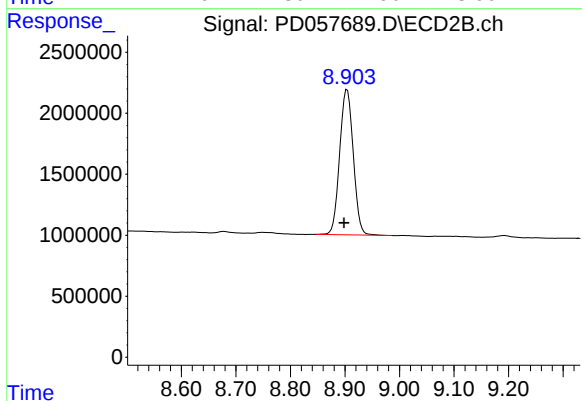

#28 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: 0.006 min
Response: 20671017
Conc: 23.50 ng/ml