

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 17:00
 Operator : AJ\MA
 Sample : L2125-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:54:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	10464226	13308738	14.656	16.964
28)	SA Decachlor...	7.868	8.901	13361826	17547874	17.549	19.951
Target Compounds							
3)	MA gamma-BHC...	3.934	0.000	2119654	0	1.969	N.D. #
5)	MB Aldrin	4.463f	0.000	374352	0	0.382	N.D. #
10)	B gamma-Chl...	5.111f	0.000	1552626	0	1.691	N.D. #
11)	B alpha-Chl...	5.146	6.053	865694	2102719	0.945	1.898 #
14)	MA Endrin	5.691	0.000	412515	0	0.568	N.D. #
15)	B Endosulfa...	5.963	0.000	172645	0	0.223	N.D. #
21)	B Endrin ke...	6.807	0.000	2639010	0	3.229	N.D. #
23)	Chlordane-1	4.057	0.000	217386	0	8.734	N.D. #
24)	Chlordane-2	4.542	0.000	446549	0	15.576	N.D. #
25)	Chlordane-3	5.111f	0.000	1552626	0	17.688	N.D. #
26)	Chlordane-4	5.146	6.053	865694	2102719	10.705	11.898
27)	Chlordane-5	5.963	0.000	172645	0	6.477	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 17:00
Operator : AJ\MA
Sample : L2125-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:54:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

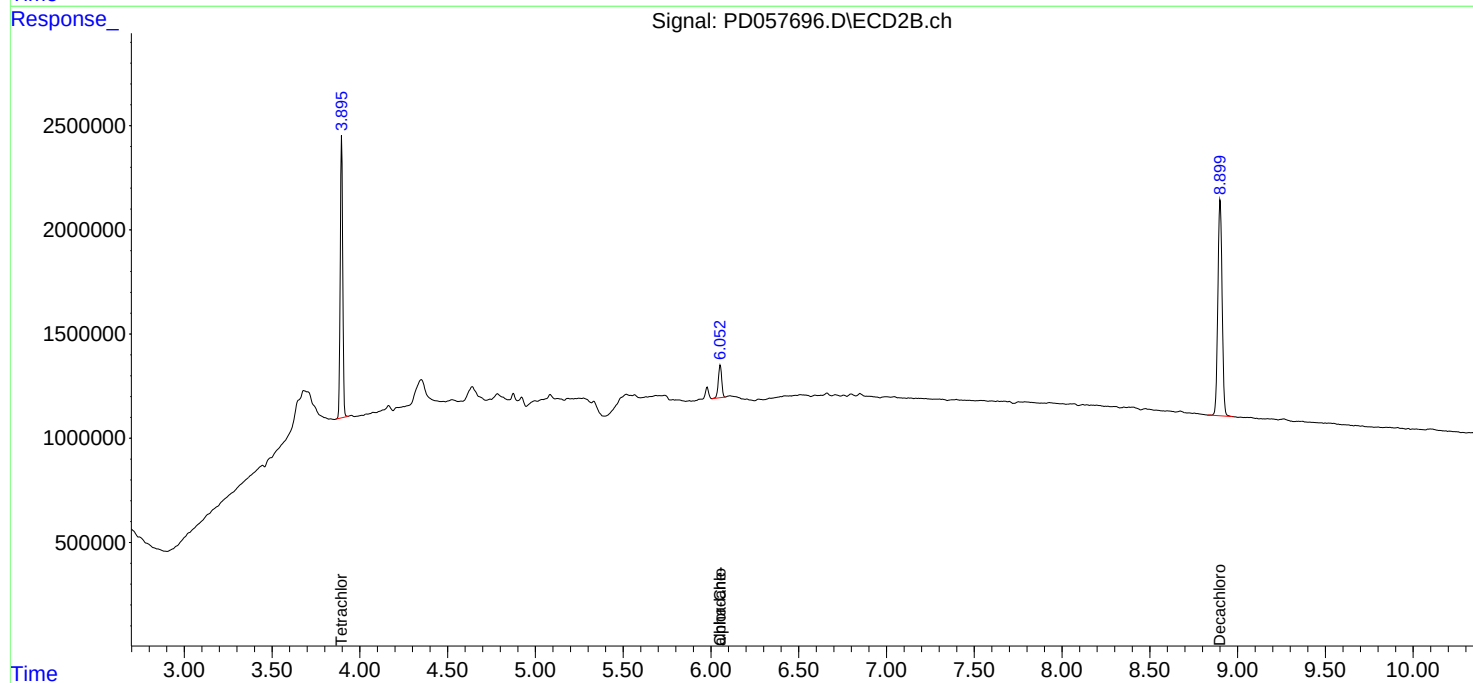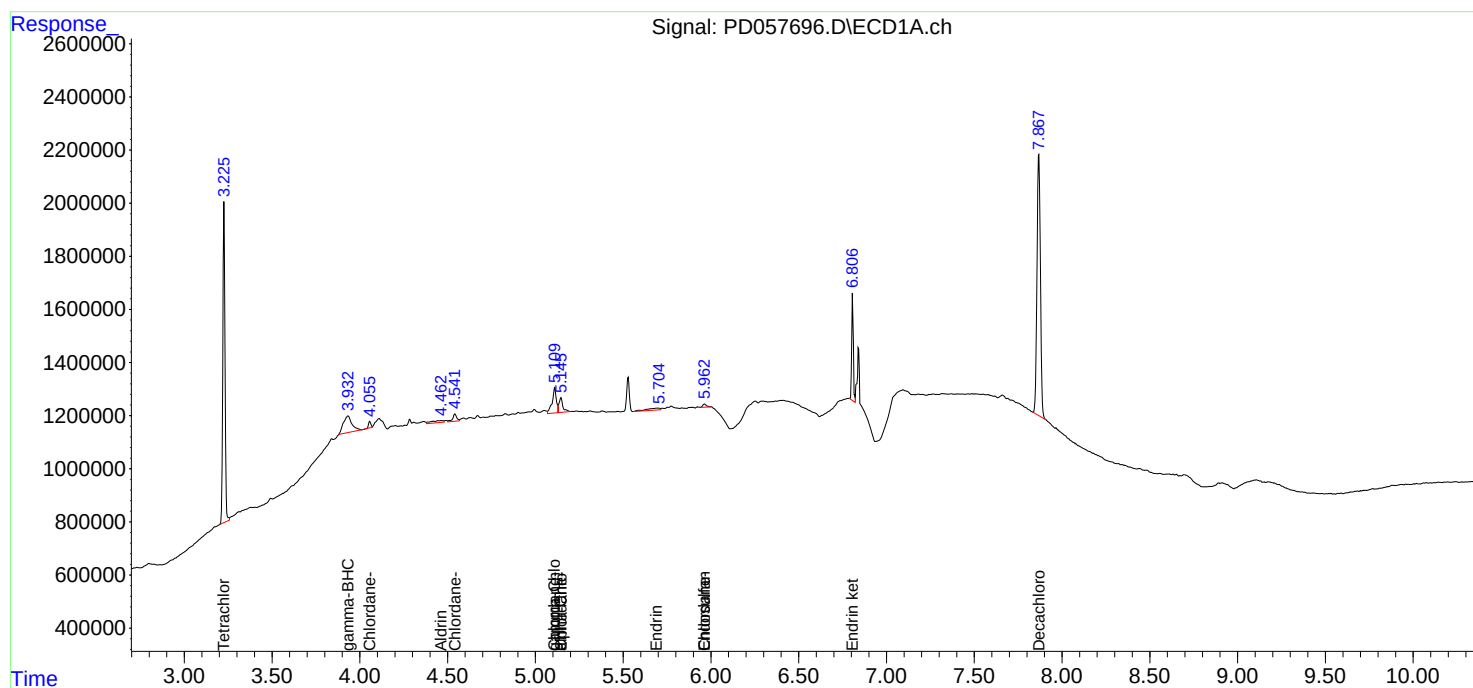


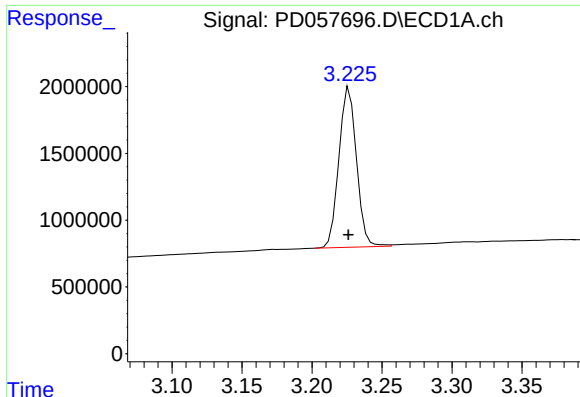

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 10464226
Conc: 14.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

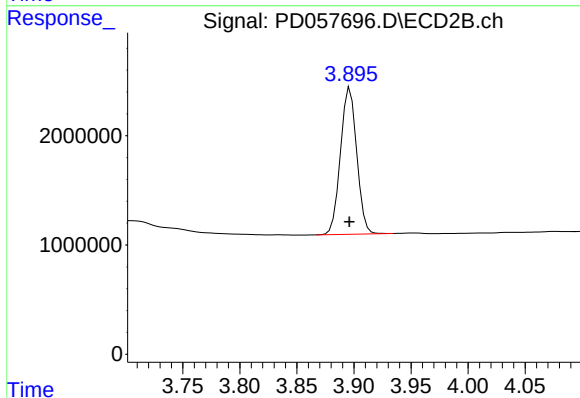


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 13308738
Conc: 16.96 ng/ml

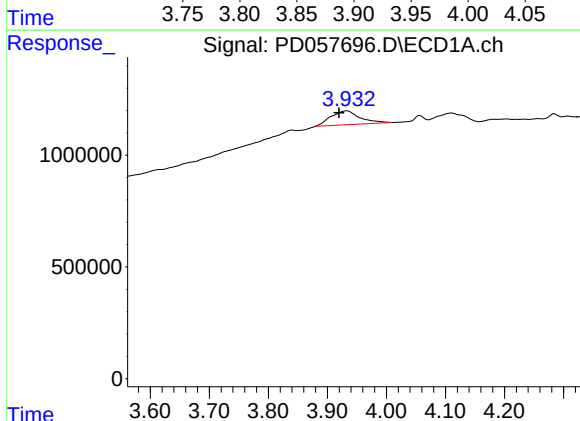


#3 gamma-BHC (Lindane)

R.T.: 3.934 min
Delta R.T.: 0.013 min
Response: 2119654
Conc: 1.97 ng/ml

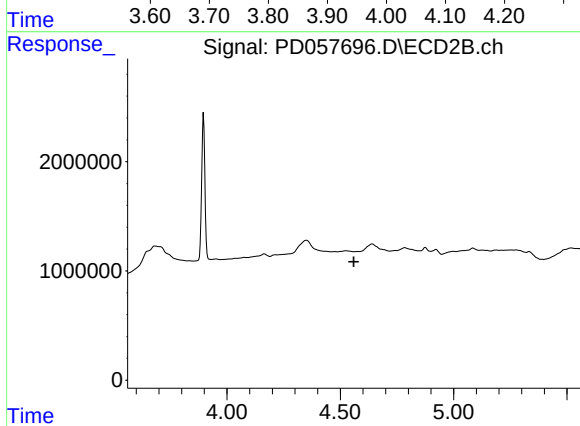

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

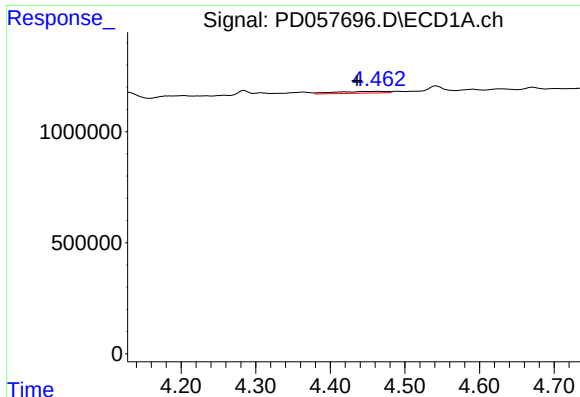

#5 Aldrin


R.T.: 4.463 min
Delta R.T.: 0.028 min
Response: 374352
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

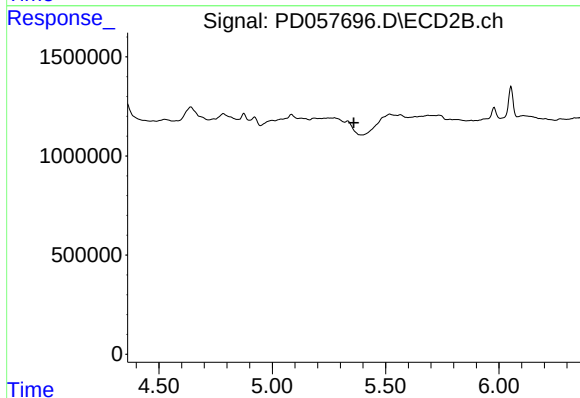


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.360 min
Response: 0
Conc: N.D.

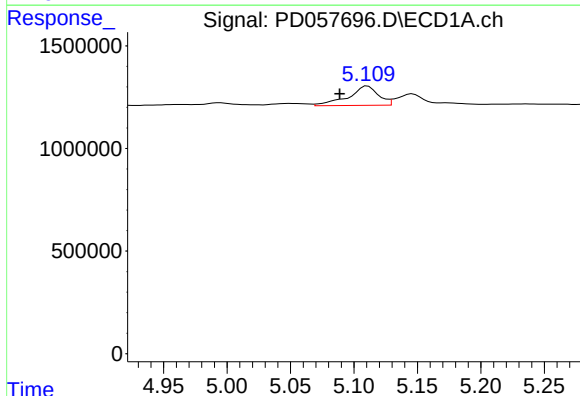


#10 gamma-Chlordane

R.T.: 5.111 min
Delta R.T.: 0.022 min
Response: 1552626
Conc: 1.69 ng/ml

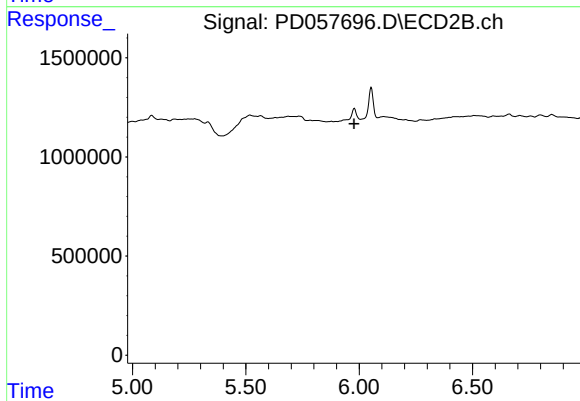

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

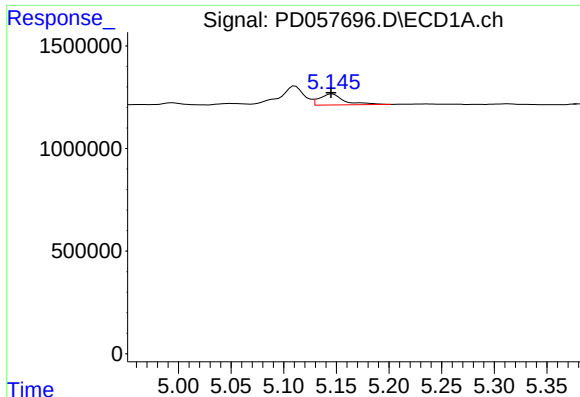

#11 alpha-Chlordane


R.T.: 5.146 min
Delta R.T.: 0.001 min
Response: 865694
Conc: 0.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

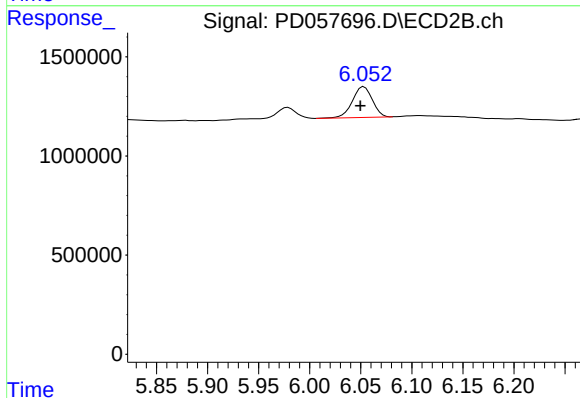


#11 alpha-Chlordane

R.T.: 6.053 min
Delta R.T.: 0.004 min
Response: 2102719
Conc: 1.90 ng/ml

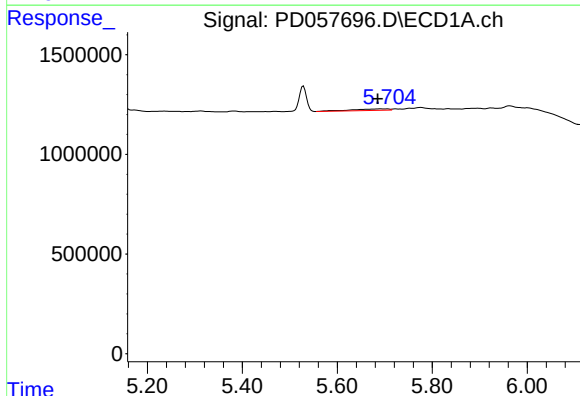


#14 Endrin

R.T.: 5.691 min
Delta R.T.: 0.006 min
Response: 412515
Conc: 0.57 ng/ml

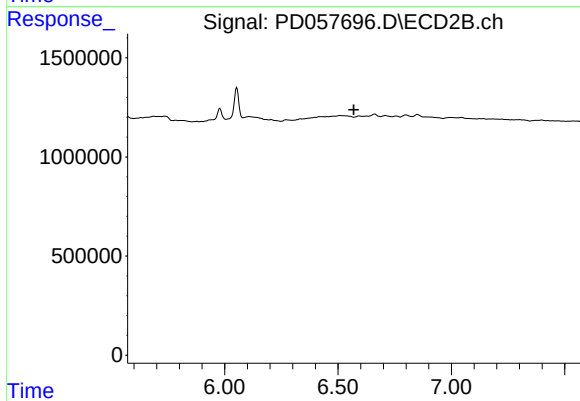

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

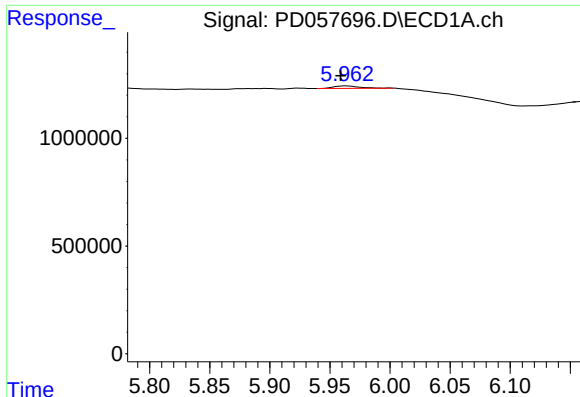

#15 Endosulfan II


R.T.: 5.963 min
Delta R.T.: 0.005 min
Response: 172645
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

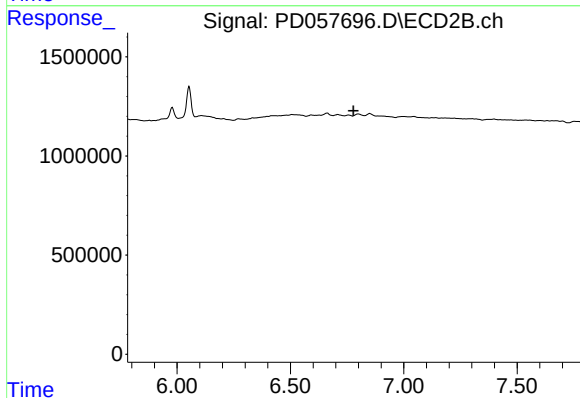


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.778 min
Response: 0
Conc: N.D.

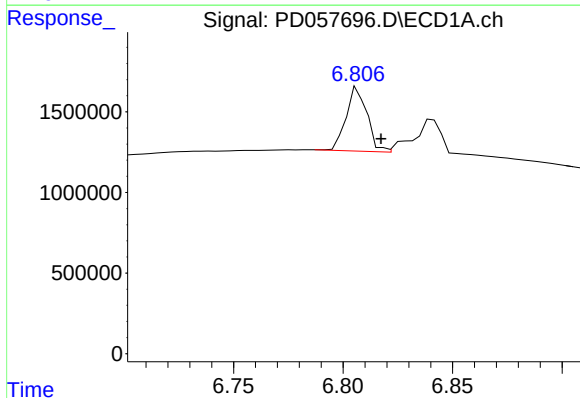


#21 Endrin ketone

R.T.: 6.807 min
Delta R.T.: -0.010 min
Response: 2639010
Conc: 3.23 ng/ml

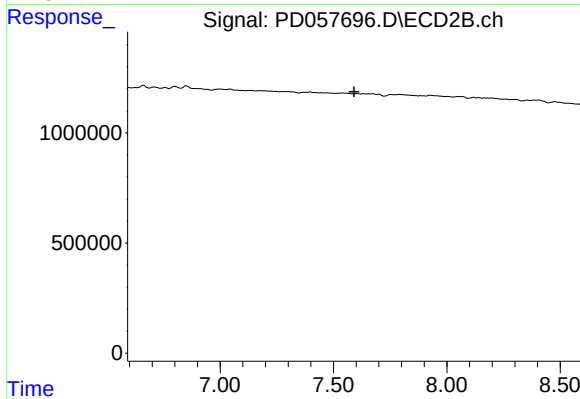

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.591 min
Response: 0
Conc: N.D.

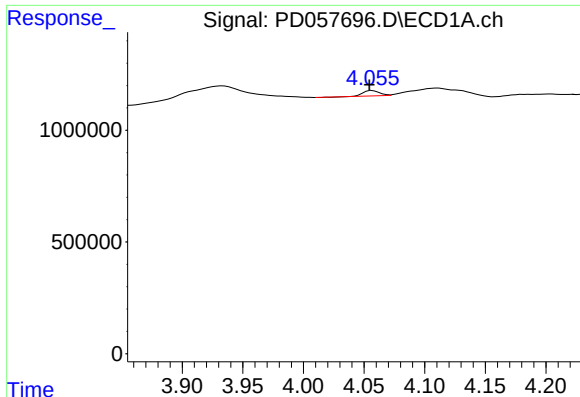

#23 Chlordane-1


R.T.: 4.057 min
Delta R.T.: 0.002 min
Response: 217386
Conc: 8.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

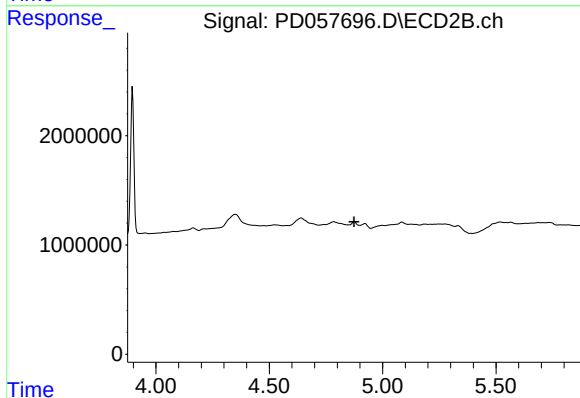


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

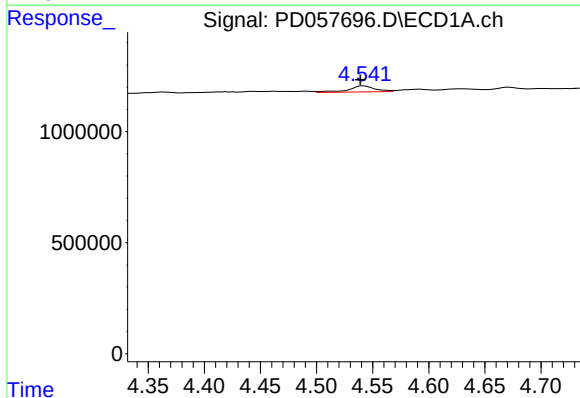


#24 Chlordane-2

R.T.: 4.542 min
Delta R.T.: 0.003 min
Response: 446549
Conc: 15.58 ng/ml

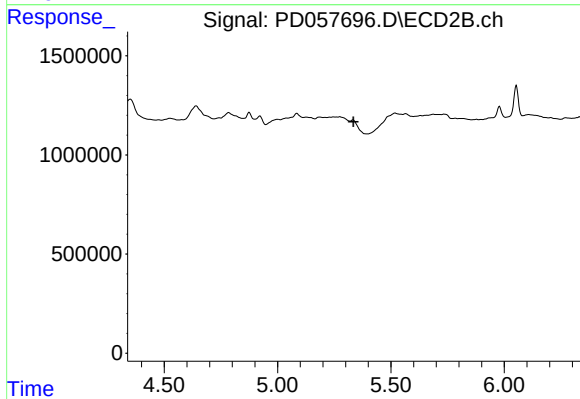

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

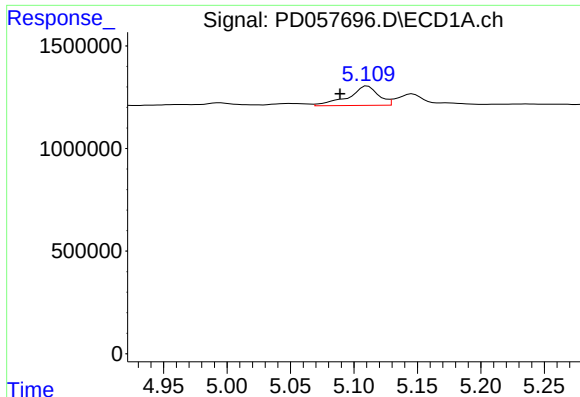

#25 Chlordane-3


R.T.: 5.111 min
Delta R.T.: 0.022 min
Response: 1552626
Conc: 17.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

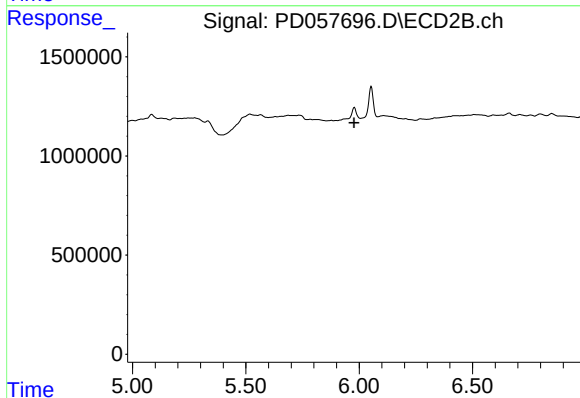


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

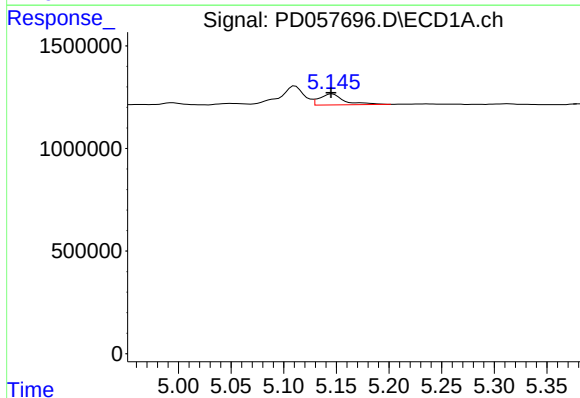


#26 Chlordane-4

R.T.: 5.146 min
Delta R.T.: 0.001 min
Response: 865694
Conc: 10.70 ng/ml

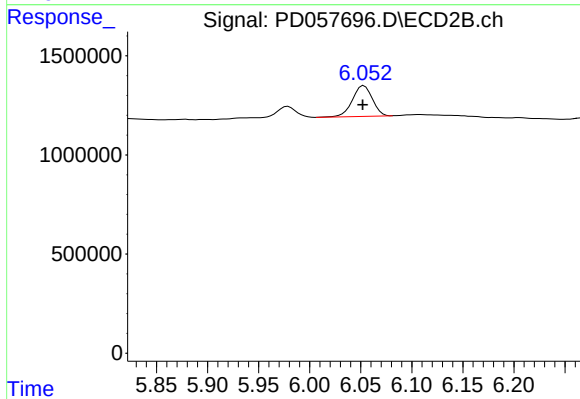

#26 Chlordane-4


R.T.: 6.053 min
Delta R.T.: 0.001 min
Response: 2102719
Conc: 11.90 ng/ml

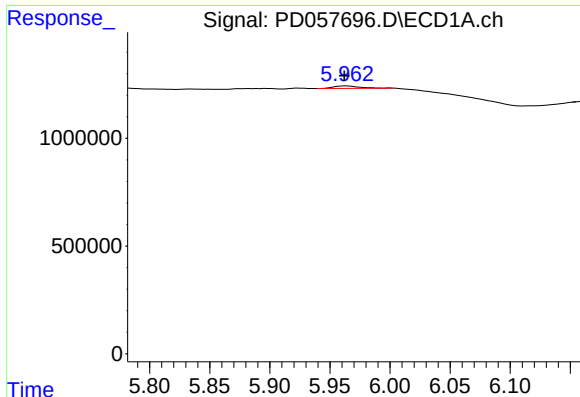

#27 Chlordane-5


R.T.: 5.963 min
Delta R.T.: 0.002 min
Response: 172645
Conc: 6.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-1

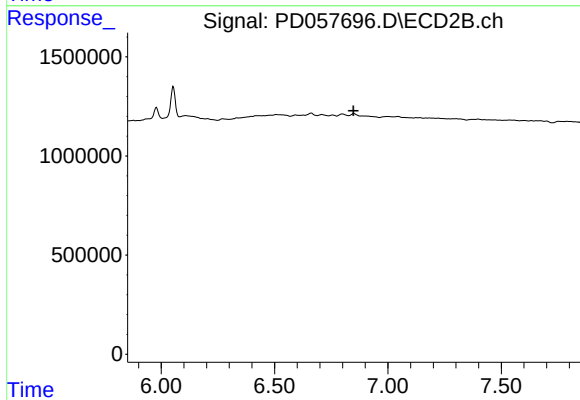


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.849 min
Response: 0
Conc: N.D.

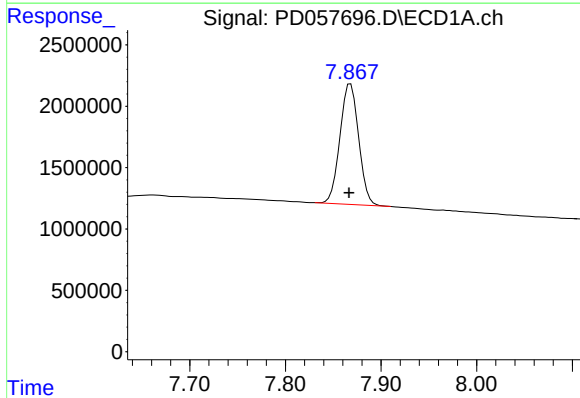

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.002 min
Response: 13361826
Conc: 17.55 ng/ml

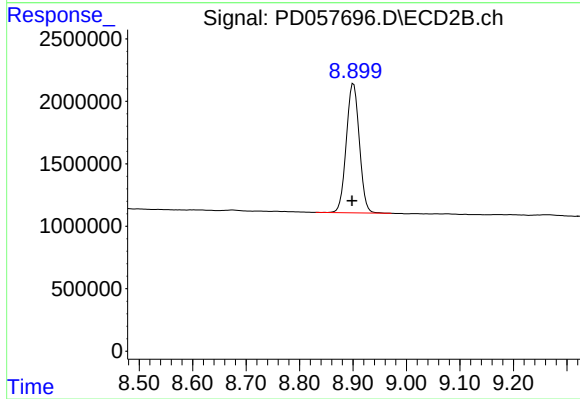

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.003 min
Response: 17547874
Conc: 19.95 ng/ml