

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 17:28
 Operator : AJ\MA
 Sample : L2104-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CHASSIE-WASH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:55:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	16558966	21198779	23.192	27.020
28)	SA Decachlor...	7.869	8.901	14428967	18808414	18.951	21.385
Target Compounds							
3)	MA gamma-BHC...	3.923	0.000	2312841	0	2.148	N.D. #
5)	MB Aldrin	4.456f	0.000	417000	0	0.425	N.D. #
11)	B alpha-Chl...	5.154	0.000	766777	0	0.837	N.D. #
13)	MA Dieldrin	5.406f	0.000	513613	0	0.658	N.D. #
14)	MA Endrin	5.713f	0.000	284120	0	0.391	N.D. #
23)	Chlordane-1	4.050	0.000	69516	0	2.793	N.D. #
25)	Chlordane-3	5.154f	0.000	766777	0	8.735	N.D. #
26)	Chlordane-4	5.154	0.000	766777	0	9.482	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 17:28
Operator : AJ\MA
Sample : L2104-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
CHASSIE-WASH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:55:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

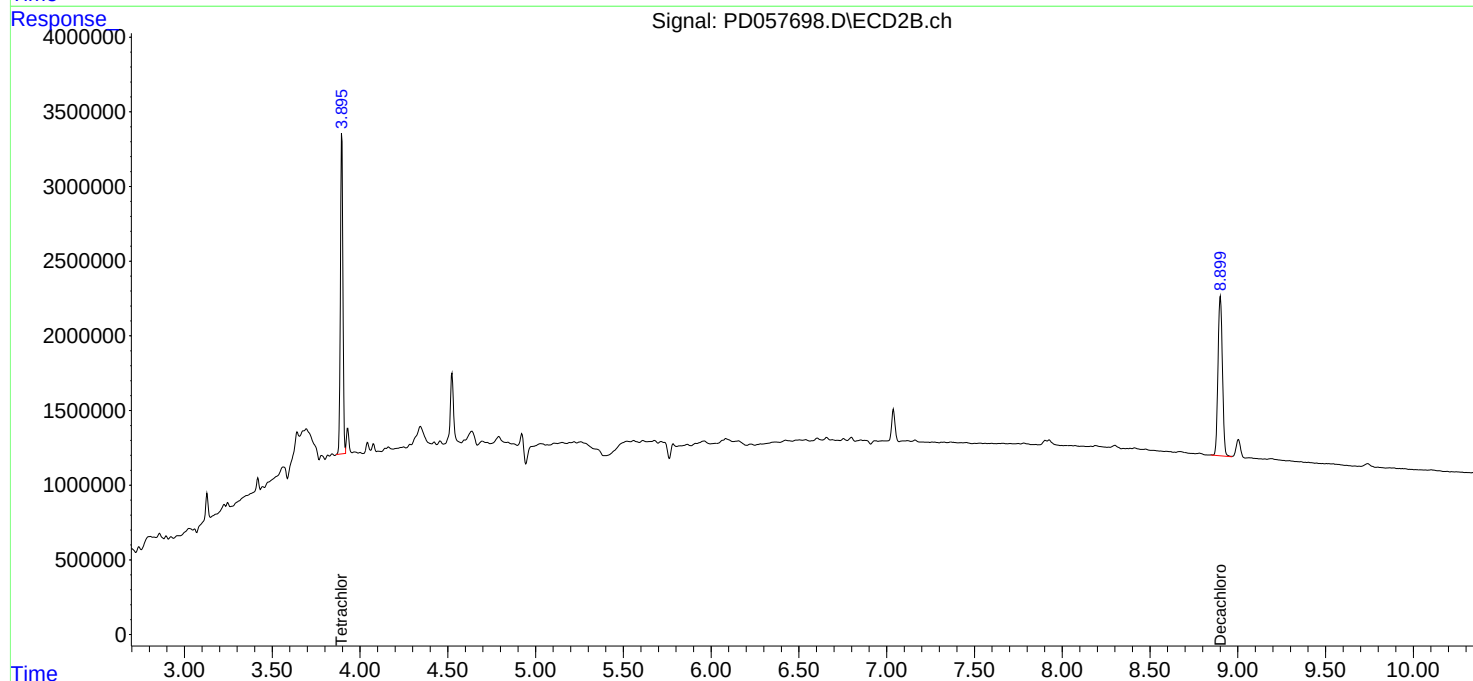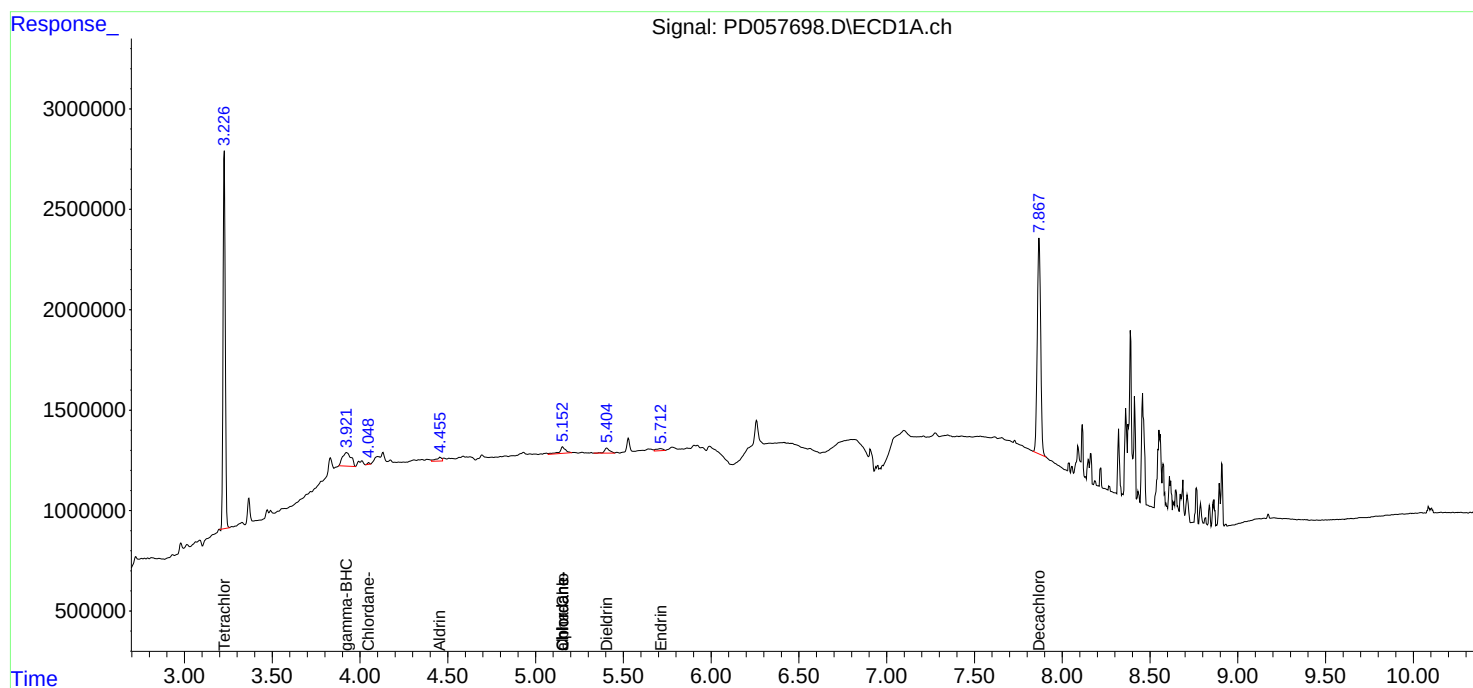


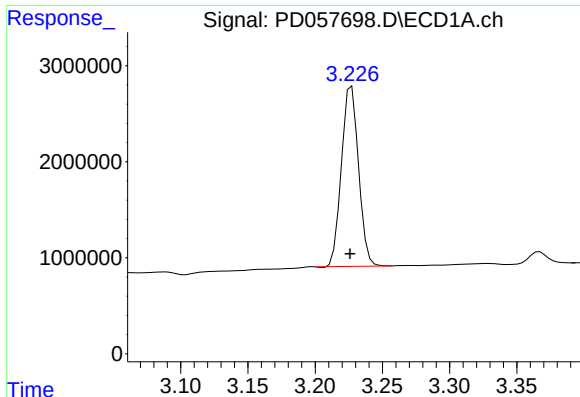

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 16558966
Conc: 23.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHASSIE-WASH

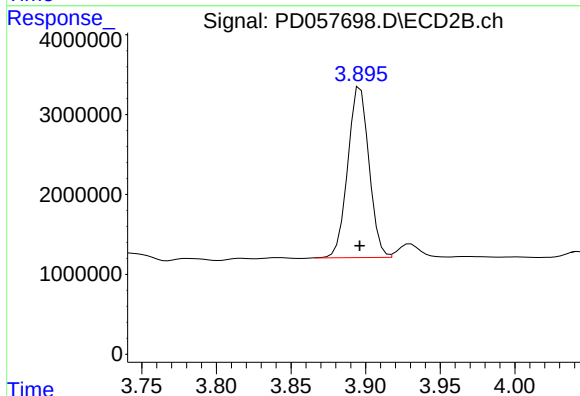


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 21198779
Conc: 27.02 ng/ml

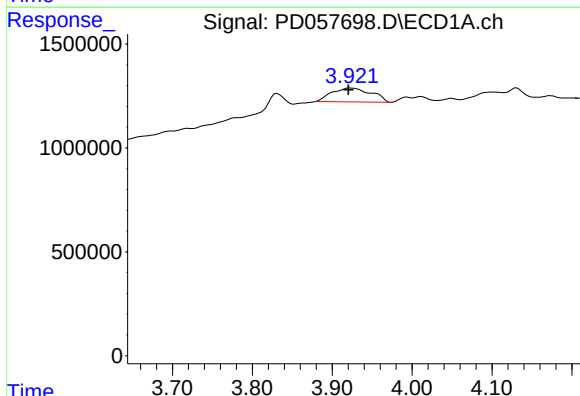


#3 gamma-BHC (Lindane)

R.T.: 3.923 min
Delta R.T.: 0.003 min
Response: 2312841
Conc: 2.15 ng/ml

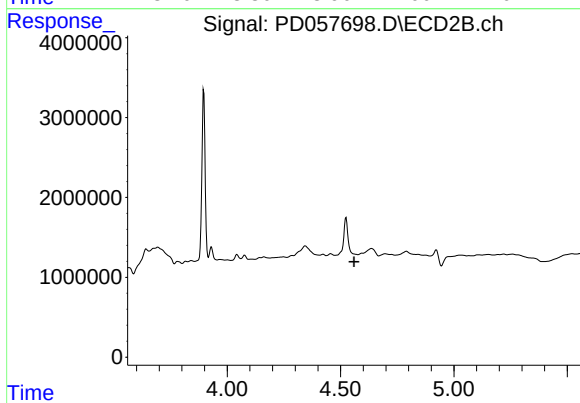

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

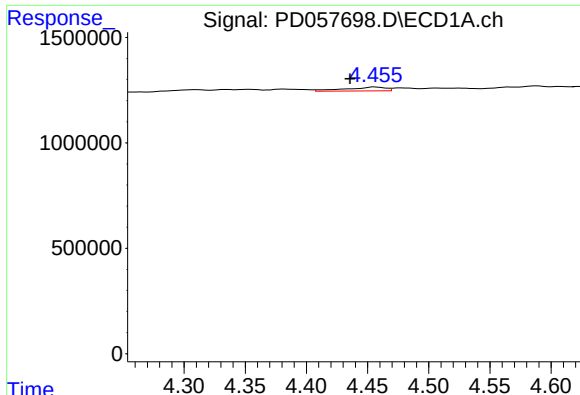

#5 Aldrin


R.T.: 4.456 min

Delta R.T.: 0.021 min

Response: 417000

Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHASSIE-WASH

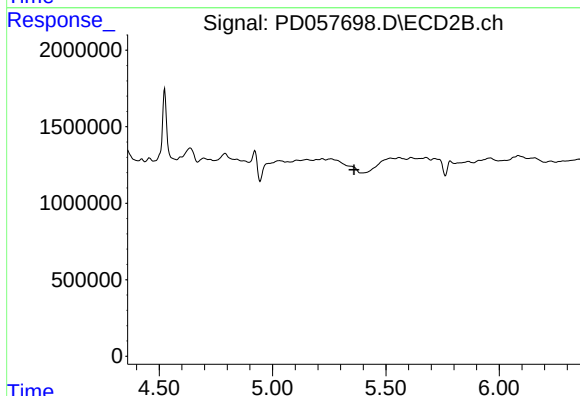


#5 Aldrin

R.T.: 0.000 min

Exp R.T. : 5.360 min

Response: 0

Conc: N.D.

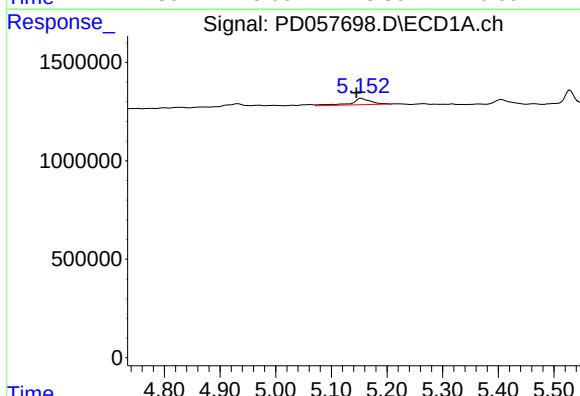


#11 alpha-Chlordane

R.T.: 5.154 min

Delta R.T.: 0.009 min

Response: 766777

Conc: 0.84 ng/ml

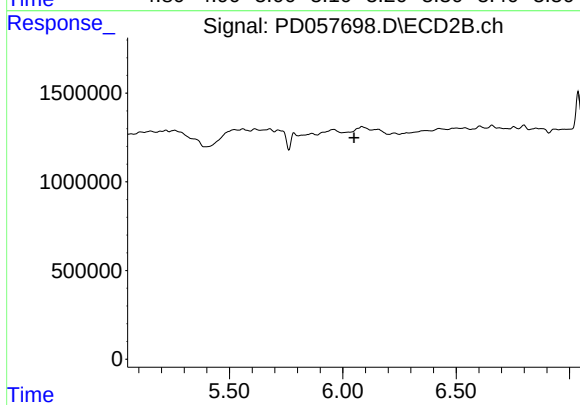


#11 alpha-Chlordane

R.T.: 0.000 min

Exp R.T. : 6.050 min

Response: 0


Conc: N.D.

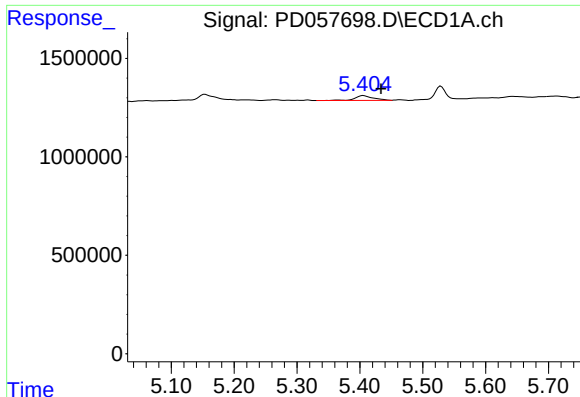

#13 Dieldrin


R.T.: 5.406 min
Delta R.T.: -0.028 min
Response: 513613
Conc: 0.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHASSIE-WASH

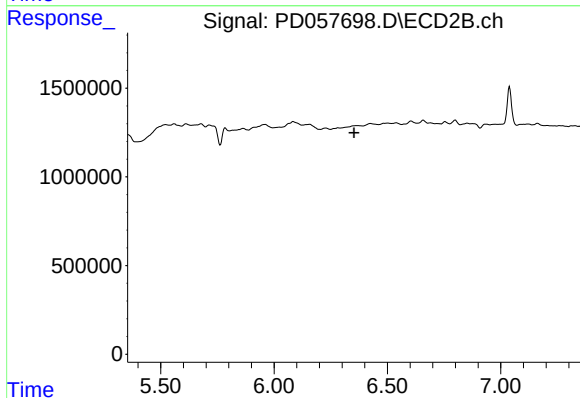


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

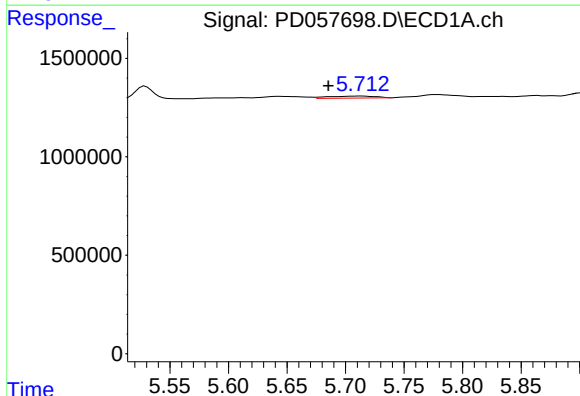


#14 Endrin

R.T.: 5.713 min
Delta R.T.: 0.028 min
Response: 284120
Conc: 0.39 ng/ml

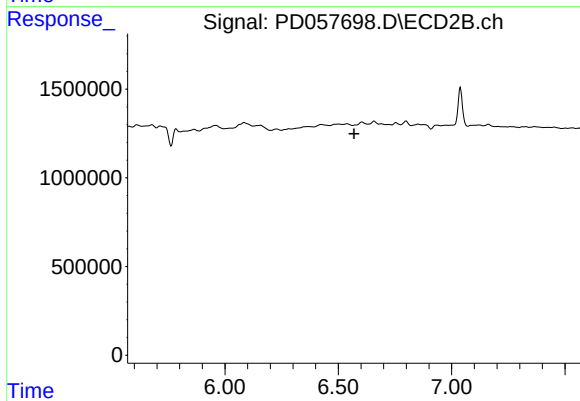

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

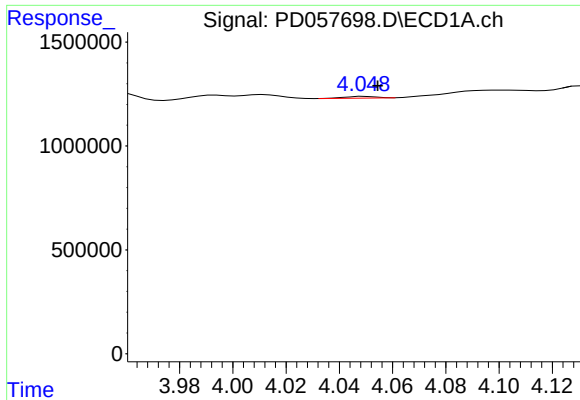

#23 Chlordane-1


R.T.: 4.050 min
Delta R.T.: -0.005 min
Response: 69516
Conc: 2.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHASSIE-WASH

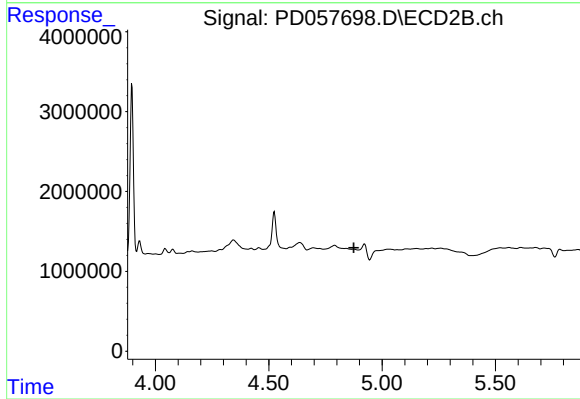


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

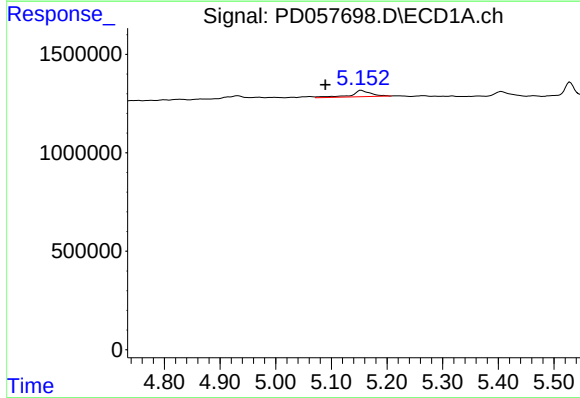


#25 Chlordane-3

R.T.: 5.154 min
Delta R.T.: 0.065 min
Response: 766777
Conc: 8.74 ng/ml

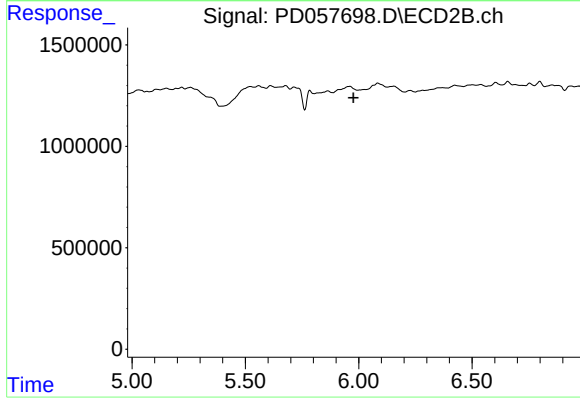

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

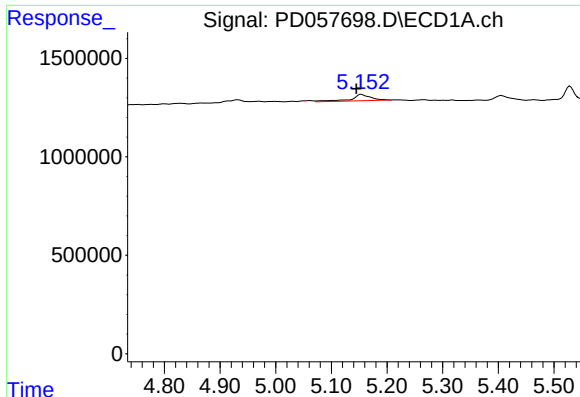

#26 Chlordane-4


R.T.: 5.154 min
Delta R.T.: 0.009 min
Response: 766777
Conc: 9.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHASSIE-WASH

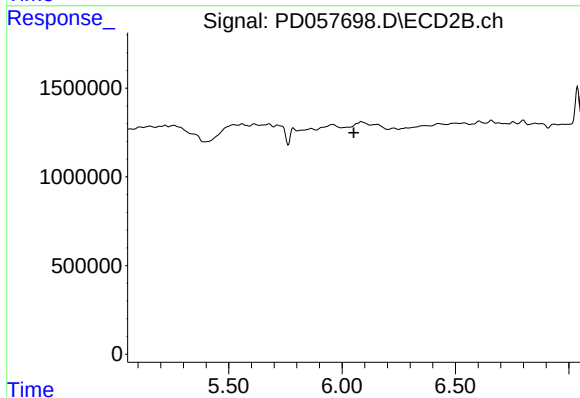


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

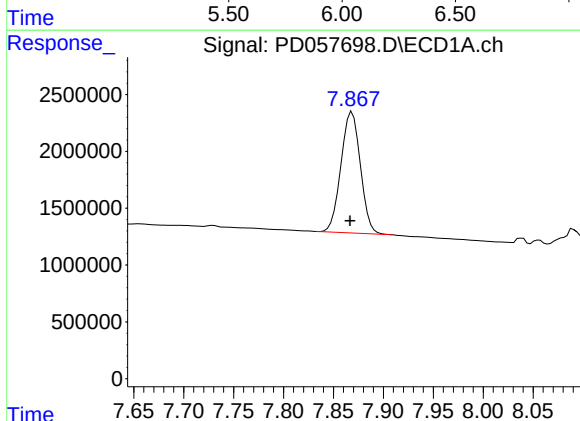

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.002 min
Response: 14428967
Conc: 18.95 ng/ml

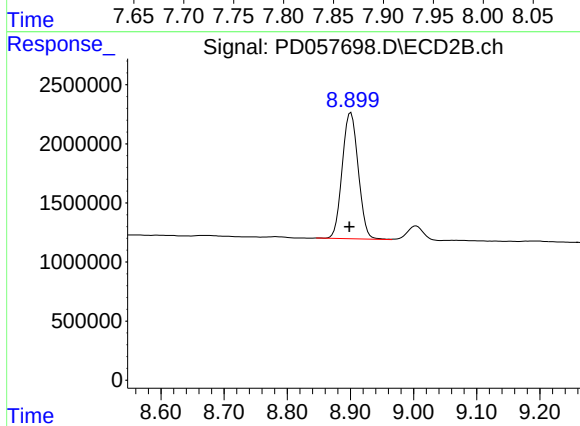

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.002 min
Response: 18808414
Conc: 21.38 ng/ml