

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 19:21
 Operator : AJ\MA
 Sample : L2122-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-01-040120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:57:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	16596640	21465162	23.245	27.360
28)	SA Decachlor...	7.868	8.902	11302428	13528724	14.845	15.382
Target Compounds							
3)	MA gamma-BHC...	3.927	0.000	1644893	0	1.528	N.D. #
5)	MB Aldrin	4.456f	0.000	106123	0	0.108	N.D. #
8)	B Heptachlo...	4.870	0.000	208990	0	0.247	N.D. #
11)	B alpha-Chl...	5.155	0.000	306675	0	0.335	N.D. #
13)	MA Dieldrin	5.420	0.000	308725	0	0.396	N.D. #
14)	MA Endrin	5.695	0.000	41559	0	0.057	N.D. #
24)	Chlordane-2	4.564f	0.000	36622	0	1.277	N.D. #
25)	Chlordane-3	5.155f	0.000	306675	0	3.494	N.D. #
26)	Chlordane-4	5.155	0.000	306675	0	3.792	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 19:21
Operator : AJ\MA
Sample : L2122-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:57:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

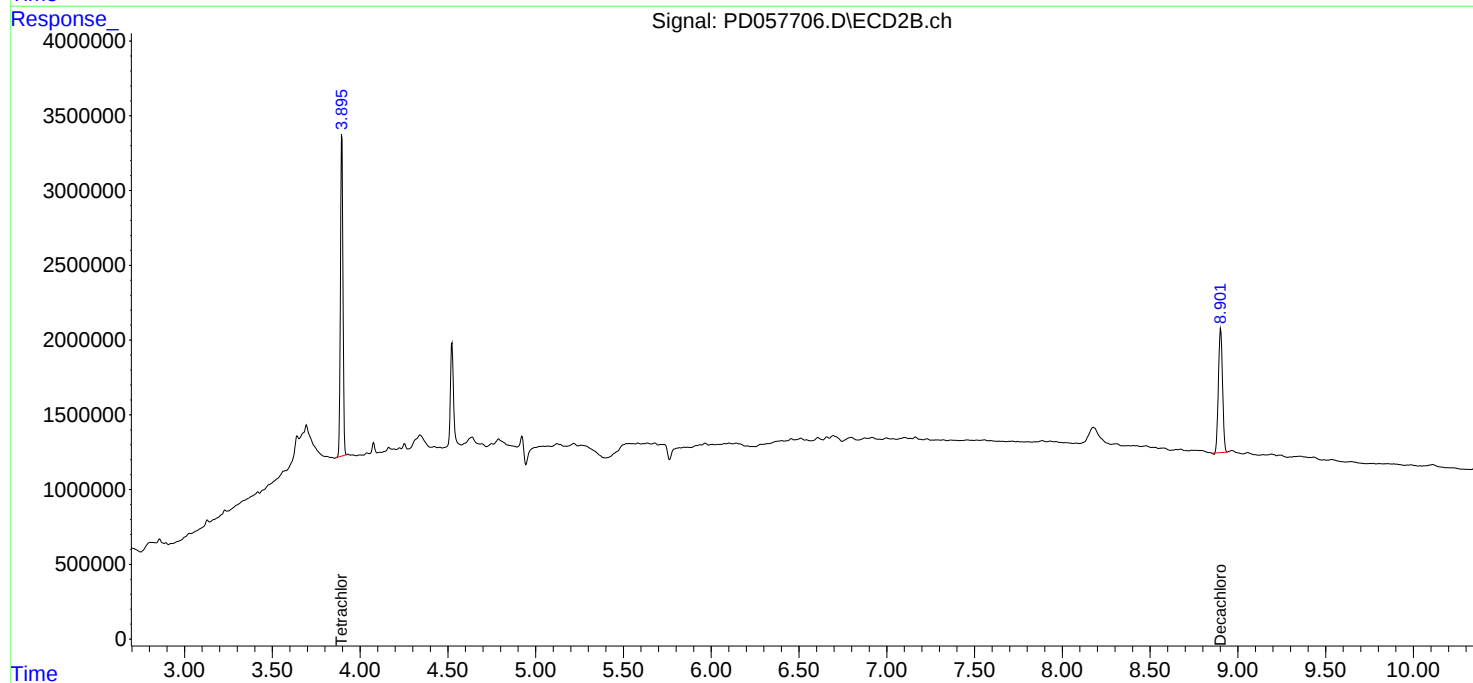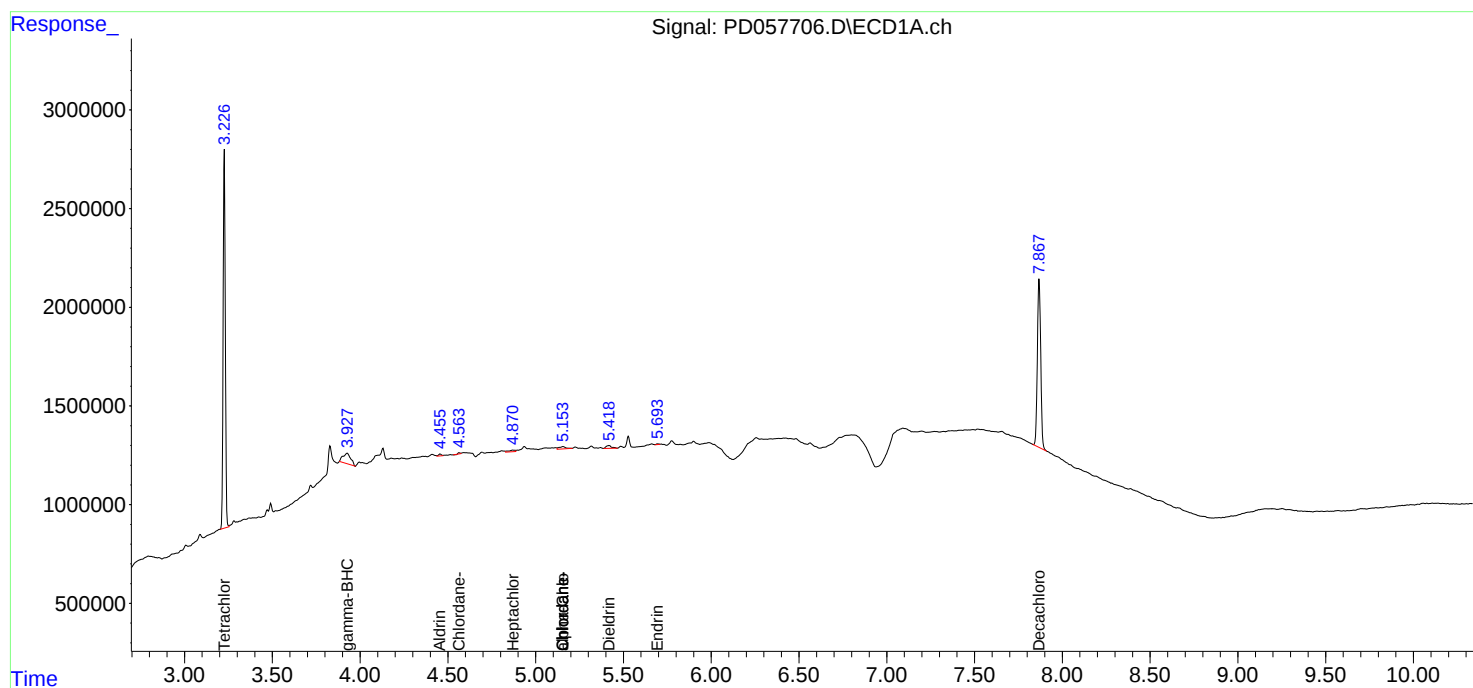


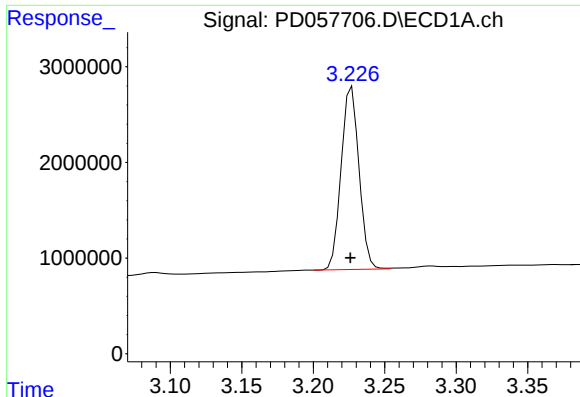

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 16596640
Conc: 23.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

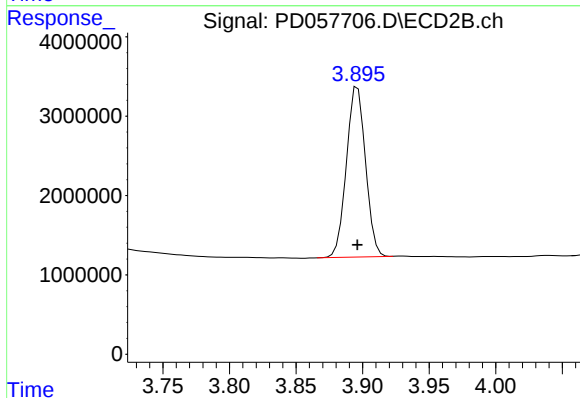


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 21465162
Conc: 27.36 ng/ml

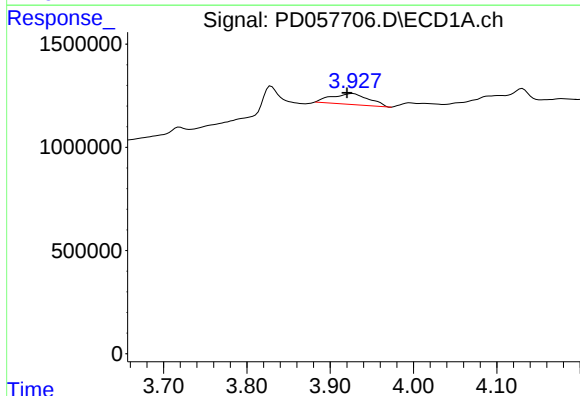


#3 gamma-BHC (Lindane)

R.T.: 3.927 min
Delta R.T.: 0.007 min
Response: 1644893
Conc: 1.53 ng/ml

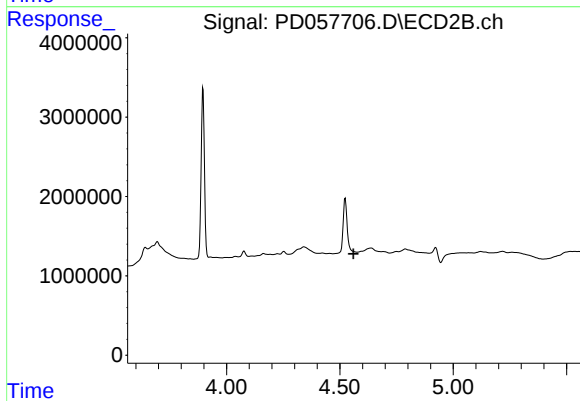

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

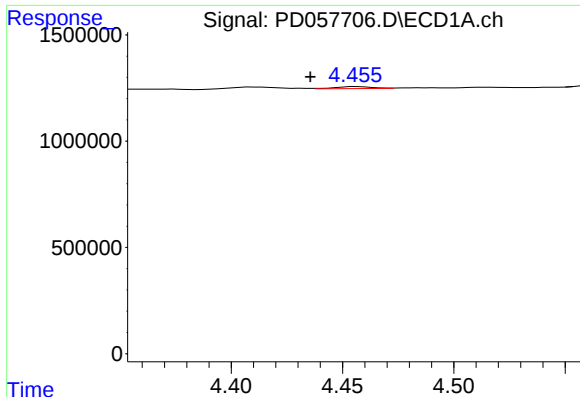

#5 Aldrin


R.T.: 4.456 min
Delta R.T.: 0.021 min
Response: 106123
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

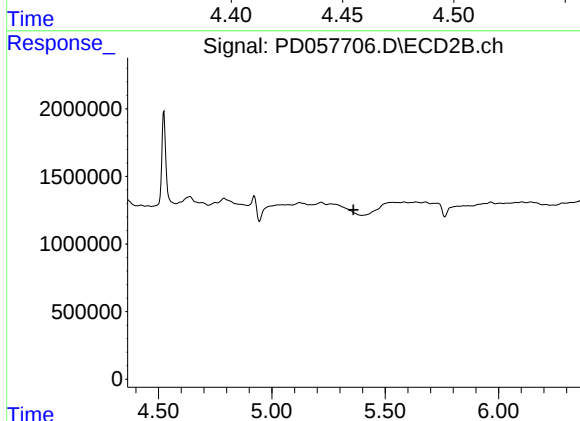


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.360 min
Response: 0
Conc: N.D.

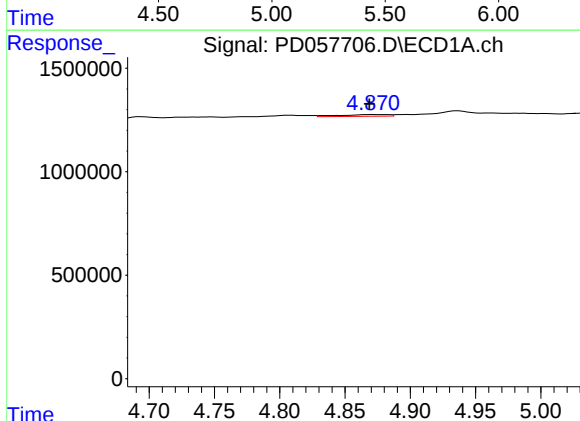


#8 Heptachlor epoxide

R.T.: 4.870 min
Delta R.T.: 0.002 min
Response: 208990
Conc: 0.25 ng/ml

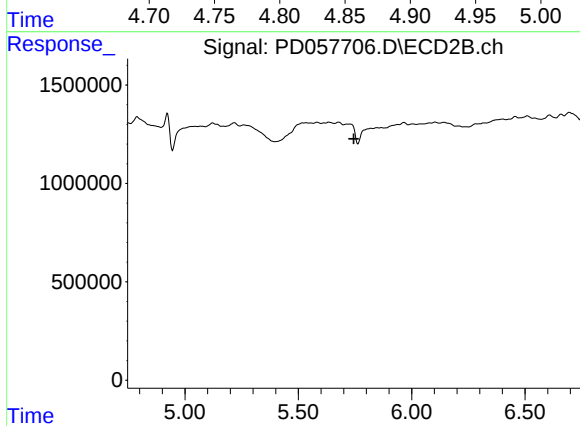

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

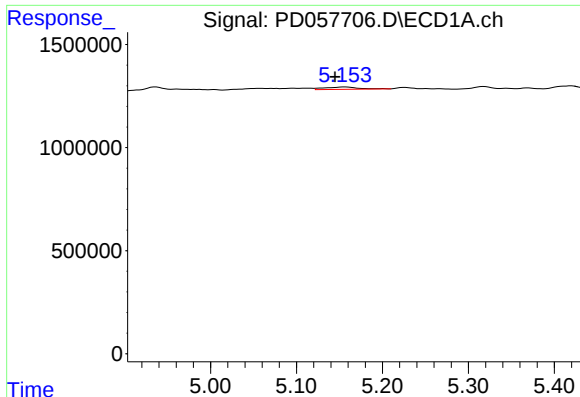

#11 alpha-Chlordane


R.T.: 5.155 min
Delta R.T.: 0.011 min
Response: 306675
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

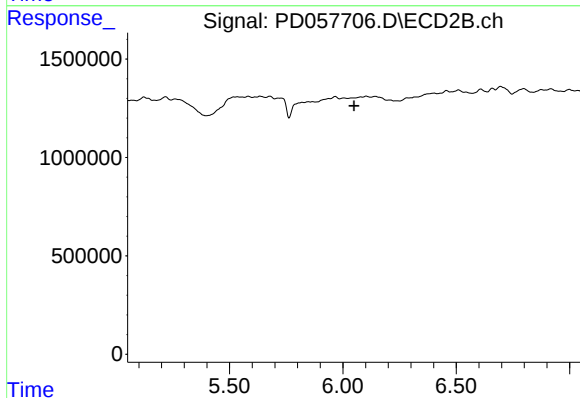


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

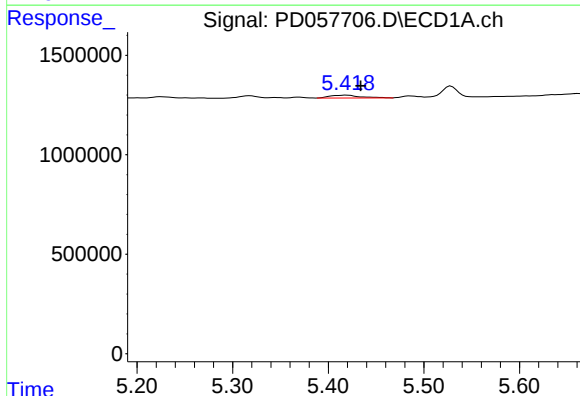


#13 Dieldrin

R.T.: 5.420 min
Delta R.T.: -0.014 min
Response: 308725
Conc: 0.40 ng/ml

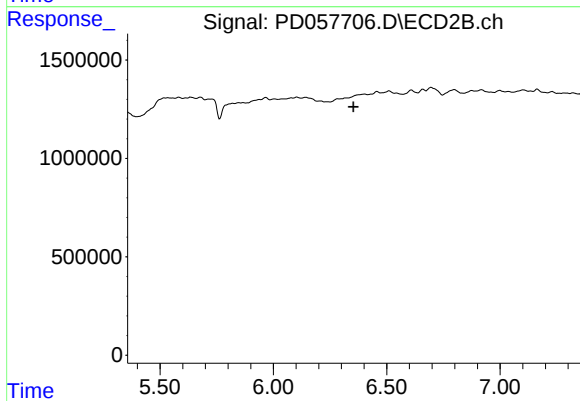

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

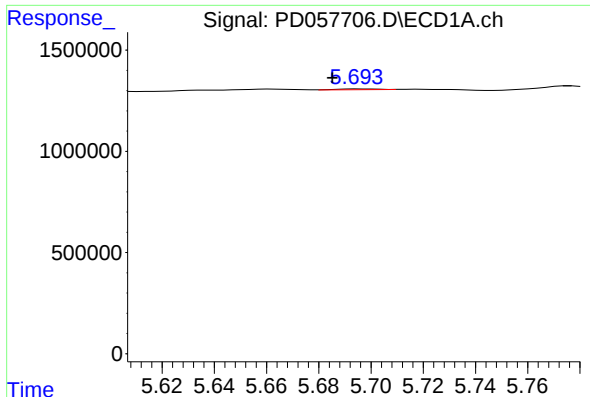

#14 Endrin


R.T.: 5.695 min
Delta R.T.: 0.010 min
Response: 41559
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

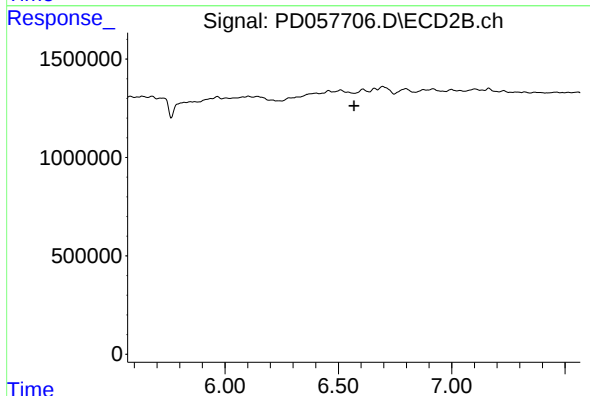


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

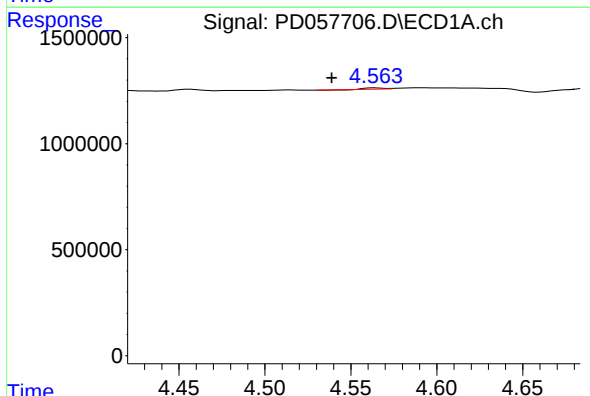


#24 Chlordane-2

R.T.: 4.564 min
Delta R.T.: 0.025 min
Response: 36622
Conc: 1.28 ng/ml

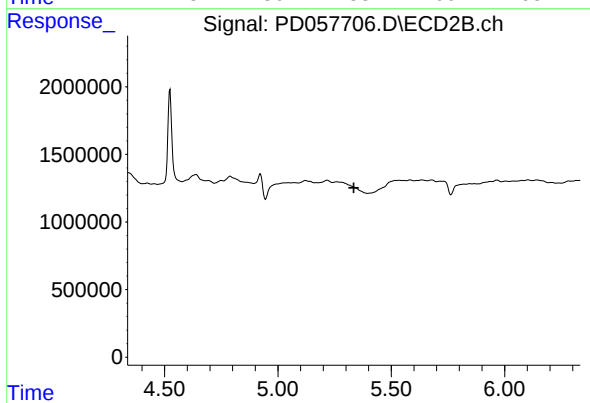

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

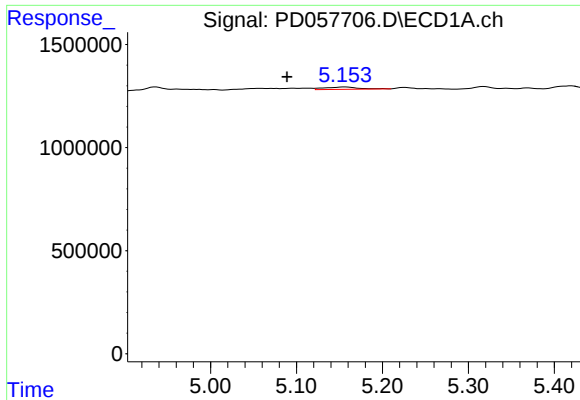

#25 Chlordane-3


R.T.: 5.155 min
Delta R.T.: 0.066 min
Response: 306675
Conc: 3.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

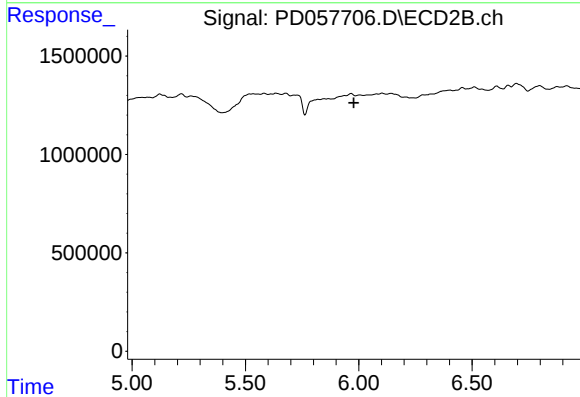


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

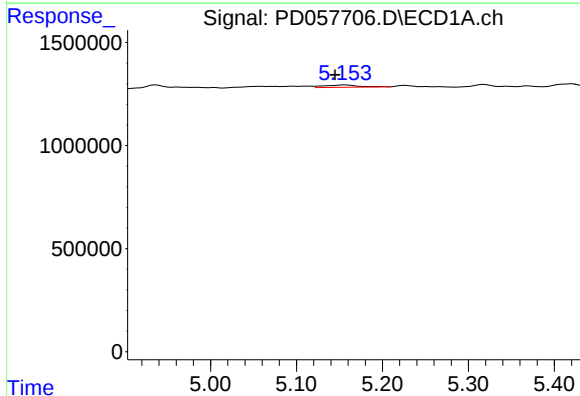


#26 Chlordane-4

R.T.: 5.155 min
Delta R.T.: 0.011 min
Response: 306675
Conc: 3.79 ng/ml

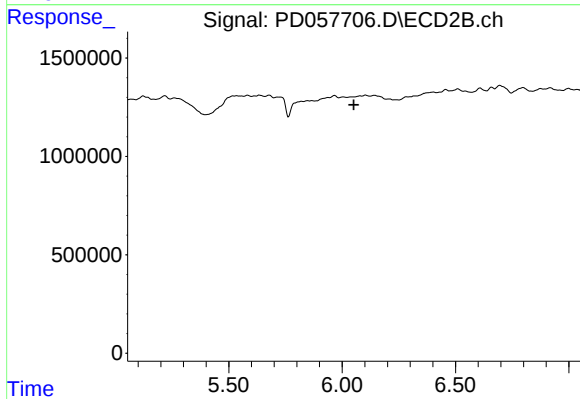

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

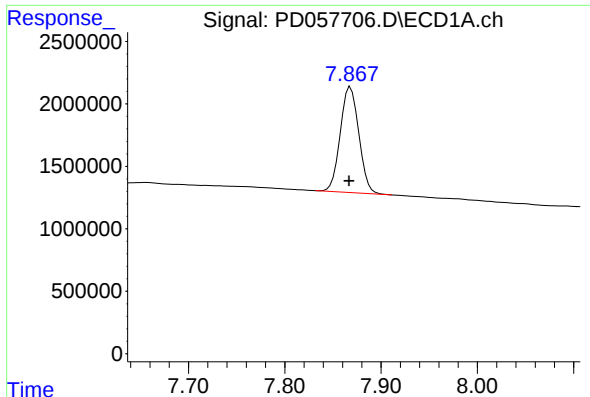

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.002 min
Response: 11302428
Conc: 14.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-040120

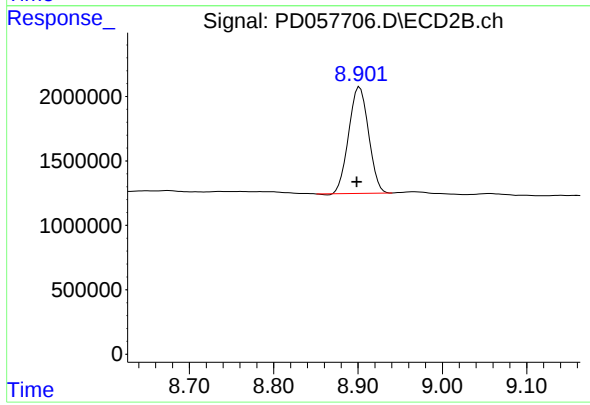

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.004 min
Response: 13528724
Conc: 15.38 ng/ml