

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 10:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:30:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:50:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.895	17256066	21355071	24.169	27.220
28)	SA Decachlor...	7.869	8.900	18772042	21621029	24.655m	24.582

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 10:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
I.BLK


Manual Integrations
APPROVED

mohammad
4/6/2020 1:30:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:50:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

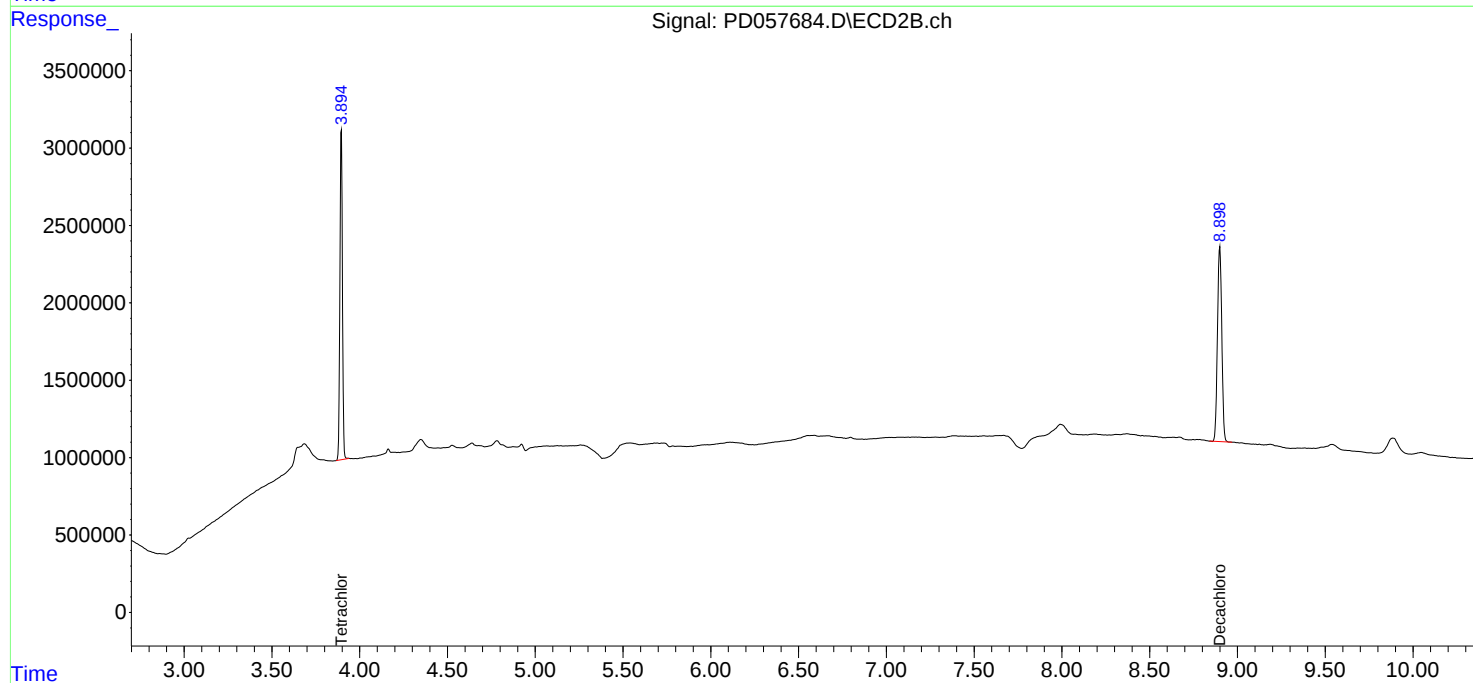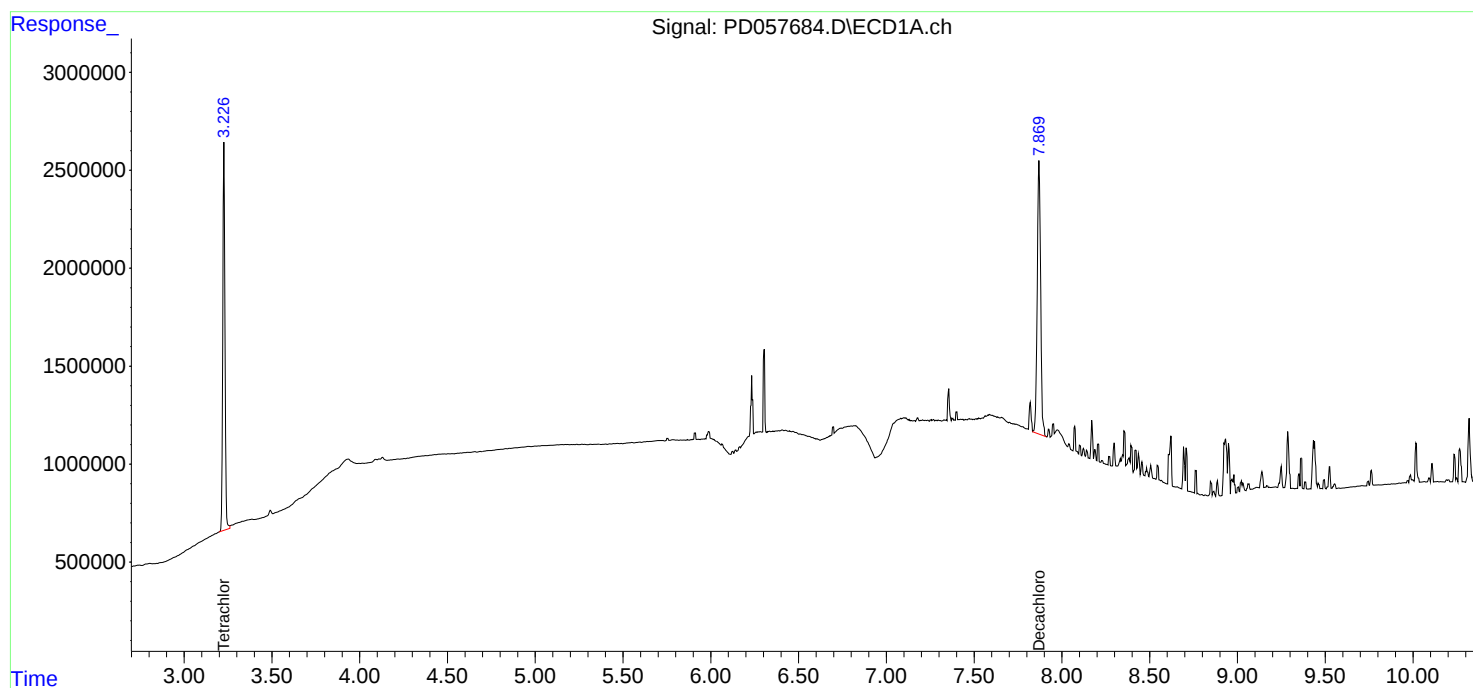

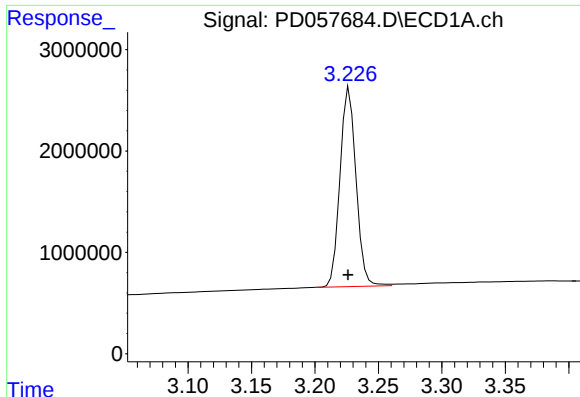


#1 Tetrachloro-m-xylene

R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 17256066
Conc: 24.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
4/6/2020 1:30:08 PM

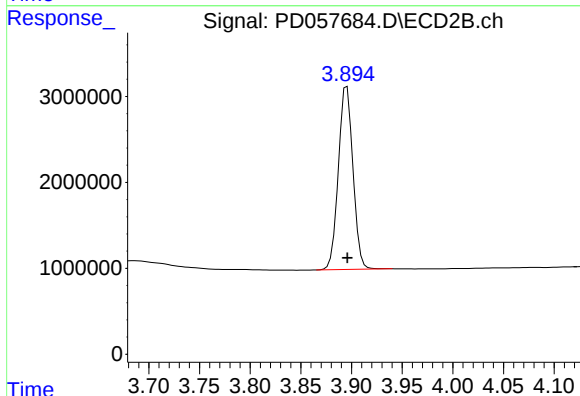


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 21355071
Conc: 27.22 ng/ml

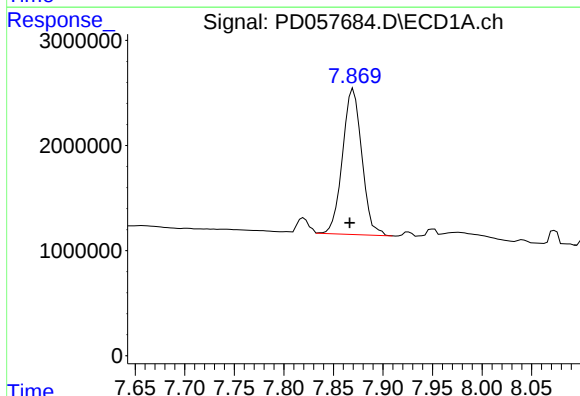

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.002 min
Response: 18772042
Conc: 24.66 ng/ml m

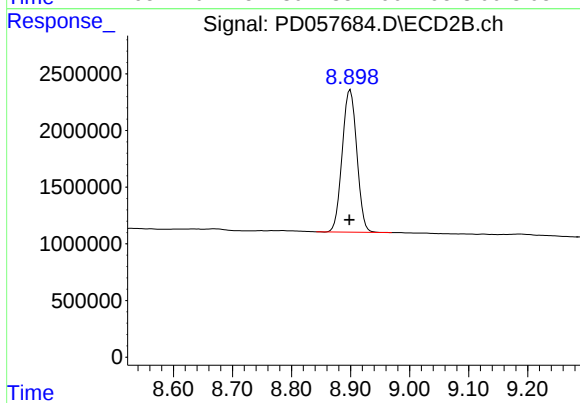

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.001 min
Response: 21621029
Conc: 24.58 ng/ml