

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
 Data File : PD057702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 18:25
 Operator : AJ\MA
 Sample : L2100-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 239-105060708-0-6

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:30:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:56:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.227	3.896	7639691	9693766	10.700	12.356
28) SA Decachlor...	7.872	8.901	12216016	11593258	16.044m	13.181
Target Compounds						
8) B Heptachlo...	4.869	5.739	4726620	1899187	5.575m	1.895 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040220\
Data File : PD057702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 18:25
Operator : AJ\MA
Sample : L2100-07
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
239-105060708-0-6


Manual Integrations
APPROVED

mohammad
4/6/2020 1:30:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:56:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

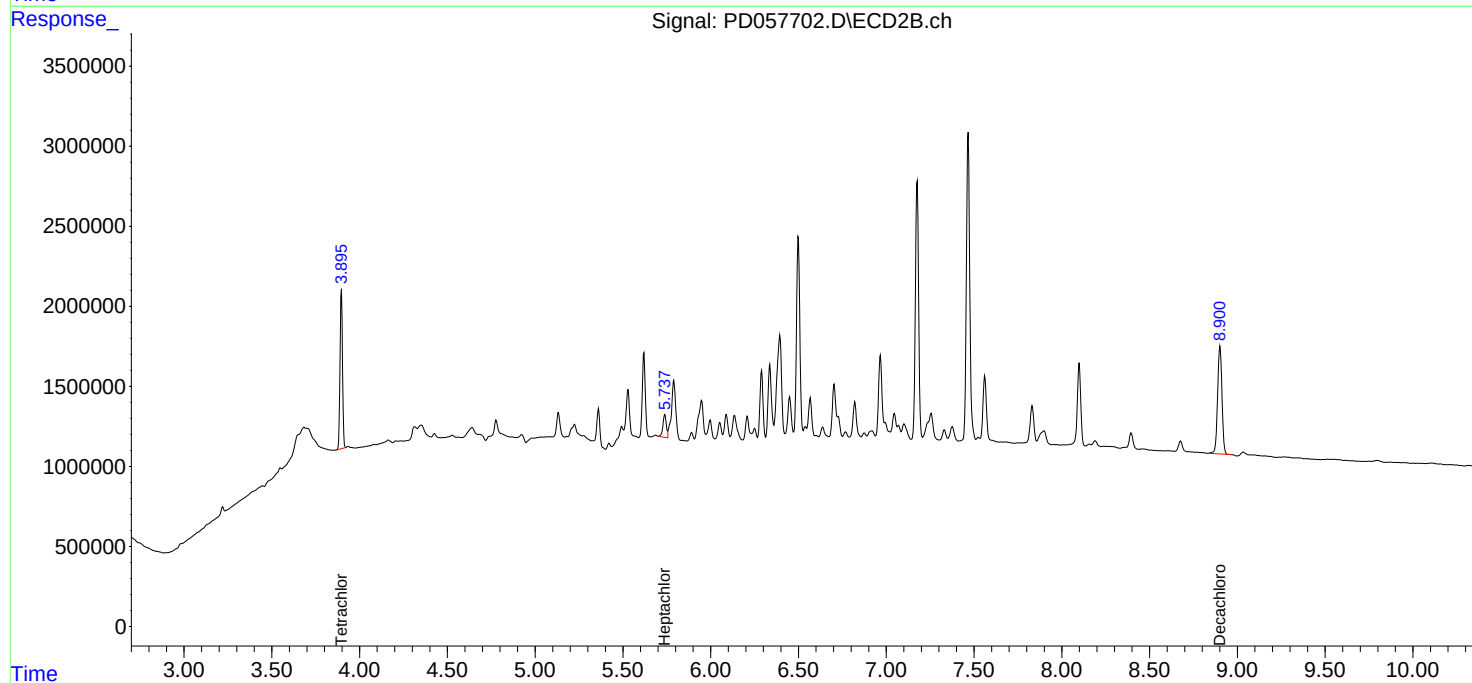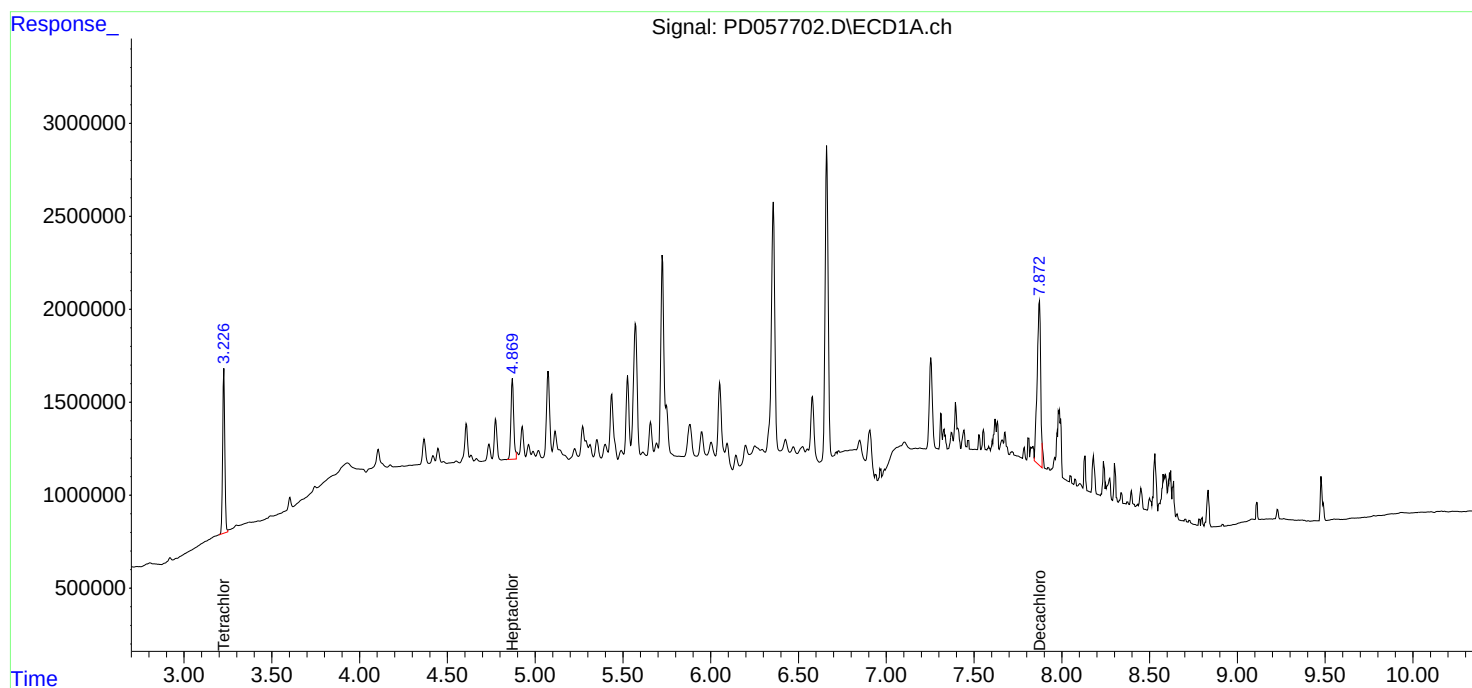

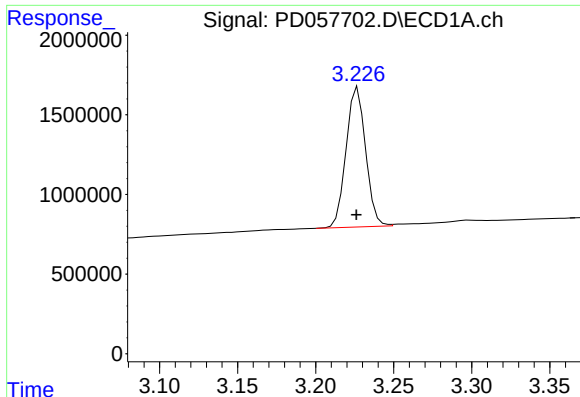


#1 Tetrachloro-m-xylene

R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 7639691
Conc: 10.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
239-105060708-0-6


Manual Integrations
APPROVED

mohammad
4/6/2020 1:30:38 PM

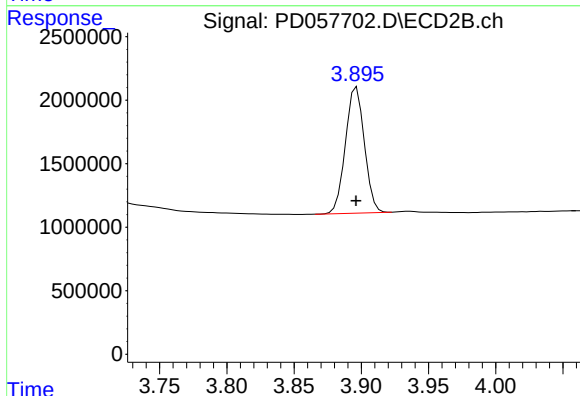


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 9693766
Conc: 12.36 ng/ml

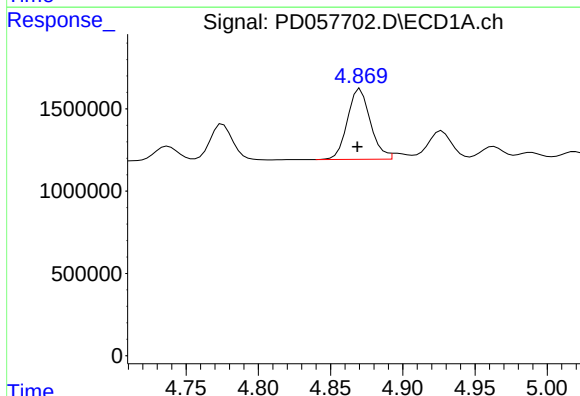


#8 Heptachlor epoxide

R.T.: 4.869 min
Delta R.T.: 0.000 min
Response: 4726620
Conc: 5.58 ng/ml m

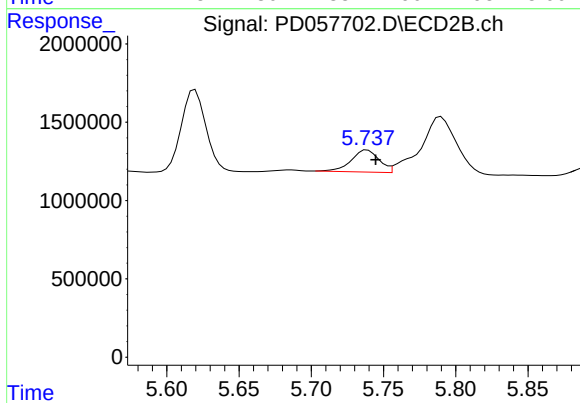

#8 Heptachlor epoxide

R.T.: 5.739 min
Delta R.T.: -0.006 min
Response: 1899187
Conc: 1.89 ng/ml

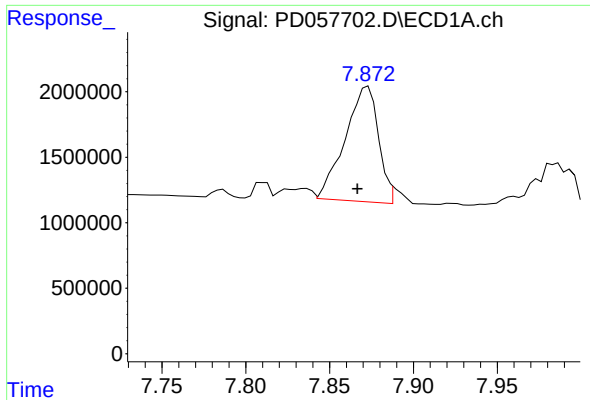


#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.005 min
Response: 12216016
Conc: 16.04 ng/ml m

Instrument :
ECD_D
ClientSampleId :
239-105060708-0-6

Manual Integrations
APPROVED

mohammad
4/6/2020 1:30:38 PM

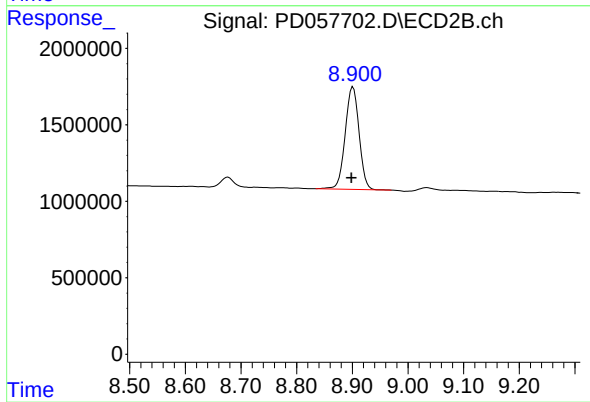

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.003 min
Response: 11593258
Conc: 13.18 ng/ml