

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD040221\  
 Data File : PD061967.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 02 Apr 2021 12:46  
 Operator : AR\AJ  
 Sample : INDA323  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA323

Manual Integrations  
 APPROVED

Ankita  
 4/5/2021 3:32:09 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 03 05:13:09 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD030421CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Mar 05 05:53:14 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 3.485 | 3.981 | 19591508 | 204.4E6 | 21.565  | 21.879  |
| 27)                         | SA Decachlor... | 8.255 | 9.039 | 50976414 | 330.0E6 | 38.061  | 35.286  |
| Target Compounds            |                 |       |       |          |         |         |         |
| 2)                          | A alpha-BHC     | 3.924 | 4.369 | 28356233 | 337.0E6 | 21.569  | 23.307  |
| 3)                          | MA gamma-BHC... | 4.209 | 4.654 | 27439847 | 306.5E6 | 21.132  | 23.137  |
| 4)                          | MA Heptachlor   | 4.512 | 5.162 | 27882762 | 301.3E6 | 20.698  | 22.116  |
| 9)                          | A Endosulfan I  | 5.547 | 6.209 | 24836411 | 243.7E6 | 20.638  | 21.399  |
| 13)                         | MA Dieldrin     | 5.789 | 6.464 | 54964552 | 522.9E6 | 41.593m | 43.002m |
| 14)                         | MA Endrin       | 6.050 | 6.683 | 45856983 | 421.3E6 | 39.647  | 41.455  |
| 16)                         | A 4,4'-DDD      | 6.173 | 6.806 | 42986610 | 394.2E6 | 41.321  | 40.886  |
| 17)                         | MA 4,4'-DDT     | 6.415 | 7.104 | 42739622 | 391.4E6 | 38.498  | 40.196  |
| 20)                         | A Methoxychlor  | 6.961 | 7.561 | 116.9E6  | 912.7E6 | 191.652 | 200.237 |
| -----                       |                 |       |       |          |         |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD040221\  
Data File : PD061967.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Apr 2021 12:46  
Operator : AR\AJ  
Sample : INDA323  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 03 05:13:09 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD030421CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Mar 05 05:53:14 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

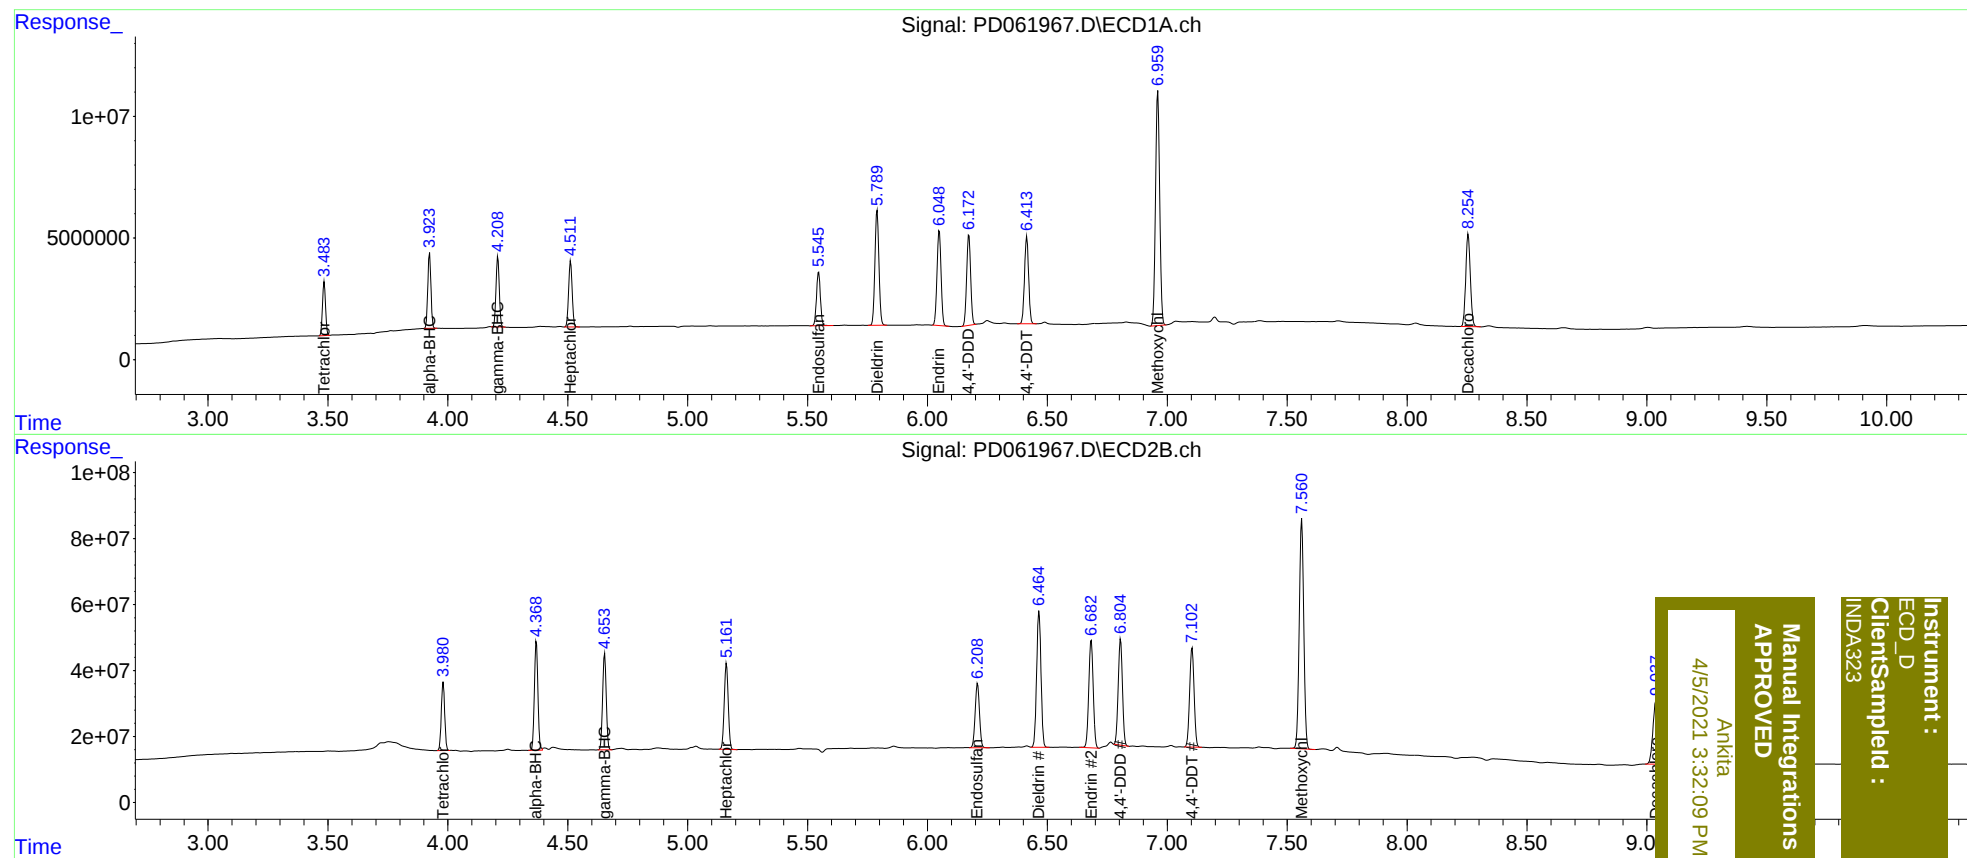

Manual Integrations  
APPROVED

Ankita  
4/5/2021 3:32:09 PM

Instrument :  
ECD\_D  
ClientSample :  
INDA323