

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040319\
 Data File : PD052494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 7:22
 Operator : AJ\SJ
 Sample : MDL-BL-TOX-S-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BL-TOX-S-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 08:36:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 14:07:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.220	4.042	27893475	586.7E6	20.530	21.030
7) SA Decachlor...	7.815	9.155	30227300	417.2E6	22.506	27.236


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040319\
Data File : PD052494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 7:22
Operator : AJ\SJ
Sample : MDL-BL-TOX-S-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 08:36:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 14:07:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

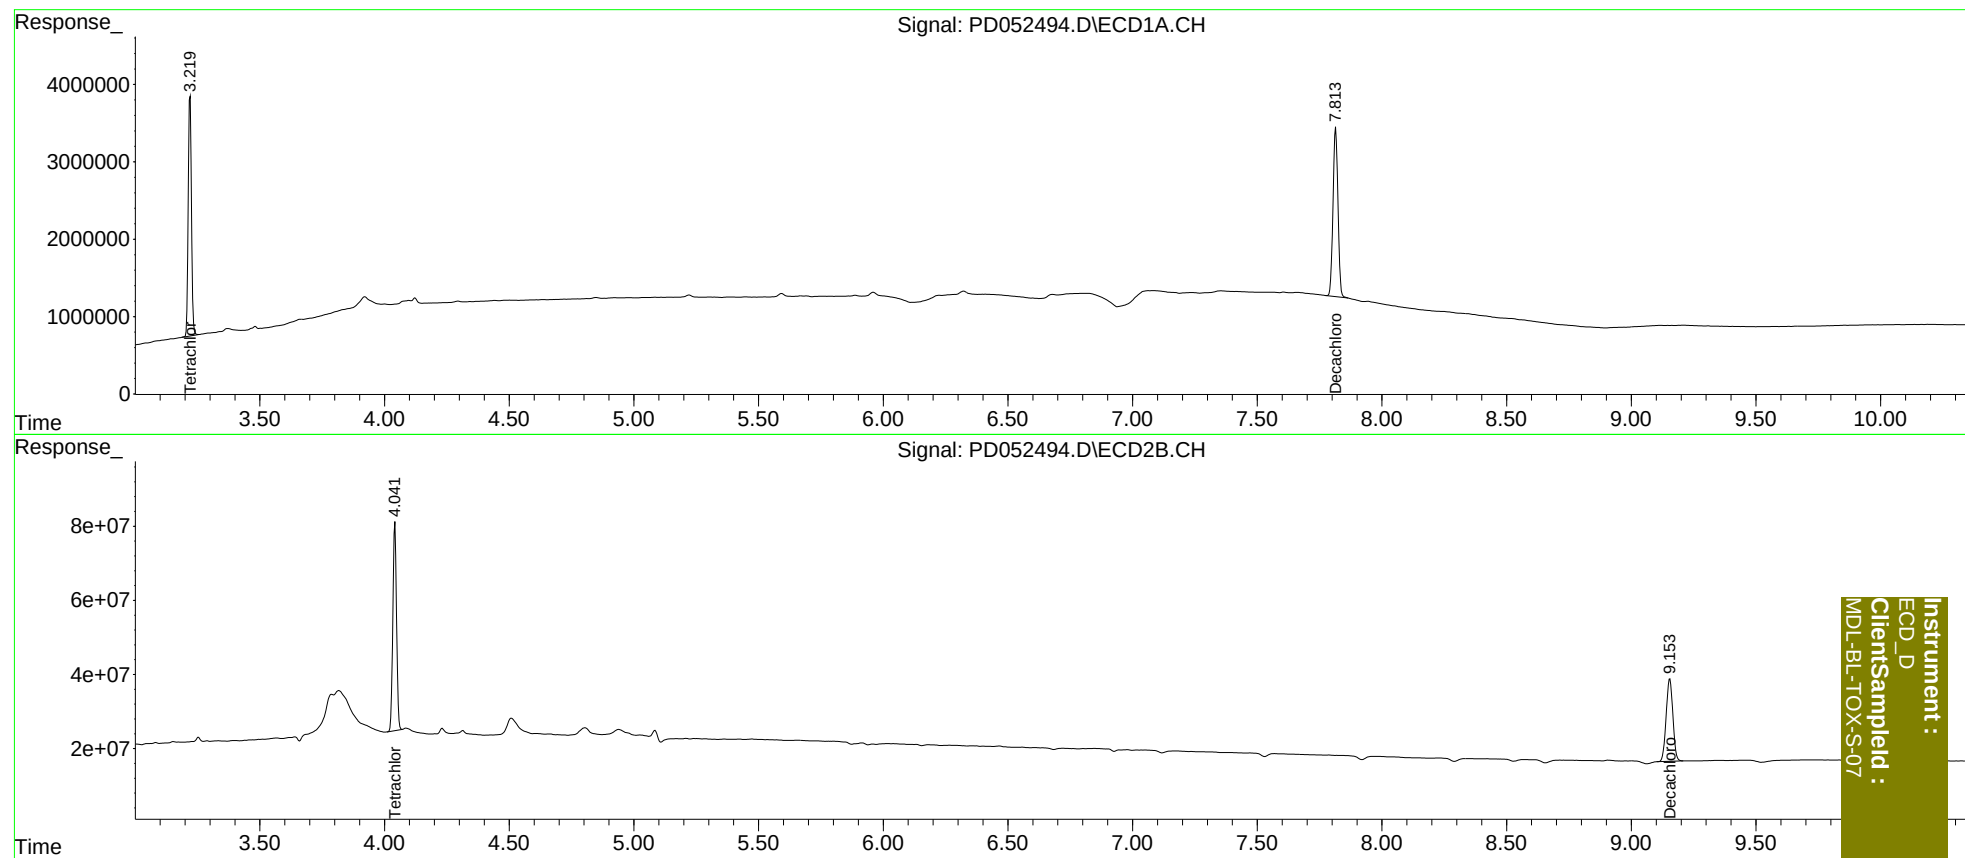


Instrument :
ECD_D
ClientSample :
MDL-BL-TOX-S-07

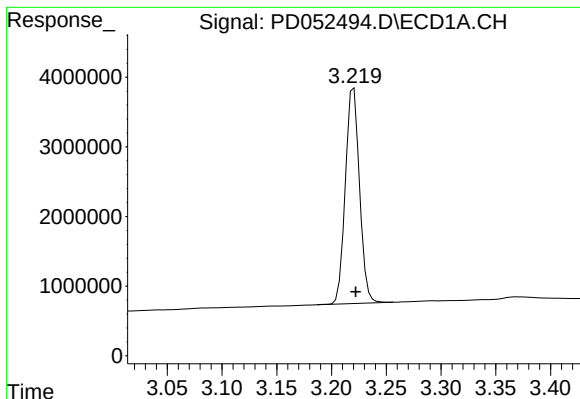

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.002 min
Response: 27893475
Conc: 20.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-TOX-S-07

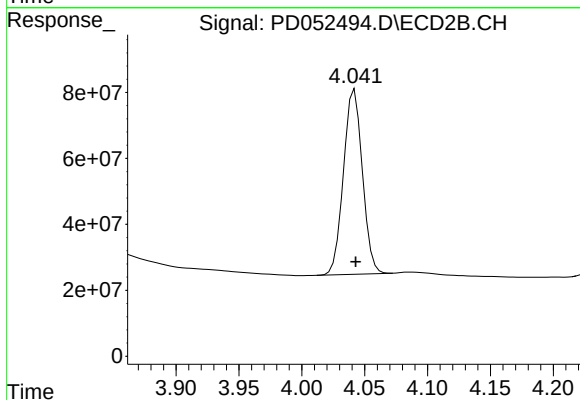


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 586691548
Conc: 21.03 ng/ml

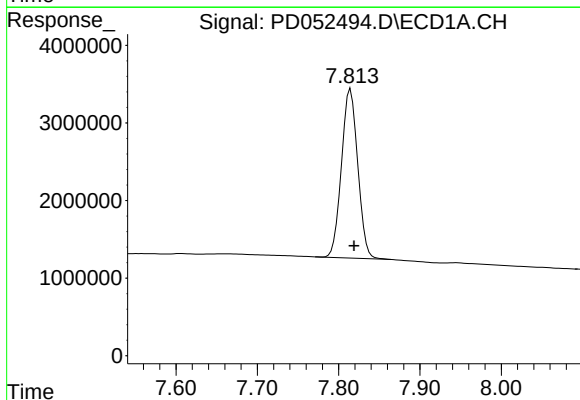

#7 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: -0.004 min
Response: 30227300
Conc: 22.51 ng/ml

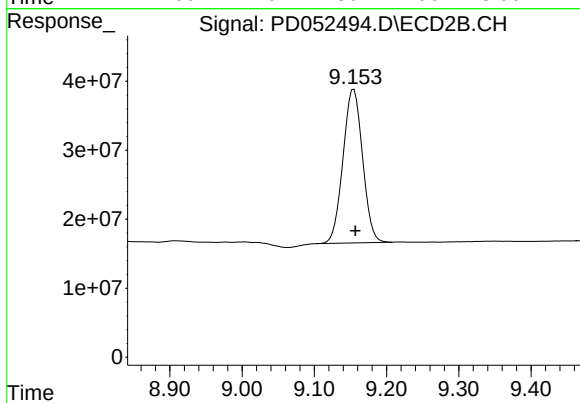

#7 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 417225471
Conc: 27.24 ng/ml