

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
 Data File : PD057717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 16:43
 Operator : AJ\MA
 Sample : L2129-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 00:53:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	16294183	21629408	22.821	27.569
28)	SA Decachlor...	7.867	8.900	16032795	20931609	21.057	23.799
Target Compounds							
3)	MA gamma-BHC...	3.927	0.000	2068842	0	1.922	N.D. #
24)	Chlordane-2	4.564f	0.000	324653	0	11.324	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
Data File : PD057717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 16:43
Operator : AJ\MA
Sample : L2129-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 00:53:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

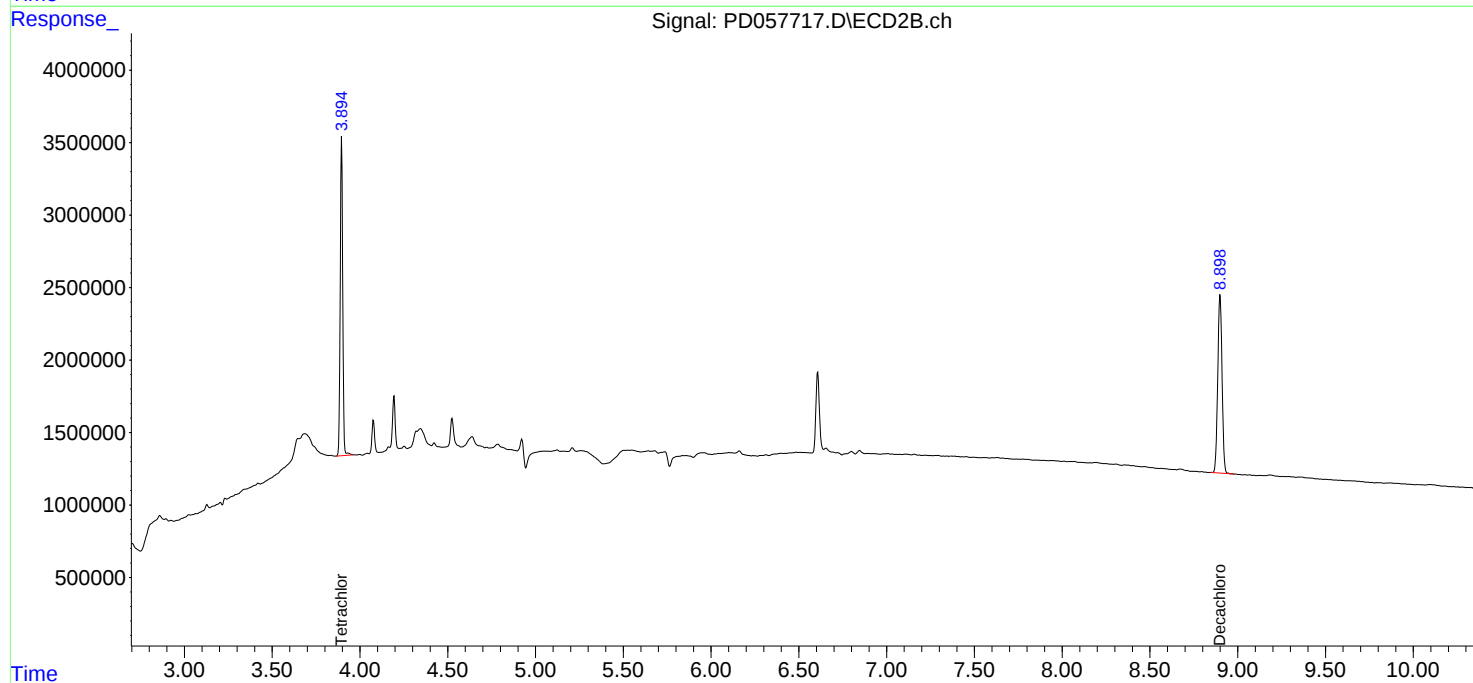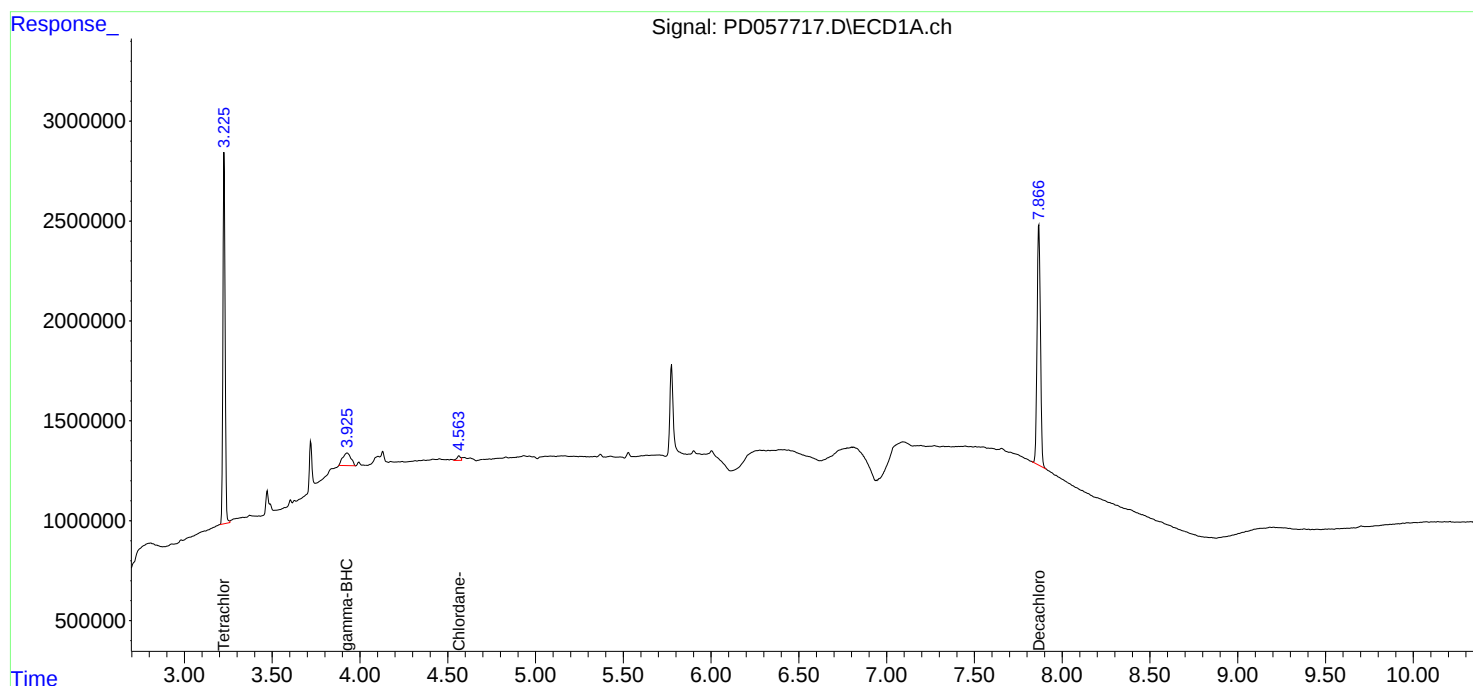


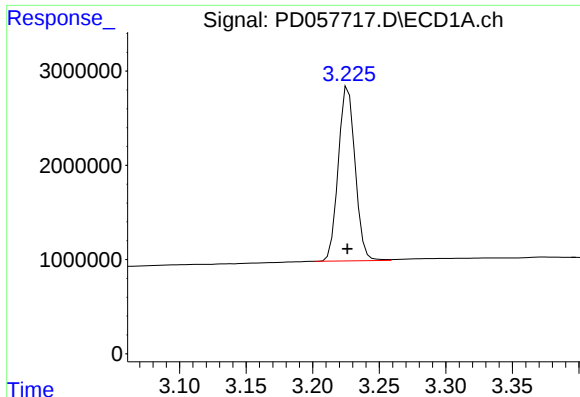

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 16294183
Conc: 22.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8

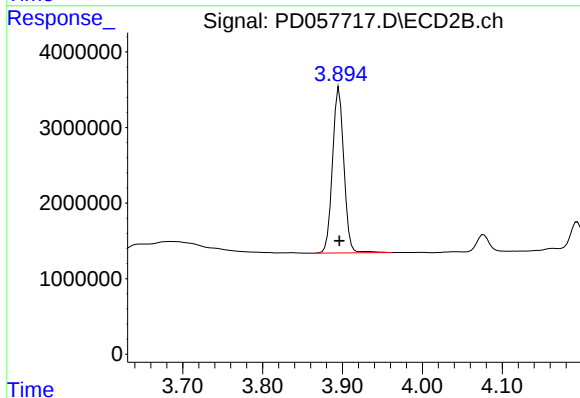


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 21629408
Conc: 27.57 ng/ml

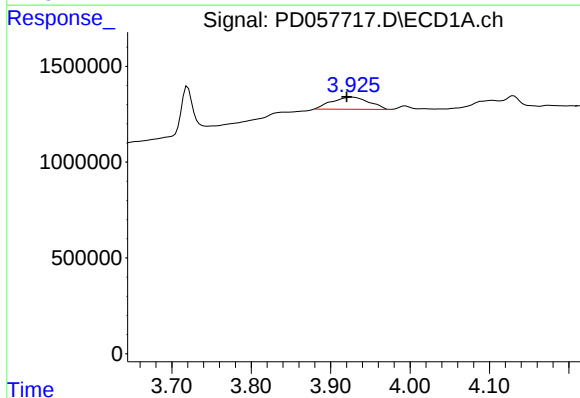


#3 gamma-BHC (Lindane)

R.T.: 3.927 min
Delta R.T.: 0.007 min
Response: 2068842
Conc: 1.92 ng/ml

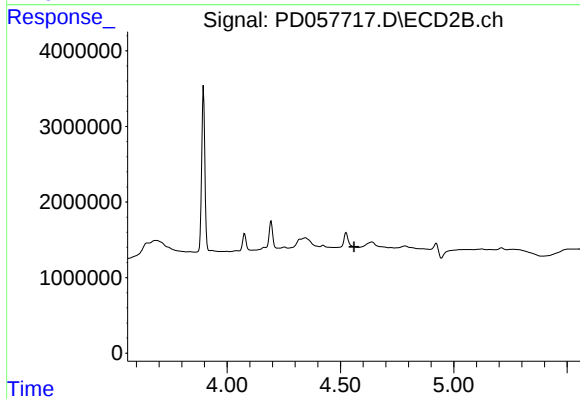

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

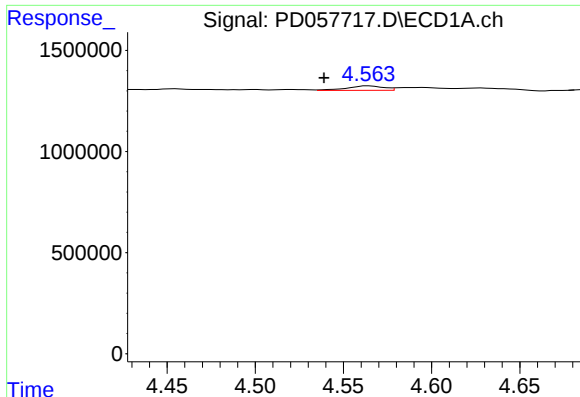

#24 Chlordane-2


R.T.: 4.564 min
Delta R.T.: 0.025 min
Response: 324653
Conc: 11.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8

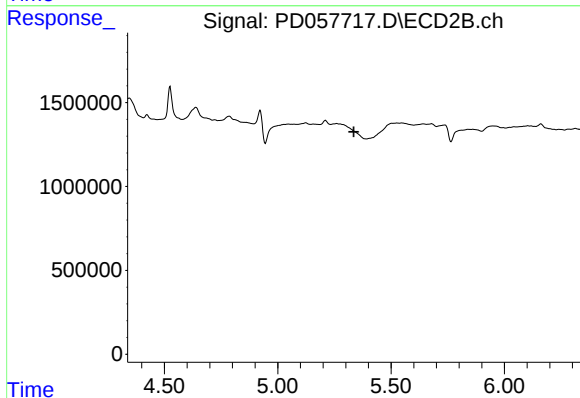


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

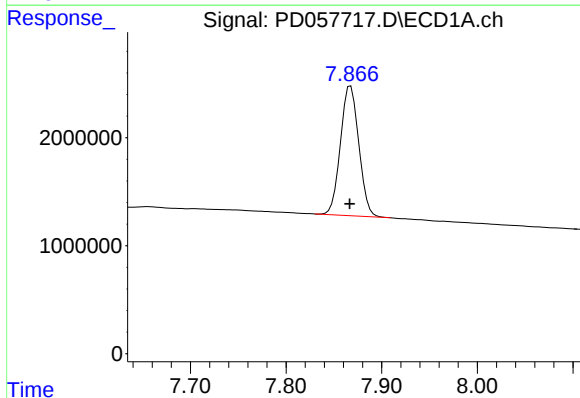

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 16032795
Conc: 21.06 ng/ml

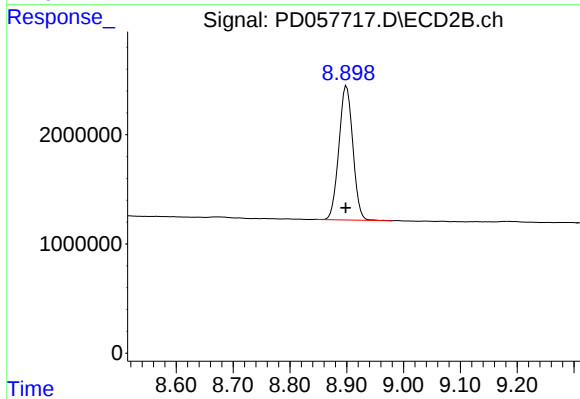

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.001 min
Response: 20931609
Conc: 23.80 ng/ml