

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
 Data File : PD057720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 17:26
 Operator : AJ\MA
 Sample : L2129-24
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 00:53:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	15233286	20020229	21.336	25.518
28)	SA Decachlor...	7.869	8.901	14694612	19051880	19.300	21.661
Target Compounds							
3)	MA gamma-BHC...	3.929	0.000	2271183	0	2.109	N.D. #
8)	B Heptachlo...	4.891f	0.000	221909	0	0.262	N.D. #
9)	A Endosulfan I	5.171f	0.000	102710	0	0.124	N.D. #
10)	B gamma-Chl...	5.093	0.000	230534	0	0.251	N.D. #
11)	B alpha-Chl...	5.140	0.000	173419	0	0.189	N.D. #
24)	Chlordane-2	4.564f	0.000	19723	0	0.688	N.D. #
25)	Chlordane-3	5.093	0.000	230534	0	2.626	N.D. #
26)	Chlordane-4	5.140	0.000	173419	0	2.144	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
Data File : PD057720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 17:26
Operator : AJ\MA
Sample : L2129-24
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 00:53:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

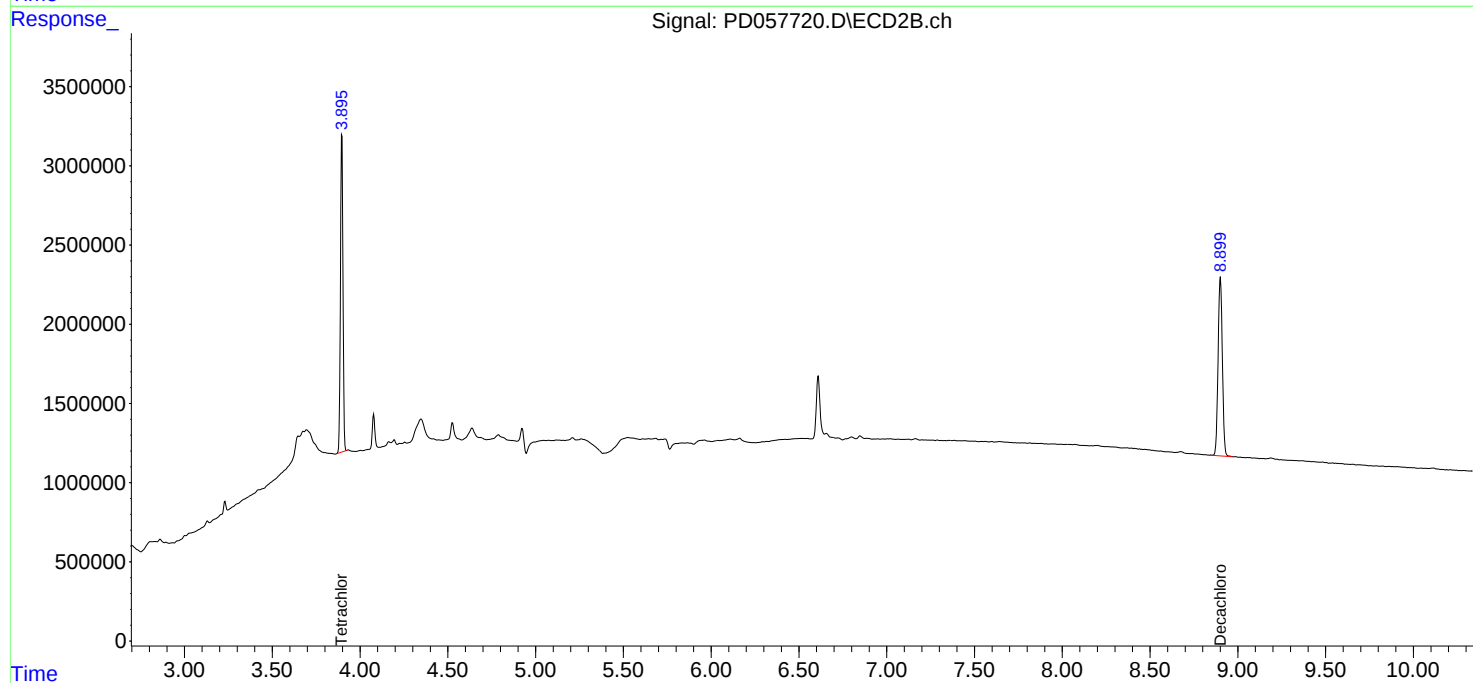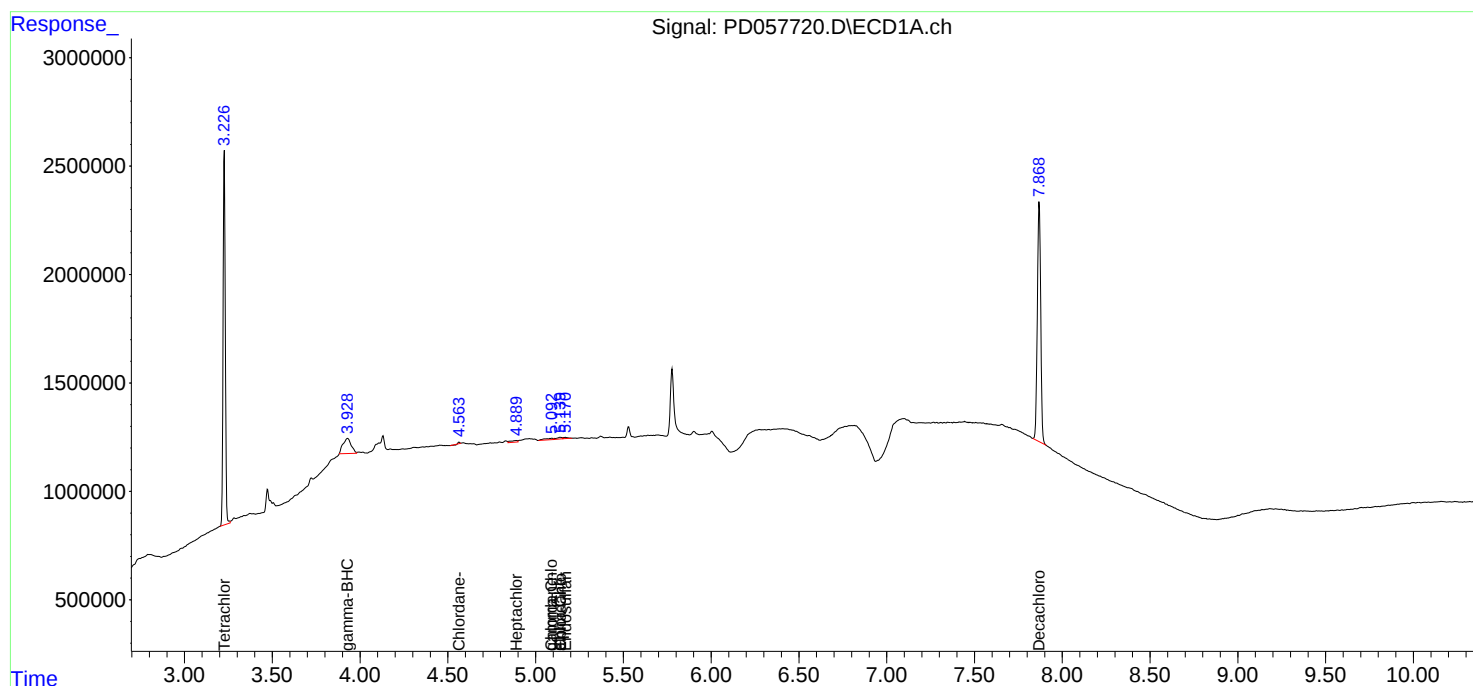


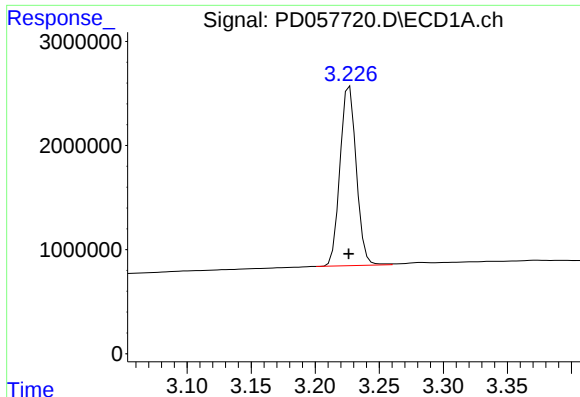

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 15233286
Conc: 21.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

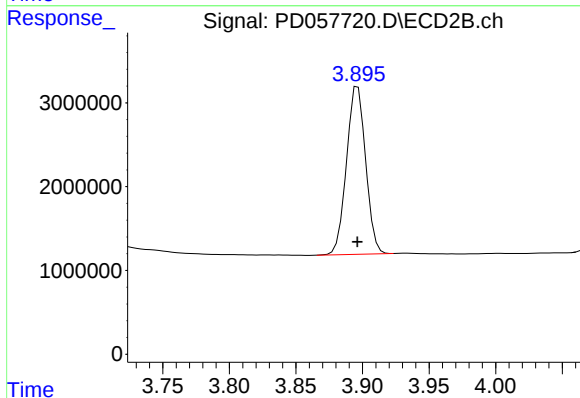


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 20020229
Conc: 25.52 ng/ml

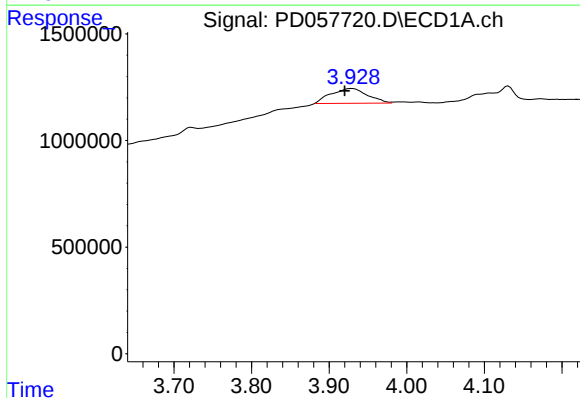


#3 gamma-BHC (Lindane)

R.T.: 3.929 min
Delta R.T.: 0.009 min
Response: 2271183
Conc: 2.11 ng/ml

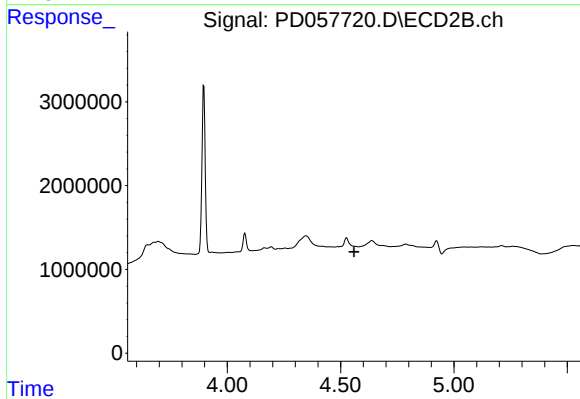

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

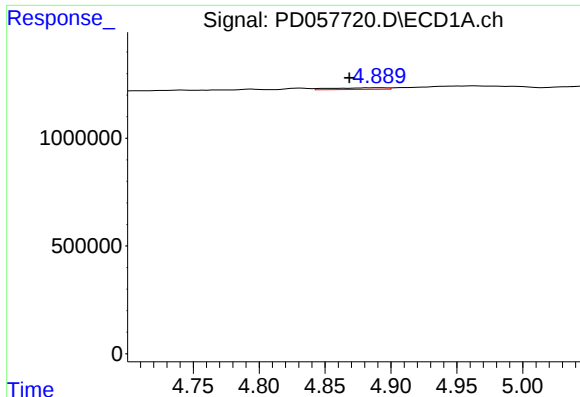

#8 Heptachlor epoxide


R.T.: 4.891 min
Delta R.T.: 0.022 min
Response: 221909
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

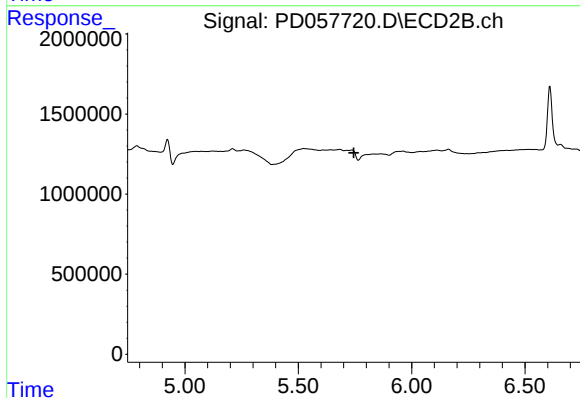


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

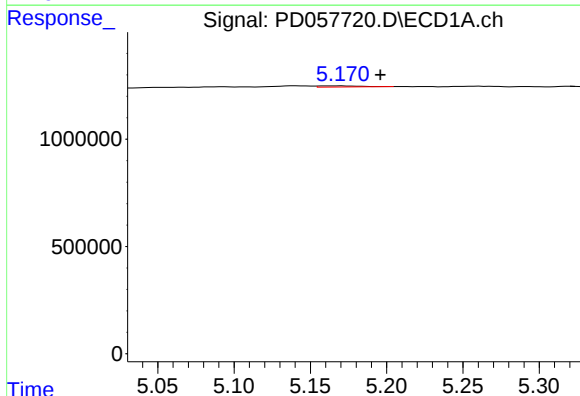


#9 Endosulfan I

R.T.: 5.171 min
Delta R.T.: -0.025 min
Response: 102710
Conc: 0.12 ng/ml

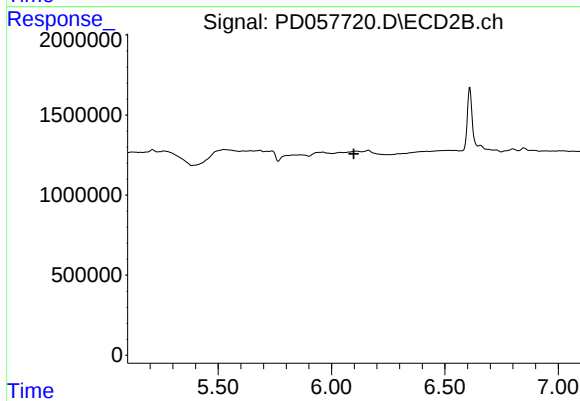

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

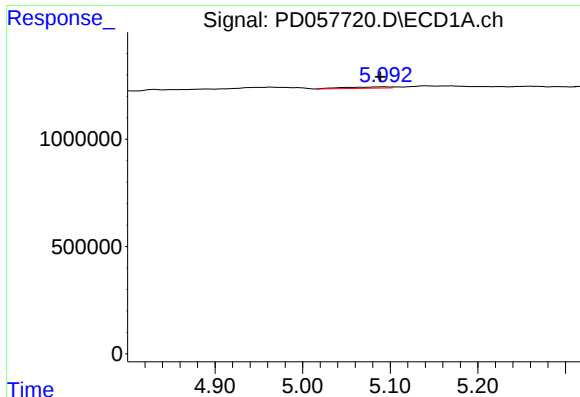

#10 gamma-Chlordane


R.T.: 5.093 min
Delta R.T.: 0.005 min
Response: 230534
Conc: 0.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

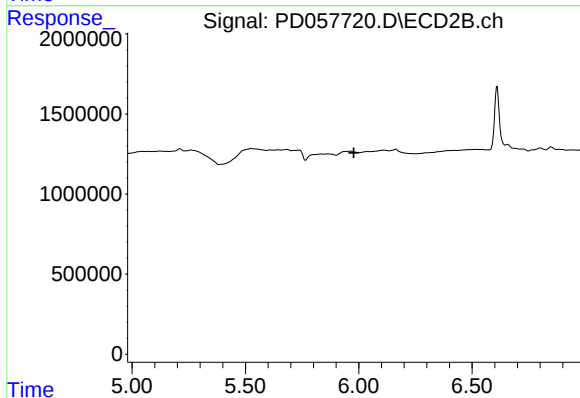


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

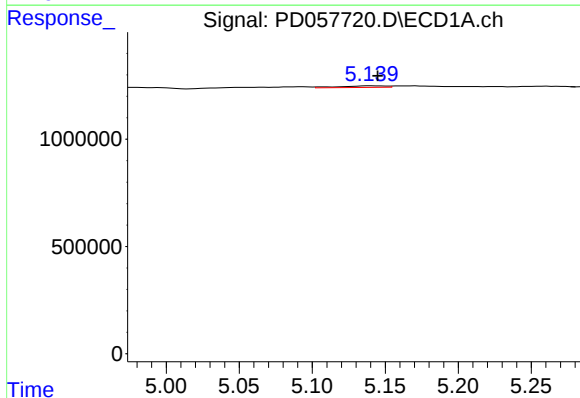


#11 alpha-Chlordane

R.T.: 5.140 min
Delta R.T.: -0.005 min
Response: 173419
Conc: 0.19 ng/ml

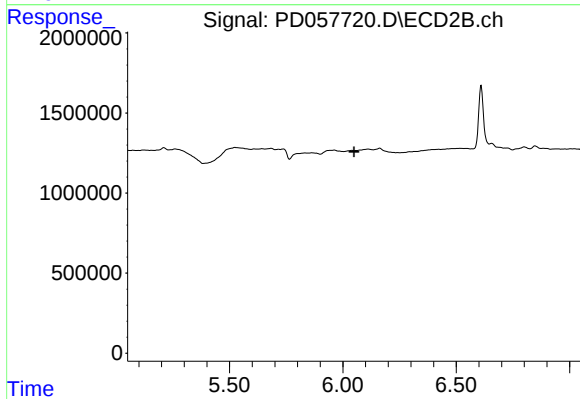

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

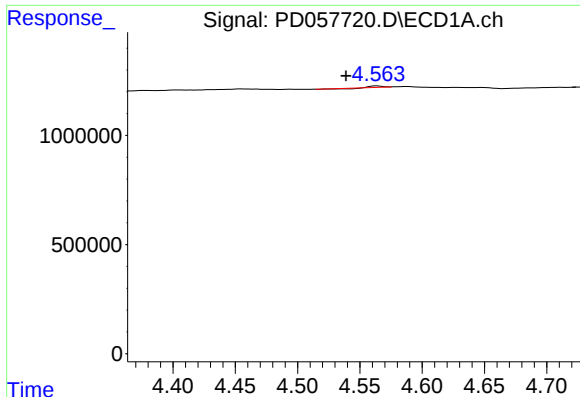

#24 Chlordane-2


R.T.: 4.564 min
Delta R.T.: 0.025 min
Response: 19723
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

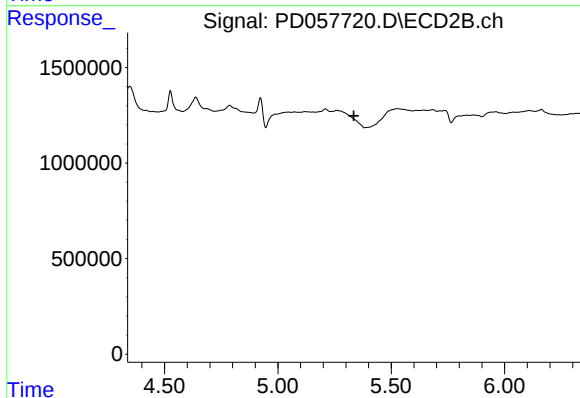


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

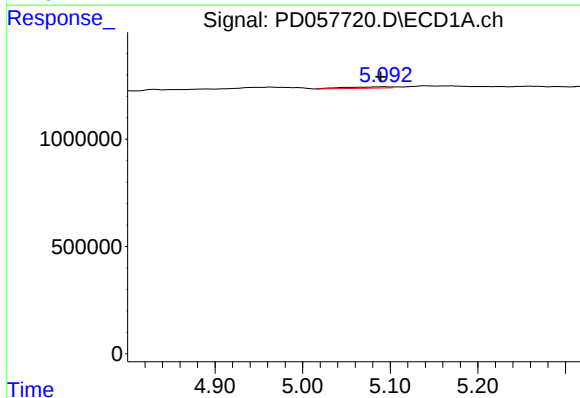


#25 Chlordane-3

R.T.: 5.093 min
Delta R.T.: 0.004 min
Response: 230534
Conc: 2.63 ng/ml

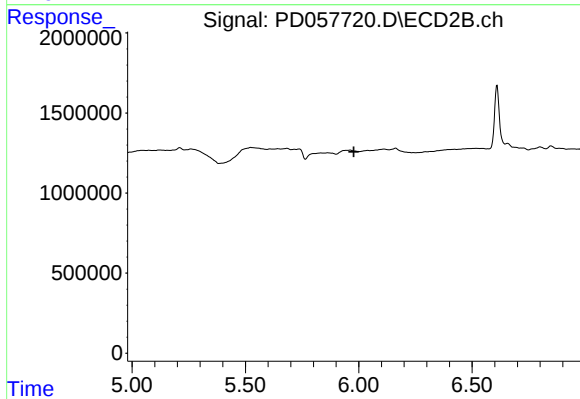

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

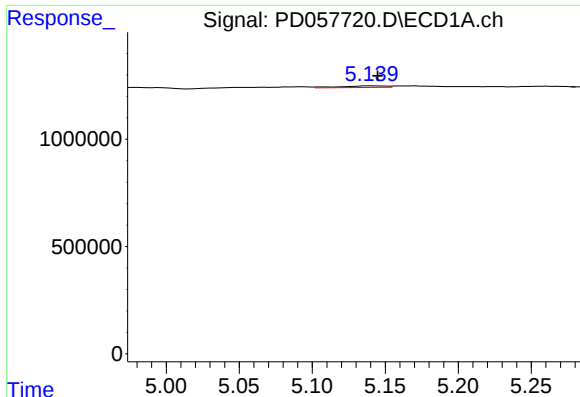

#26 Chlordane-4


R.T.: 5.140 min
Delta R.T.: -0.005 min
Response: 173419
Conc: 2.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

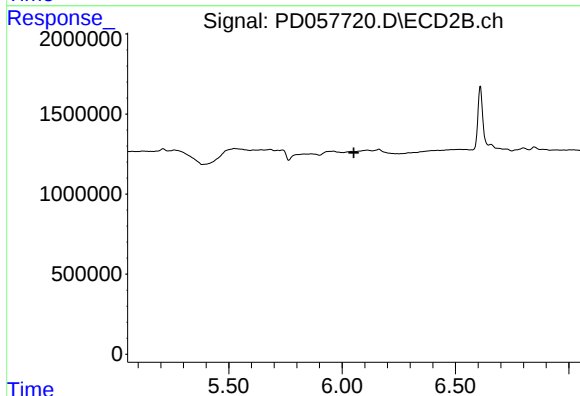


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

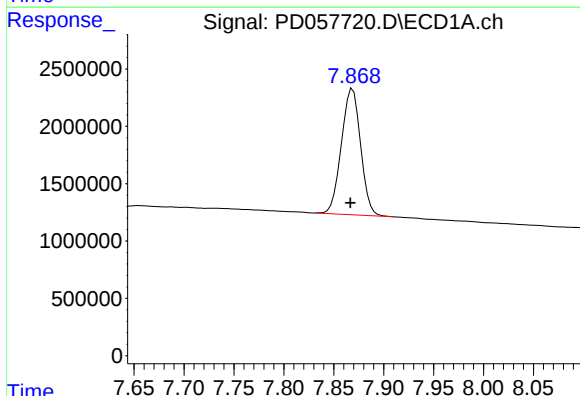

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.002 min
Response: 14694612
Conc: 19.30 ng/ml

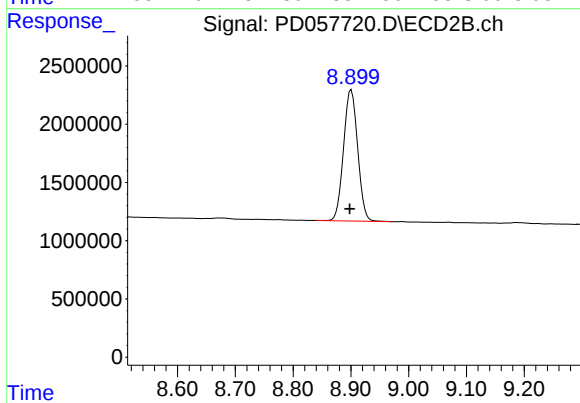

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.002 min
Response: 19051880
Conc: 21.66 ng/ml