

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
 Data File : PD057723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 18:08
 Operator : AJ\MA
 Sample : L2129-39
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 00:54:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	17292215	22450986	24.219	28.617
28)	SA Decachlor...	7.868	8.899	15371422	19990111	20.189	22.728
Target Compounds							
2)	A alpha-BHC	3.627f	0.000	167473	0	0.153	N.D. #
3)	MA gamma-BHC...	3.927	0.000	1866468	0	1.734	N.D. #
5)	MB Aldrin	4.413f	0.000	215379	0	0.220	N.D. #
10)	B gamma-Chl...	5.064f	0.000	61598	0	0.067	N.D. #
24)	Chlordane-2	4.564f	0.000	578166	0	20.167	N.D. #
25)	Chlordane-3	5.064f	0.000	61598	0	0.702	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
Data File : PD057723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 18:08
Operator : AJ\MA
Sample : L2129-39
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 00:54:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

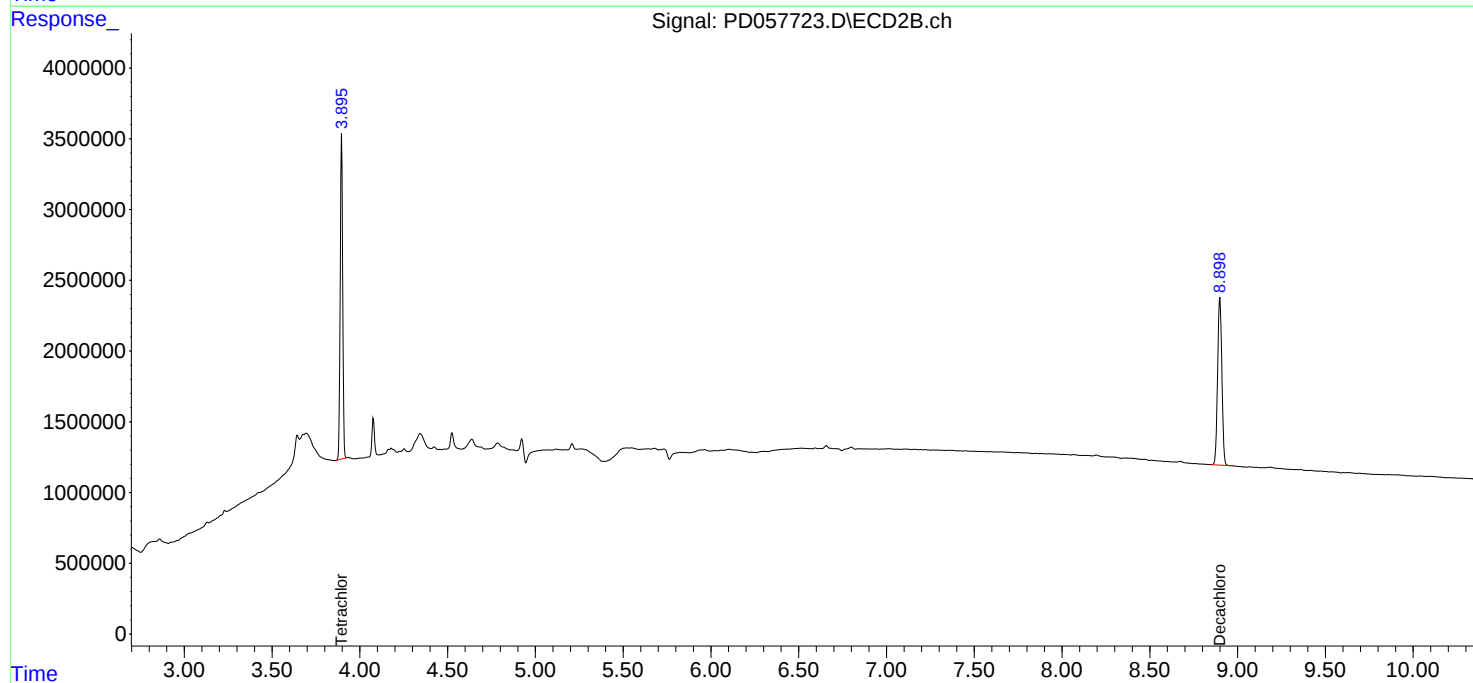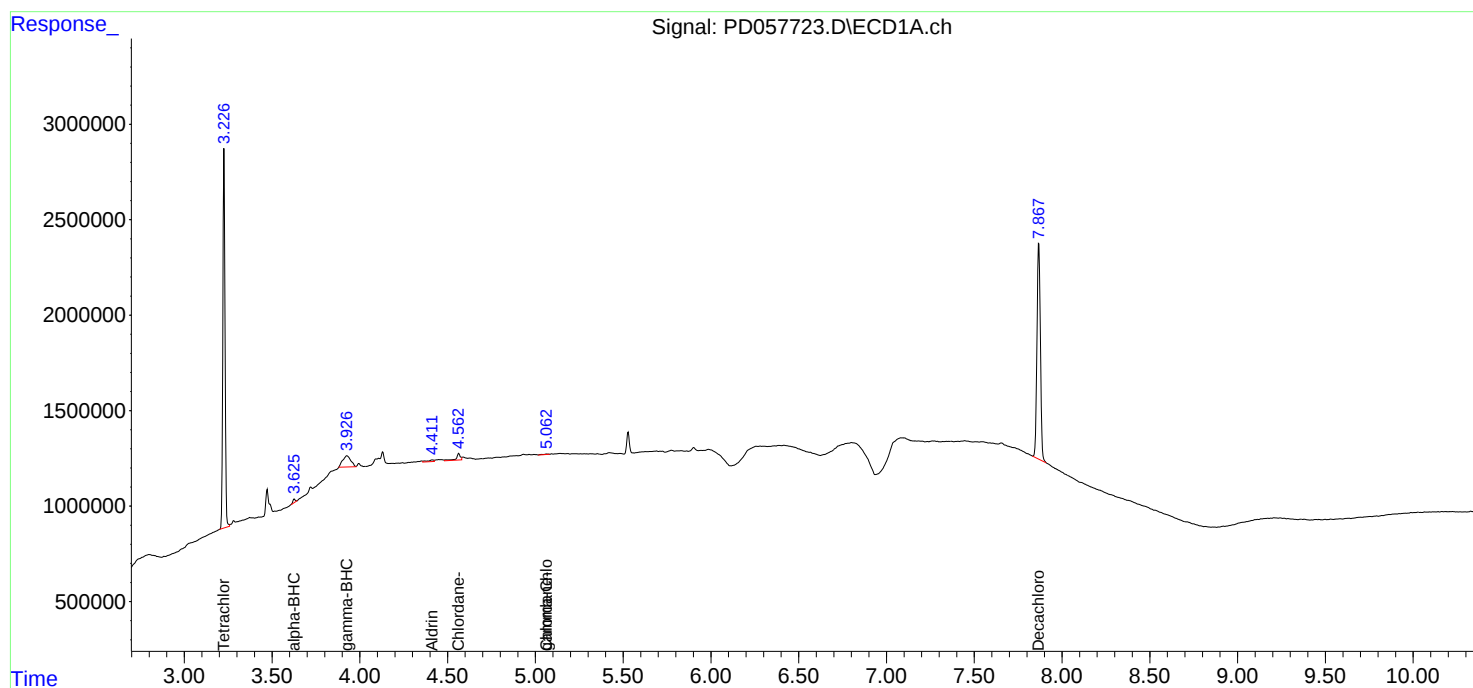


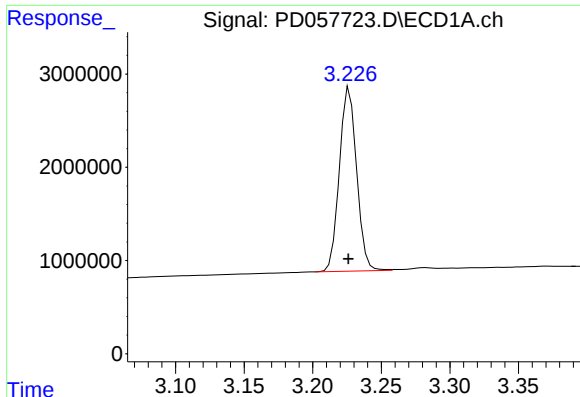

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 17292215
Conc: 24.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

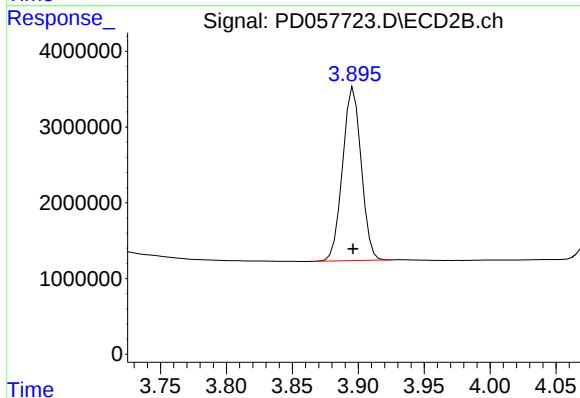


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 22450986
Conc: 28.62 ng/ml

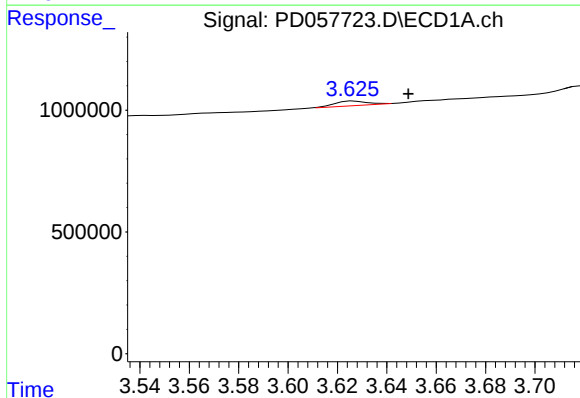


#2 alpha-BHC

R.T.: 3.627 min
Delta R.T.: -0.022 min
Response: 167473
Conc: 0.15 ng/ml

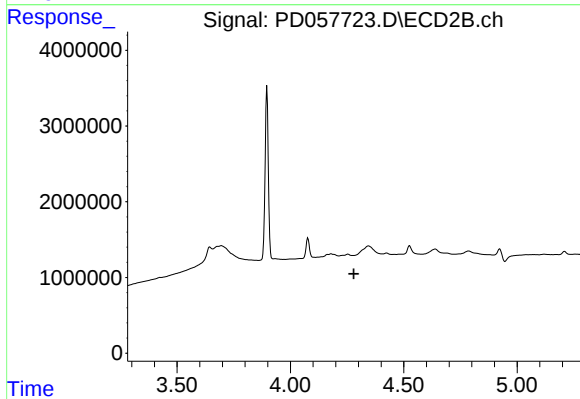

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.279 min
Response: 0
Conc: N.D.

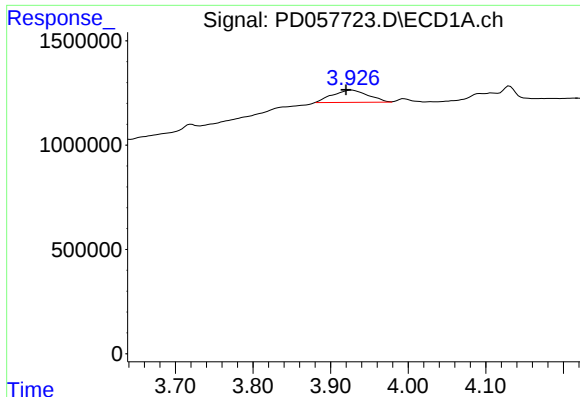

#3 gamma-BHC (Lindane)


R.T.: 3.927 min
Delta R.T.: 0.007 min
Response: 1866468
Conc: 1.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

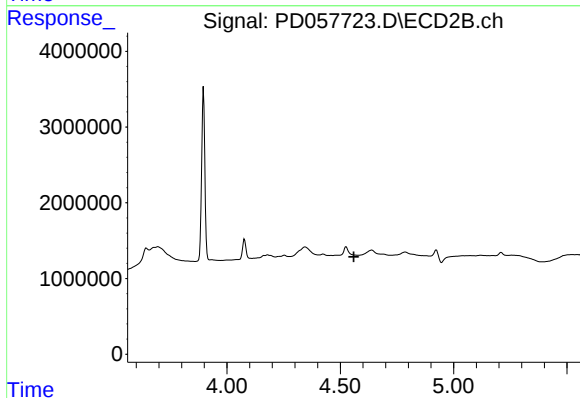


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

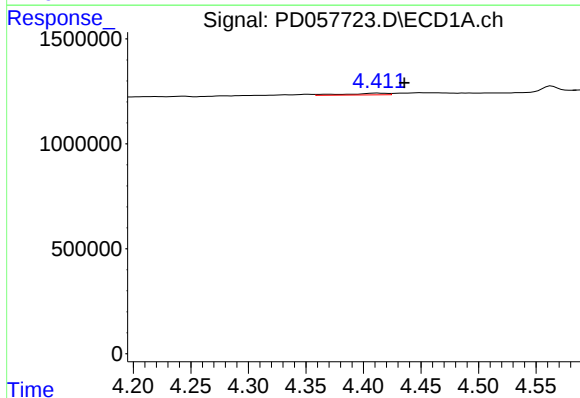


#5 Aldrin

R.T.: 4.413 min
Delta R.T.: -0.023 min
Response: 215379
Conc: 0.22 ng/ml

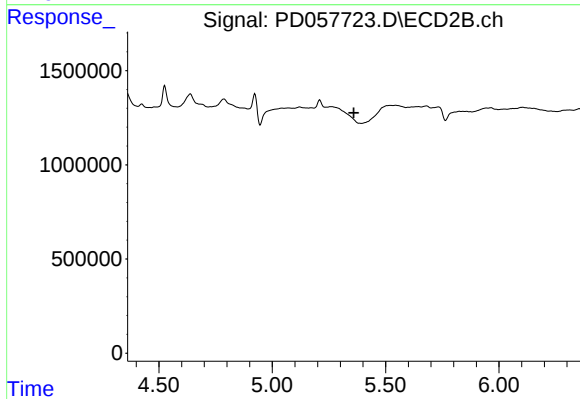

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.360 min
Response: 0
Conc: N.D.

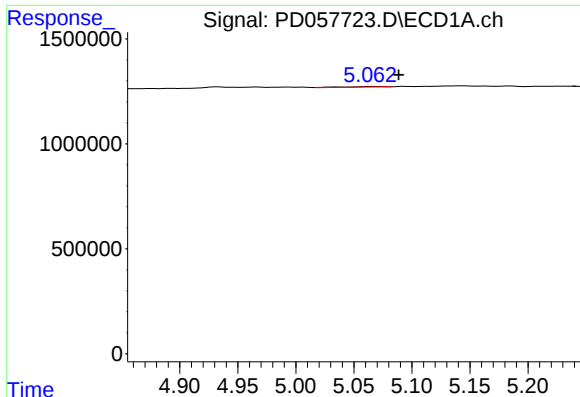

#10 gamma-Chlordane


R.T.: 5.064 min
Delta R.T.: -0.025 min
Response: 61598
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

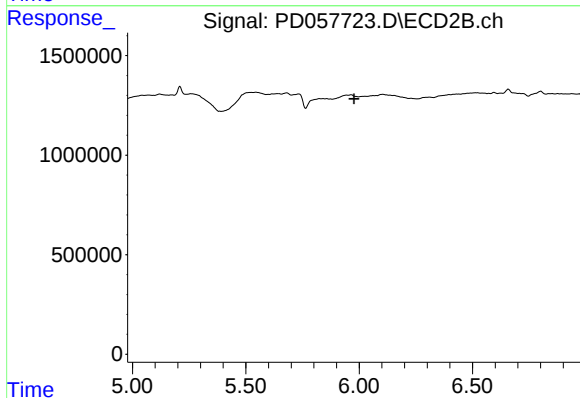


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

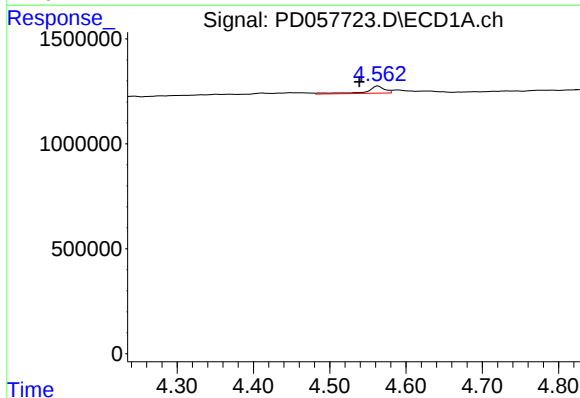


#24 Chlordane-2

R.T.: 4.564 min
Delta R.T.: 0.025 min
Response: 578166
Conc: 20.17 ng/ml

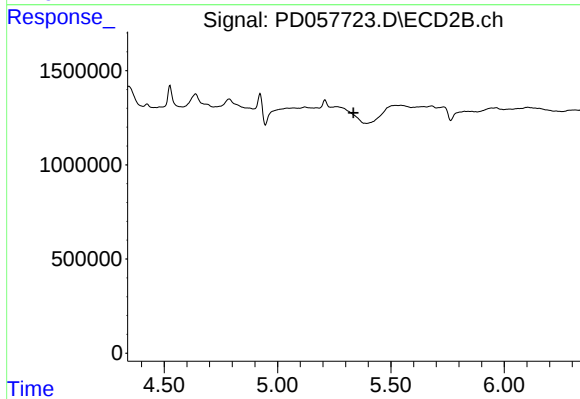

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

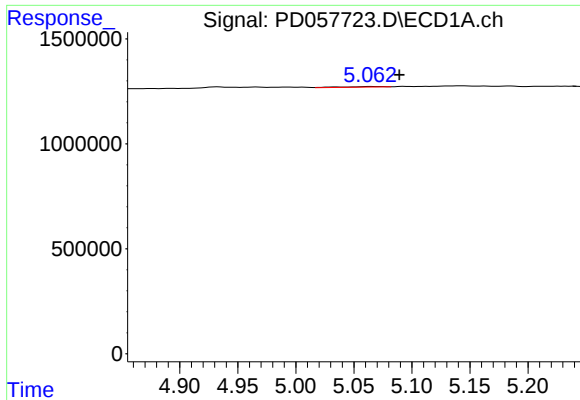

#25 Chlordane-3


R.T.: 5.064 min
Delta R.T.: -0.025 min
Response: 61598
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

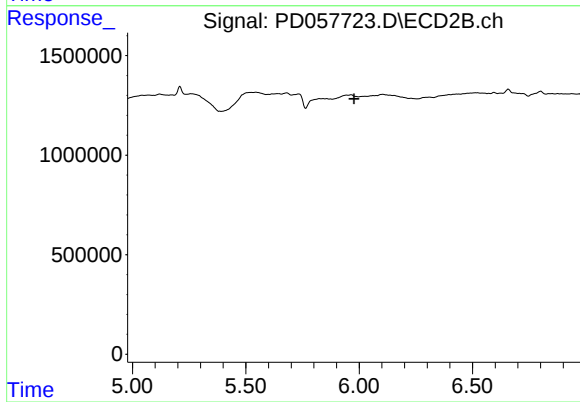


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

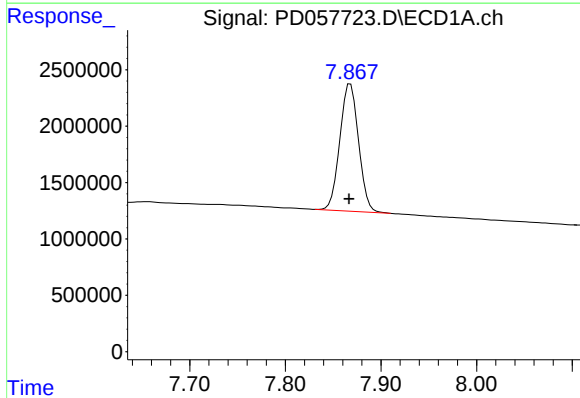

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.001 min
Response: 15371422
Conc: 20.19 ng/ml

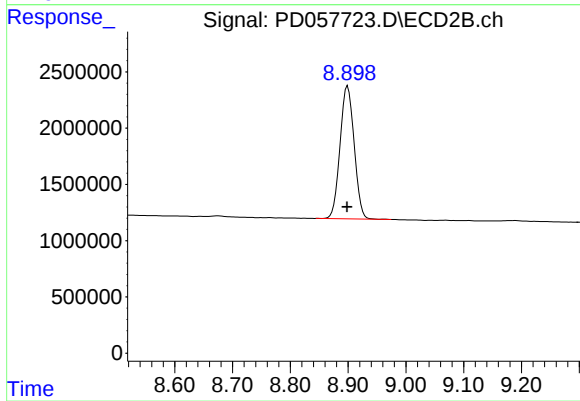

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.001 min
Response: 19990111
Conc: 22.73 ng/ml