

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
 Data File : PD057732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 20:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 00:56:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.247f	3.896	16300381	21214369	22.830	27.040
28)	SA Decachlor...	7.886f	8.899	16770729	21819550	22.027	24.808
Target Compounds							
7)	B delta-BHC	4.367	0.000	83632	0	0.081	N.D. #
8)	B Heptachlo...	4.855	0.000	10765	0	0.013	N.D. #
14)	MA Endrin	5.711f	0.000	365148	0	0.502	N.D. #
16)	A 4,4'-DDD	5.799f	0.000	125196	0	0.219	N.D. #
24)	Chlordane-2	4.533	0.000	19271	0	0.672	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
Data File : PD057732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 20:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 00:56:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

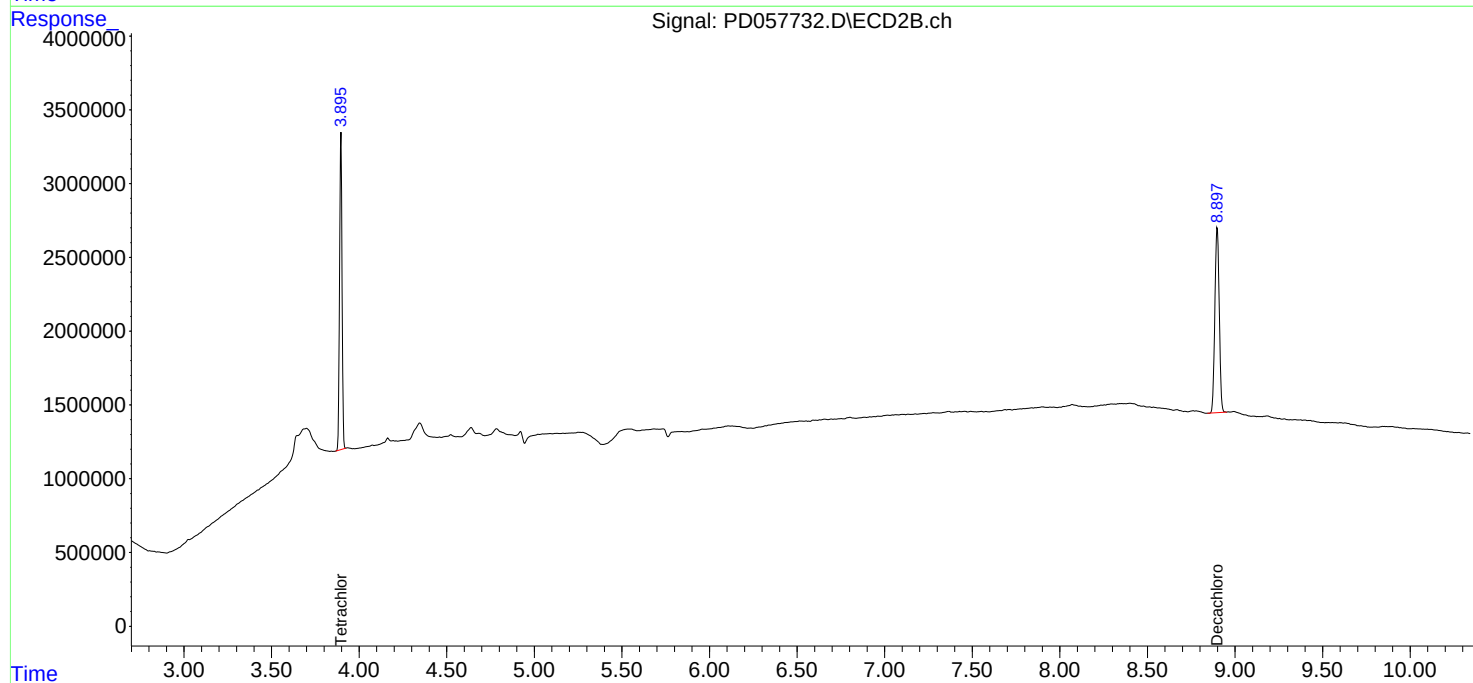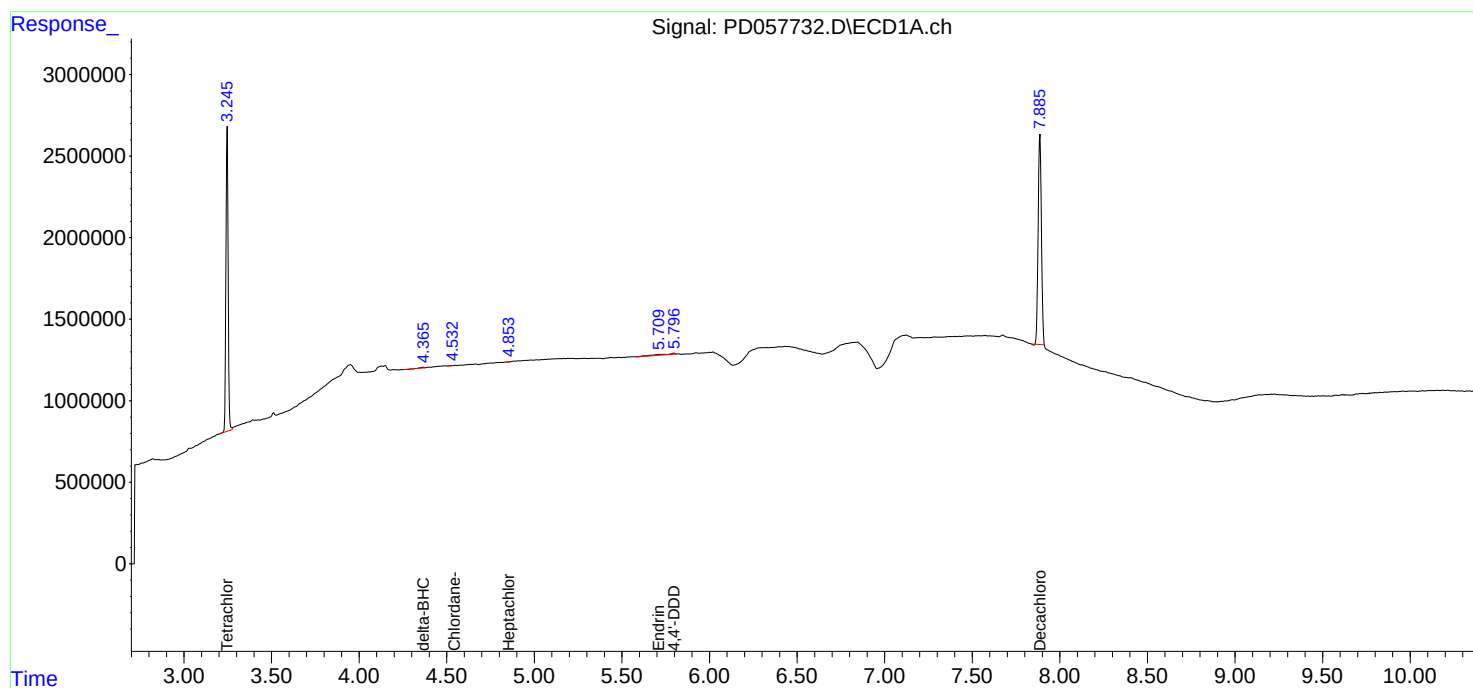


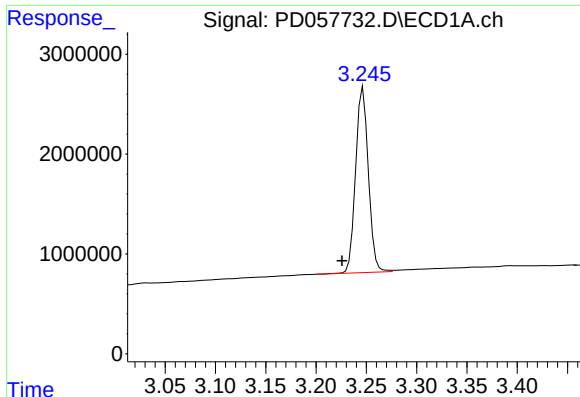

#1 Tetrachloro-m-xylene


R.T.: 3.247 min
Delta R.T.: 0.021 min
Response: 16300381
Conc: 22.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

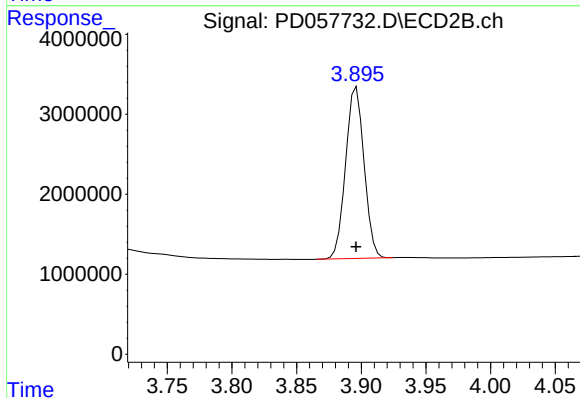


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 21214369
Conc: 27.04 ng/ml

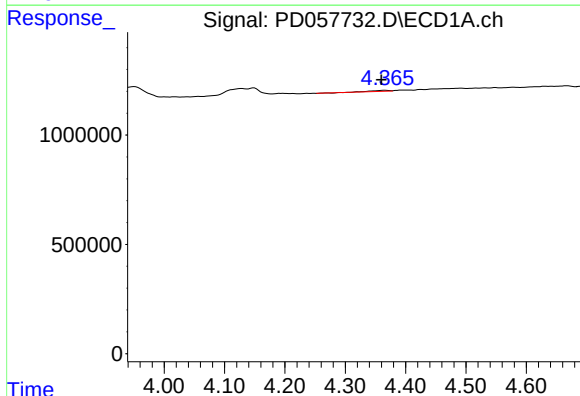


#7 delta-BHC

R.T.: 4.367 min
Delta R.T.: 0.006 min
Response: 83632
Conc: 0.08 ng/ml

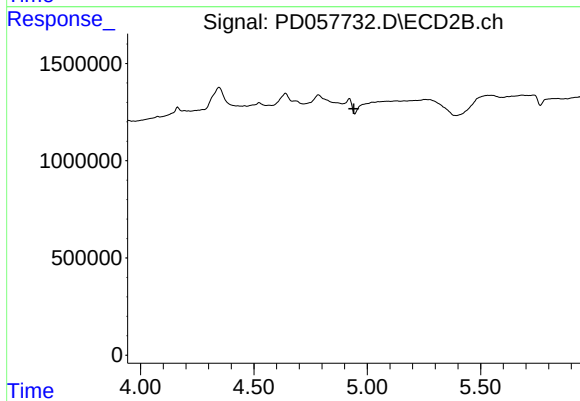

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

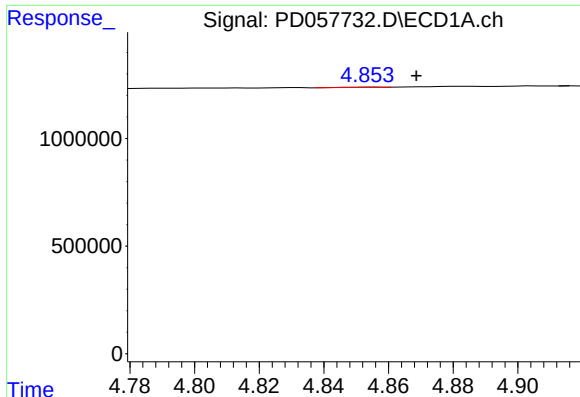

#8 Heptachlor epoxide


R.T.: 4.855 min
Delta R.T.: -0.014 min
Response: 10765
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

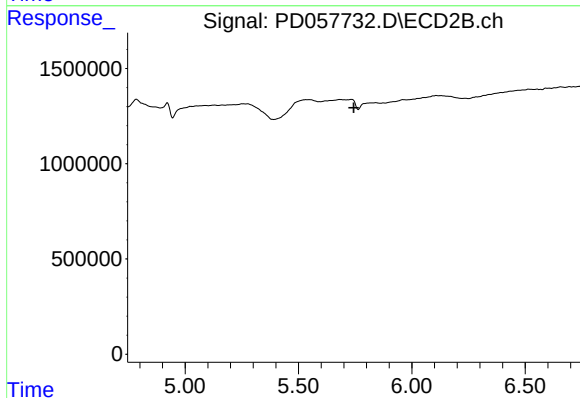


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

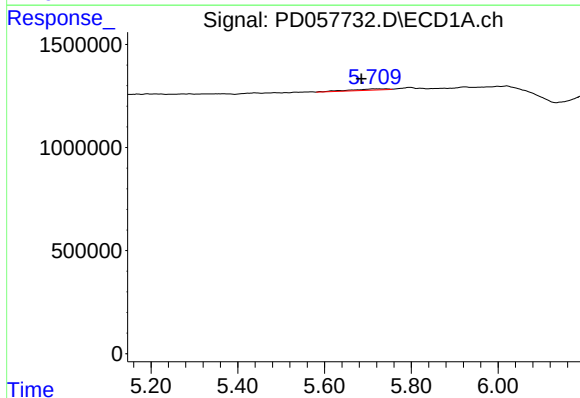


#14 Endrin

R.T.: 5.711 min
Delta R.T.: 0.026 min
Response: 365148
Conc: 0.50 ng/ml

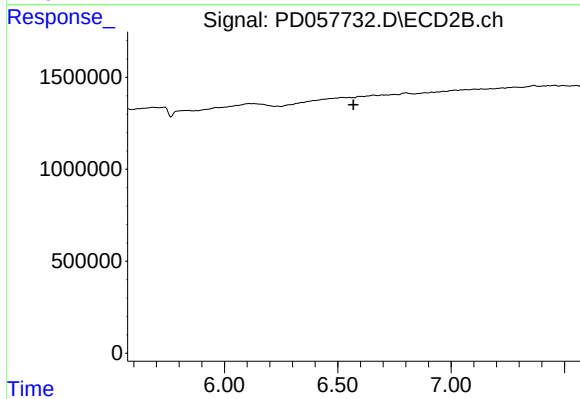

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

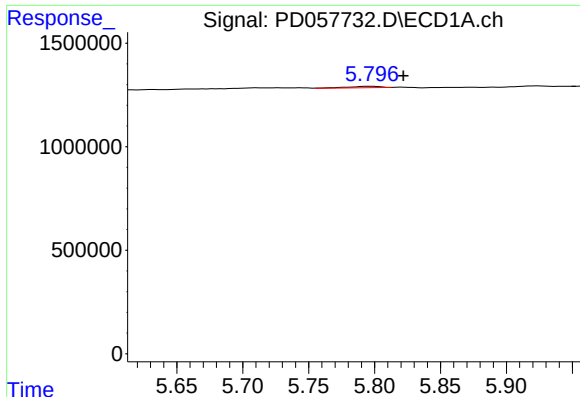

#16 4,4'-DDD


R.T.: 5.799 min
Delta R.T.: -0.023 min
Response: 125196
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

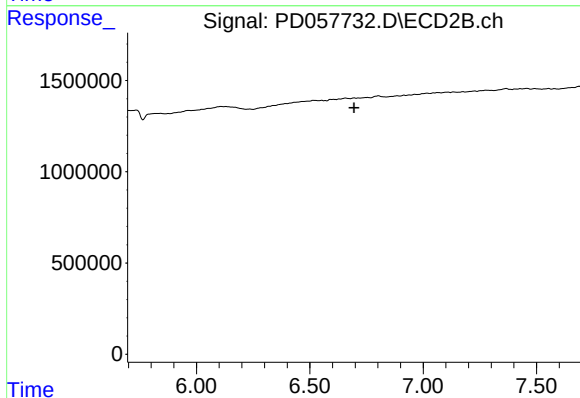


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

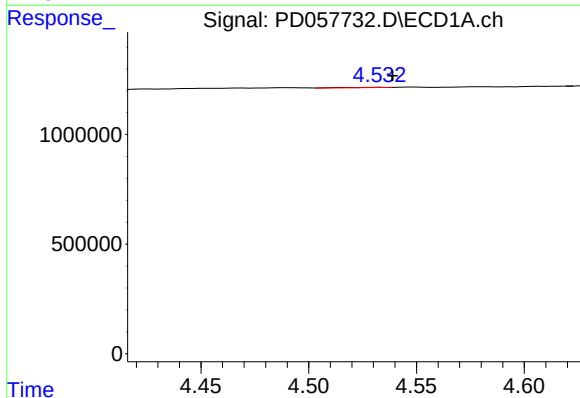


#24 Chlordane-2

R.T.: 4.533 min
Delta R.T.: -0.006 min
Response: 19271
Conc: 0.67 ng/ml

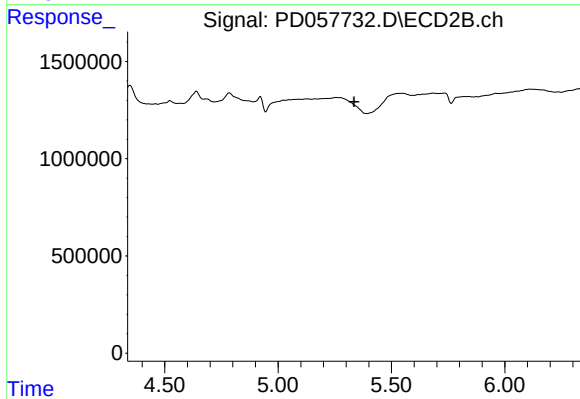

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

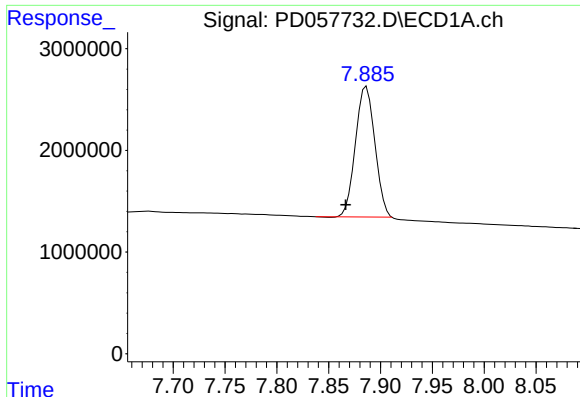

#28 Decachlorobiphenyl

R.T.: 7.886 min
Delta R.T.: 0.020 min
Response: 16770729
Conc: 22.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

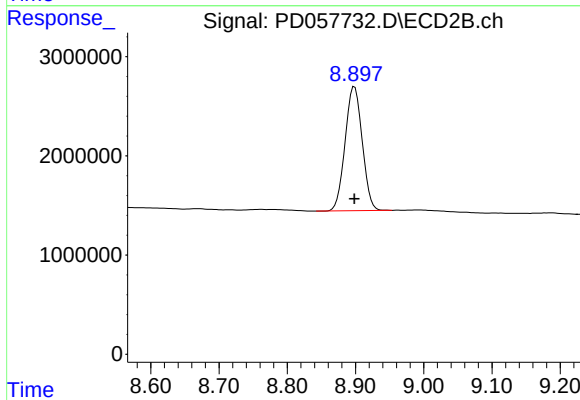

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 21819550
Conc: 24.81 ng/ml