

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
 Data File : PD057735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 21:27
 Operator : AJ\MA
 Sample : L2146-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 00:57:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	15463640	21304065	21.658	27.155 #
28)	SA Decachlor...	7.868	8.900	14093943	18275726	18.511	20.779
Target Compounds							
2)	A alpha-BHC	3.651	0.000	81063	0	0.074	N.D. #
3)	MA gamma-BHC...	3.927	0.000	2396866	0	2.226	N.D. #
8)	B Heptachlo...	4.867	0.000	353261	0	0.417	N.D. #
10)	B gamma-Chl...	5.102	0.000	303544	0	0.331	N.D. #
11)	B alpha-Chl...	5.142	0.000	228103	0	0.249	N.D. #
13)	MA Dieldrin	5.424	0.000	654028	0	0.838	N.D. #
14)	MA Endrin	5.704f	0.000	559588	0	0.770	N.D. #
16)	A 4,4'-DDD	5.839f	0.000	104704	0	0.184	N.D. #
25)	Chlordane-3	5.102	0.000	303544	0	3.458	N.D. #
26)	Chlordane-4	5.142	0.000	228103	0	2.821	N.D. #
27)	Chlordane-5	5.990f	0.000	77117	0	2.893	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040320\
Data File : PD057735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 21:27
Operator : AJ\MA
Sample : L2146-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 00:57:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

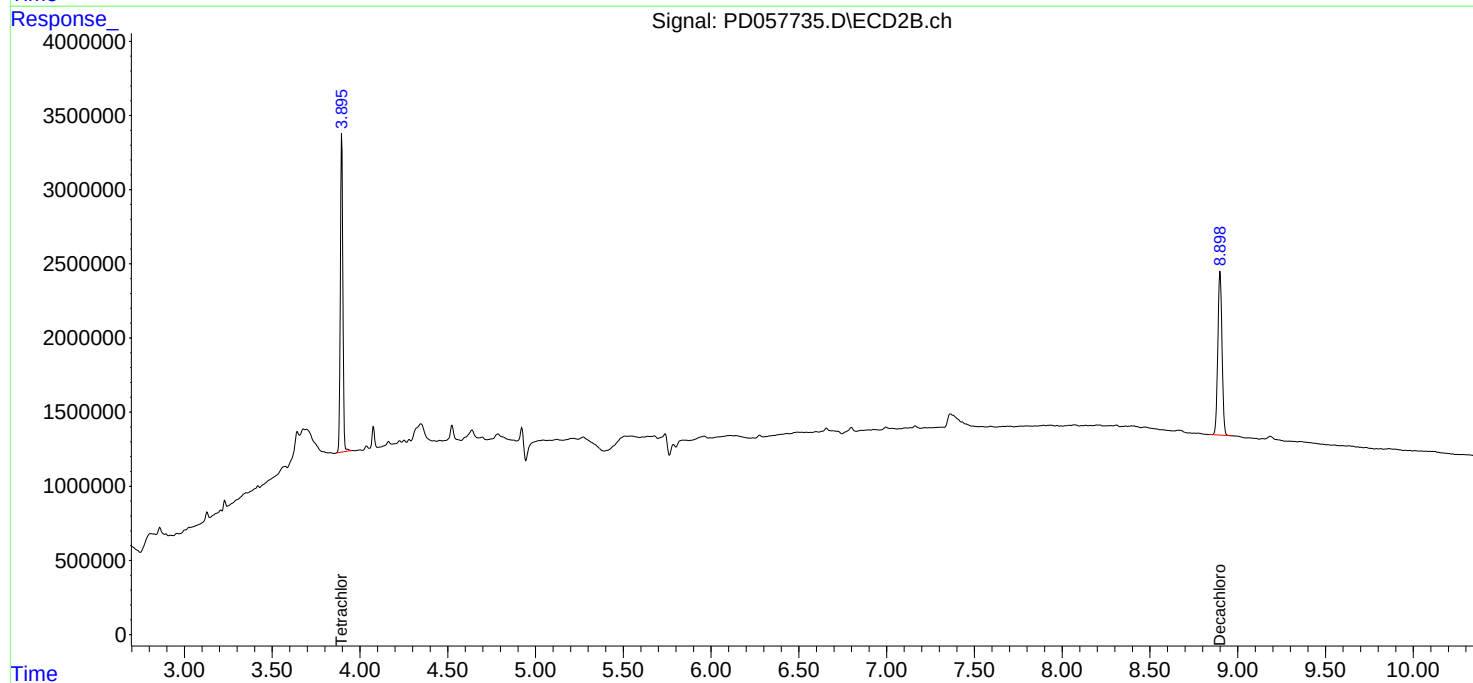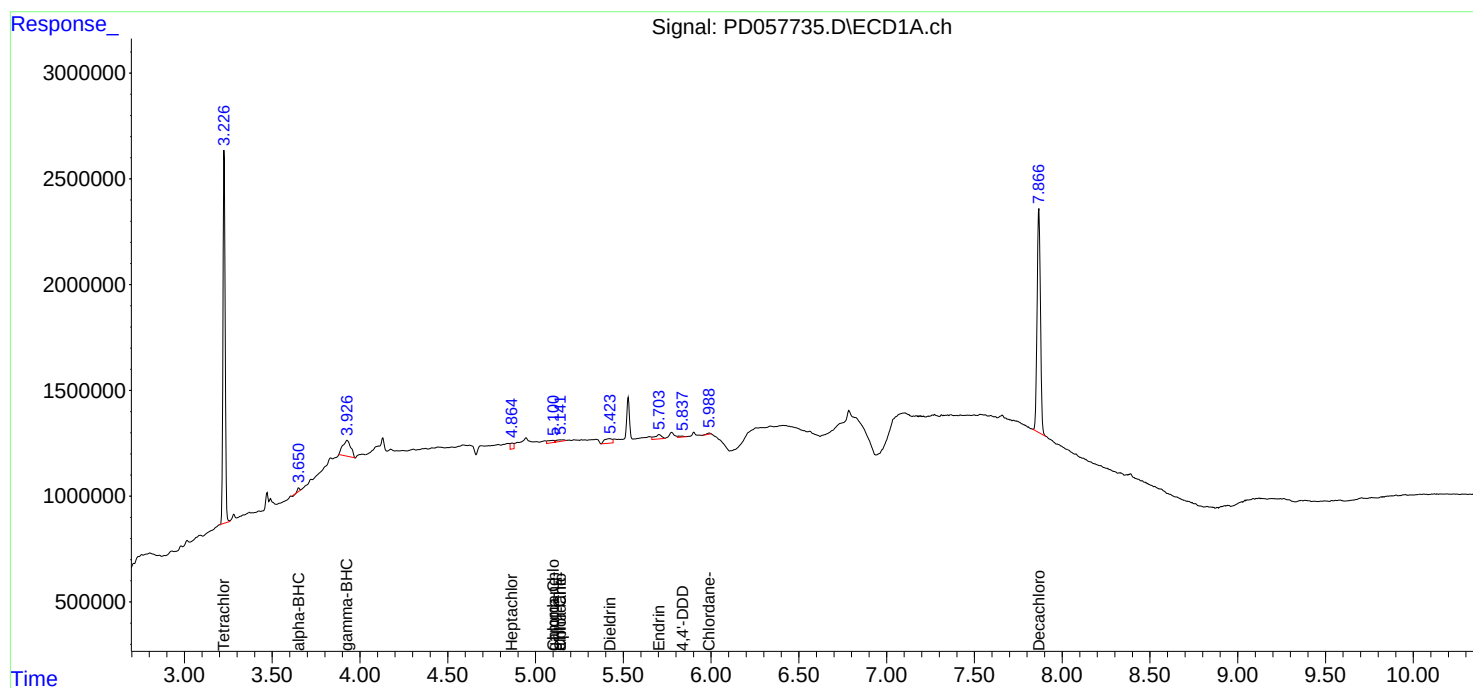


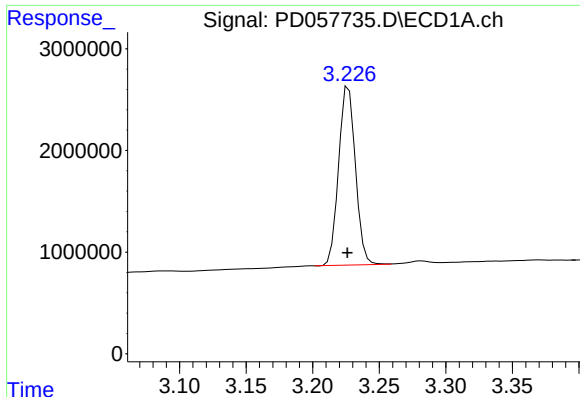

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.001 min
Response: 15463640
Conc: 21.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

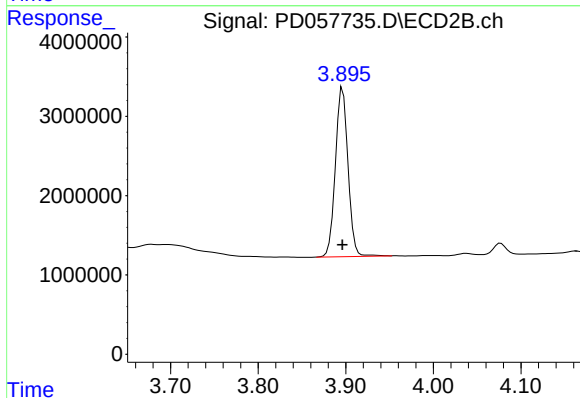


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 21304065
Conc: 27.15 ng/ml

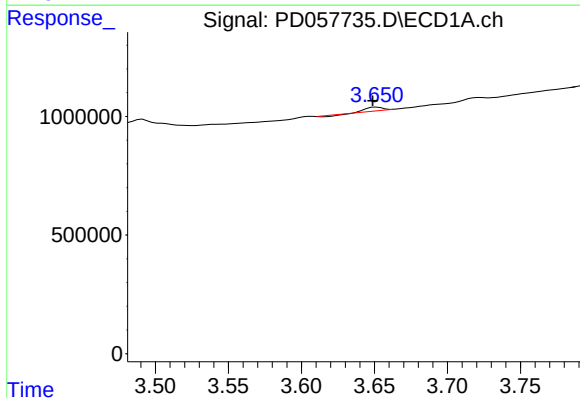


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.003 min
Response: 81063
Conc: 0.07 ng/ml

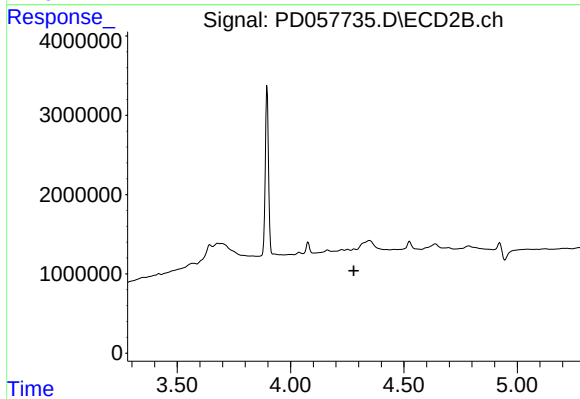

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.279 min
Response: 0
Conc: N.D.

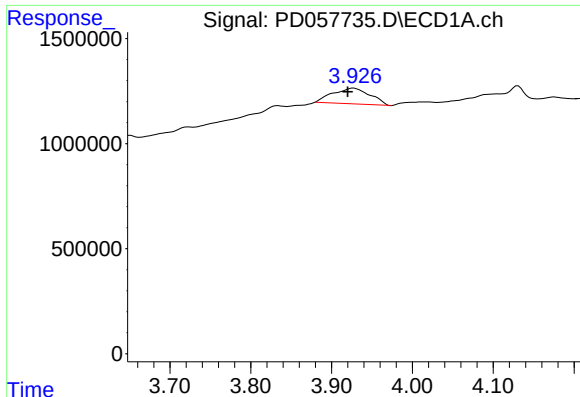

#3 gamma-BHC (Lindane)


R.T.: 3.927 min
Delta R.T.: 0.007 min
Response: 2396866
Conc: 2.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

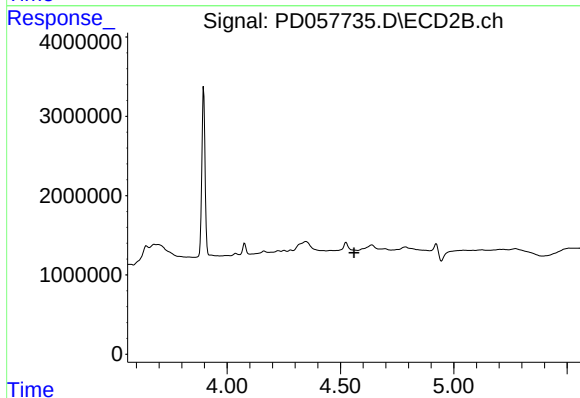


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

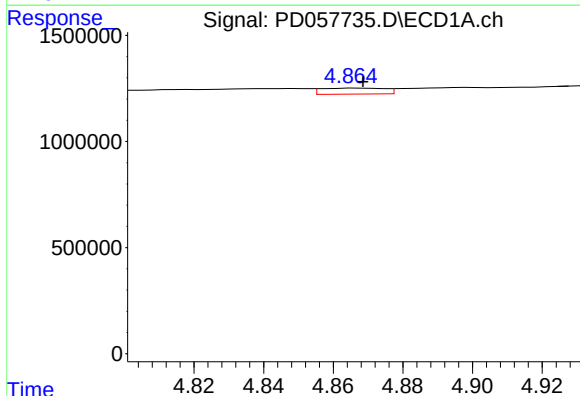


#8 Heptachlor epoxide

R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 353261
Conc: 0.42 ng/ml

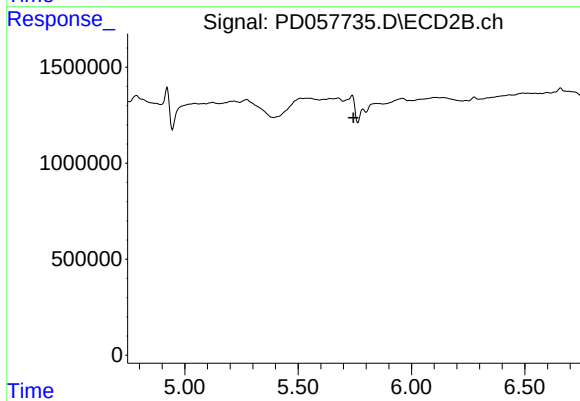

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

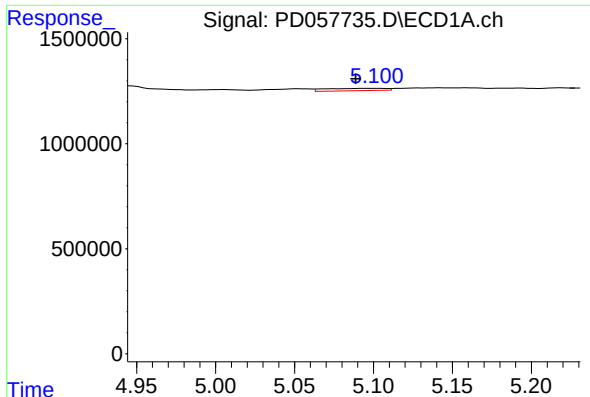

#10 gamma-Chlordane


R.T.: 5.102 min
Delta R.T.: 0.013 min
Response: 303544
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

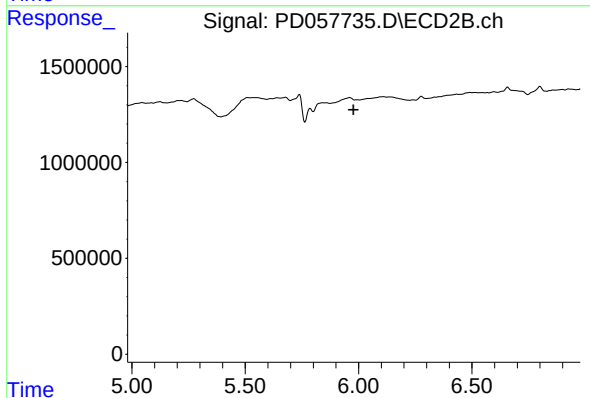


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

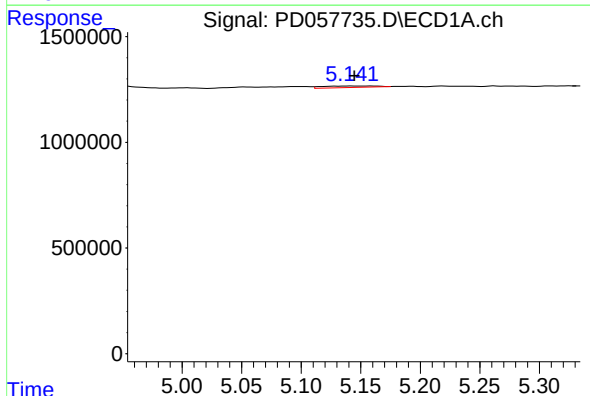


#11 alpha-Chlordane

R.T.: 5.142 min
Delta R.T.: -0.003 min
Response: 228103
Conc: 0.25 ng/ml

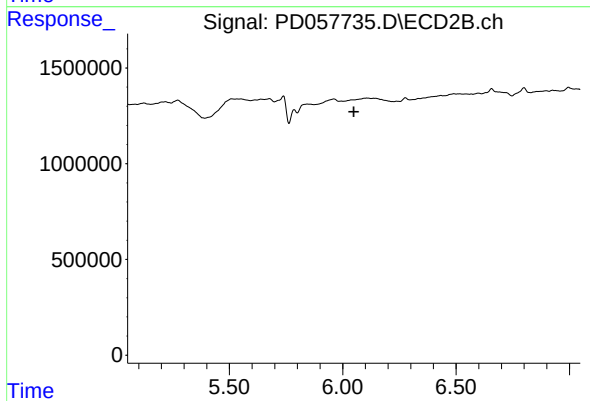

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

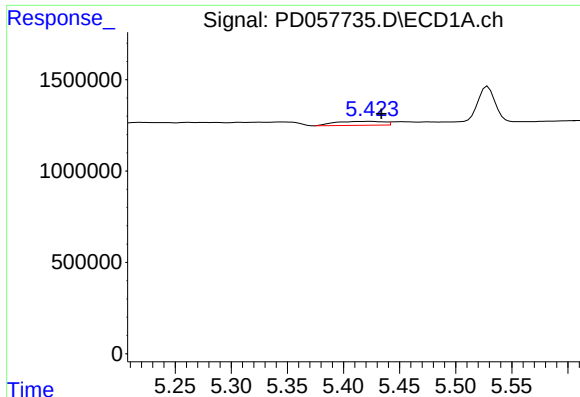

#13 Dieldrin


R.T.: 5.424 min
Delta R.T.: -0.010 min
Response: 654028
Conc: 0.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

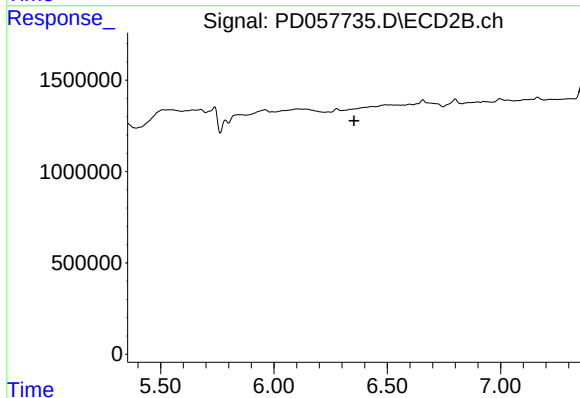


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

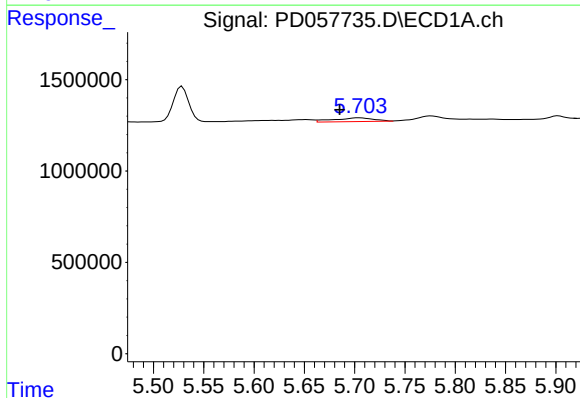


#14 Endrin

R.T.: 5.704 min
Delta R.T.: 0.019 min
Response: 559588
Conc: 0.77 ng/ml

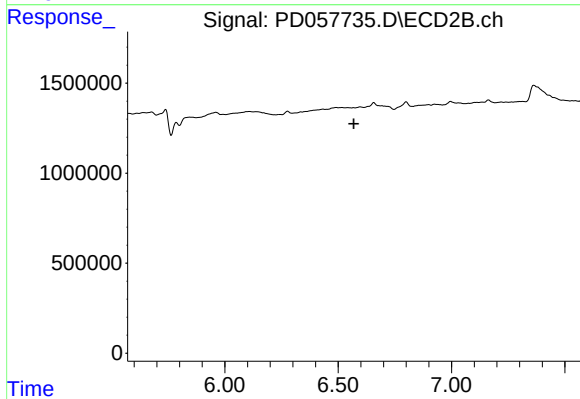

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

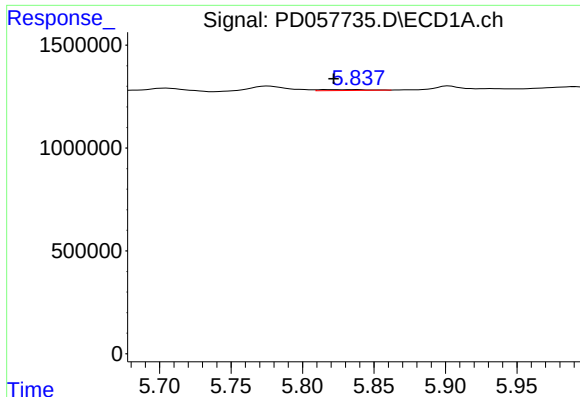

#16 4,4'-DDD


R.T.: 5.839 min
Delta R.T.: 0.017 min
Response: 104704
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

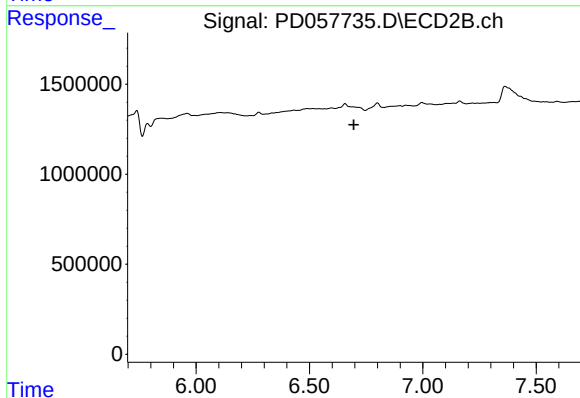


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

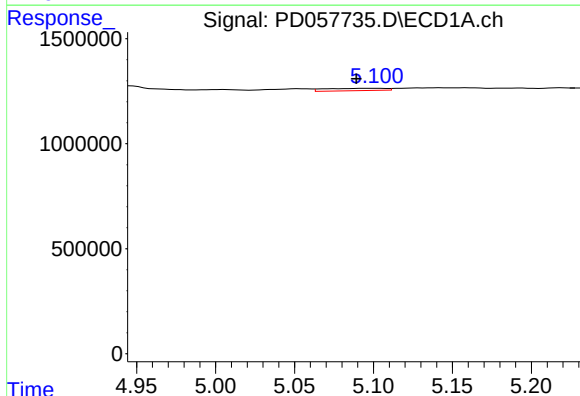


#25 Chlordane-3

R.T.: 5.102 min
Delta R.T.: 0.013 min
Response: 303544
Conc: 3.46 ng/ml

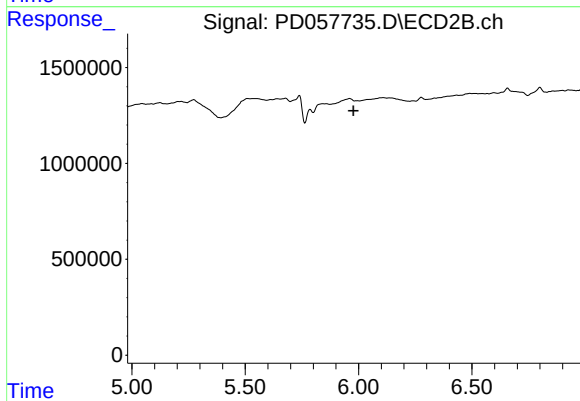

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

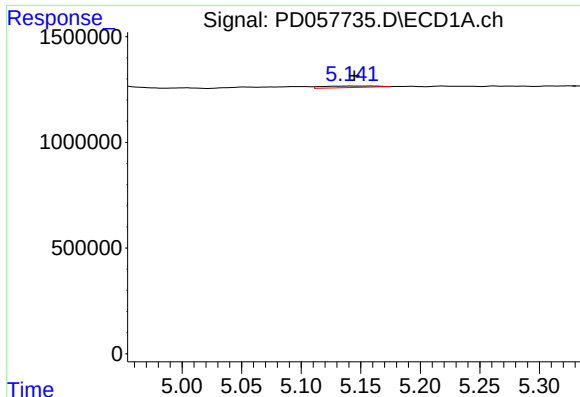

#26 Chlordane-4


R.T.: 5.142 min
Delta R.T.: -0.003 min
Response: 228103
Conc: 2.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

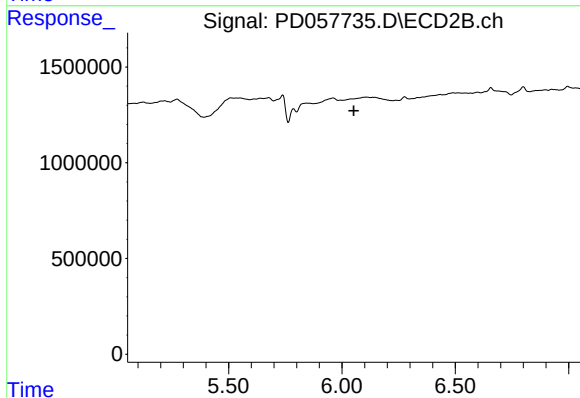


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

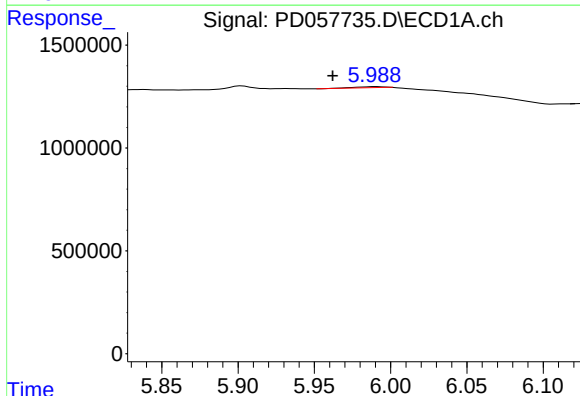


#27 Chlordane-5

R.T.: 5.990 min
Delta R.T.: 0.028 min
Response: 77117
Conc: 2.89 ng/ml

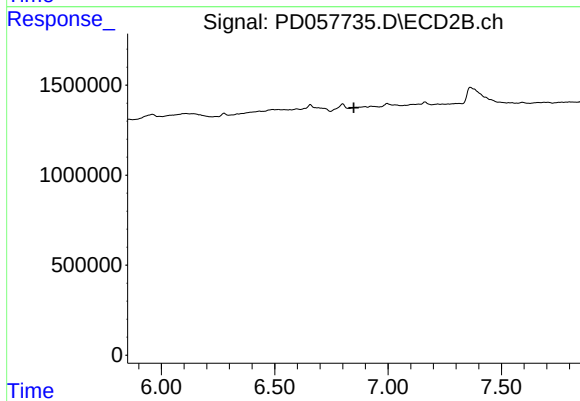

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.849 min
Response: 0
Conc: N.D.

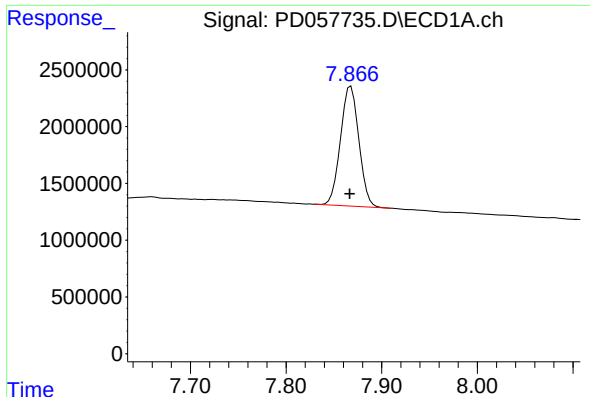

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.001 min
Response: 14093943
Conc: 18.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

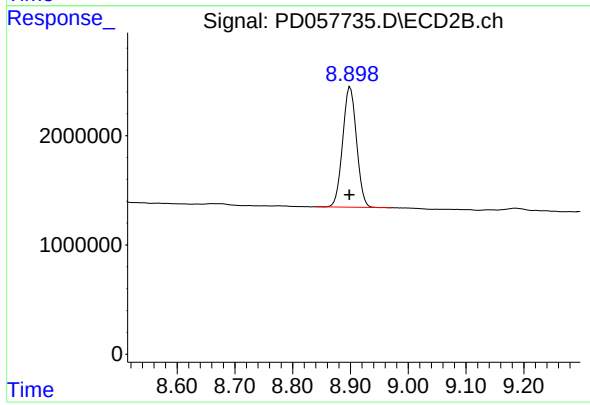

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.001 min
Response: 18275726
Conc: 20.78 ng/ml