

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 18:09
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:28:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	5193914	49819750	5.435	5.049
27)	SA Decachlor...	8.257	9.040	15375952	104.5E6	11.753	11.595
Target Compounds							
2)	A alpha-BHC	3.924	4.370	6973716	89921278	5.053	5.713
3)	MA gamma-BHC...	4.209	4.654	7154638	79989736	5.312	5.698
4)	MA Heptachlor	4.513	5.162	7154657	79945667	5.138	5.833
9)	A Endosulfan I	5.547	6.210	6514104	65556306	5.244	5.388
13)	MA Dieldrin	5.791	6.466	13888700	139.3E6	10.128	10.654
14)	MA Endrin	6.049	6.684	11877955	113.1E6	10.183	10.593
16)	A 4,4'-DDD	6.173	6.805	10700354	112.6E6	9.997	10.915
17)	MA 4,4'-DDT	6.416	7.104	9935062	100.8E6	9.471	10.091
20)	A Methoxychlor	6.961	7.562	31448654	249.3E6	52.909	53.053


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 18:09
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:28:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

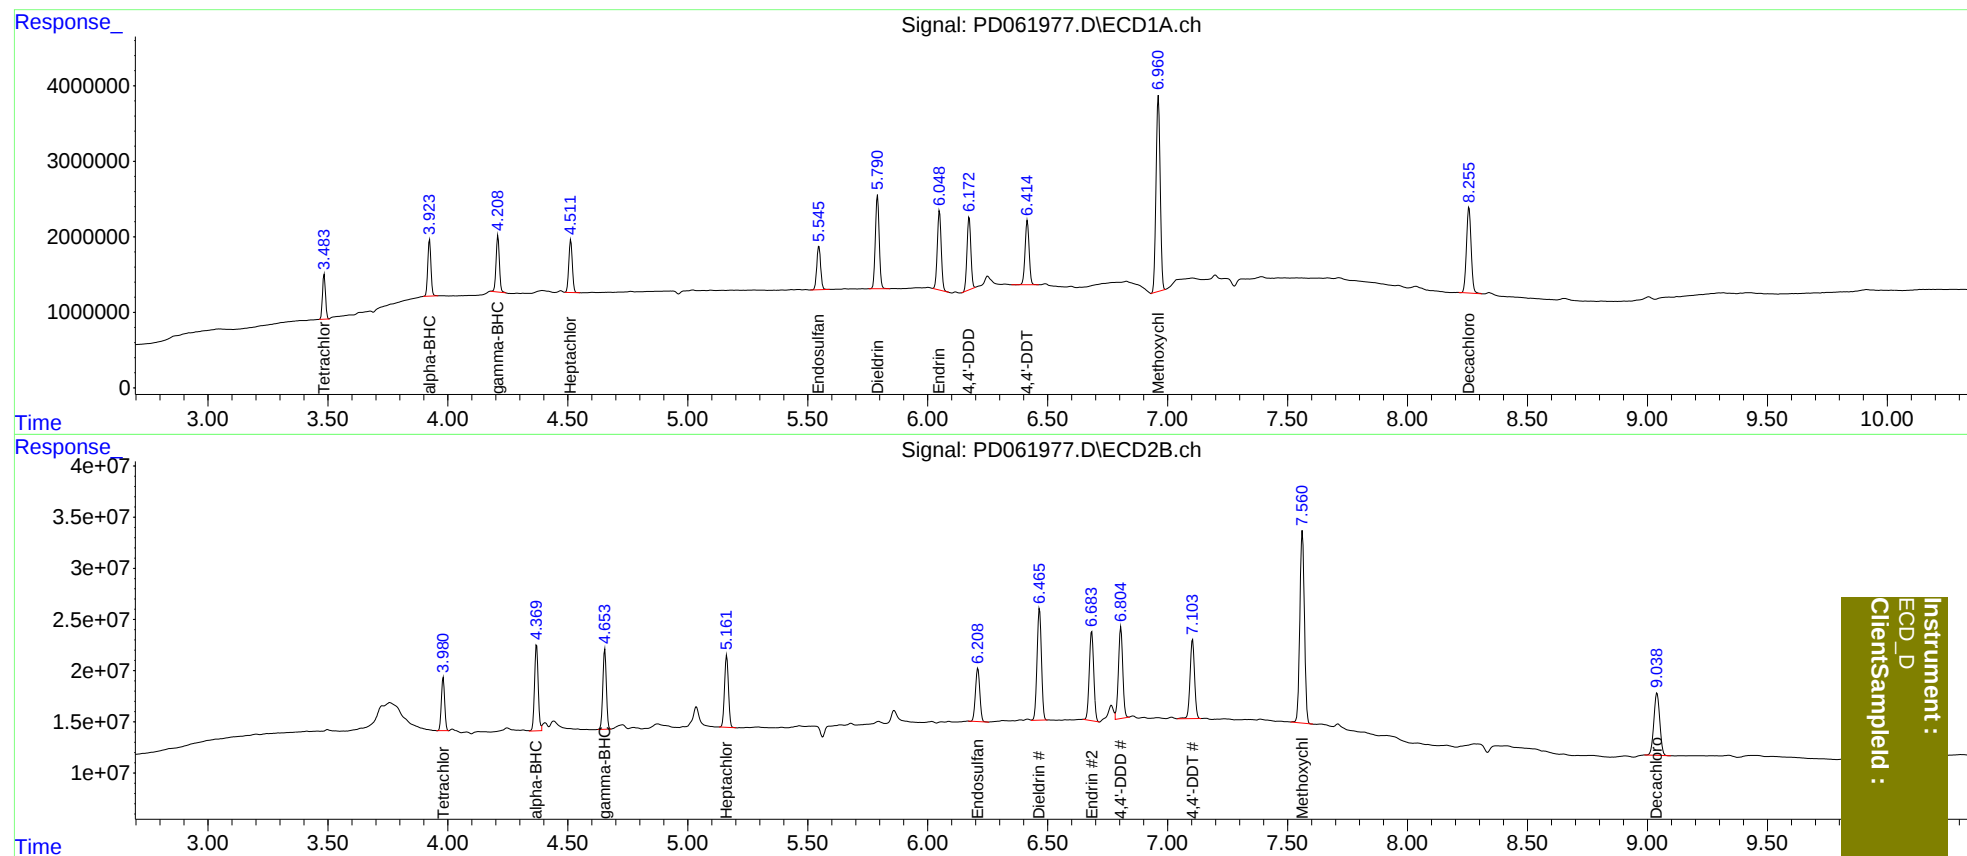


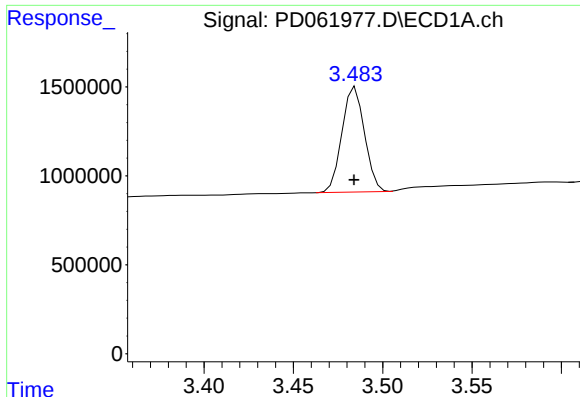

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 5193914
Conc: 5.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

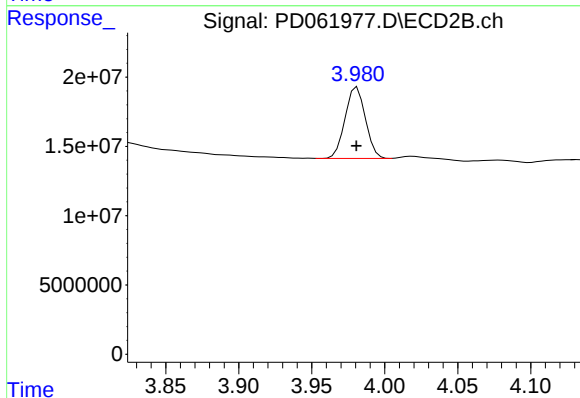


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 49819750
Conc: 5.05 ng/ml

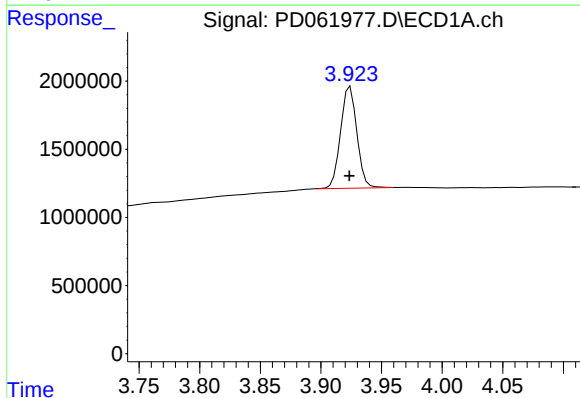


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 6973716
Conc: 5.05 ng/ml

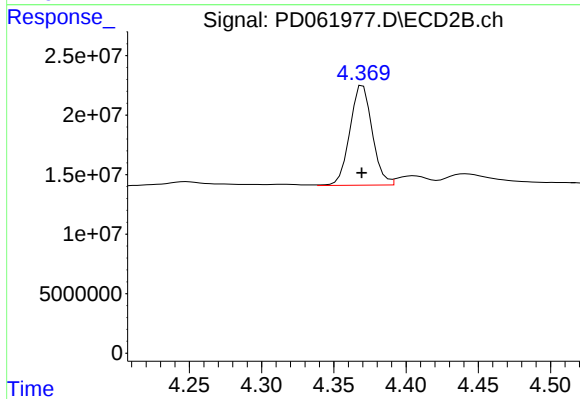

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 89921278
Conc: 5.71 ng/ml

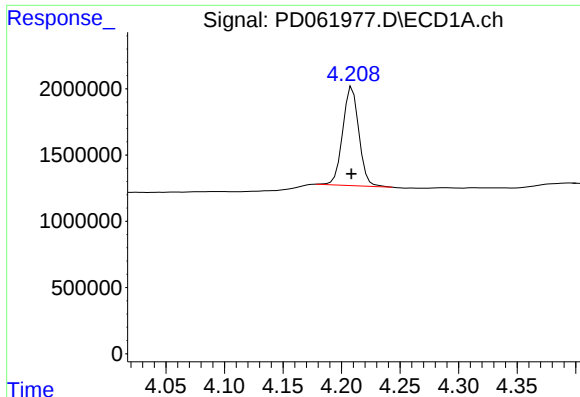

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 7154638
Conc: 5.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

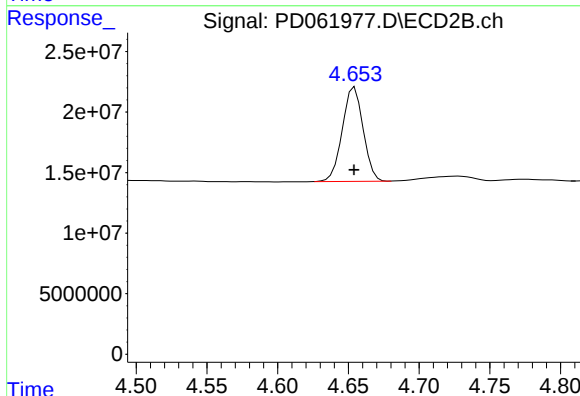


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 79989736
Conc: 5.70 ng/ml

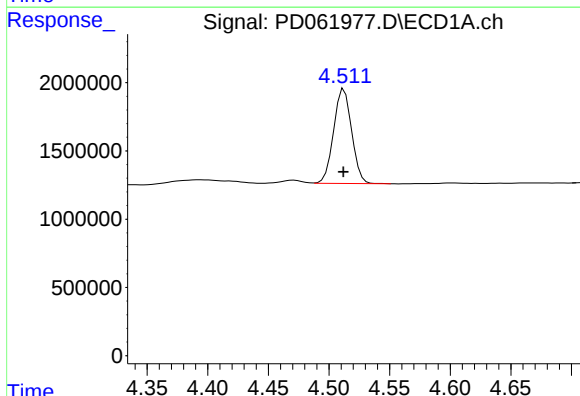


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 7154657
Conc: 5.14 ng/ml

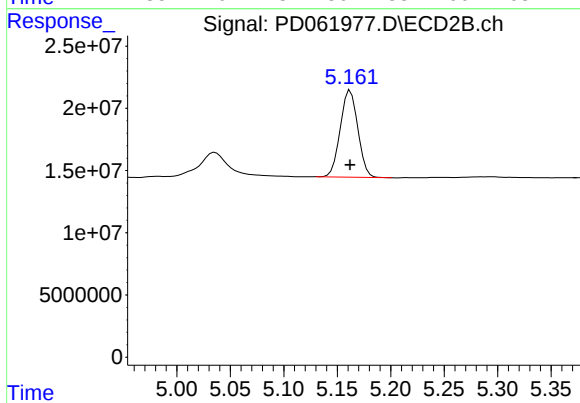

#4 Heptachlor


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 79945667
Conc: 5.83 ng/ml

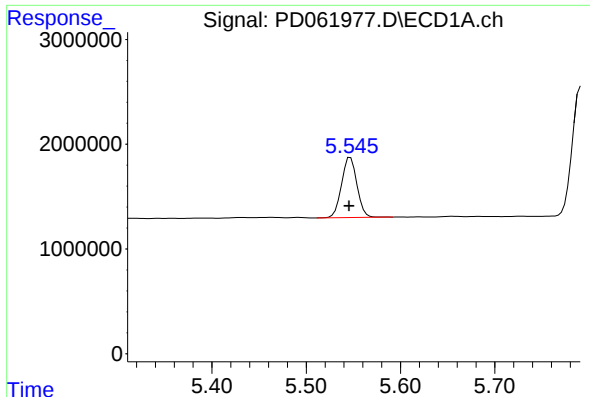

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.001 min
Response: 6514104
Conc: 5.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

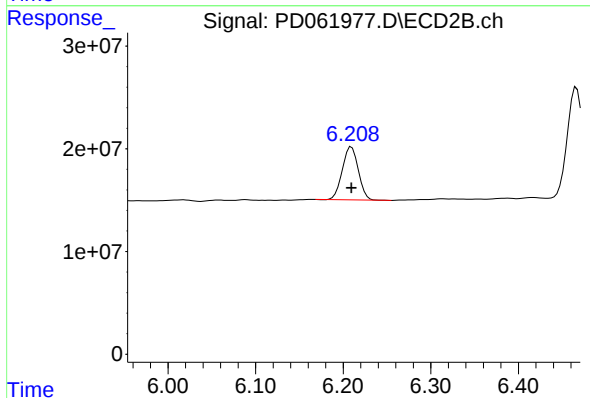


#9 Endosulfan I

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 65556306
Conc: 5.39 ng/ml

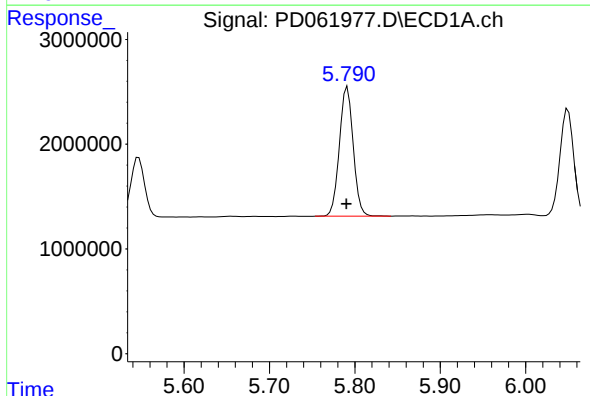


#13 Dieldrin

R.T.: 5.791 min
Delta R.T.: 0.001 min
Response: 13888700
Conc: 10.13 ng/ml

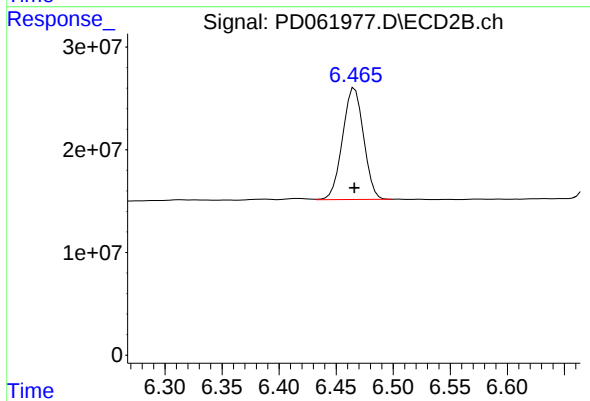

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 139289901
Conc: 10.65 ng/ml

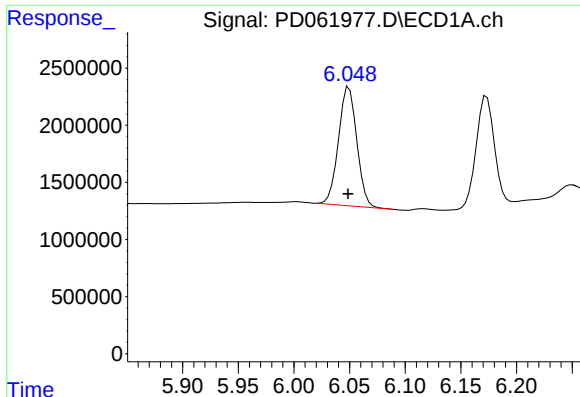

#14 Endrin


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 11877955
Conc: 10.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

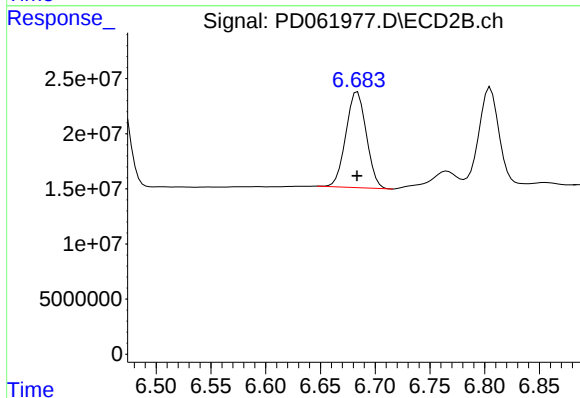


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 113087494
Conc: 10.59 ng/ml

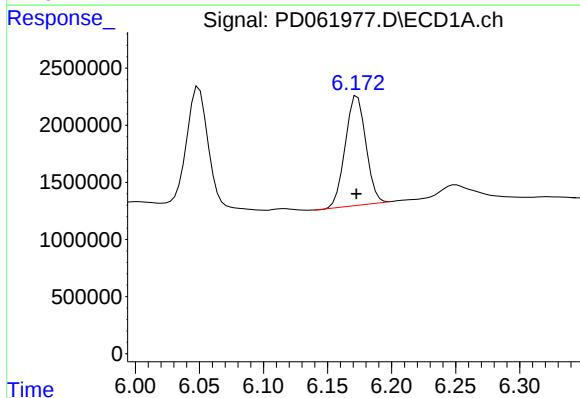


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 10700354
Conc: 10.00 ng/ml

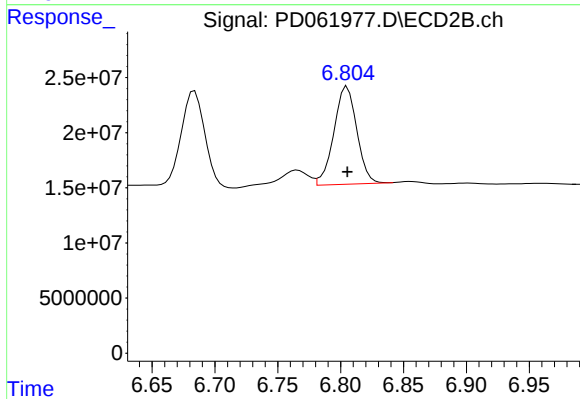

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 112632341
Conc: 10.91 ng/ml

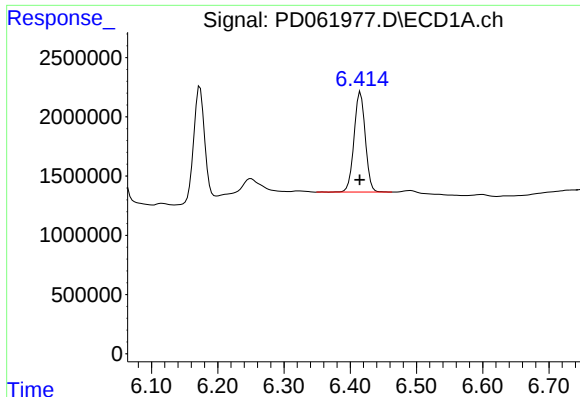

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: 0.001 min
Response: 9935062
Conc: 9.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

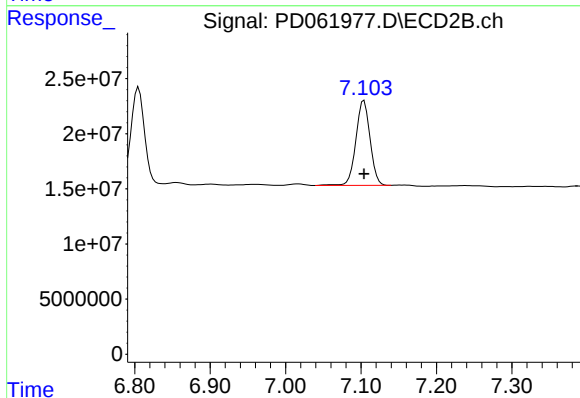


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 100812024
Conc: 10.09 ng/ml

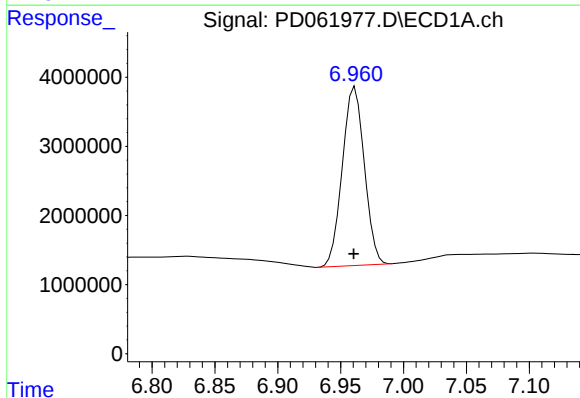


#20 Methoxychlor

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 31448654
Conc: 52.91 ng/ml

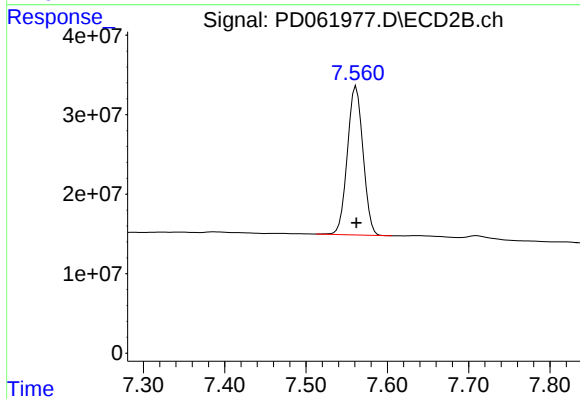

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 249329698
Conc: 53.05 ng/ml

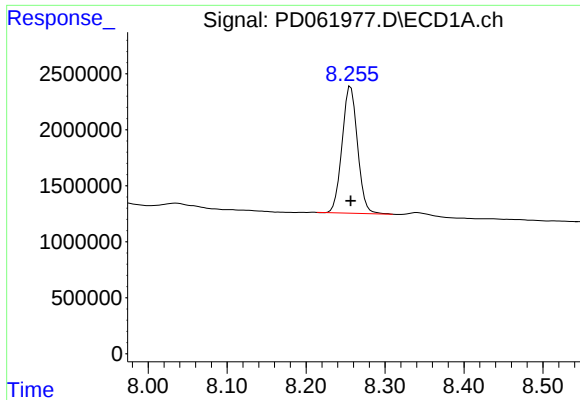

#27 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 15375952
Conc: 11.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

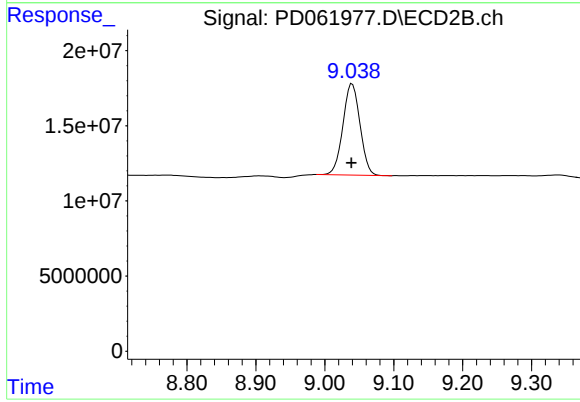

#27 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 104519633
Conc: 11.60 ng/ml