

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 18:37
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:28:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10175660	105.1E6	10.648	10.648
27)	SA Decachlor...	8.256	9.039	29297727	197.9E6	22.395	21.954
Target Compounds							
2)	A alpha-BHC	3.924	4.370	14058857	174.3E6	10.186	11.073
3)	MA gamma-BHC...	4.209	4.654	14070717	158.2E6	10.447	11.270
4)	MA Heptachlor	4.513	5.162	14482843	159.1E6	10.401	11.608
9)	A Endosulfan I	5.547	6.209	13112381	130.6E6	10.556	10.736
13)	MA Dieldrin	5.791	6.466	28304837	279.8E6	20.641	21.398
14)	MA Endrin	6.049	6.683	24113687	229.0E6	20.672	21.454
16)	A 4,4'-DDD	6.173	6.805	22089692	223.4E6	20.639	21.645
17)	MA 4,4'-DDT	6.415	7.104	21276750	206.7E6	20.284	20.694
20)	A Methoxychlor	6.961	7.562	63398488	498.9E6	106.661	106.165


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 18:37
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:28:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

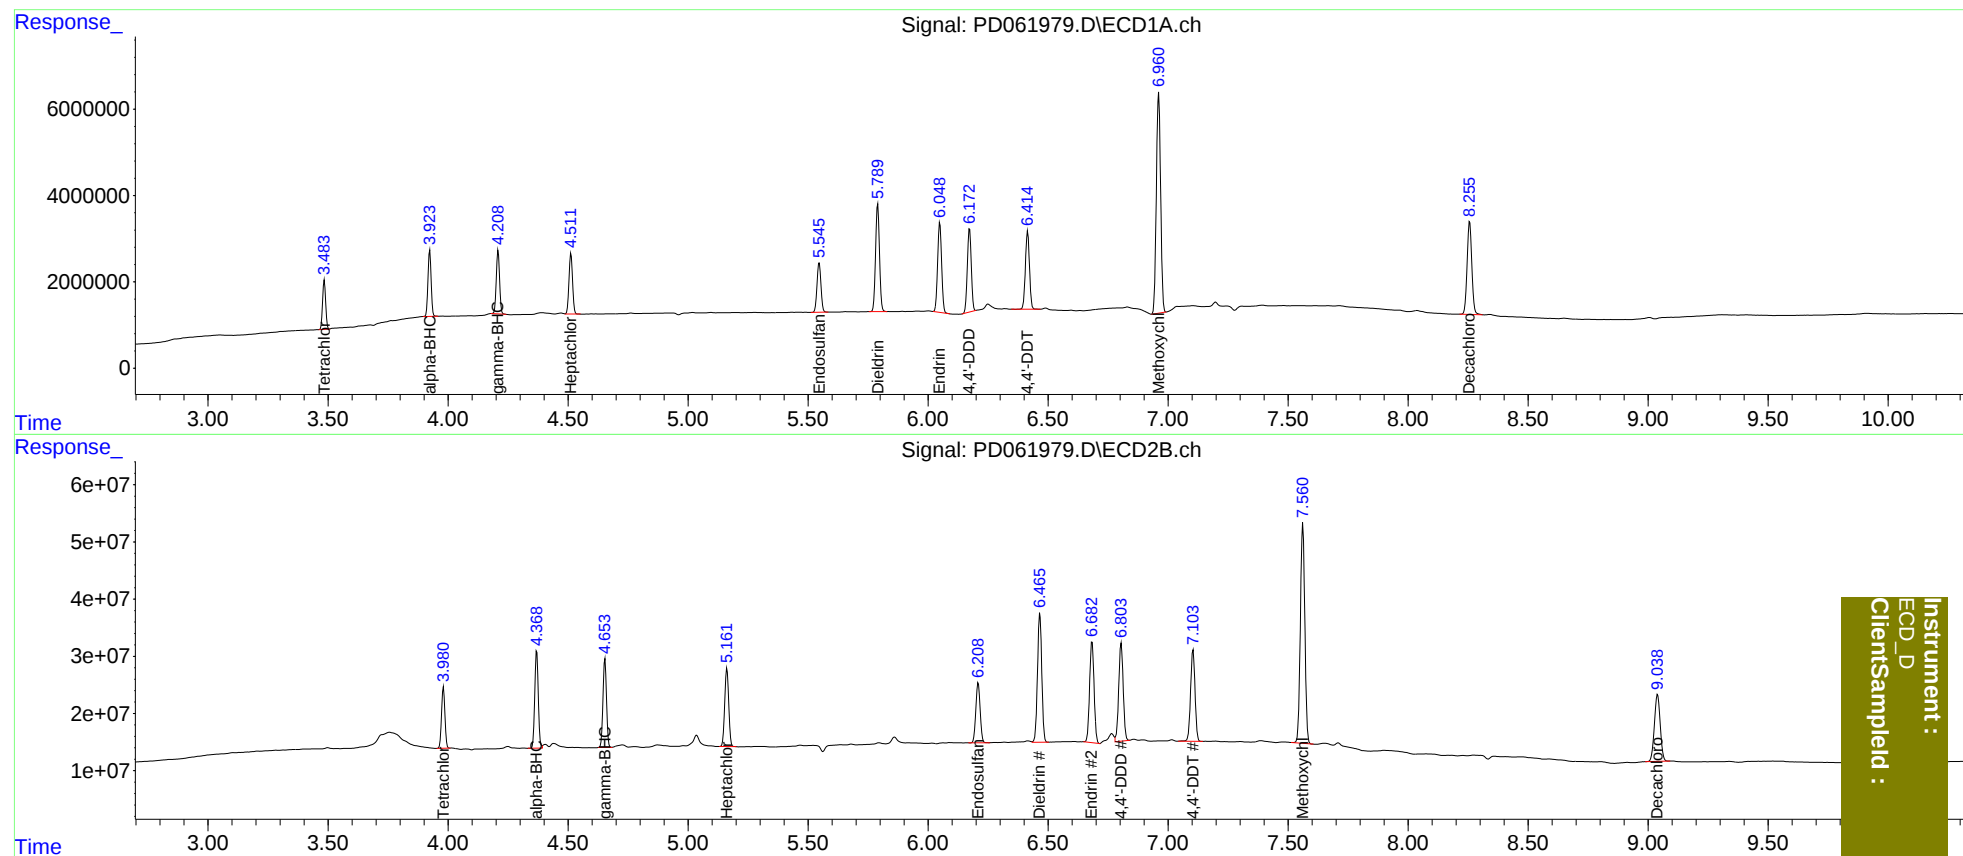


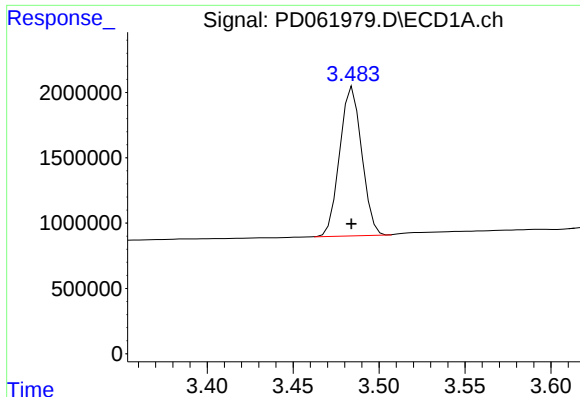

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 10175660
Conc: 10.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

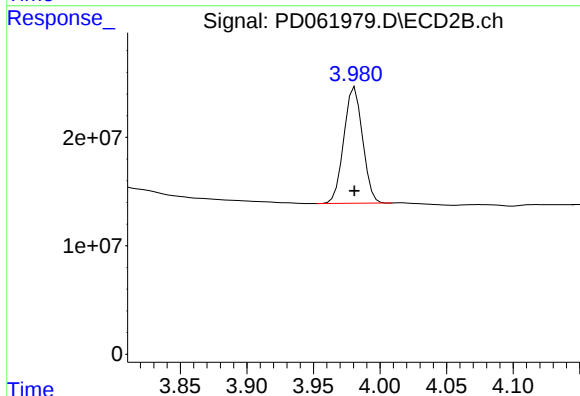


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 105071992
Conc: 10.65 ng/ml

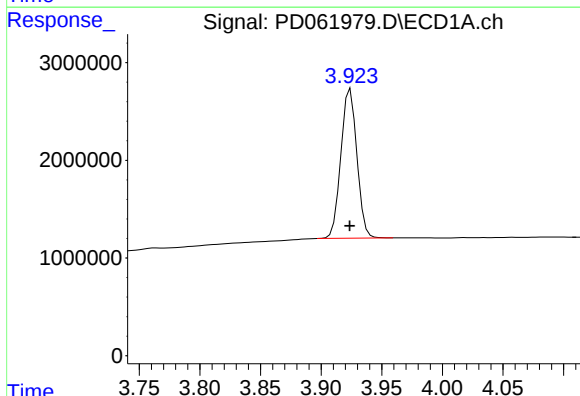


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 14058857
Conc: 10.19 ng/ml

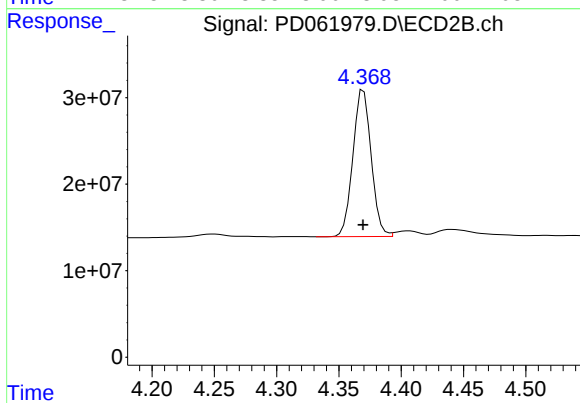

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 174264826
Conc: 11.07 ng/ml

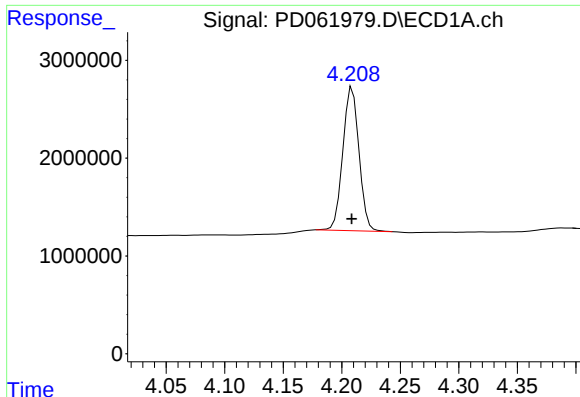

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 14070717
Conc: 10.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

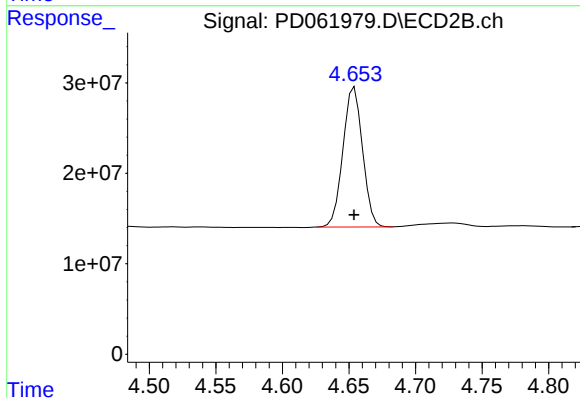


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 158195299
Conc: 11.27 ng/ml

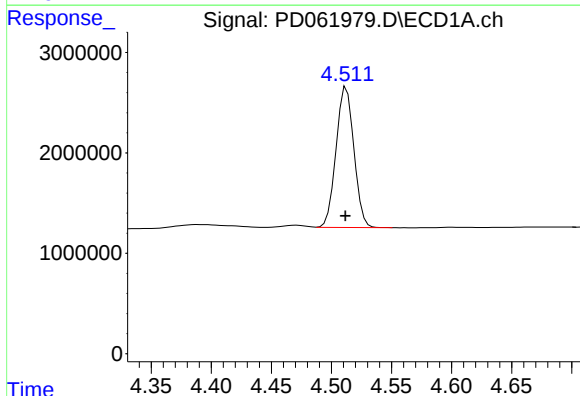


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 14482843
Conc: 10.40 ng/ml

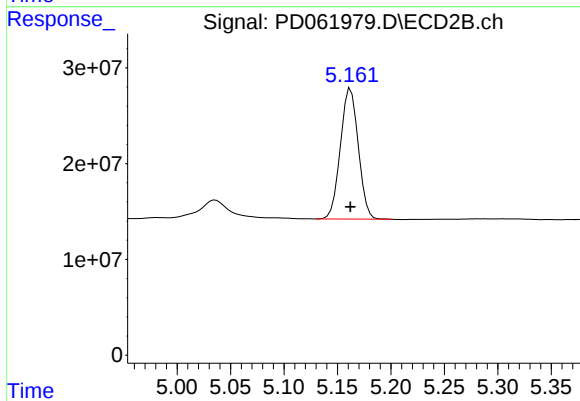

#4 Heptachlor


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 159096284
Conc: 11.61 ng/ml

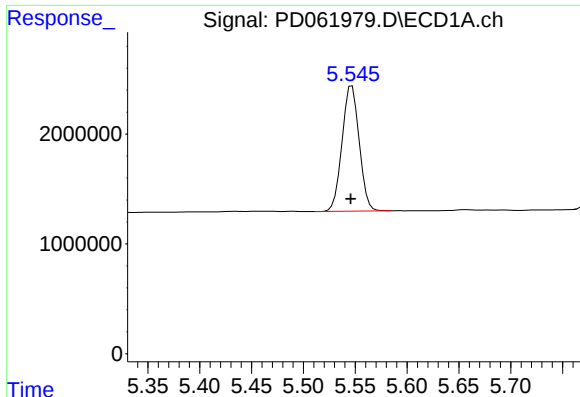

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.001 min
Response: 13112381
Conc: 10.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

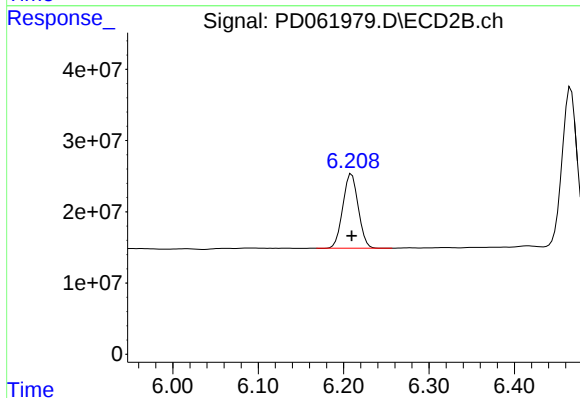


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 130632690
Conc: 10.74 ng/ml

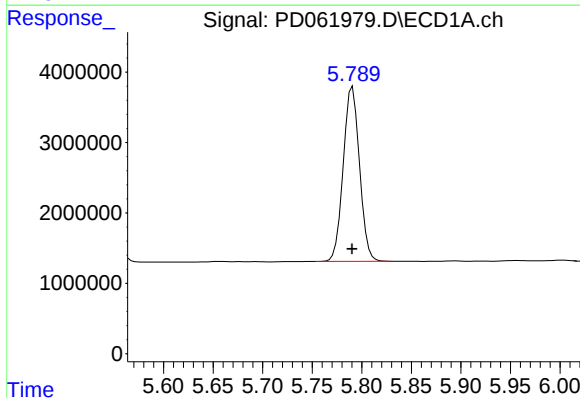


#13 Dieldrin

R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 28304837
Conc: 20.64 ng/ml

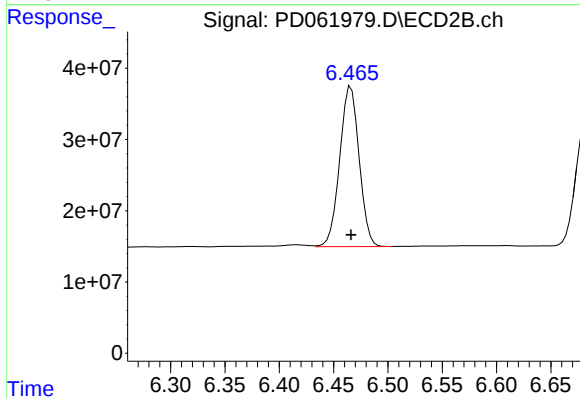

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 279760162
Conc: 21.40 ng/ml

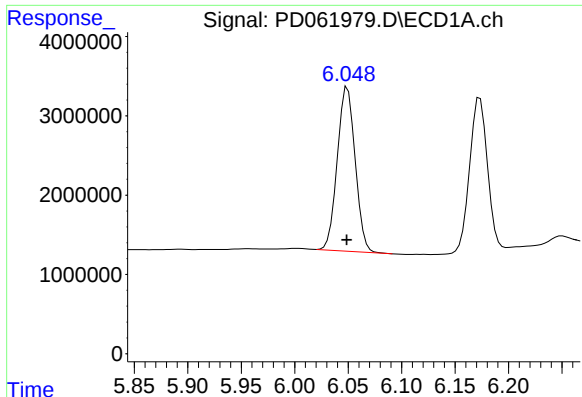

#14 Endrin


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 24113687
Conc: 20.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

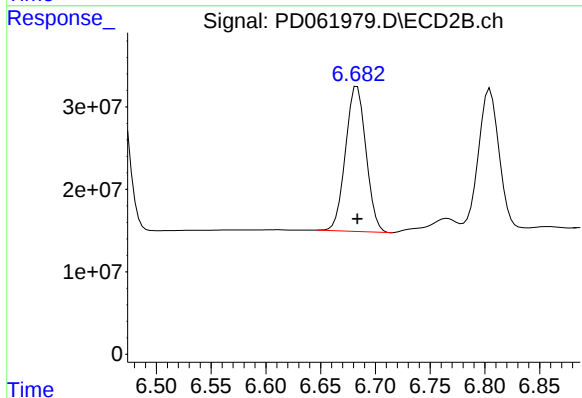


#14 Endrin

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 229046122
Conc: 21.45 ng/ml

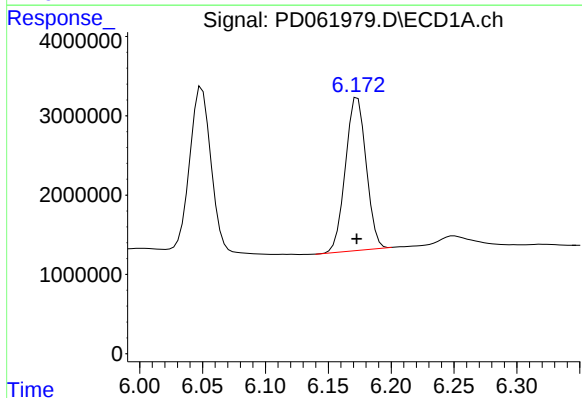


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 22089692
Conc: 20.64 ng/ml

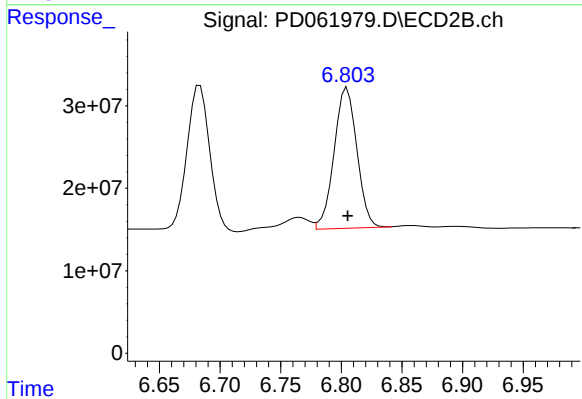

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 223358743
Conc: 21.64 ng/ml

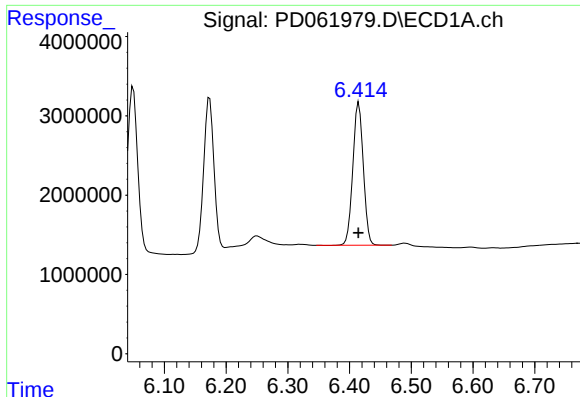

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 21276750
Conc: 20.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

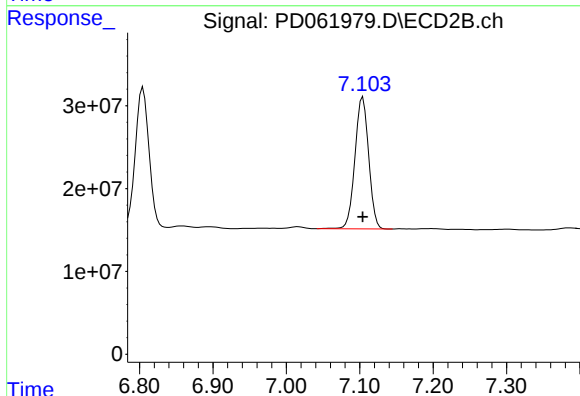


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 206744769
Conc: 20.69 ng/ml

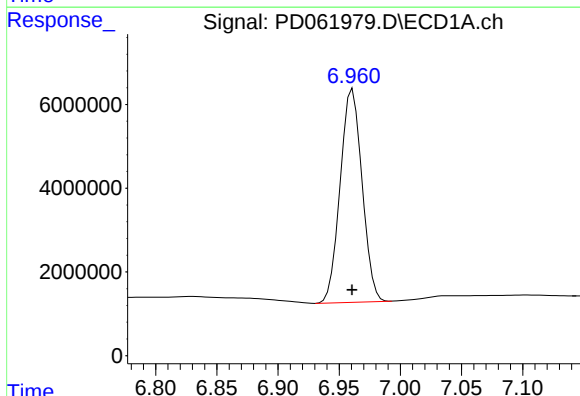


#20 Methoxychlor

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 63398488
Conc: 106.66 ng/ml

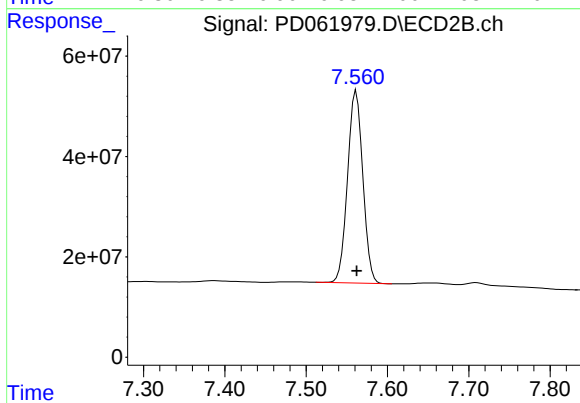

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 498934988
Conc: 106.17 ng/ml

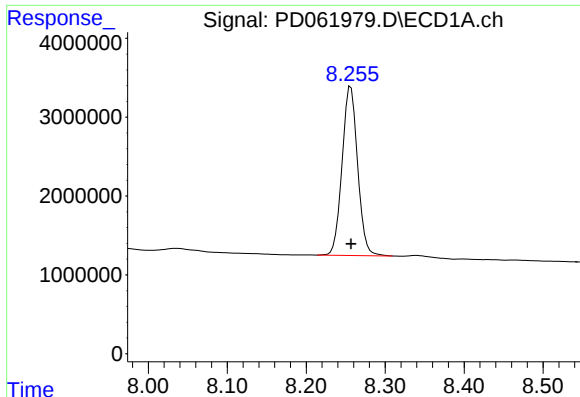

#27 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 29297727
Conc: 22.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

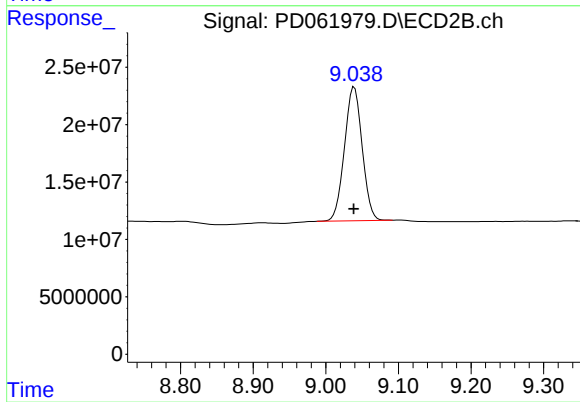

#27 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 197886052
Conc: 21.95 ng/ml