

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 19:05
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:29:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	19113295	197.4E6	20.000	20.000
27)	SA Decachlor...	8.257	9.038	52329038	360.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.924	4.369	27604912	314.8E6	20.000	20.000
3)	MA gamma-BHC...	4.209	4.654	26937790	280.7E6	20.000	20.000
4)	MA Heptachlor	4.512	5.162	27848782	274.1E6	20.000	20.000
9)	A Endosulfan I	5.546	6.209	24842845	243.3E6	20.000	20.000
13)	MA Dieldrin	5.790	6.466	54851418	523.0E6	40.000	40.000
14)	MA Endrin	6.049	6.684	46659870	427.0E6	40.000	40.000
16)	A 4,4'-DDD	6.173	6.805	42812280	412.8E6	40.000	40.000
17)	MA 4,4'-DDT	6.414	7.104	41958007	399.6E6	40.000	40.000
20)	A Methoxychlor	6.961	7.562	118.9E6	939.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 19:05
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:29:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

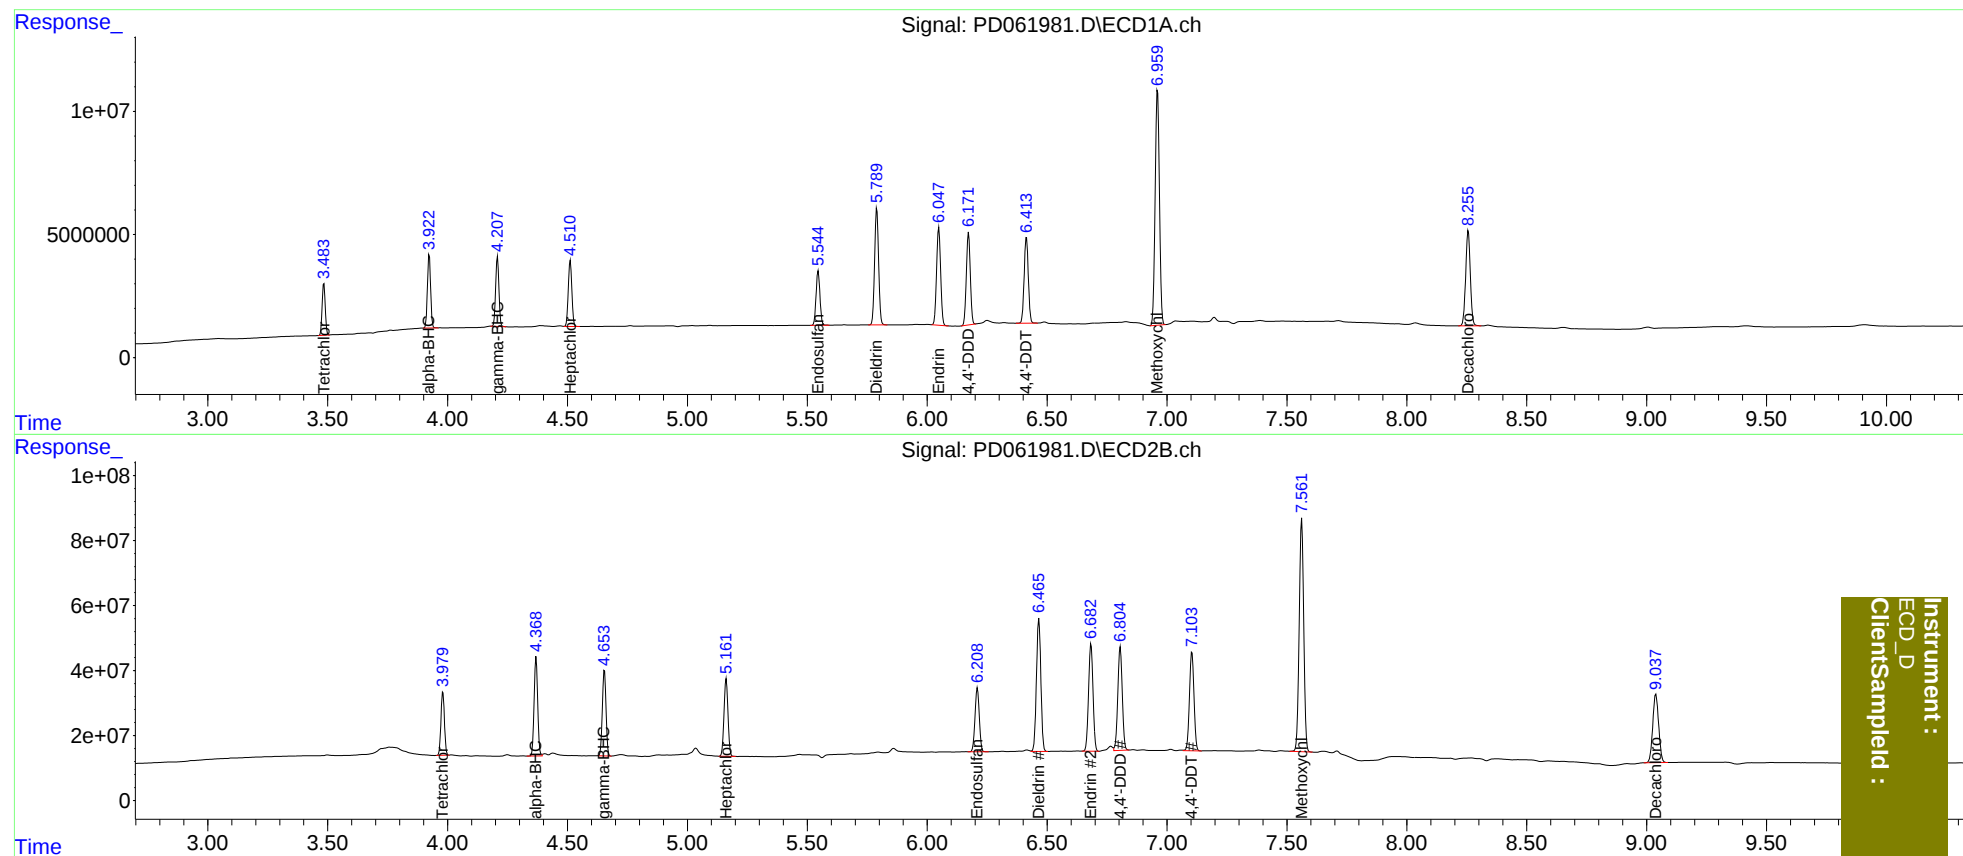


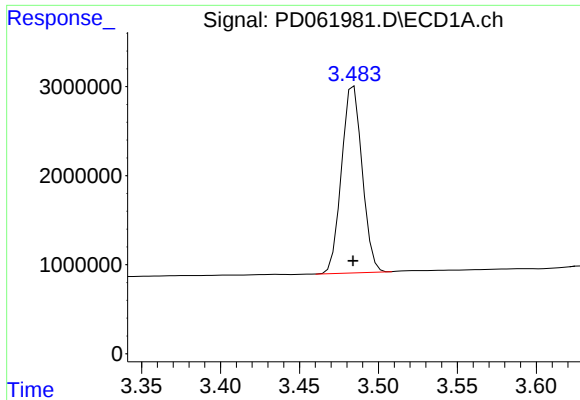

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 19113295
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

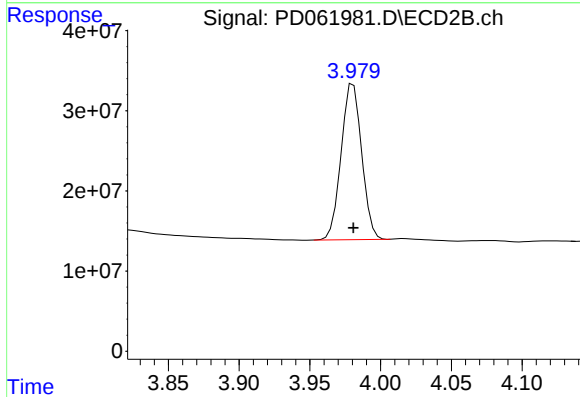


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 197350173
Conc: 20.00 ng/ml

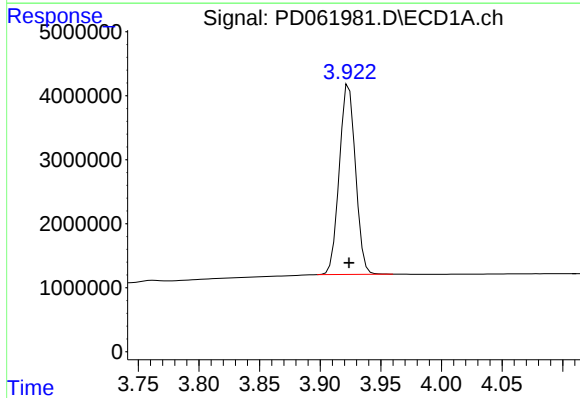


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 27604912
Conc: 20.00 ng/ml

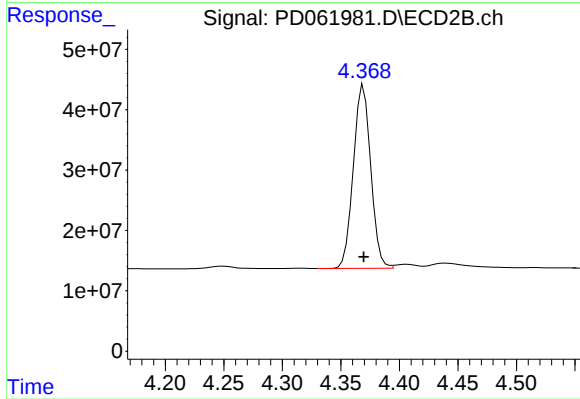

#2 alpha-BHC


R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 314770230
Conc: 20.00 ng/ml

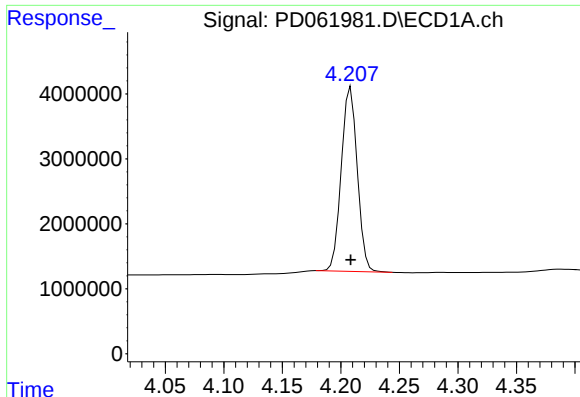

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 26937790
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

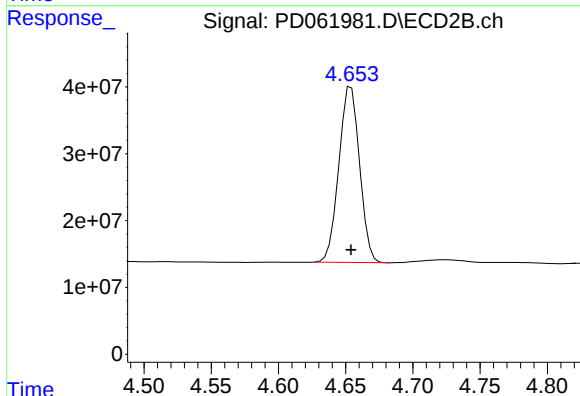


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 280742023
Conc: 20.00 ng/ml

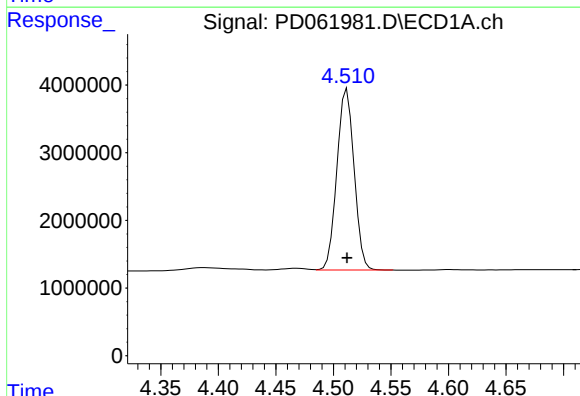


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 27848782
Conc: 20.00 ng/ml

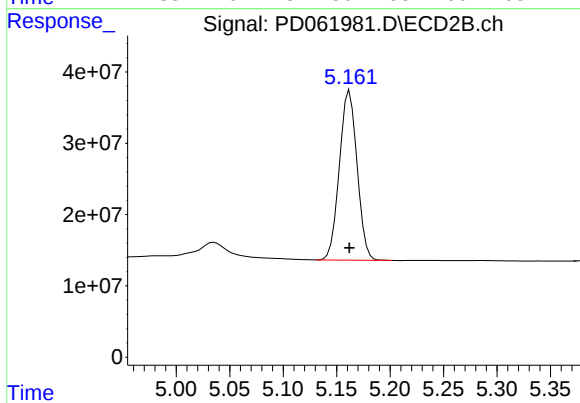

#4 Heptachlor


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 274116640
Conc: 20.00 ng/ml

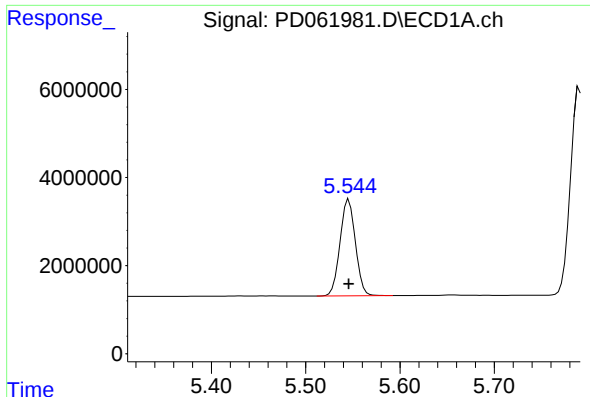

#9 Endosulfan I


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 24842845
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

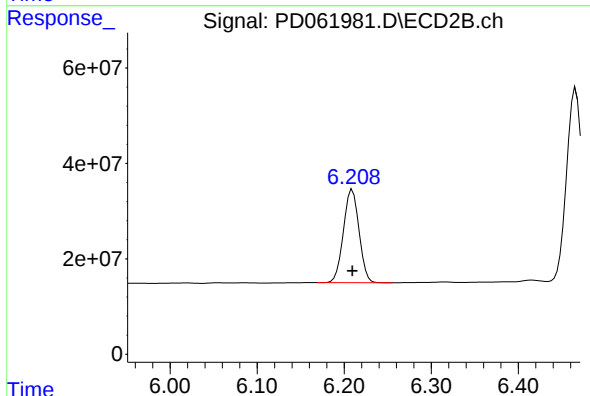


#9 Endosulfan I

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 243348987
Conc: 20.00 ng/ml

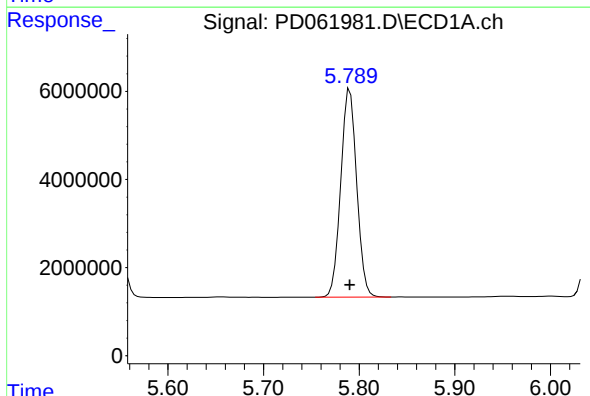


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 54851418
Conc: 40.00 ng/ml

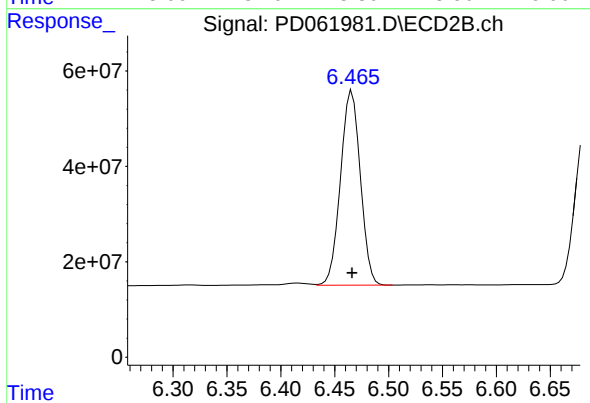

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 522964671
Conc: 40.00 ng/ml

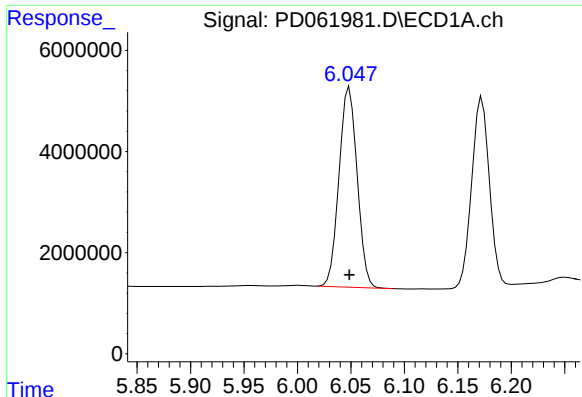

#14 Endrin


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 46659870
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

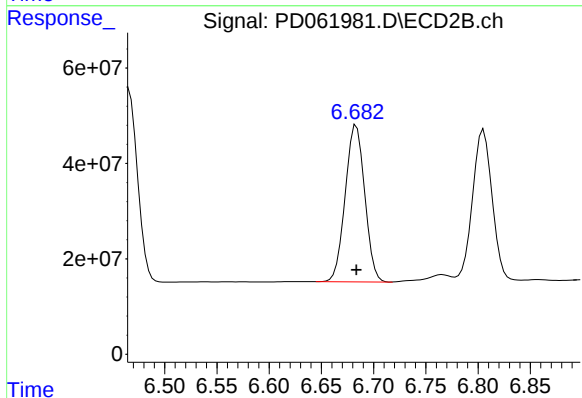


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 427041257
Conc: 40.00 ng/ml

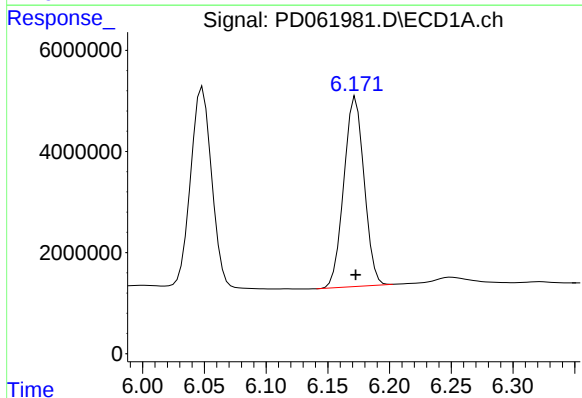


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 42812280
Conc: 40.00 ng/ml

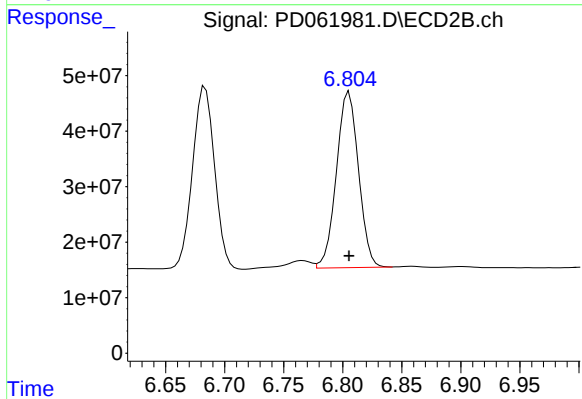

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: 0.000 min
Response: 412771737
Conc: 40.00 ng/ml

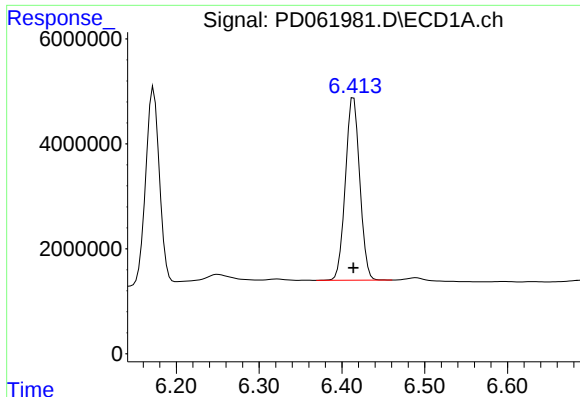

#17 4,4'-DDT


R.T.: 6.414 min
Delta R.T.: 0.000 min
Response: 41958007
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

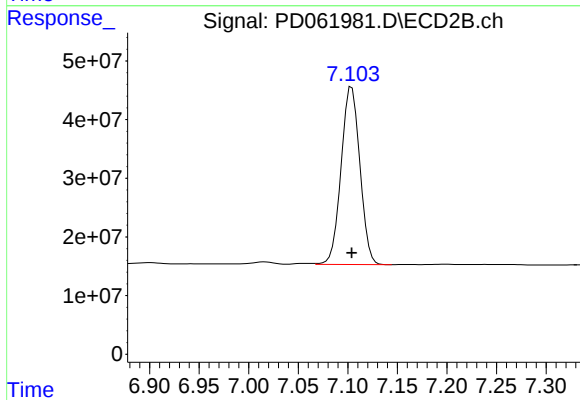


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 399621306
Conc: 40.00 ng/ml

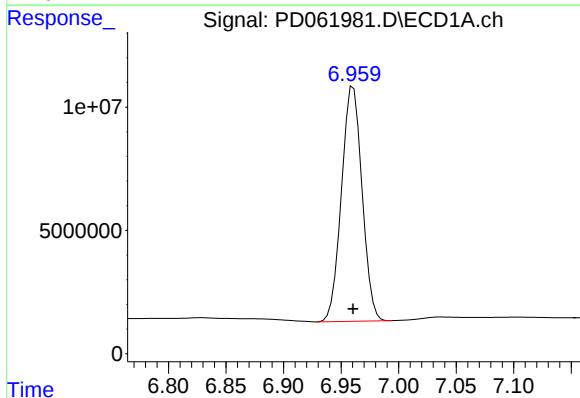


#20 Methoxychlor

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 118877996
Conc: 200.00 ng/ml

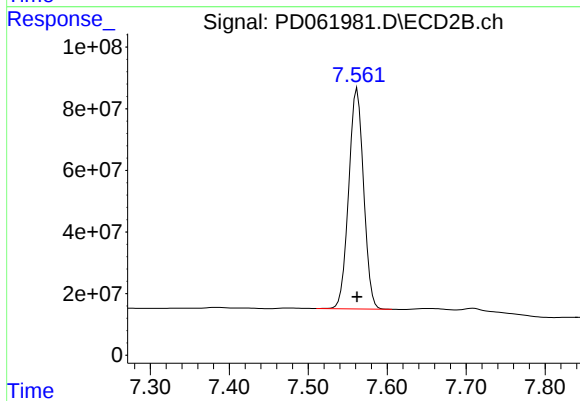

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 939919820
Conc: 200.00 ng/ml

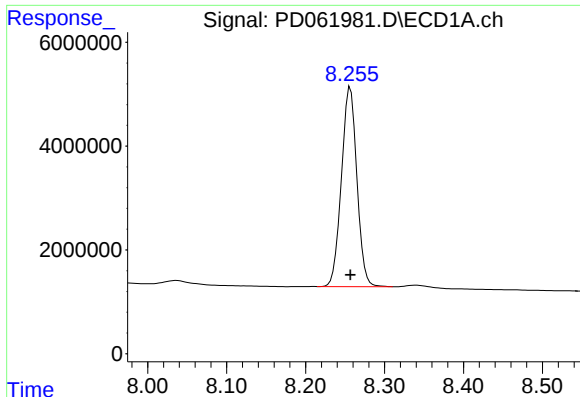

#27 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 52329038
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

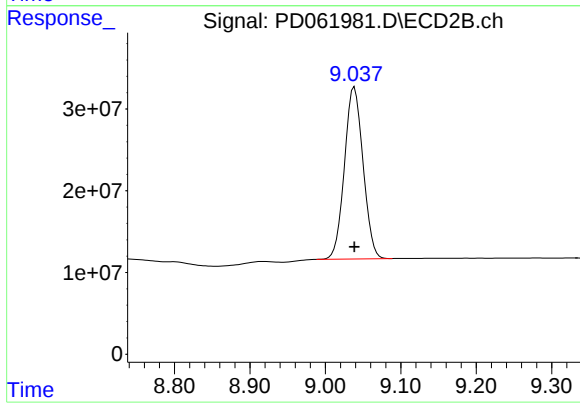

#27 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 360552456
Conc: 40.00 ng/ml