

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 19:33
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:29:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	37301127	388.8E6	39.032	39.406
27)	SA Decachlor...	8.256	9.039	97597874	675.8E6	74.603	74.974
Target Compounds							
2)	A alpha-BHC	3.925	4.370	56616424	632.3E6	41.019	40.174
3)	MA gamma-BHC...	4.209	4.655	54353030	577.5E6	40.354	41.140
4)	MA Heptachlor	4.512	5.163	55253594	574.3E6	39.681	41.899
9)	A Endosulfan I	5.547	6.210	48975931	470.0E6	39.429	38.625
13)	MA Dieldrin	5.791	6.466	111.1E6	1004.5E6	81.008	76.829
14)	MA Endrin	6.050	6.684	91943251	794.9E6	78.820	74.460
16)	A 4,4'-DDD	6.173	6.806	87232955	787.0E6	81.503	76.268
17)	MA 4,4'-DDT	6.415	7.104	87892883	769.6E6	83.791	77.028
20)	A Methoxychlor	6.961	7.562	229.9E6	1736.9E6	386.744	369.595

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 19:33
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:29:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

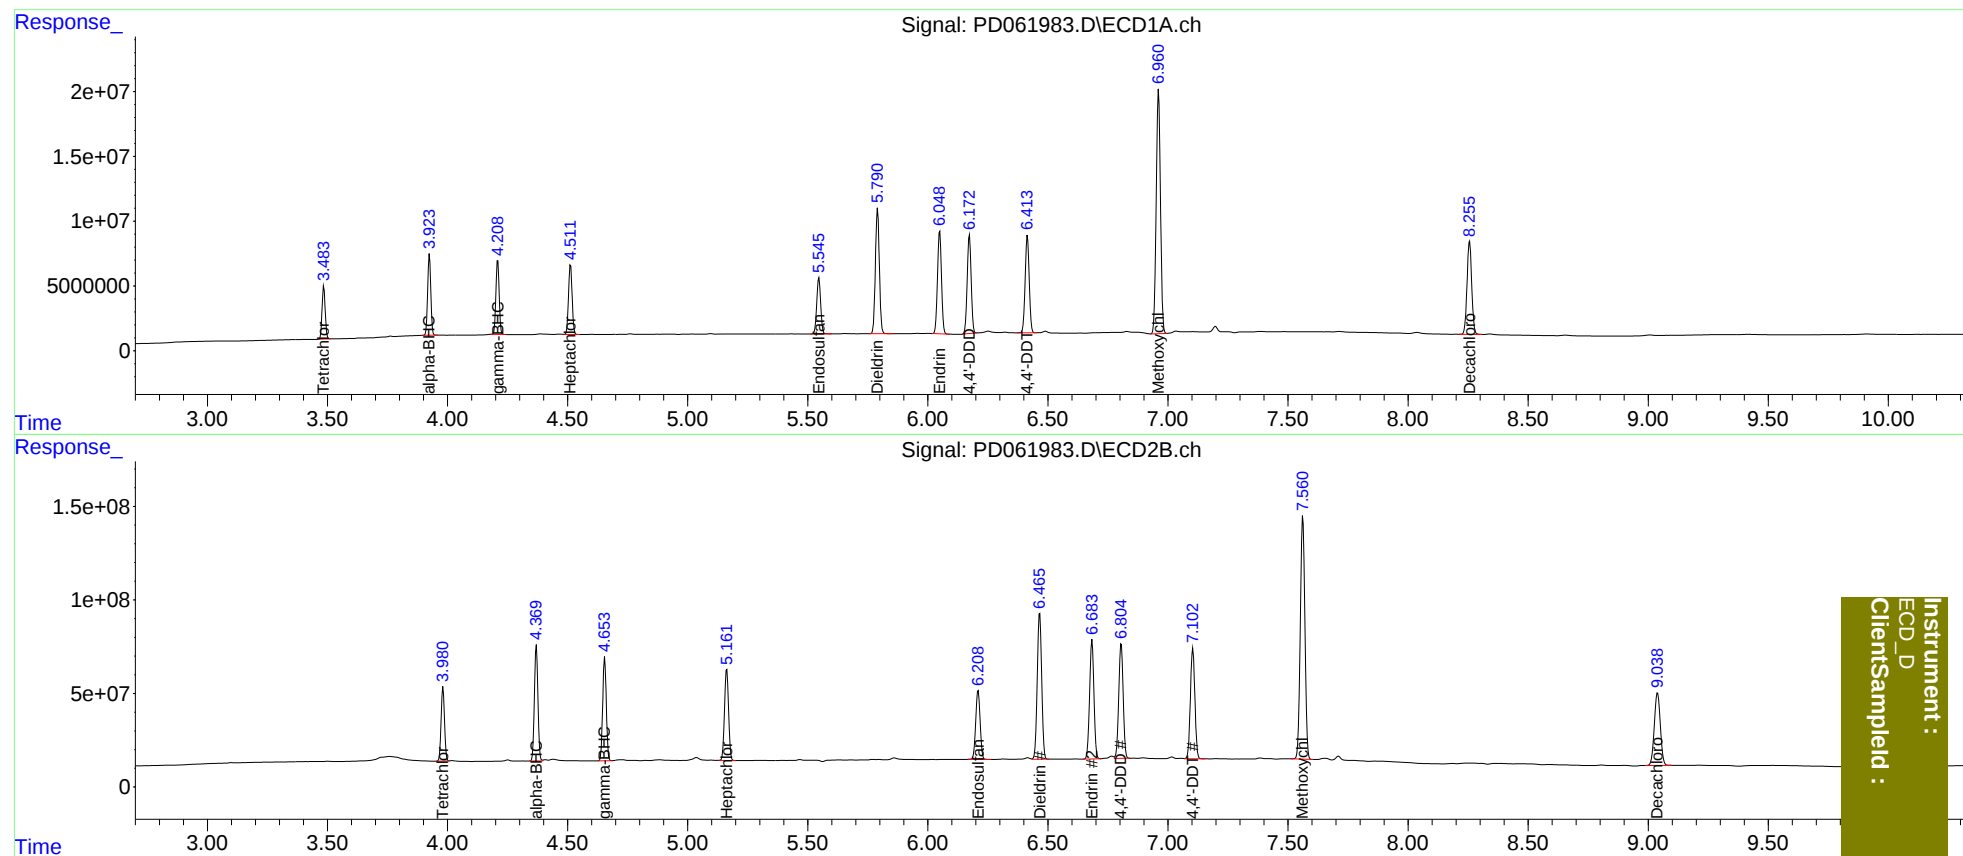


Instrument :
ECD_D
ClientSampled :

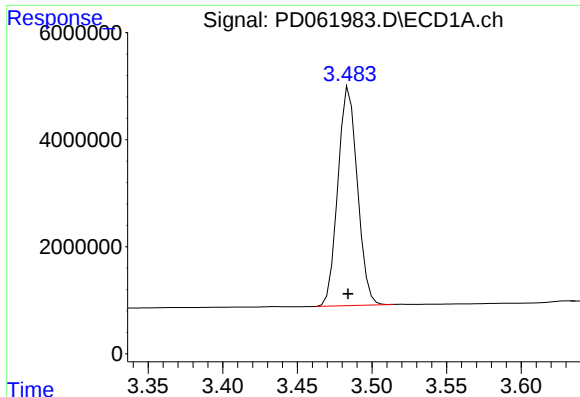

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 37301127
Conc: 39.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

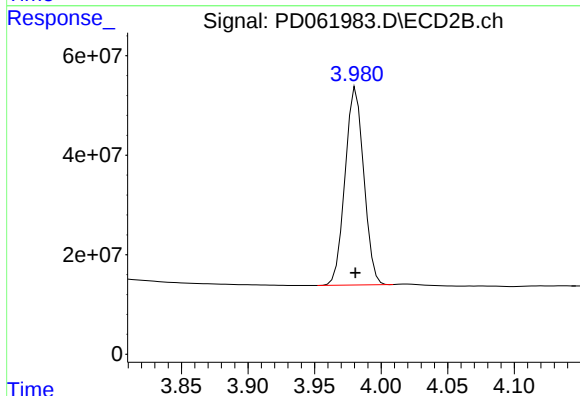


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 388836036
Conc: 39.41 ng/ml

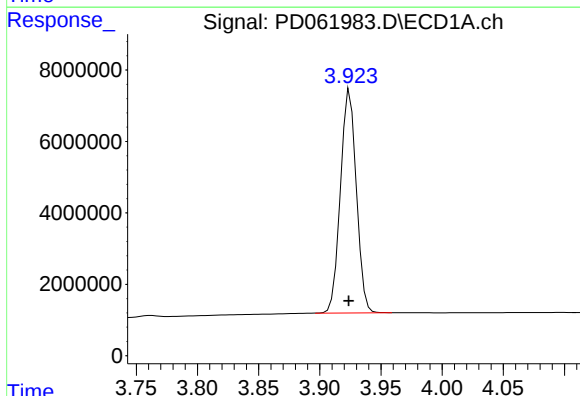


#2 alpha-BHC

R.T.: 3.925 min
Delta R.T.: 0.000 min
Response: 56616424
Conc: 41.02 ng/ml

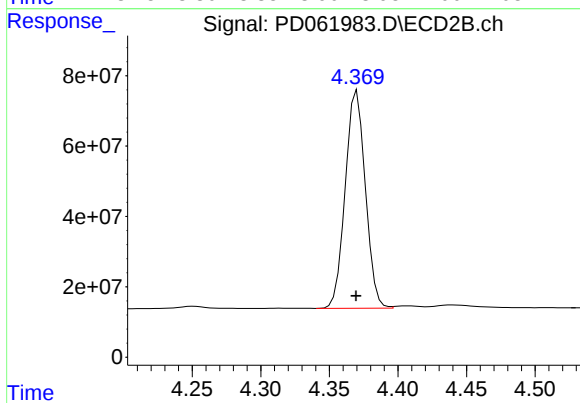

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 632273308
Conc: 40.17 ng/ml

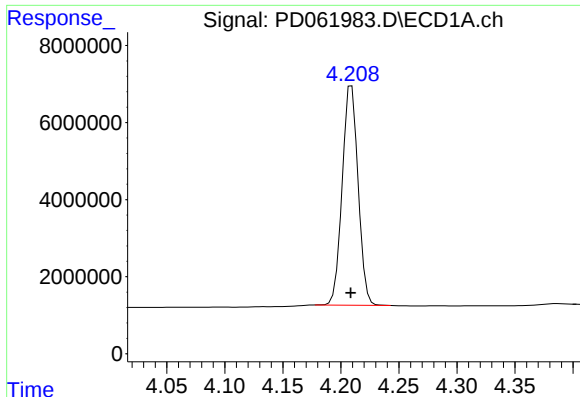

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 54353030
Conc: 40.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

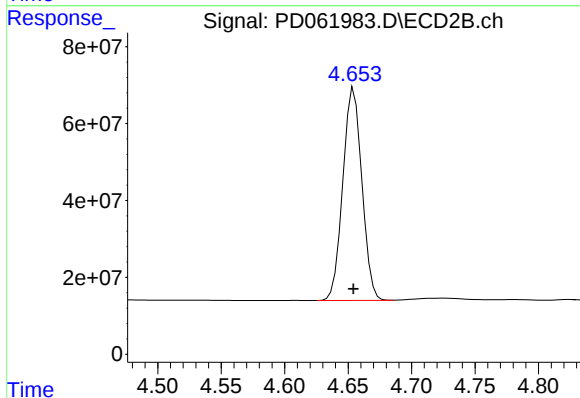


#3 gamma-BHC (Lindane)

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 577487852
Conc: 41.14 ng/ml

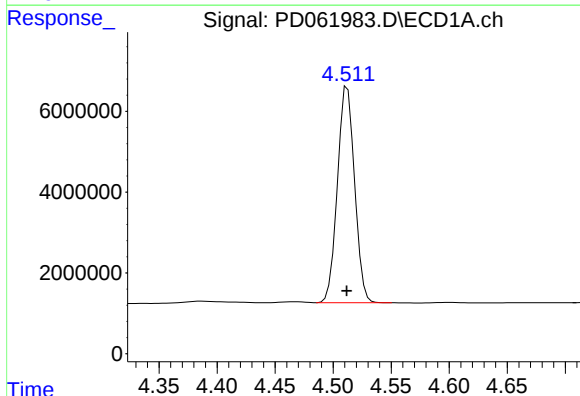


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 55253594
Conc: 39.68 ng/ml

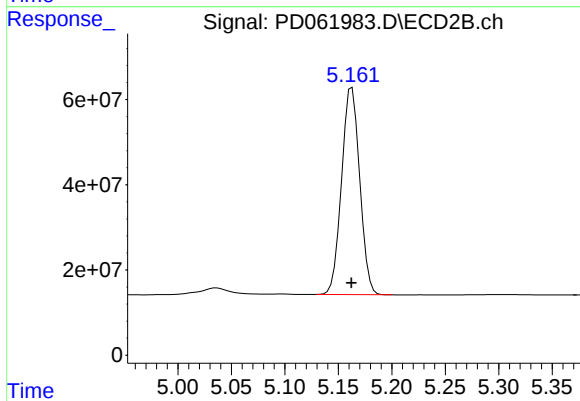

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 574255406
Conc: 41.90 ng/ml

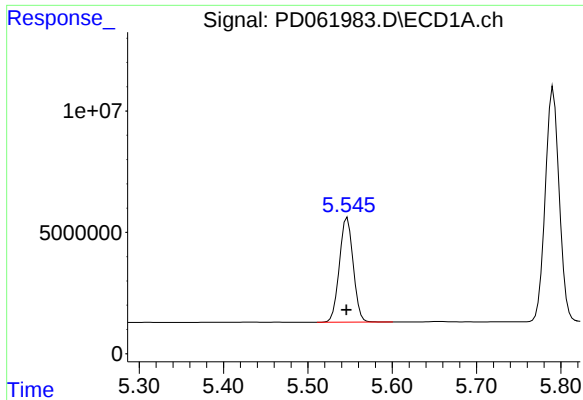

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.001 min
Response: 48975931
Conc: 39.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

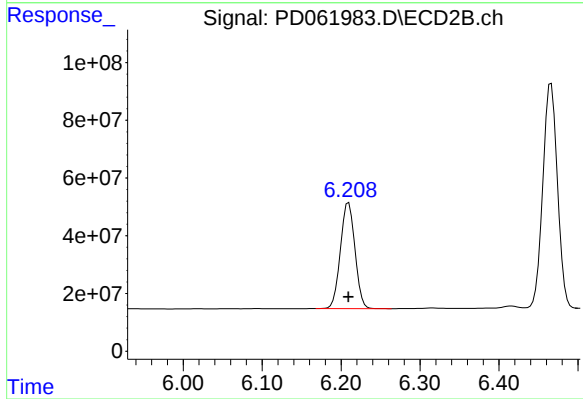


#9 Endosulfan I

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 469967036
Conc: 38.62 ng/ml

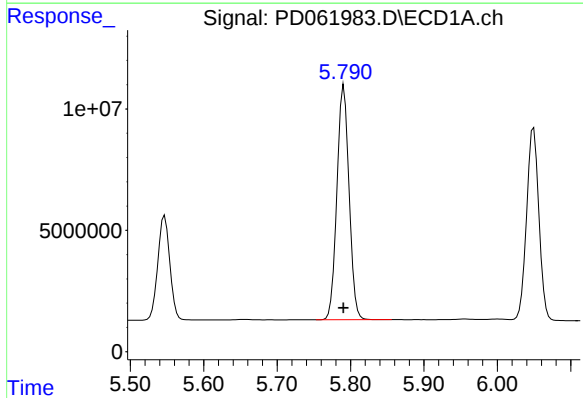


#13 Dieldrin

R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 111084544
Conc: 81.01 ng/ml

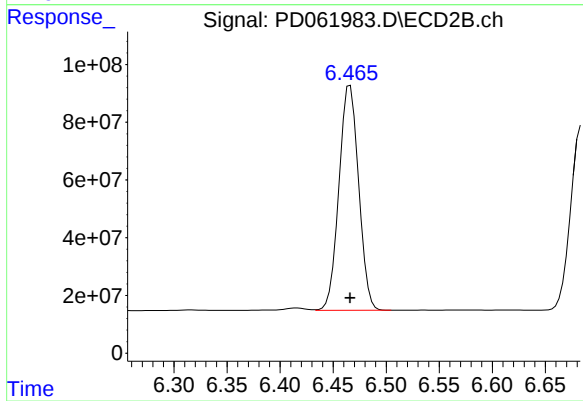

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 1004468750
Conc: 76.83 ng/ml

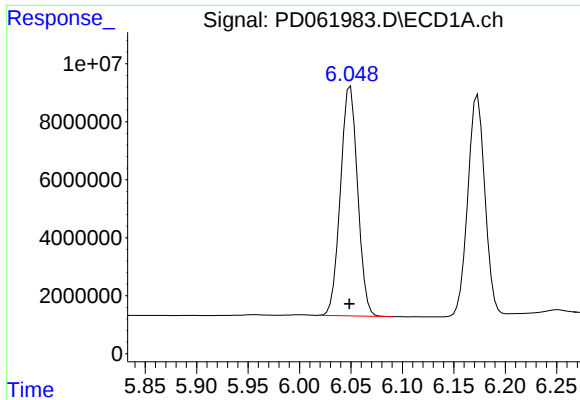

#14 Endrin


R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 91943251
Conc: 78.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

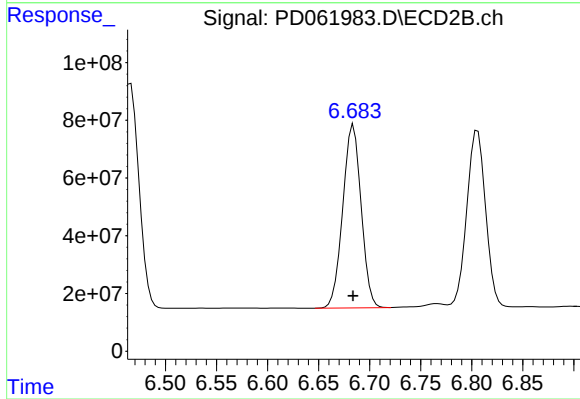


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 794935594
Conc: 74.46 ng/ml

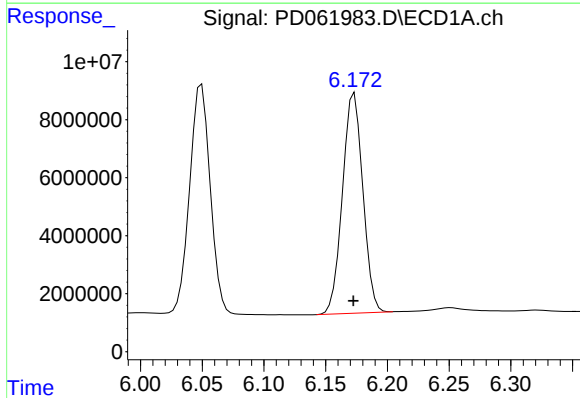


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 87232955
Conc: 81.50 ng/ml

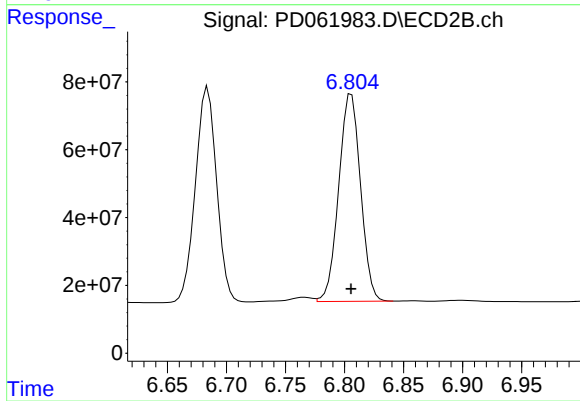

#16 4,4'-DDD


R.T.: 6.806 min
Delta R.T.: 0.000 min
Response: 787029073
Conc: 76.27 ng/ml

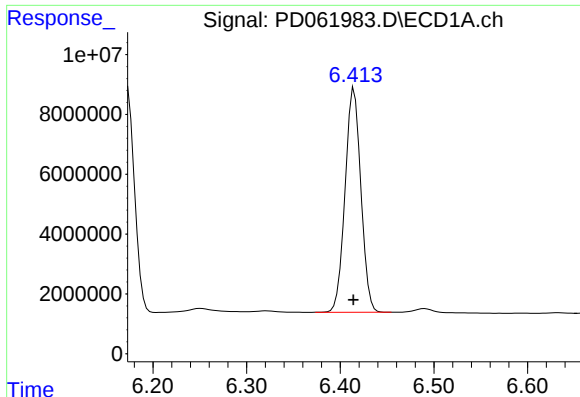

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 87892883
Conc: 83.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

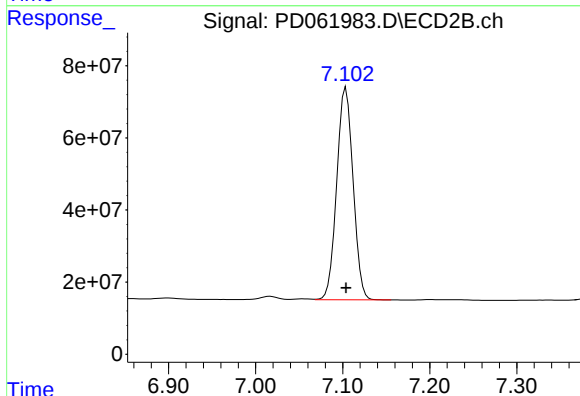


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 769552212
Conc: 77.03 ng/ml

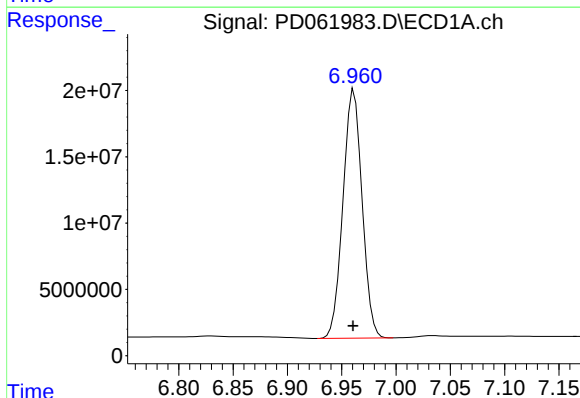


#20 Methoxychlor

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 229876648
Conc: 386.74 ng/ml

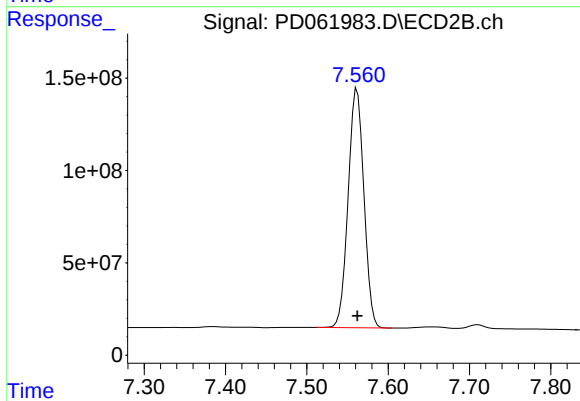

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 1736947031
Conc: 369.59 ng/ml

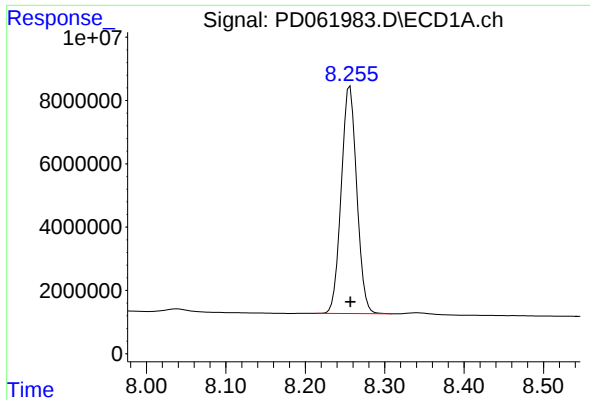

#27 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 97597874
Conc: 74.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

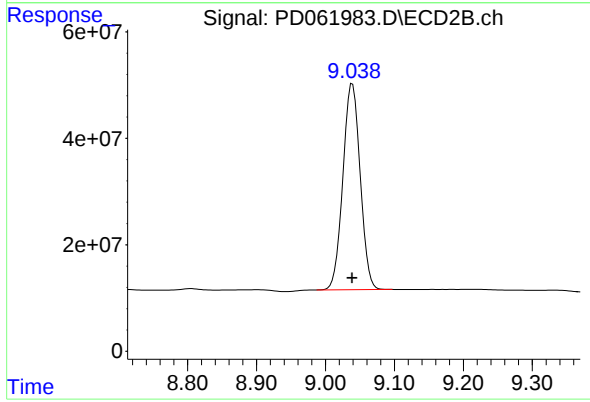

#27 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 675797699
Conc: 74.97 ng/ml