

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 19:47
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 02:18:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 02:16:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	37091722	387.6E6	39.111	39.005
27)	SA Decachlor...	8.256	9.039	98516402	667.6E6	75.470	73.232
Target Compounds							
5)	MB Aldrin	4.763	5.467	55014379	556.9E6	40.451	38.664
6)	B beta-BHC	4.459	4.824	25376529	245.1E6	38.406	38.379
7)	B delta-BHC	4.666	5.041	56069507	530.8E6	40.982	37.674
8)	B Heptachlo...	5.207	5.852	51836579	482.4E6	39.617	37.431
10)	B trans-Chl...	5.434	6.087	54096464	526.9E6	39.689	38.094
11)	B cis-Chlor...	5.493	6.160	52965175	492.5E6	39.394	37.983
12)	B 4,4'-DDE	5.656	6.316	105.2E6	989.8E6	81.402	76.962
15)	B Endosulfa...	6.323	6.892	86277535	780.6E6	77.800	76.875
18)	B Endrin al...	6.491	7.017	75724757	664.3E6	79.660	76.488
19)	B Endosulfa...	6.705	7.239	87749507	794.0E6	77.165	77.830
21)	B Endrin ke...	7.199	7.710	102.3E6	726.1E6	78.418	74.966

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 19:47
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 02:18:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 02:16:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

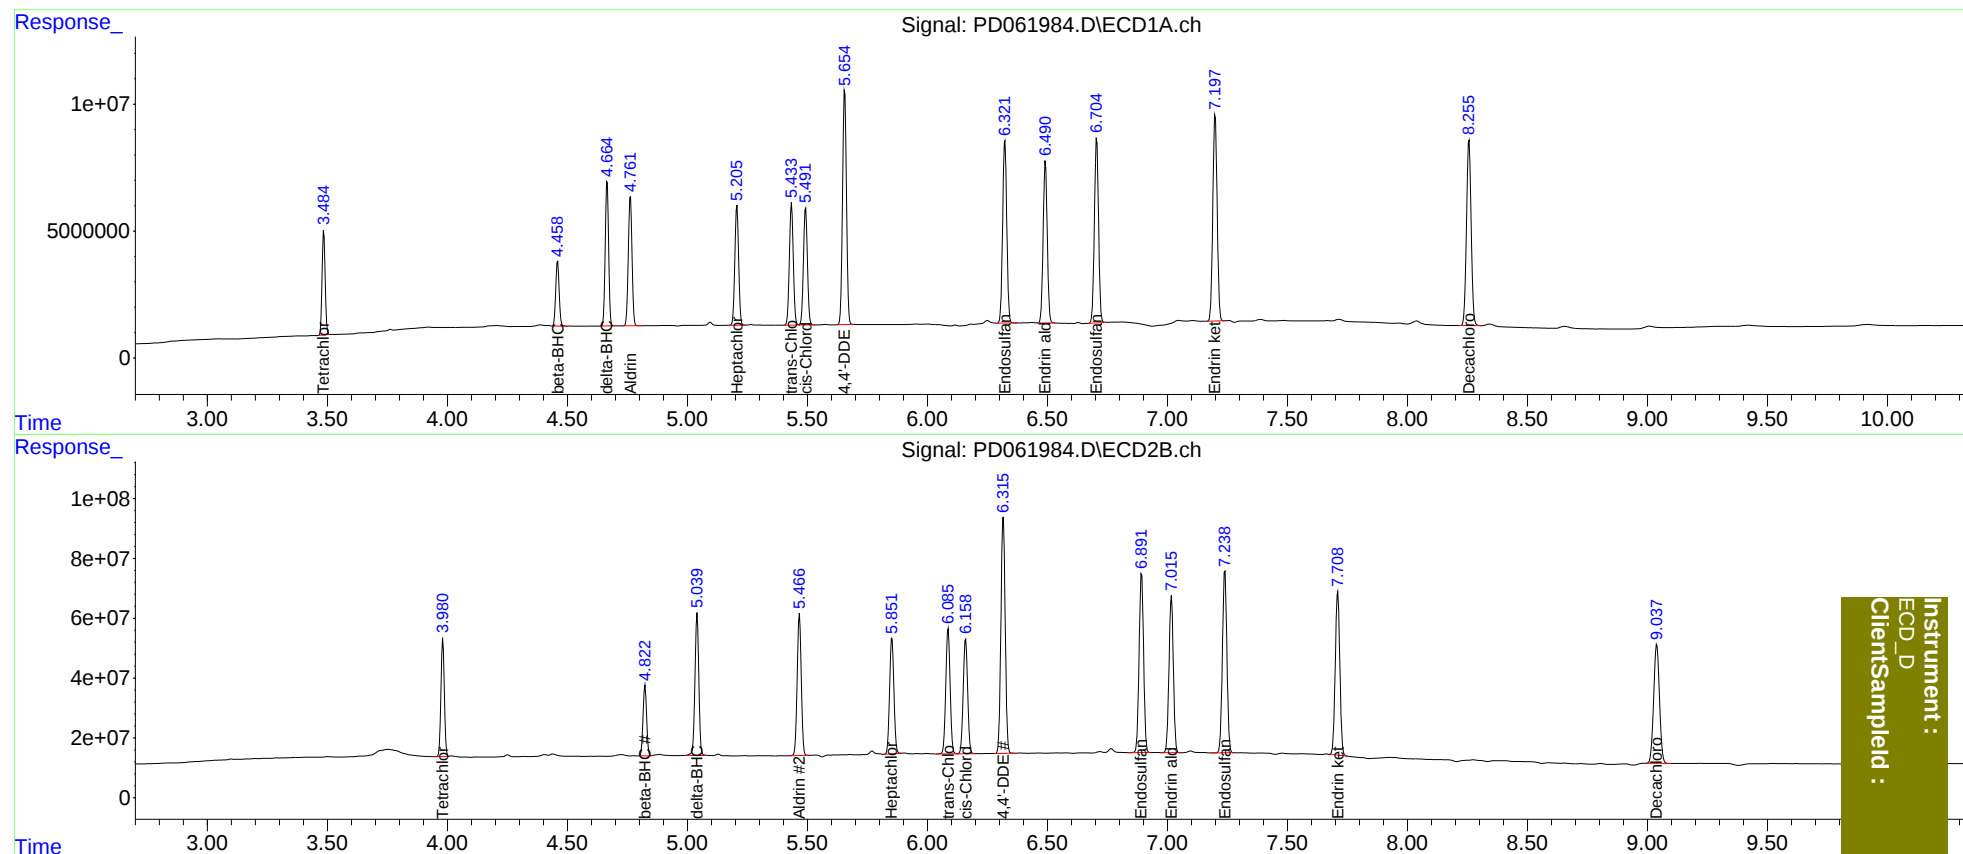


Instrument :
ECD_D
ClientSampled :

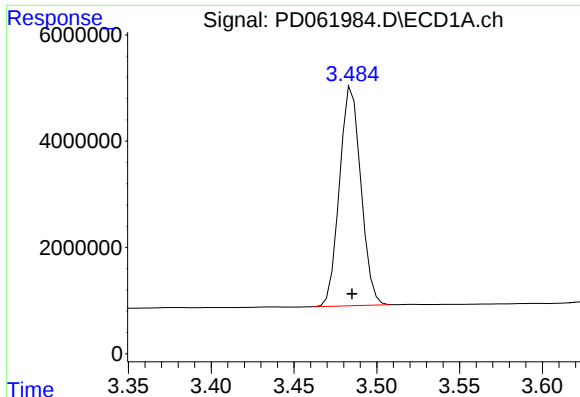

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 37091722
Conc: 39.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

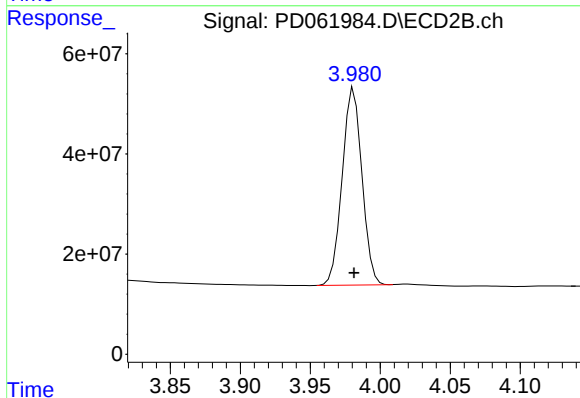


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 387581298
Conc: 39.00 ng/ml

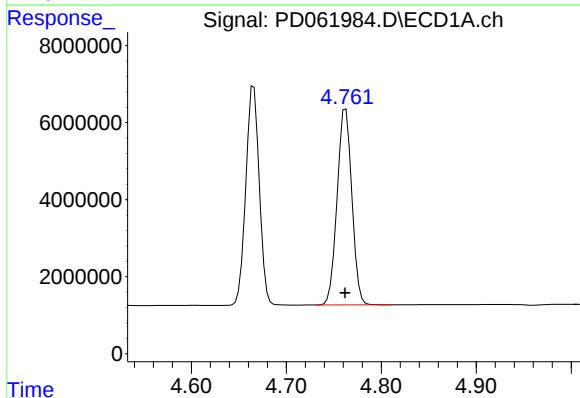


#5 Aldrin

R.T.: 4.763 min
Delta R.T.: 0.000 min
Response: 55014379
Conc: 40.45 ng/ml

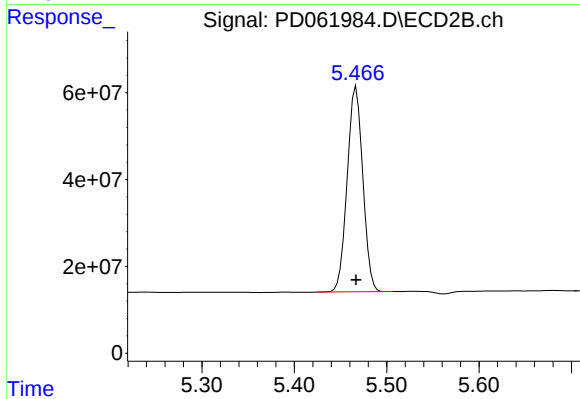

#5 Aldrin


R.T.: 5.467 min
Delta R.T.: 0.000 min
Response: 556943295
Conc: 38.66 ng/ml

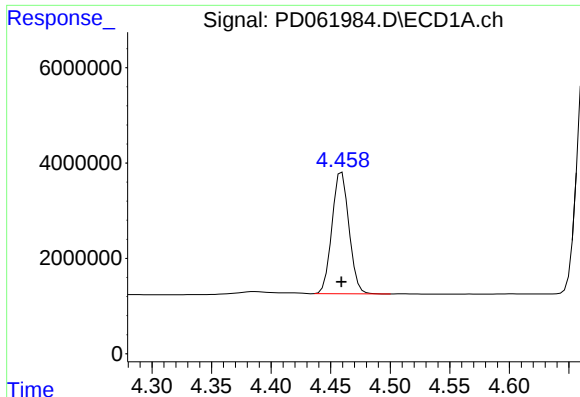

#6 beta-BHC


R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 25376529
Conc: 38.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

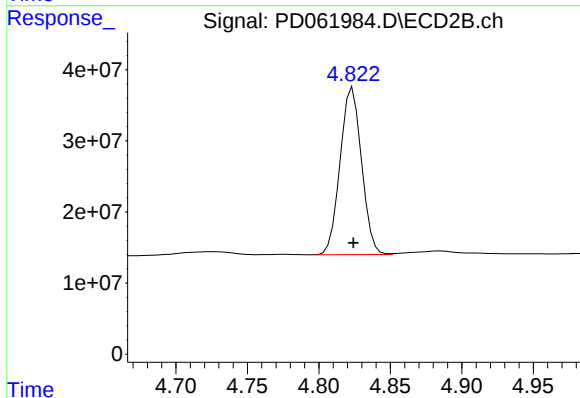


#6 beta-BHC

R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 245052513
Conc: 38.38 ng/ml

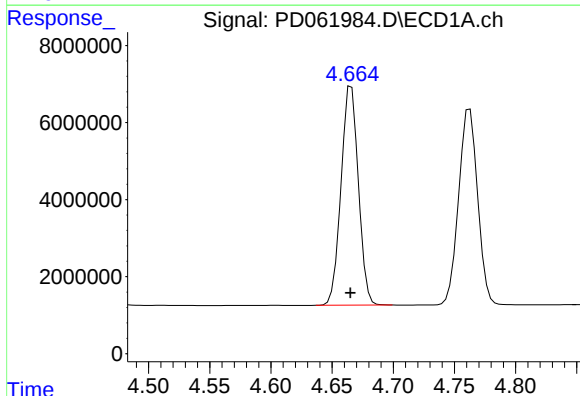


#7 delta-BHC

R.T.: 4.666 min
Delta R.T.: 0.000 min
Response: 56069507
Conc: 40.98 ng/ml

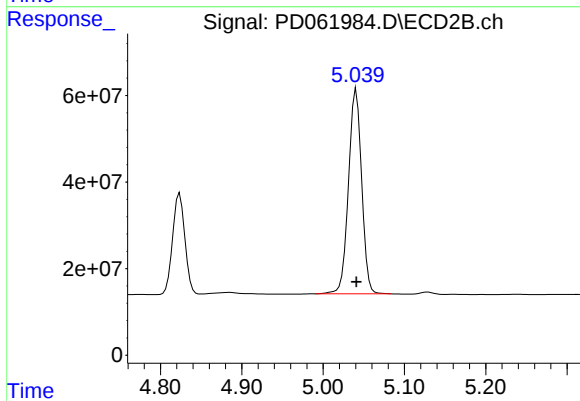

#7 delta-BHC


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 530818241
Conc: 37.67 ng/ml

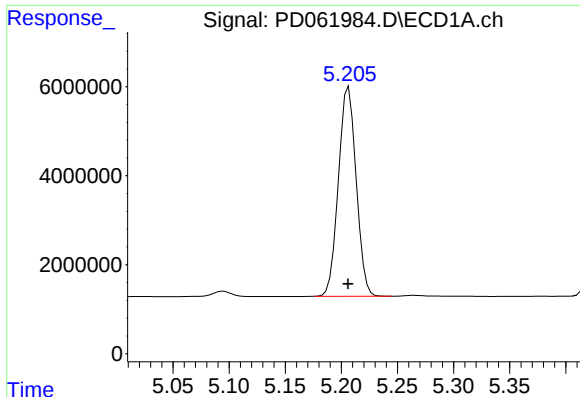

#8 Heptachlor epoxide


R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 51836579
Conc: 39.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

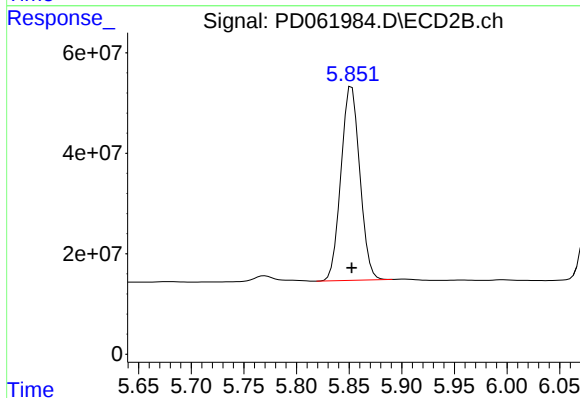


#8 Heptachlor epoxide

R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 482403604
Conc: 37.43 ng/ml

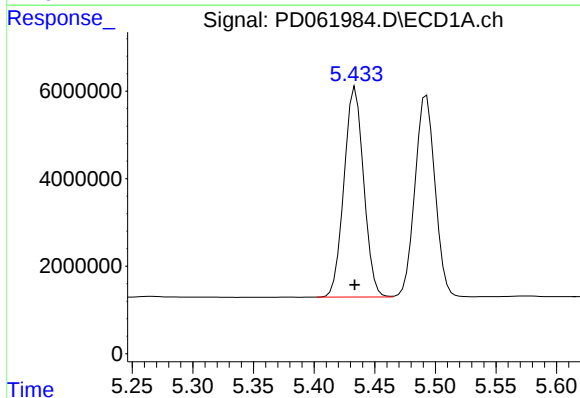


#10 trans-Chlordane

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 54096464
Conc: 39.69 ng/ml

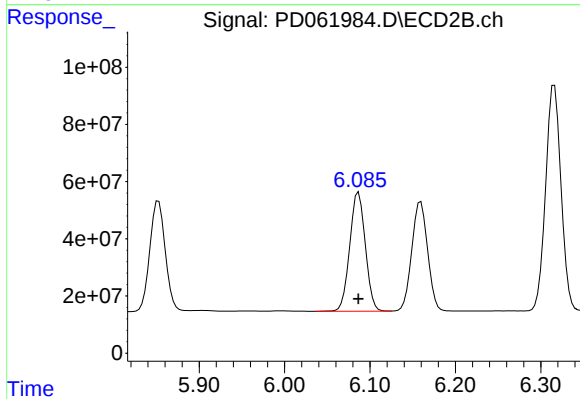

#10 trans-Chlordane


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 526945513
Conc: 38.09 ng/ml

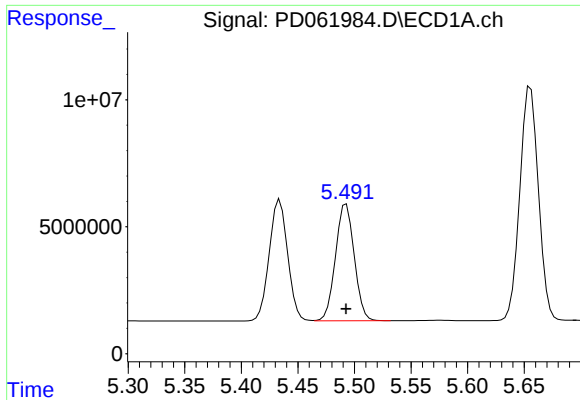

#11 cis-Chlordane


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 52965175
Conc: 39.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

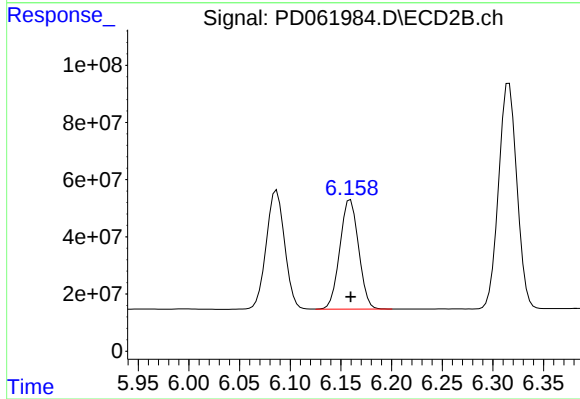


#11 cis-Chlordane

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 492450481
Conc: 37.98 ng/ml

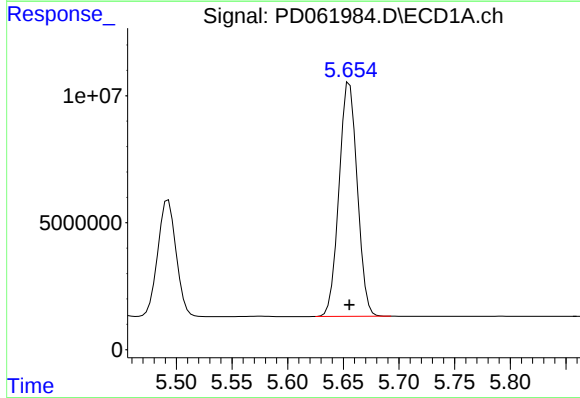


#12 4,4'-DDE

R.T.: 5.656 min
Delta R.T.: 0.000 min
Response: 105179091
Conc: 81.40 ng/ml

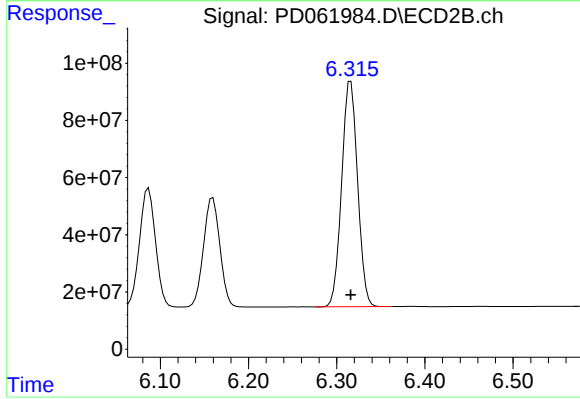

#12 4,4'-DDE


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 989796982
Conc: 76.96 ng/ml

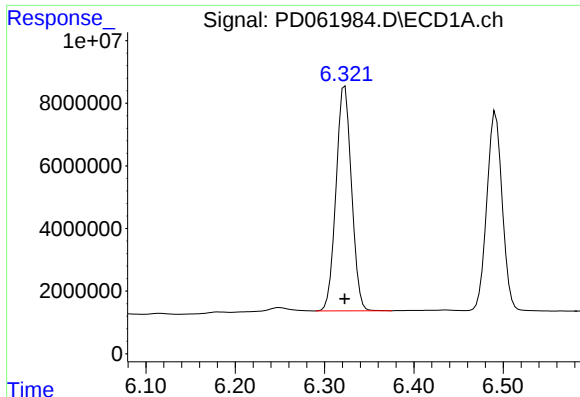

#15 Endosulfan II


R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 86277535
Conc: 77.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

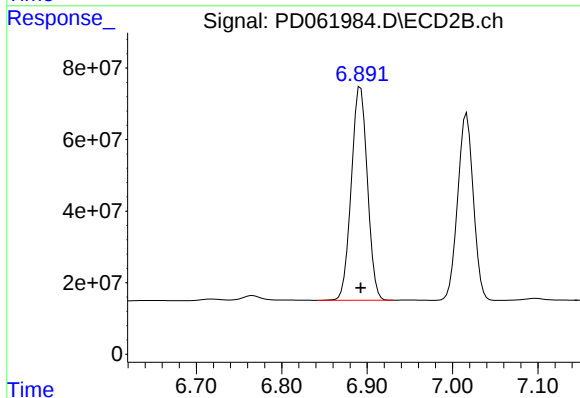


#15 Endosulfan II

R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 780614716
Conc: 76.87 ng/ml

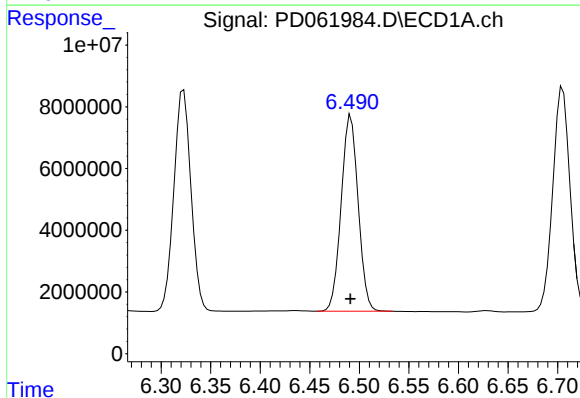


#18 Endrin aldehyde

R.T.: 6.491 min
Delta R.T.: 0.000 min
Response: 75724757
Conc: 79.66 ng/ml

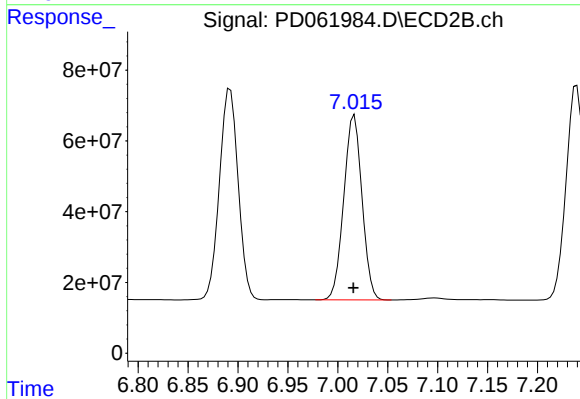

#18 Endrin aldehyde


R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 664274357
Conc: 76.49 ng/ml

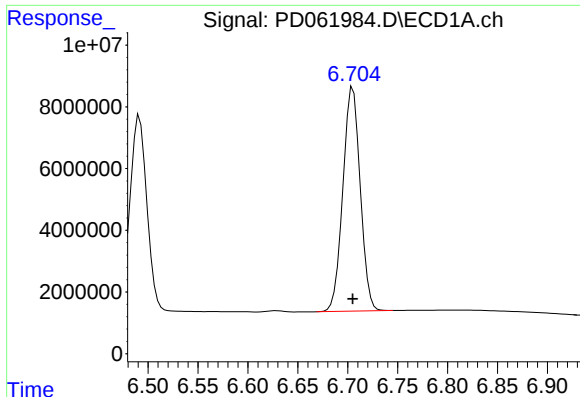

#19 Endosulfan Sulfate


R.T.: 6.705 min
Delta R.T.: 0.000 min
Response: 87749507
Conc: 77.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

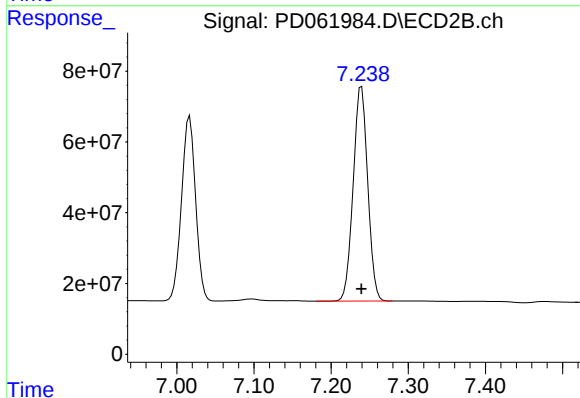


#19 Endosulfan Sulfate

R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 793964031
Conc: 77.83 ng/ml

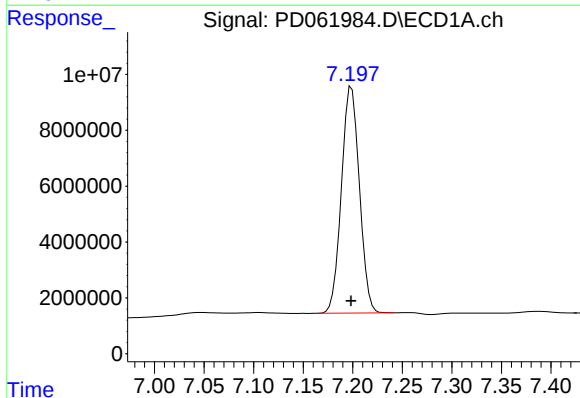


#21 Endrin ketone

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 102319662
Conc: 78.42 ng/ml

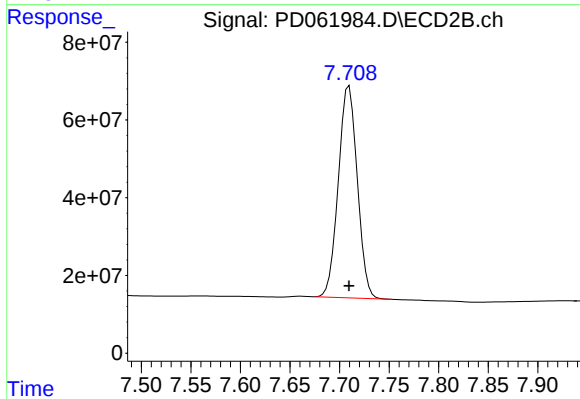

#21 Endrin ketone


R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 726084737
Conc: 74.97 ng/ml

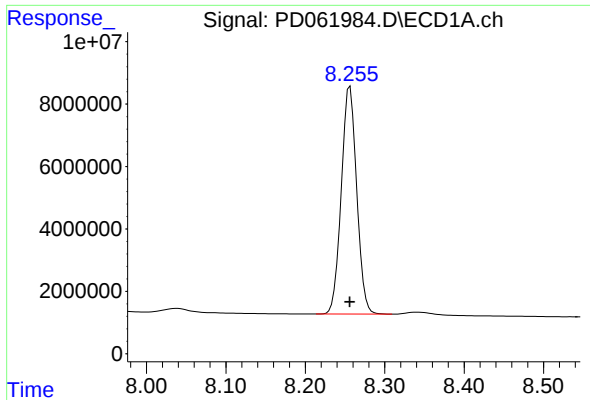

#27 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 98516402
Conc: 75.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

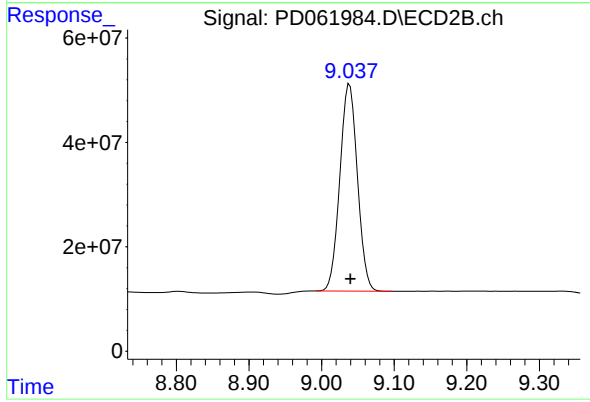

#27 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 667599944
Conc: 73.23 ng/ml