

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 20:01
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:29:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	75974208	786.9E6	79.499	79.752
27)	SA Decachlor...	8.257	9.039	187.8E6	1315.1E6	143.564	145.902
Target Compounds							
2)	A alpha-BHC	3.925	4.370	121.1E6	1253.4E6	87.719	79.639
3)	MA gamma-BHC...	4.210	4.654	113.5E6	1126.8E6	84.255	80.270
4)	MA Heptachlor	4.512	5.163	114.4E6	1087.8E6	82.155	79.370
9)	A Endosulfan I	5.547	6.210	99733045	928.0E6	80.291	76.269
13)	MA Dieldrin	5.791	6.466	230.3E6	1995.0E6	167.952	152.595
14)	MA Endrin	6.050	6.684	179.9E6	1524.6E6	154.226	142.811
16)	A 4,4'-DDD	6.173	6.806	179.7E6	1577.7E6	167.858	152.890
17)	MA 4,4'-DDT	6.415	7.105	179.4E6	1544.2E6	171.049	154.567
20)	A Methoxychlor	6.961	7.562	450.8E6	3304.0E6	758.490	703.046


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 20:01
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:29:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

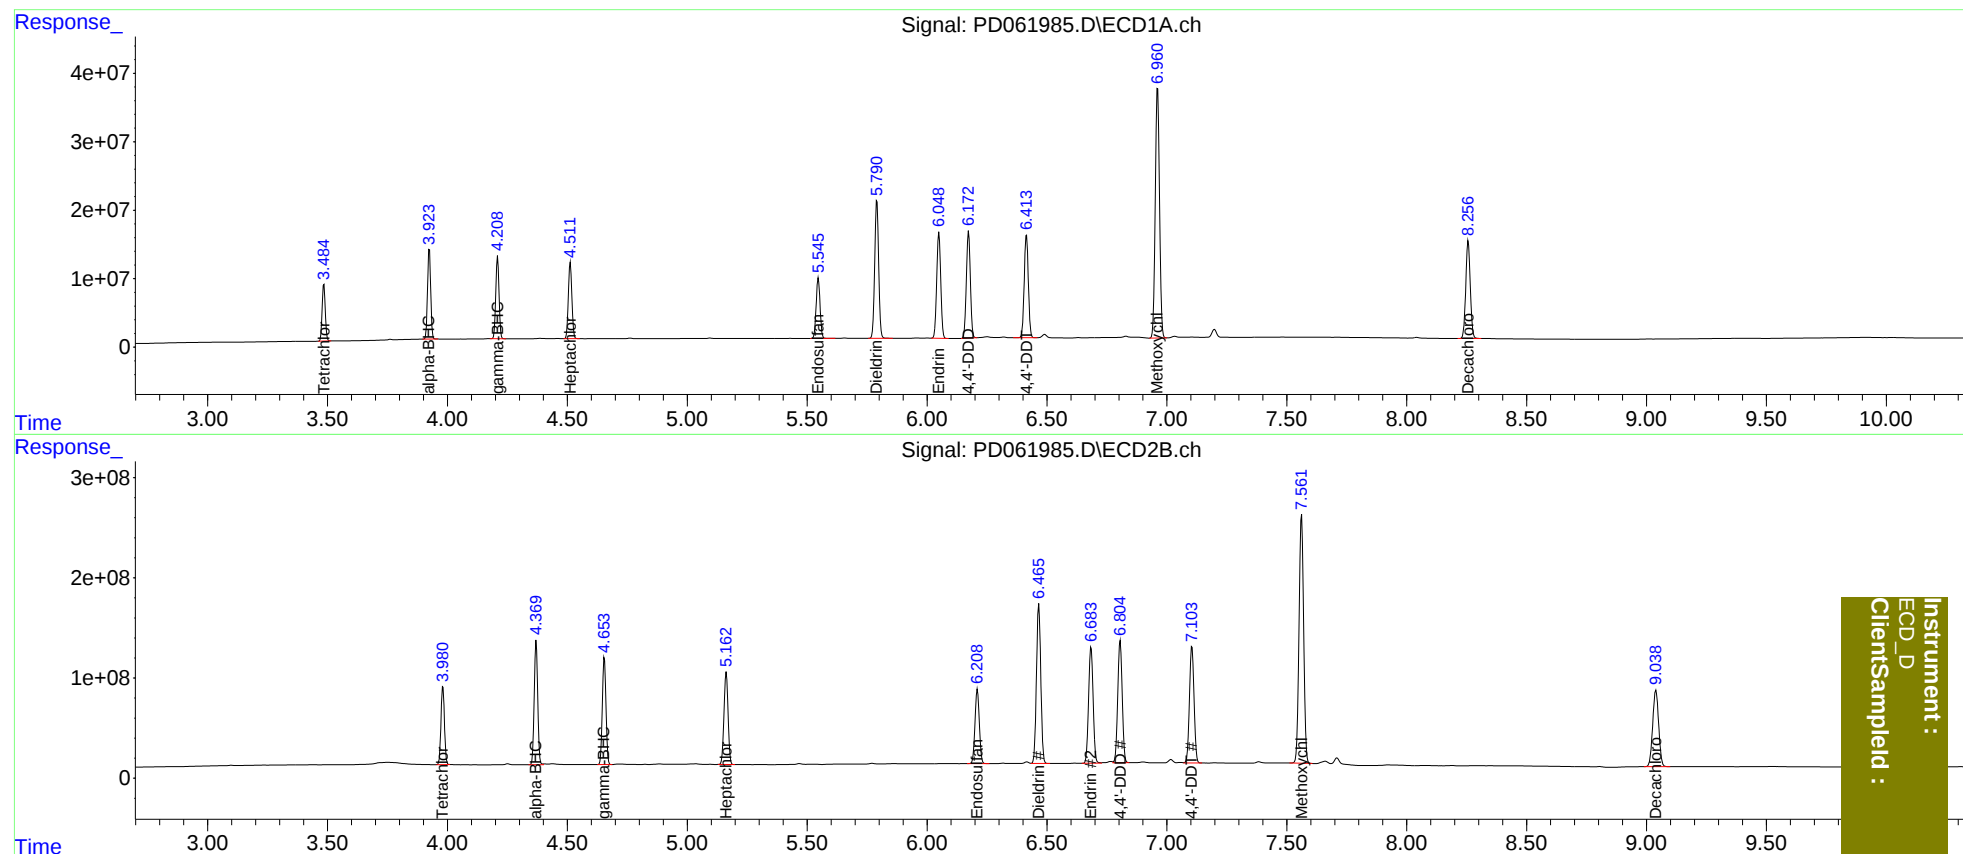


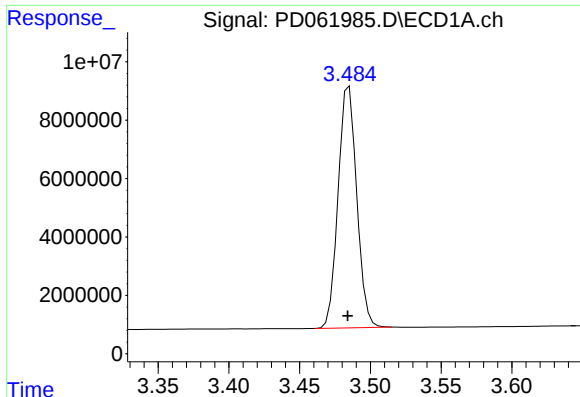

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 75974208
Conc: 79.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

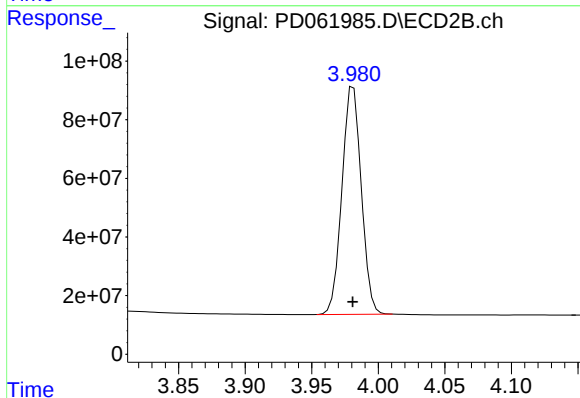


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 786949322
Conc: 79.75 ng/ml

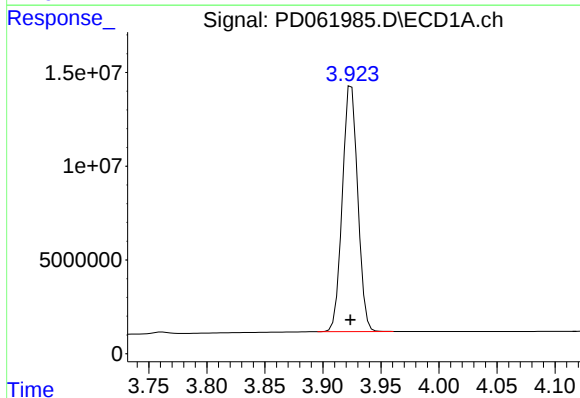


#2 alpha-BHC

R.T.: 3.925 min
Delta R.T.: 0.000 min
Response: 121074401
Conc: 87.72 ng/ml

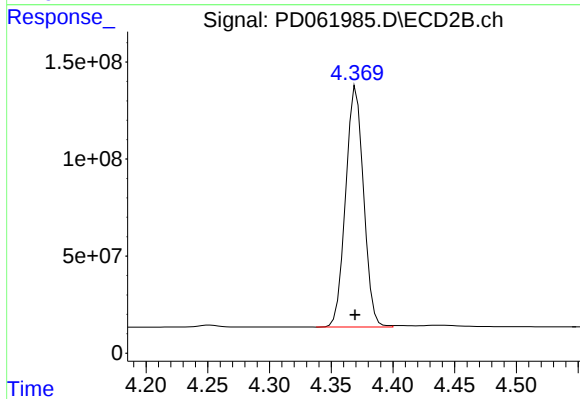

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 1253396094
Conc: 79.64 ng/ml

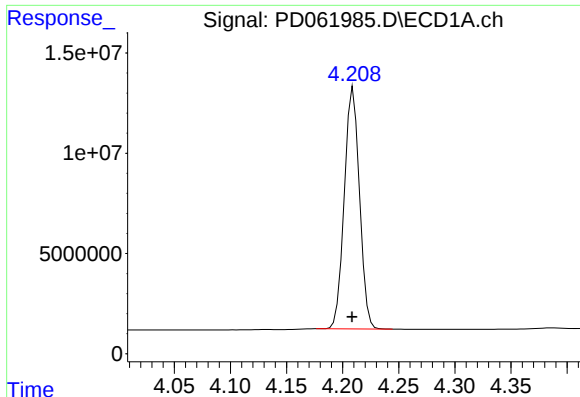

#3 gamma-BHC (Lindane)


R.T.: 4.210 min
Delta R.T.: 0.001 min
Response: 113481505
Conc: 84.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

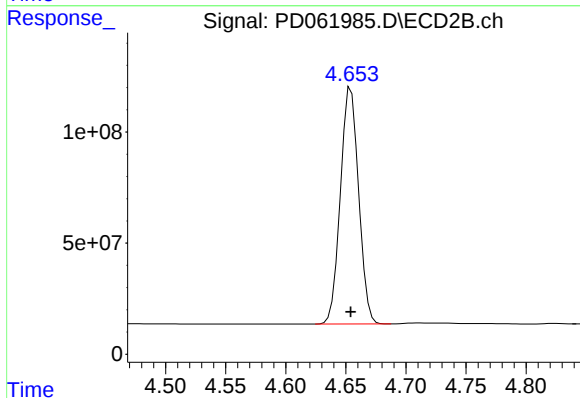


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 1126764436
Conc: 80.27 ng/ml

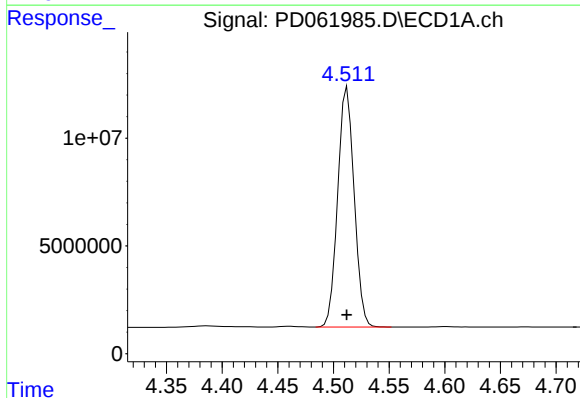


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 114396267
Conc: 82.16 ng/ml

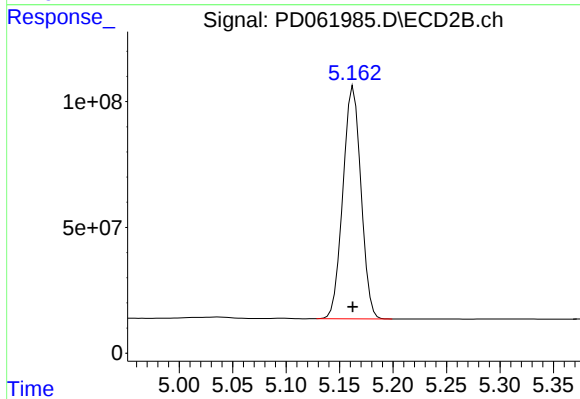

#4 Heptachlor


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 1087831687
Conc: 79.37 ng/ml

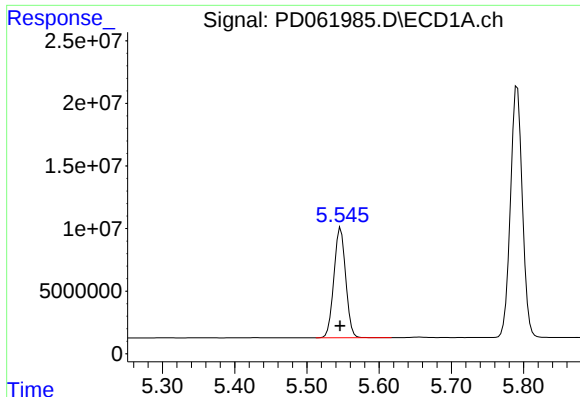

#9 Endosulfan I


R.T.: 5.547 min
Delta R.T.: 0.001 min
Response: 99733045
Conc: 80.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

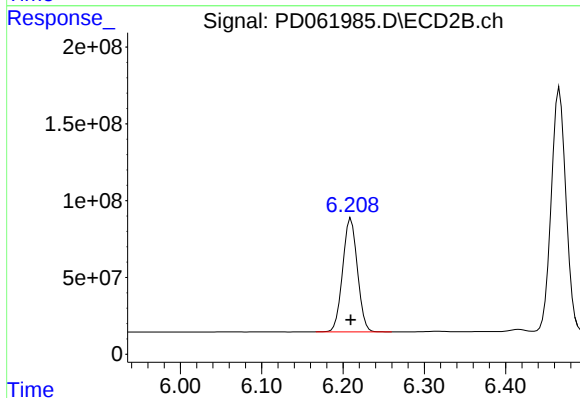


#9 Endosulfan I

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 928002793
Conc: 76.27 ng/ml

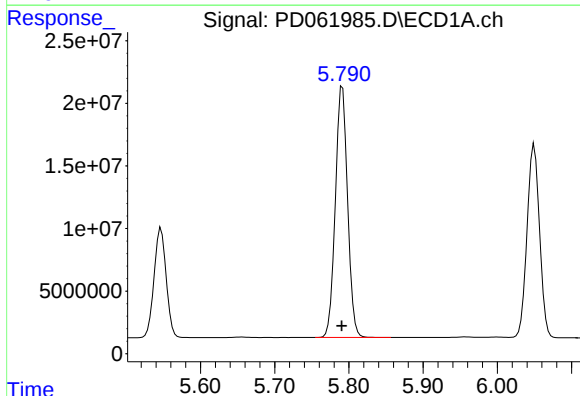


#13 Dieldrin

R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 230310197
Conc: 167.95 ng/ml

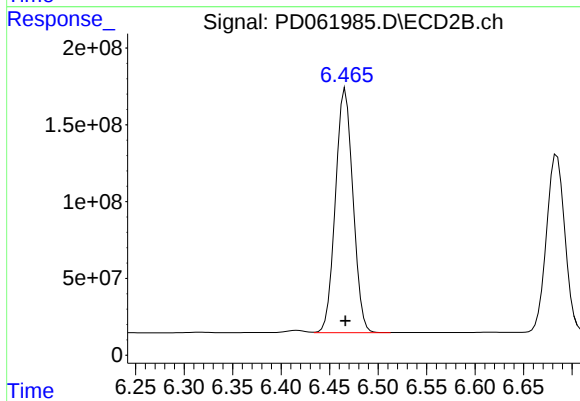

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 1995040140
Conc: 152.59 ng/ml

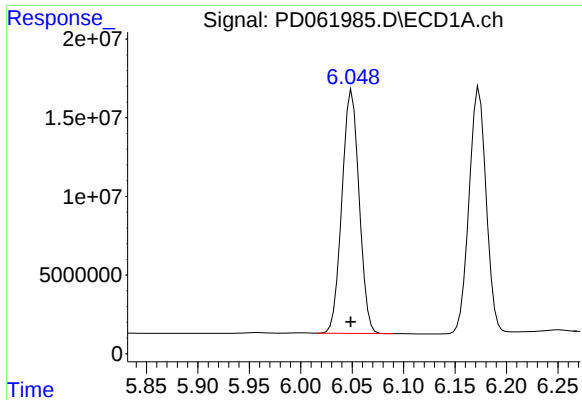

#14 Endrin


R.T.: 6.050 min
Delta R.T.: 0.001 min
Response: 179904421
Conc: 154.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

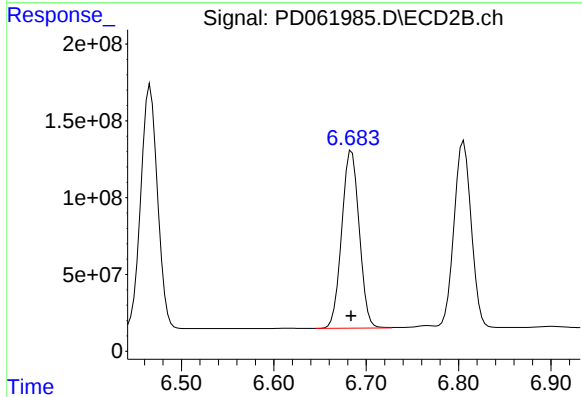


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 1524649785
Conc: 142.81 ng/ml

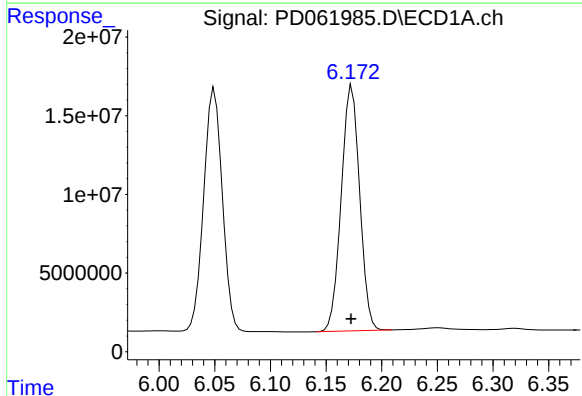


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 179659357
Conc: 167.86 ng/ml

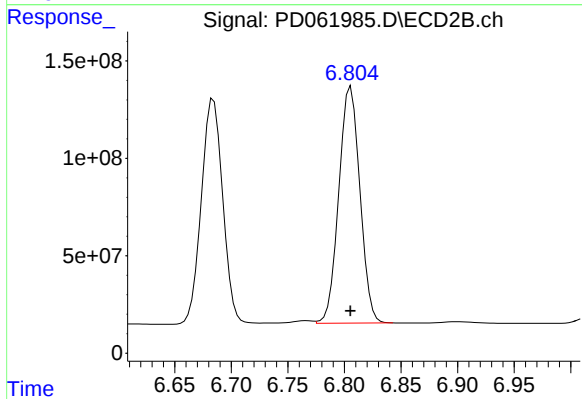

#16 4,4'-DDD


R.T.: 6.806 min
Delta R.T.: 0.000 min
Response: 1577717696
Conc: 152.89 ng/ml

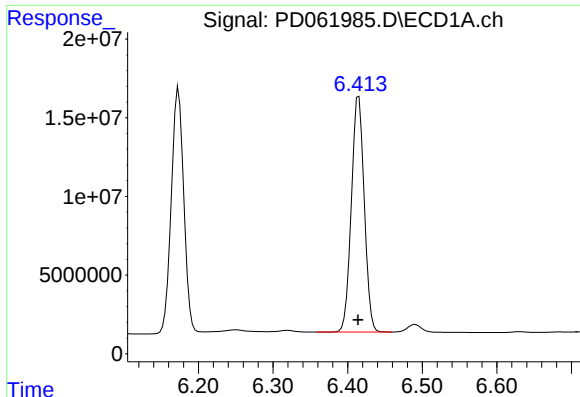

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 179421691
Conc: 171.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

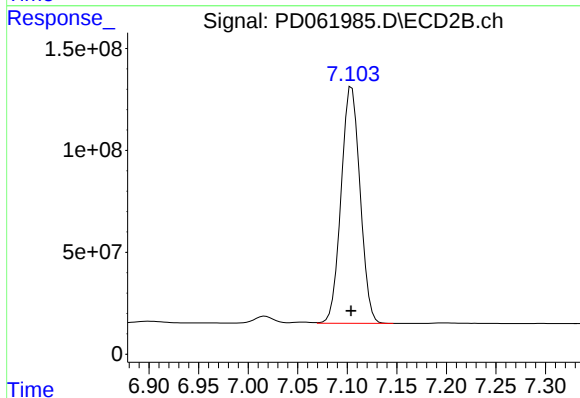


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 1544206712
Conc: 154.57 ng/ml

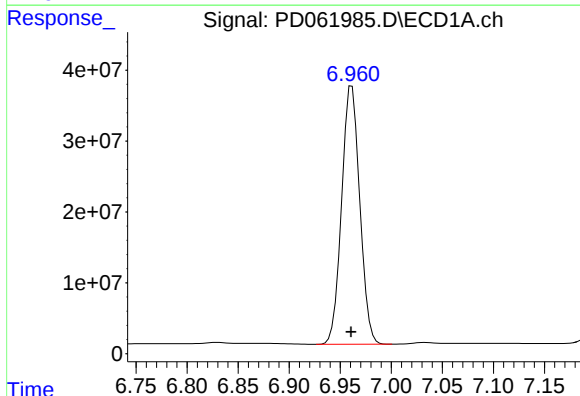


#20 Methoxychlor

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 450838813
Conc: 758.49 ng/ml

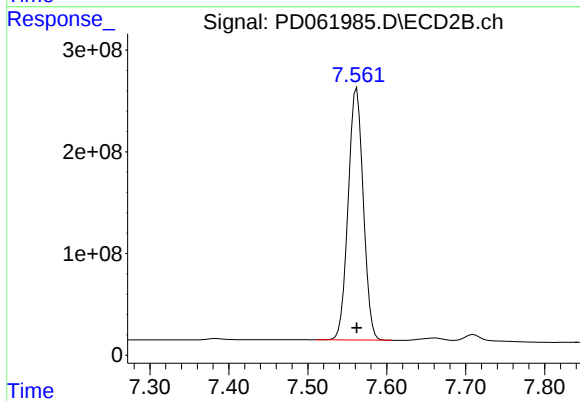

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.000 min
Response: 3304034874
Conc: 703.05 ng/ml

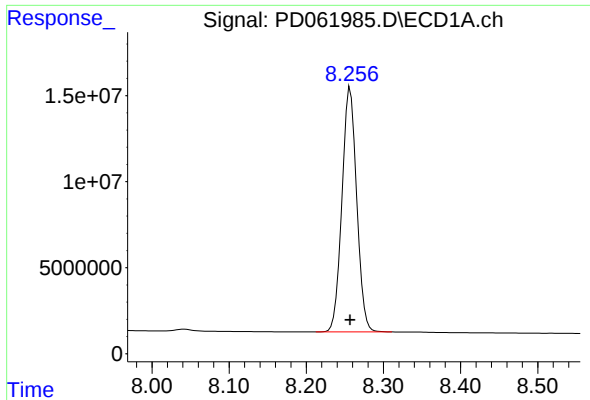

#27 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 187814395
Conc: 143.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

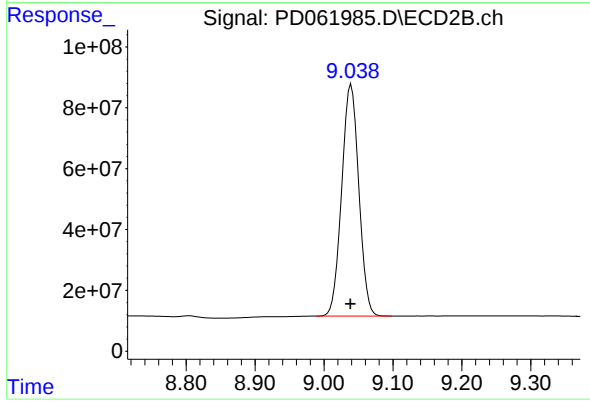

#27 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.001 min
Response: 1315131331
Conc: 145.90 ng/ml