

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
 Data File : PD061983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 19:33
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 04:29:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 04:27:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	37301127	388.8E6	39.032	39.406
27)	SA Decachlor...	8.256	9.039	97597874	675.8E6	74.603	74.974
Target Compounds							
2)	A alpha-BHC	3.925	4.370	56616424	632.3E6	41.019	40.174
3)	MA gamma-BHC...	4.209	4.655	54353030	577.5E6	40.354	41.140
4)	MA Heptachlor	4.512	5.163	55253594	574.3E6	39.681	41.899
9)	A Endosulfan I	5.547	6.210	48975931	470.0E6	39.429	38.625
13)	MA Dieldrin	5.791	6.466	111.1E6	1004.5E6	81.008	76.829
14)	MA Endrin	6.050	6.684	91943251	794.9E6	78.820	74.460
16)	A 4,4'-DDD	6.173	6.806	87232955	787.0E6	81.503	76.268
17)	MA 4,4'-DDT	6.415	7.104	87892883	769.6E6	83.791	77.028
20)	A Methoxychlor	6.961	7.562	229.9E6	1736.9E6	386.744	369.595

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040321\
Data File : PD061983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 19:33
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 04:29:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 04:27:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

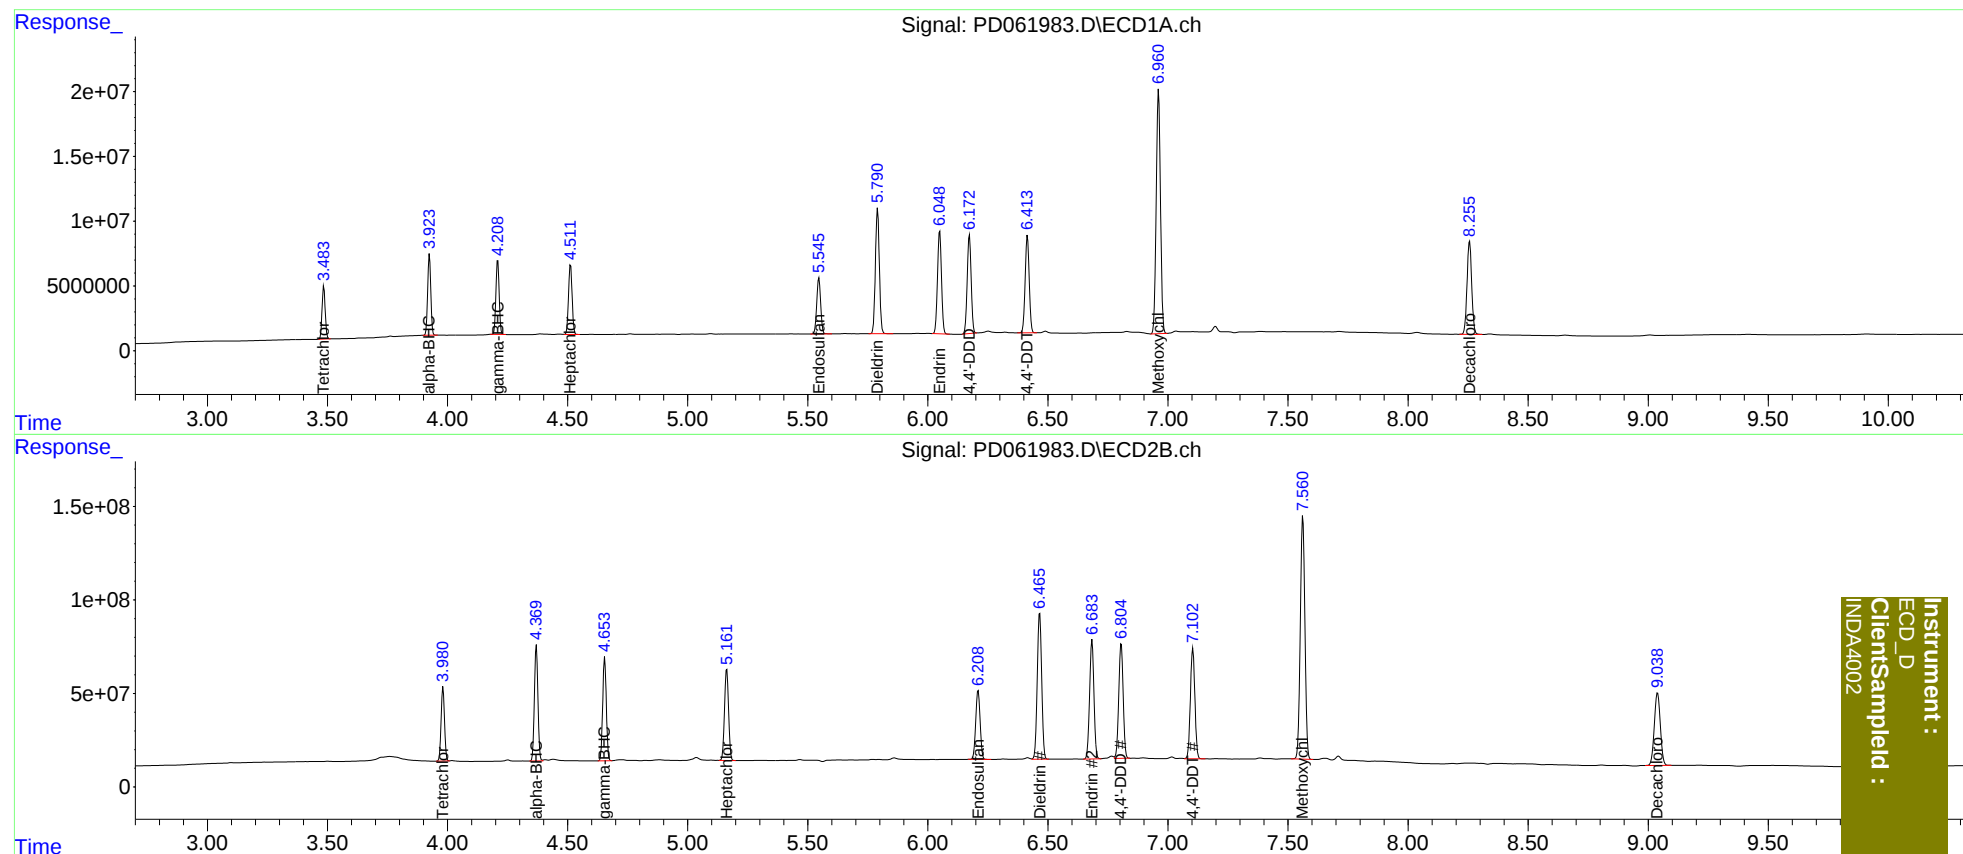

Instrument :
ECD_D
ClientSampled :
INDA4002