

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040322\
 Data File : PD068891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 12:37
 Operator : AR\AJ
 Sample : N2207-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20220340-096-21-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 23:26:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.454	4.174	25087155	233.8E6	20.662	24.457
28) SA Decachlor...	8.215	9.376	24459445	122.7E6	19.360	21.659

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040322\
Data File : PD068891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 12:37
Operator : AR\AJ
Sample : N2207-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20220340-096-21-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 23:26:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

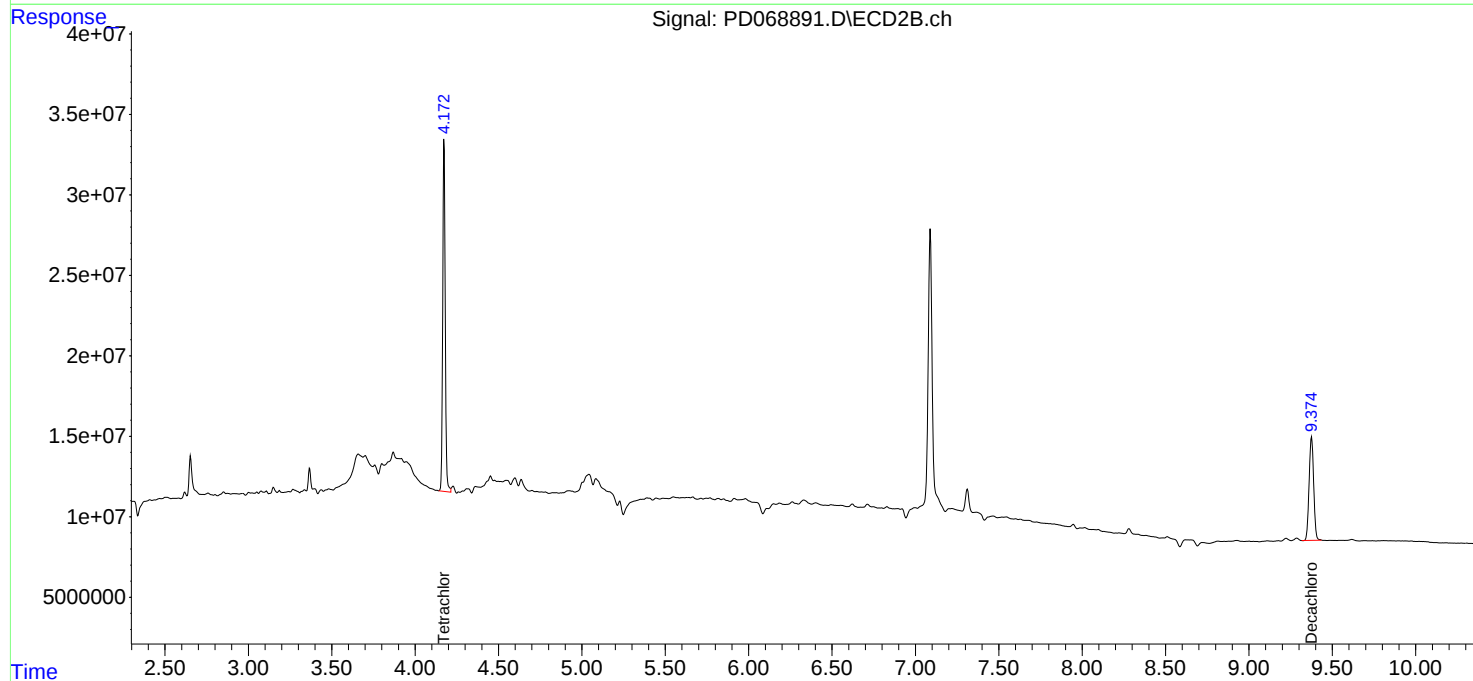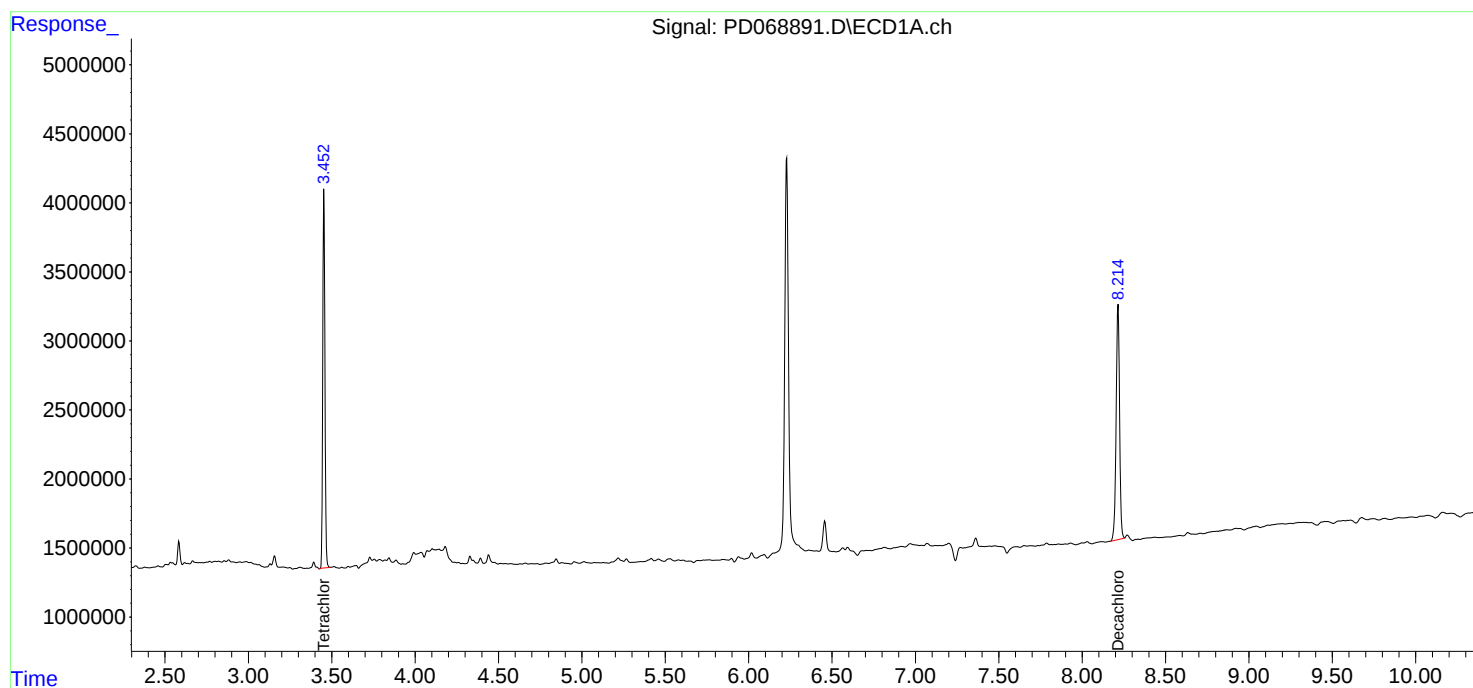


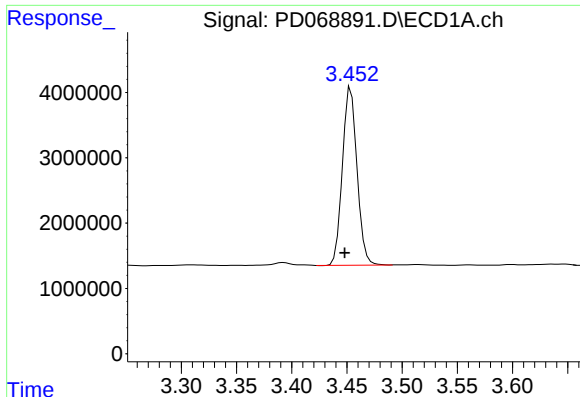

#1 Tetrachloro-m-xylene


R.T.: 3.454 min
Delta R.T.: 0.006 min
Response: 25087155
Conc: 20.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
20220340-096-21-01

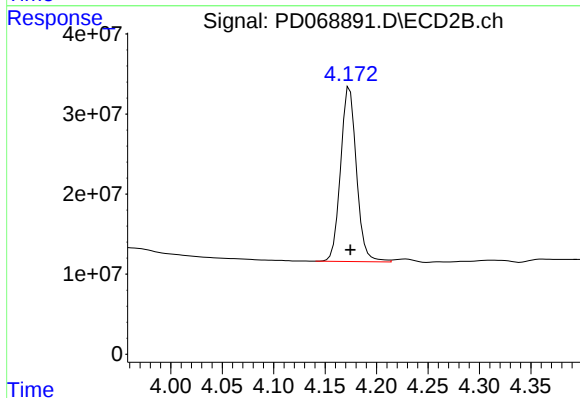


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: 0.000 min
Response: 233824792
Conc: 24.46 ng/ml

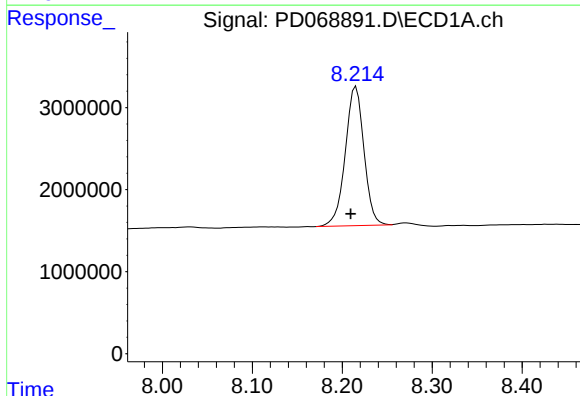

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.006 min
Response: 24459445
Conc: 19.36 ng/ml

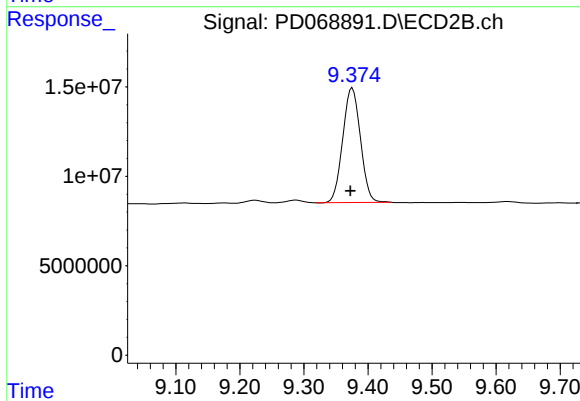

#28 Decachlorobiphenyl

R.T.: 9.376 min
Delta R.T.: 0.003 min
Response: 122735080
Conc: 21.66 ng/ml