

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040322\
 Data File : PD068900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 15:14
 Operator : AR\AJ
 Sample : N2207-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20220352-AMENDED-098-21-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 23:36:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.173	13122918	125.4E6	10.808	13.117
28) SA Decachlor...	8.207	9.372	13509194	70443852	10.693	12.431
Target Compounds						
12) B 4,4'-DDE	5.610	6.552	496254	5735530	0.363	0.619 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040322\
Data File : PD068900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 15:14
Operator : AR\AJ
Sample : N2207-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20220352-AMENDED-098-21-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 23:36:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

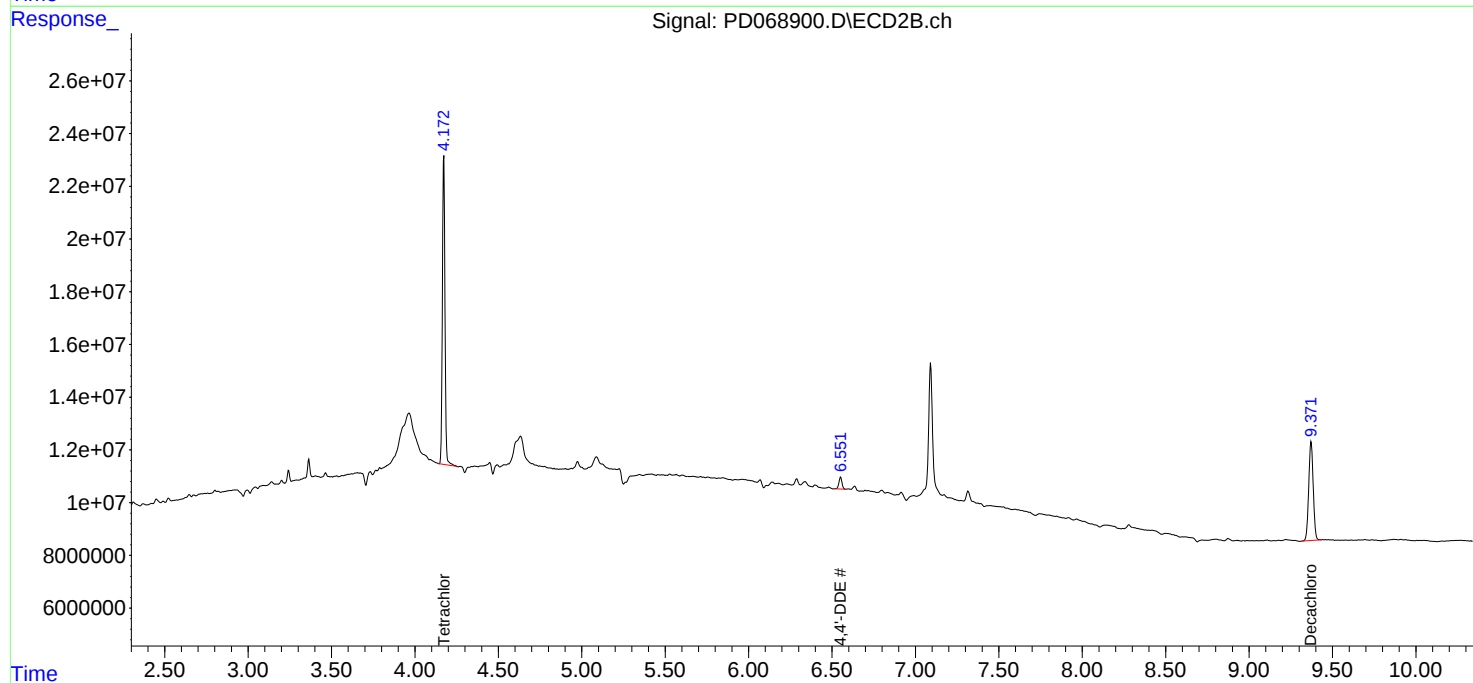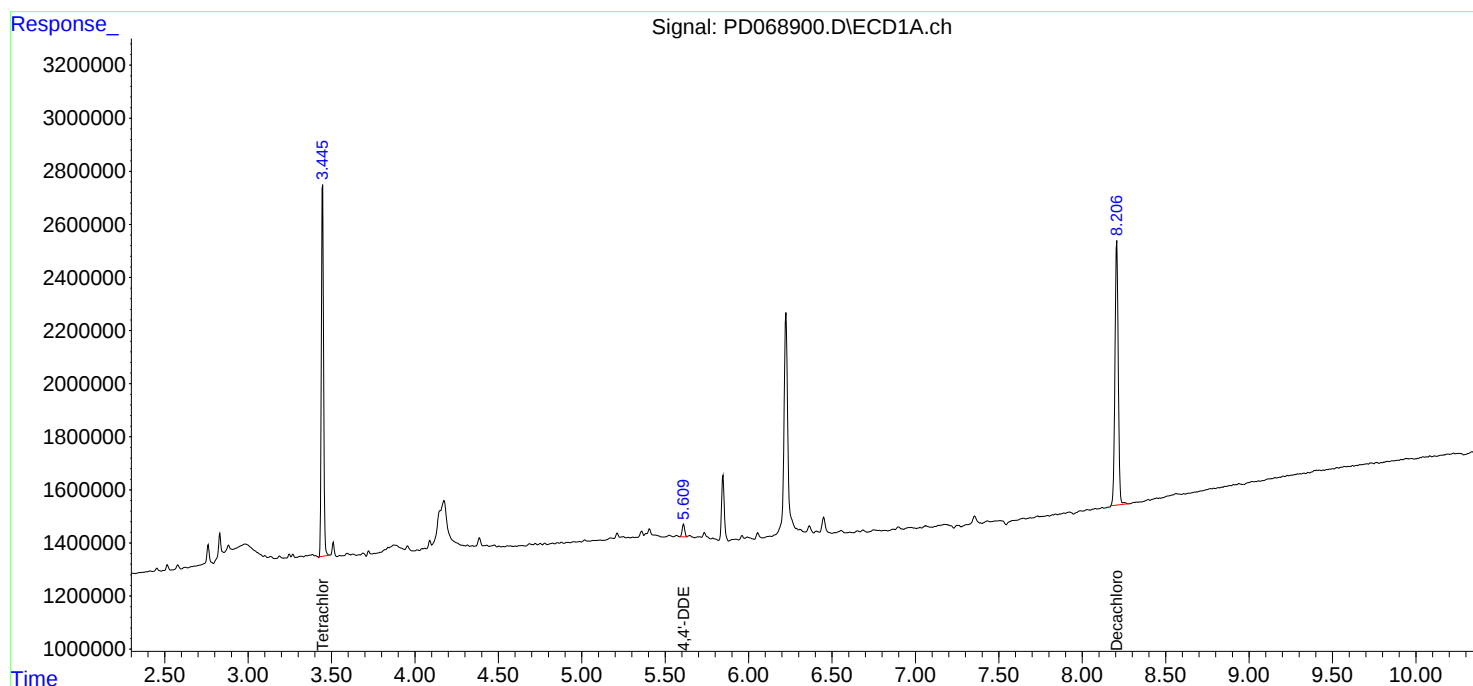


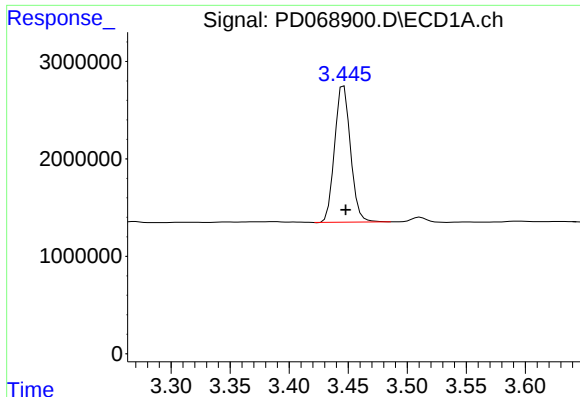

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 13122918
Conc: 10.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
20220352-AMENDED-098-21-01

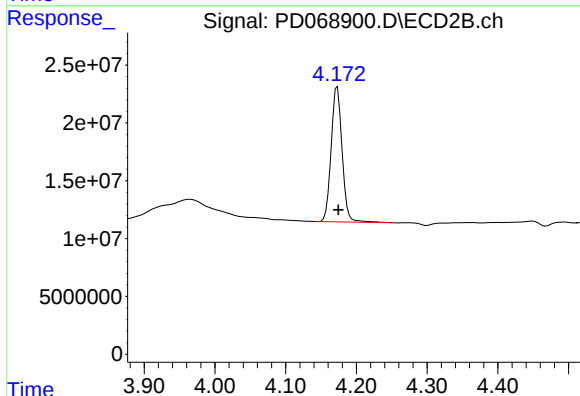


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.002 min
Response: 125411896
Conc: 13.12 ng/ml

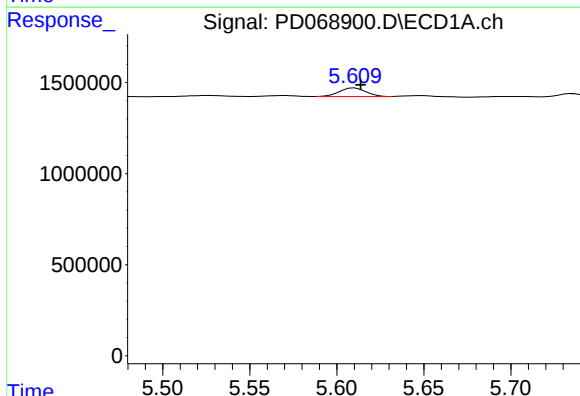


#12 4,4'-DDE

R.T.: 5.610 min
Delta R.T.: -0.003 min
Response: 496254
Conc: 0.36 ng/ml

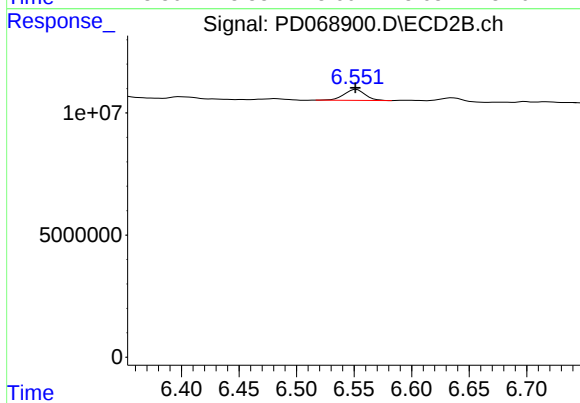

#12 4,4'-DDE


R.T.: 6.552 min
Delta R.T.: 0.000 min
Response: 5735530
Conc: 0.62 ng/ml

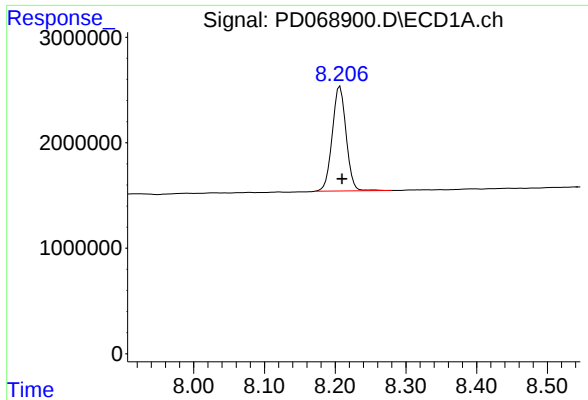

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.003 min
Response: 13509194
Conc: 10.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
20220352-AMENDED-098-21-01

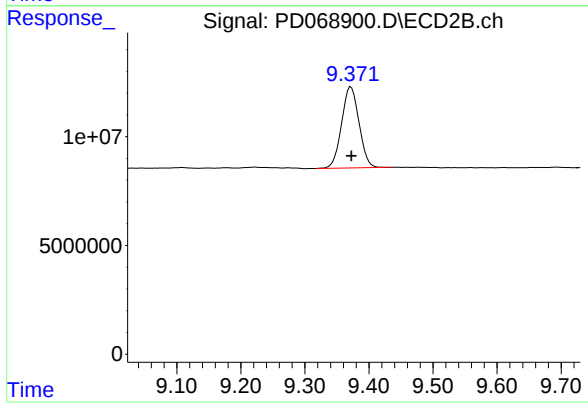

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 70443852
Conc: 12.43 ng/ml