

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
 Data File : PD074566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 14:54
 Operator : AR\AJ
 Sample : 02122-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9A8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/04/2023
 Supervised By : Ankita Jodhani 04/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 22:17:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.560	2.773	47893635	25111543	19.278	19.960
27) SA Decachlor...	9.110	7.928	98256428	43406528	35.900	36.251
Target Compounds						
9) A Endosulfan I	6.092	5.143	4317725	870115	1.447m	0.621m#
12) B 4,4'-DDE	6.190	5.250	1096448	1198127	0.366m	0.825 #
13) MA Dieldrin	6.374	5.367	1901031	721124	0.599m	0.465m
17) MA 4,4'-DDT	7.045	6.062	932144	3396191	0.371m	2.711m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
Data File : PD074566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 14:54
Operator : AR\AJ
Sample : 02122-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 22:17:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

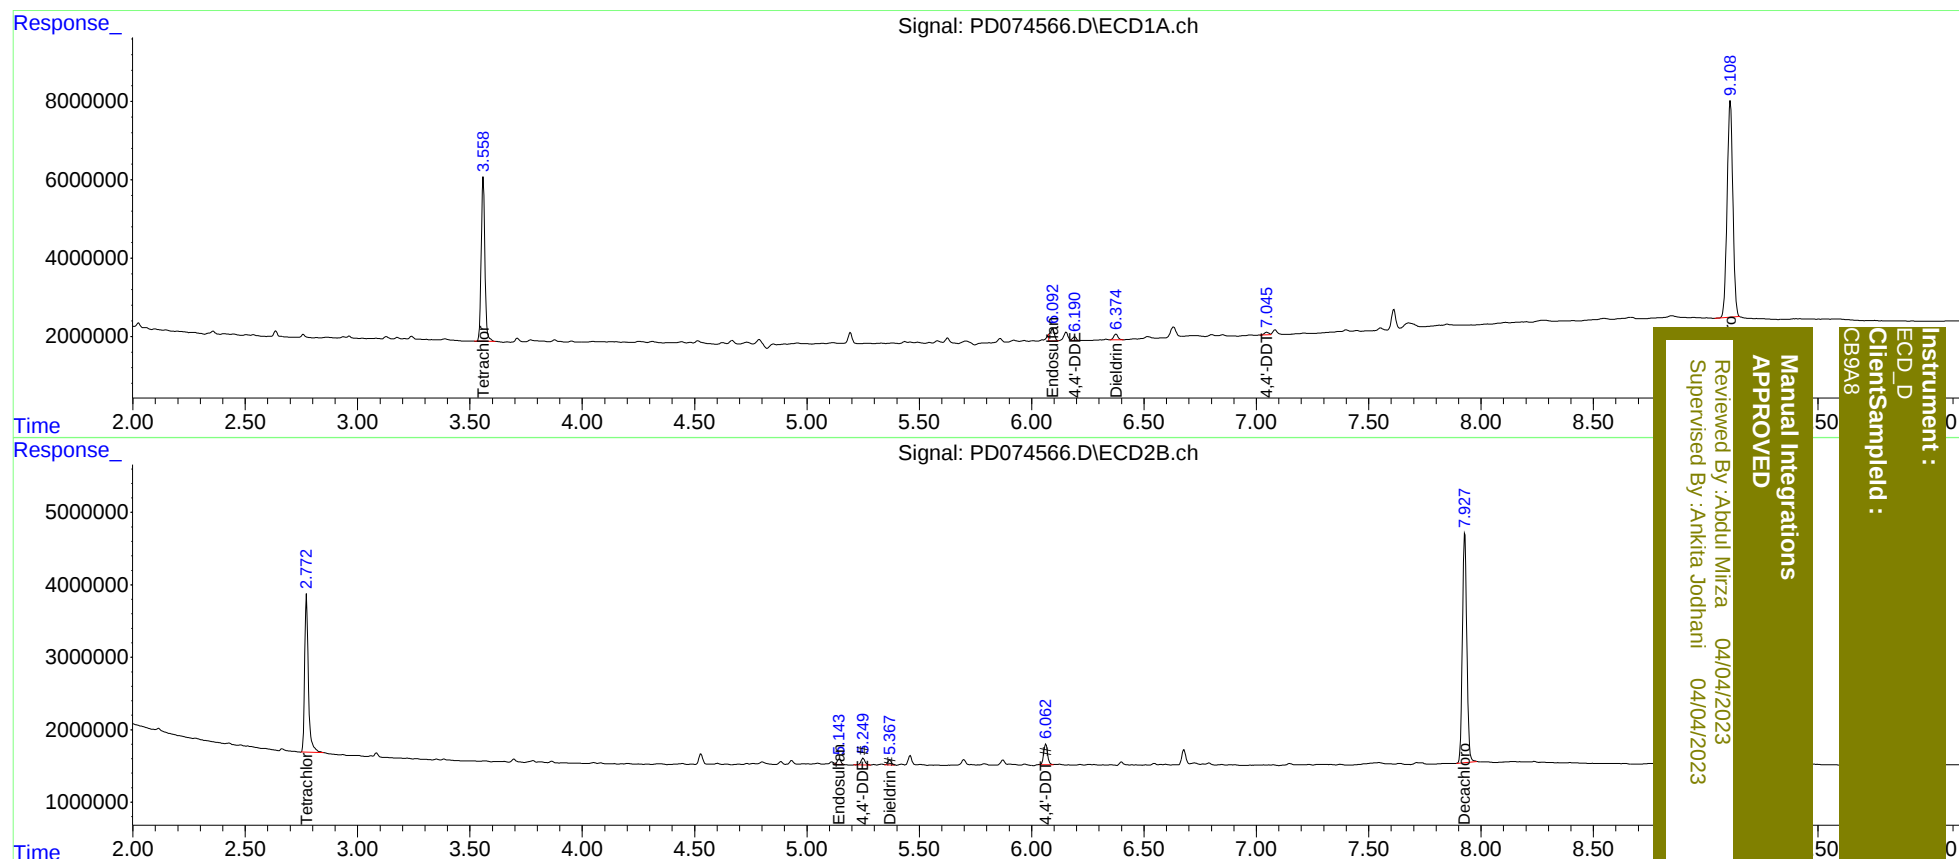

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/04/2023
Supervised By: Ankita Jodhani 04/04/2023

Instrument :
ECD_D
Client Sampled :
CB9A8