

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
 Data File : PD074570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 15:48
 Operator : AR\AJ
 Sample : 02122-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9B2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/04/2023
 Supervised By : Ankita Jodhani 04/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 22:18:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.772	49753596	25781117	20.026	20.492
27) SA Decachlor...	9.098	7.925	105.3E6	45656026	38.474	38.129
Target Compounds						
12) B 4,4'-DDE	6.180	5.248	1302056	917246	0.435m	0.631 #
13) MA Dieldrin	6.365	5.365	2751627	1179666	0.867m	0.761m
17) MA 4,4'-DDT	7.036	6.060	771482	3385354	0.307m	2.702 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
Data File : PD074570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 15:48
Operator : AR\AJ
Sample : 02122-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 22:18:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

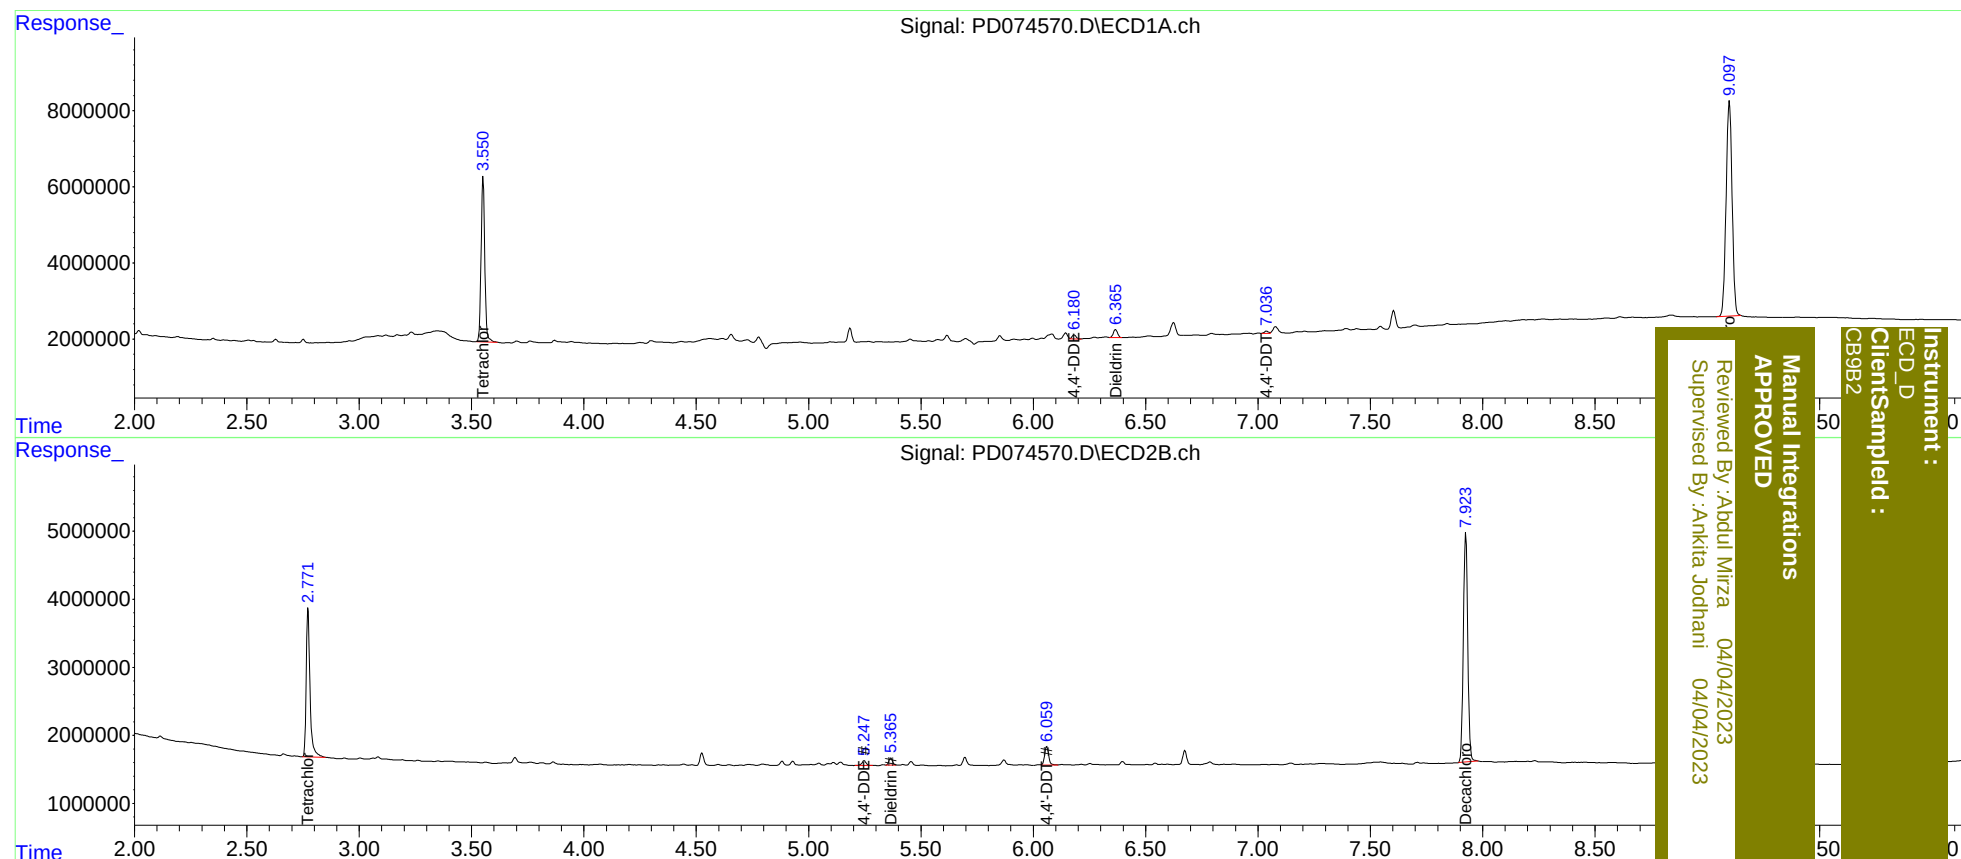

Instrument :
ECD_D
ClientSampled :
CB9B2

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/04/2023
Supervised By: Ankita Jodhani 04/04/2023