

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
 Data File : PD074567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 15:07
 Operator : AR\AJ
 Sample : 02122-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB9B0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/04/2023
 Supervised By : Ankita Jodhani 04/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:03:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.552	2.772	47631887	24197951	19.172	19.234
27) SA Decachlor...	9.100	7.924	93412886	40063703	34.130	33.459
Target Compounds						
9) A Endosulfan I	6.075	5.141	2268123	1267739	0.760m	0.904m
12) B 4,4'-DDE	6.181	5.248	1591872	1121107	0.531m	0.772 #
13) MA Dieldrin	6.365	5.364	7045625	3064579	2.221m	1.977m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040323\
Data File : PD074567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 15:07
Operator : AR\AJ
Sample : 02122-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:03:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

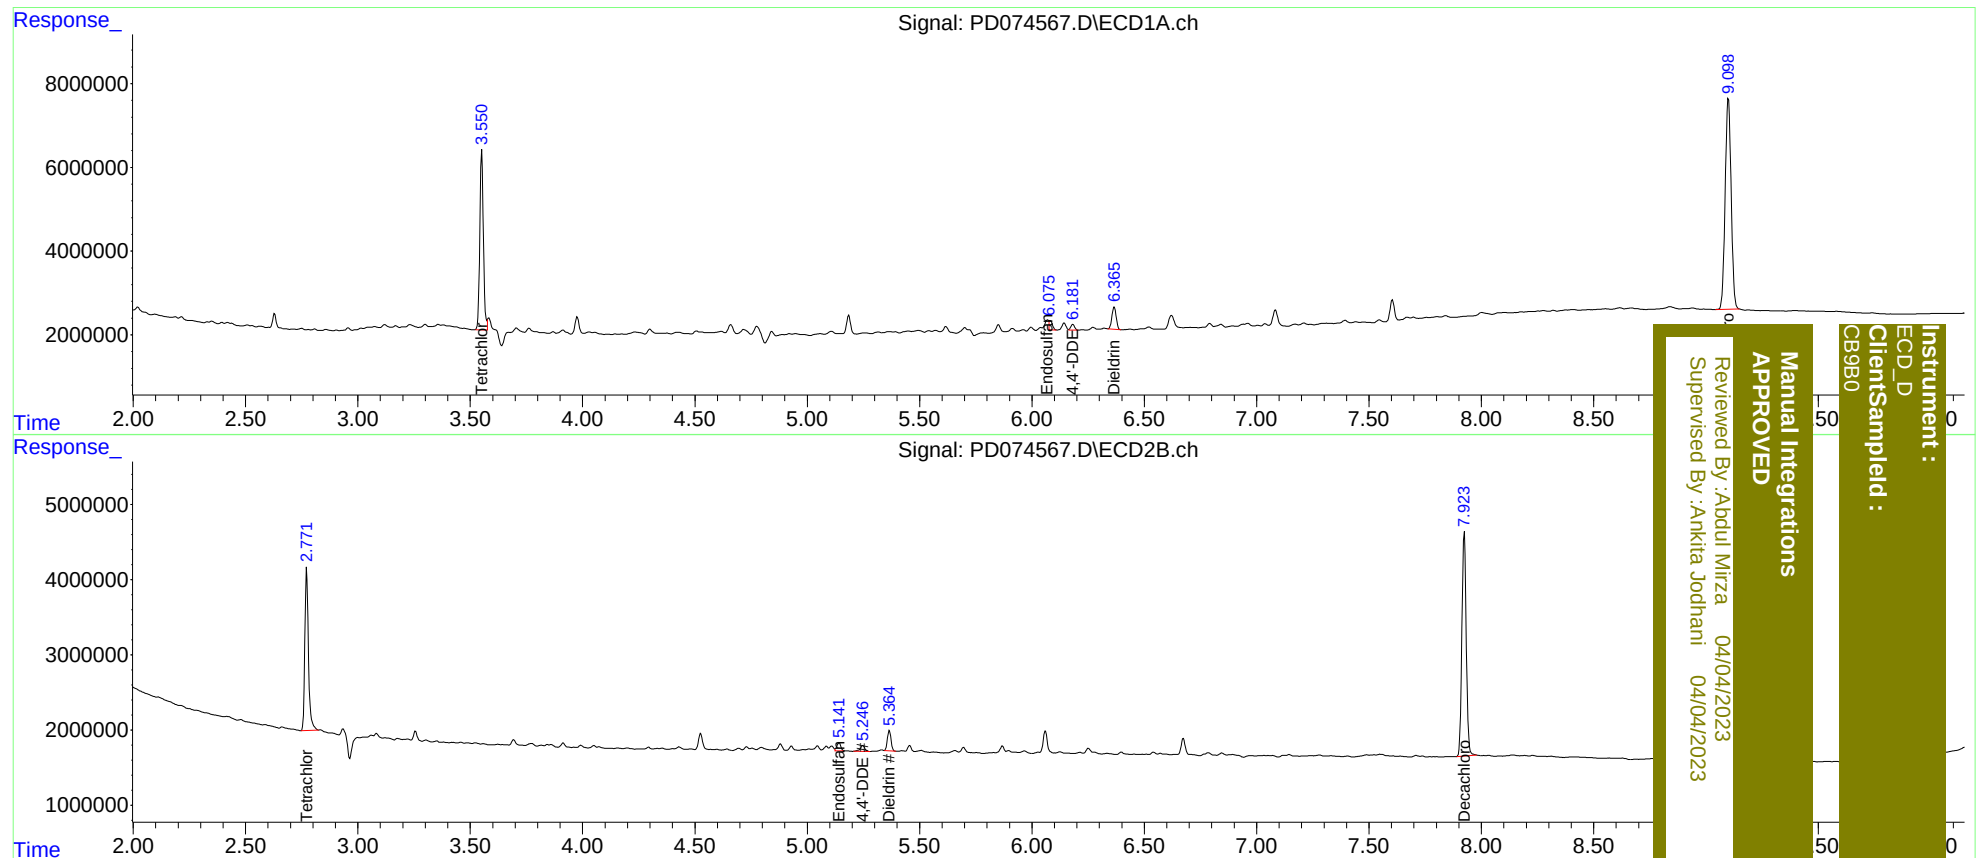

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/04/2023
Supervised By: Ankita Jodhani 04/04/2023

Instrument :
ECD_D
ClientSampled :
CB9B0