

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040324\
 Data File : PD082282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 10:44
 Operator : AR\AJ
 Sample : P1933-06MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZZZ5MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/03/2024
 Supervised By :Ankita Jodhani 04/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 12:29:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 30 04:18:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	15327507	29265360	10.365	8.748
27)	SA Decachlor...	9.118	7.911	16690668	22099980	8.983m	8.378
Target Compounds							
2)	A alpha-BHC	4.024	3.278	90130629	183.4E6	36.136	36.232
3)	MA gamma-BHC...	4.357	3.605	96948441	174.3E6	40.505m	37.741m
4)	MA Heptachlor	4.950	3.945	94224579	169.4E6	38.014m	39.524m
5)	MB Aldrin	5.295	4.226	91553277	161.3E6	39.104	38.462
6)	B beta-BHC	4.554	3.901	35899101	72568674	34.268	37.480m
7)	B delta-BHC	4.803	4.132	55543894	104.5E6	23.846	23.282
8)	B Heptachlo...	5.722	4.727	81539798	144.9E6	37.139	39.068
9)	A Endosulfan I	6.108	5.098	76561268	126.8E6	36.636m	37.332
10)	B trans-Chl...	5.979	4.978	83391643	156.8E6	40.072	43.578
11)	B cis-Chlor...	6.057	5.042	84864668	158.0E6	40.046m	42.817
12)	B 4,4'-DDE	6.230	5.230	162.1E6	334.3E6	79.605	98.078
13)	MA Dieldrin	6.386	5.361	165.2E6	311.9E6	76.676	84.959
14)	MA Endrin	6.616	5.637	144.6E6	269.8E6	81.431	87.173
15)	B Endosulfa...	6.835	5.930	138.7E6	253.5E6	78.429	83.644
16)	A 4,4'-DDD	6.749	5.784	119.5E6	226.6E6	79.746	84.104
17)	MA 4,4'-DDT	7.064	6.035	127.5E6	240.5E6	81.945	87.041
18)	B Endrin al...	6.965	6.109	99773849	187.8E6	75.276	83.243
19)	B Endosulfa...	7.201	6.332	115.8E6	220.8E6	71.055	77.485
20)	A Methoxychlor	7.540	6.610	307.0E6	522.9E6	374.545	375.124
21)	B Endrin ke...	7.688	6.837	135.2E6	257.8E6	79.074	80.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040324\
Data File : PD082282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 10:44
Operator : AR\AJ
Sample : P1933-06MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 12:29:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 30 04:18:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

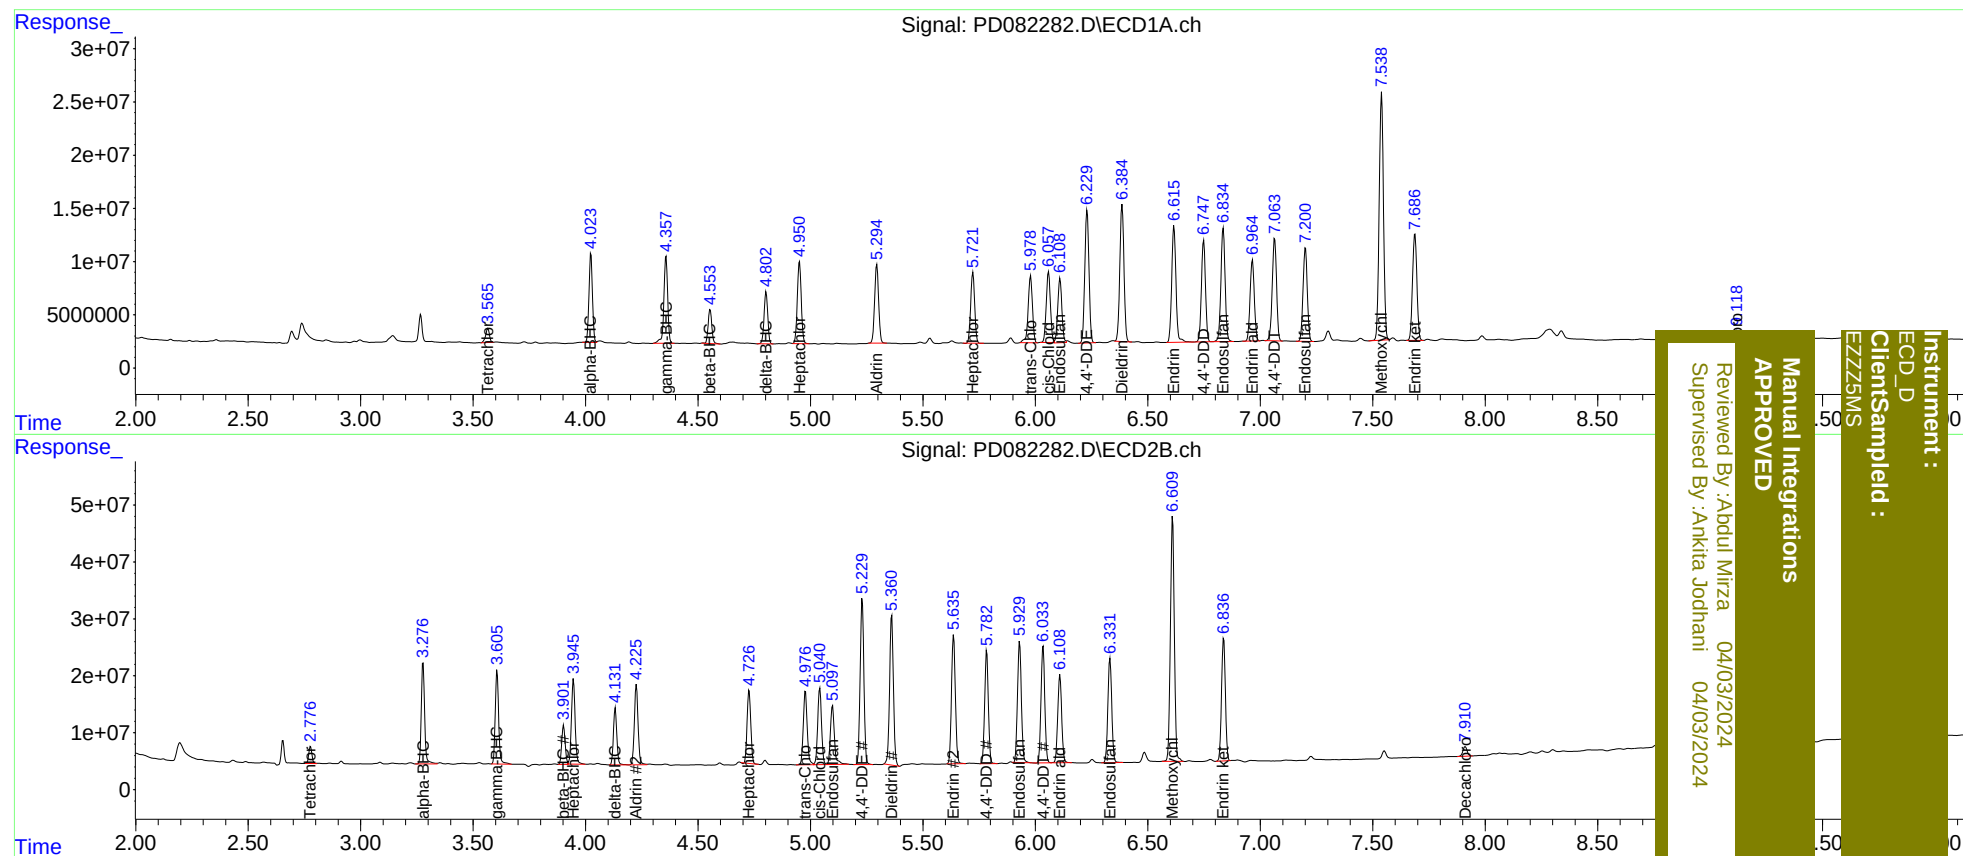

Instrument :
ECD_D
ClientSampled :
EZZZSMS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/03/2024
Supervised By :Ankita Jodhani 04/03/2024