

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040324\
 Data File : PD082283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 10:58
 Operator : AR\AJ
 Sample : P1933-07MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZZZ5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/03/2024
 Supervised By :Ankita Jodhani 04/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 12:29:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 30 04:18:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.776	16756512	31550644	11.331	9.431m
2)	SA Decachlor...	9.121	7.912	17281817	23835749	9.301m	9.036
Target Compounds							
2)	A alpha-BHC	4.024	3.278	85395598	172.3E6	34.237	34.028
3)	MA gamma-BHC...	4.356	3.607	91296467	165.3E6	38.143m	35.792
4)	MA Heptachlor	4.950	3.945	88668528	162.0E6	35.772m	37.799m
5)	MB Aldrin	5.295	4.226	81188369	152.7E6	34.677	36.426
6)	B beta-BHC	4.554	3.901	33426497	67739117	31.908	34.986m
7)	B delta-BHC	4.803	4.133	51386688	98615427	22.061	21.973
8)	B Heptachlo...	5.722	4.727	77718461	142.1E6	35.399	38.335
9)	A Endosulfan I	6.108	5.098	73664807	116.0E6	35.250m	34.166
10)	B trans-Chl...	5.978	4.977	79325250	147.2E6	38.118	40.906
11)	B cis-Chlor...	6.057	5.042	81836307	149.2E6	38.617m	40.418
12)	B 4,4'-DDE	6.230	5.230	153.3E6	322.4E6	75.296	94.580 #
13)	MA Dieldrin	6.386	5.362	154.5E6	297.0E6	71.703	80.916
14)	MA Endrin	6.616	5.637	133.6E6	254.5E6	75.254	82.210
15)	B Endosulfa...	6.835	5.930	127.6E6	243.2E6	72.105	80.252
16)	A 4,4'-DDD	6.748	5.784	112.6E6	212.8E6	75.104	78.980
17)	MA 4,4'-DDT	7.064	6.035	118.4E6	225.5E6	76.103	81.607
18)	B Endrin al...	6.966	6.109	92100629	175.9E6	69.487	77.957
19)	B Endosulfa...	7.201	6.332	107.4E6	207.6E6	65.900	72.830
20)	A Methoxychlor	7.540	6.610	282.4E6	493.4E6	344.541	354.000
21)	B Endrin ke...	7.688	6.838	124.1E6	242.1E6	72.584	75.687

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040324\
Data File : PD082283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 10:58
Operator : AR\AJ
Sample : P1933-07MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 12:29:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 30 04:18:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

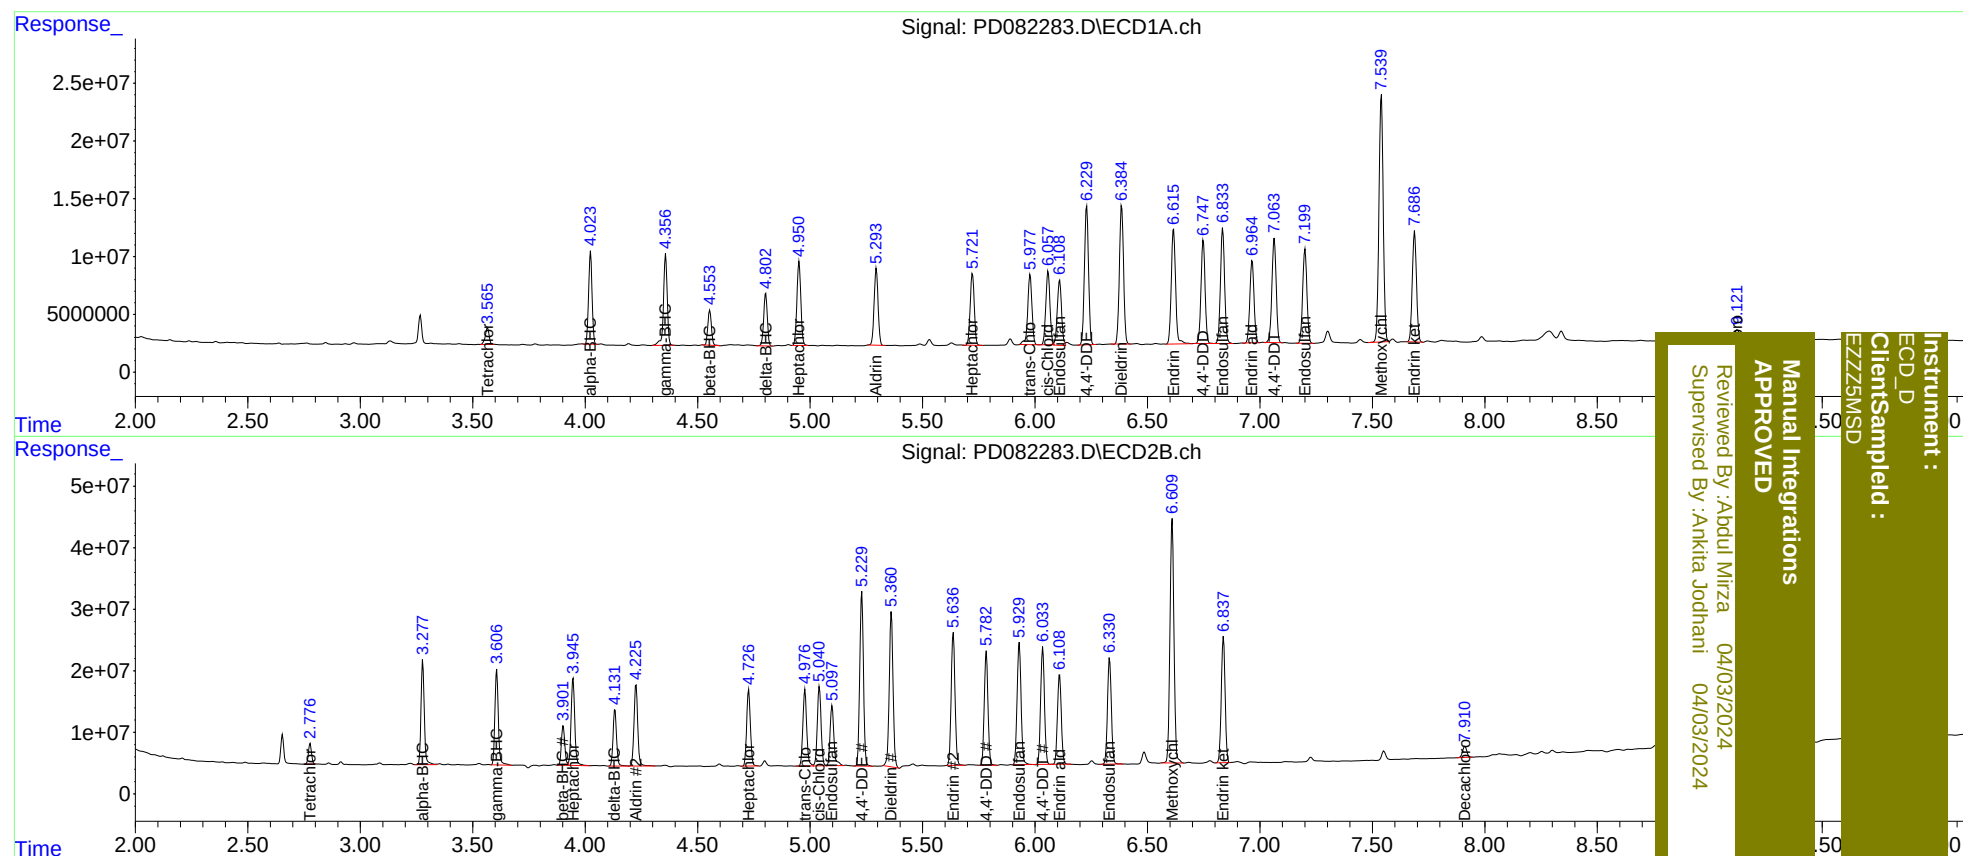

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/03/2024
Supervised By: Ankita Jodhani 04/03/2024

Instrument :
ECD_D
Client Sampled :
EZZZ5MSD