

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
 Data File : PD052535.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2019 19:56
 Operator : AJ\SJ
 Sample : K2148-08
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5G5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:26:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 01 19:09:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.042	20565751	473.3E6	14.499	14.810
27)	SA Decachlor...	7.816	9.157	35606538	430.3E6	23.701	22.133
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0 48847486	N.D.	1.014	
3)	MA gamma-BHC...	3.920	4.688f	4339828 15900120	1.962	0.363	#
7)	B delta-BHC	0.000	5.080f	0 54375072	N.D.	1.240	
8)	B Heptachlo...	0.000	5.909	0 90008906	N.D.	2.361	
10)	B trans-Chl...	0.000	6.179	0 4079862	N.D.	0.108	
11)	B cis-Chlor...	0.000	6.179f	0 4079862	N.D.	0.113	
13)	MA Dieldrin	0.000	6.546	0 15875605	N.D.	0.460	
15)	B Endosulfa...	0.000	6.985	0 55062777	N.D.	1.933	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040419\
Data File : PD052535.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2019 19:56
Operator : AJ\SJ
Sample : K2148-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:26:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040219CLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 01 19:09:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

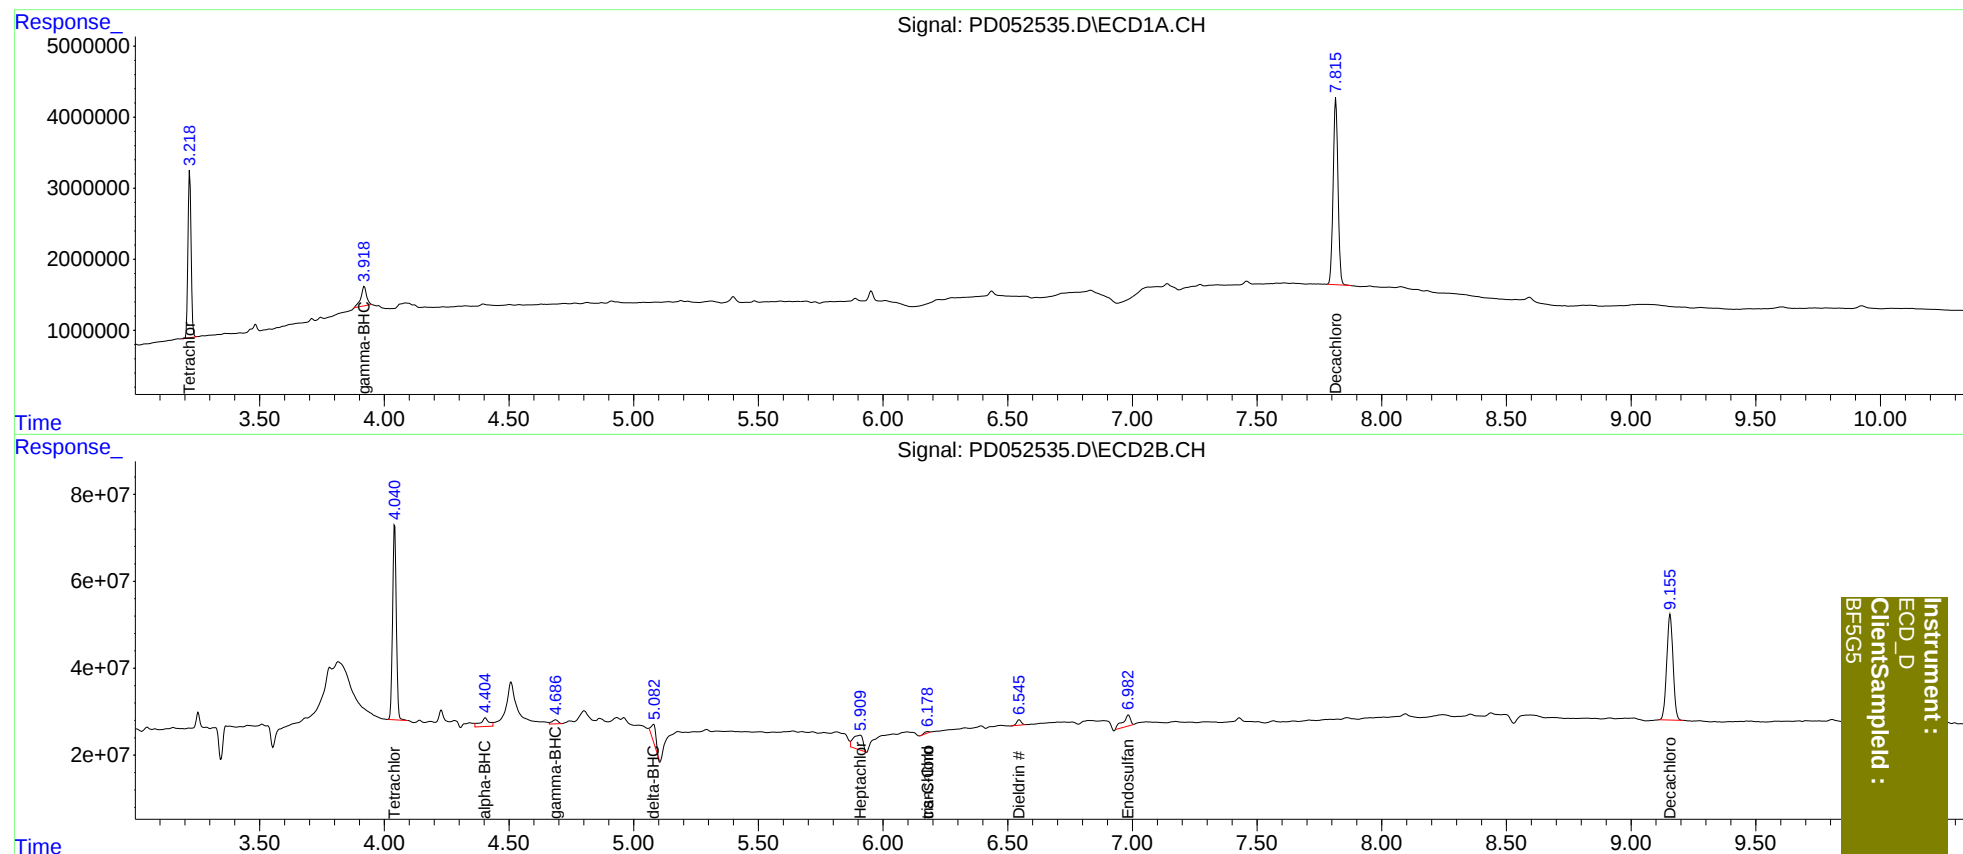


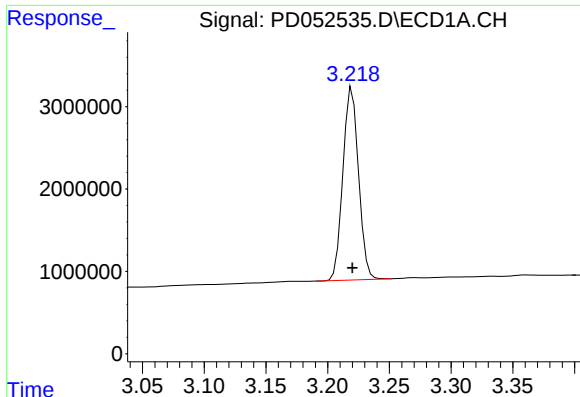

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 20565751
Conc: 14.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5G5

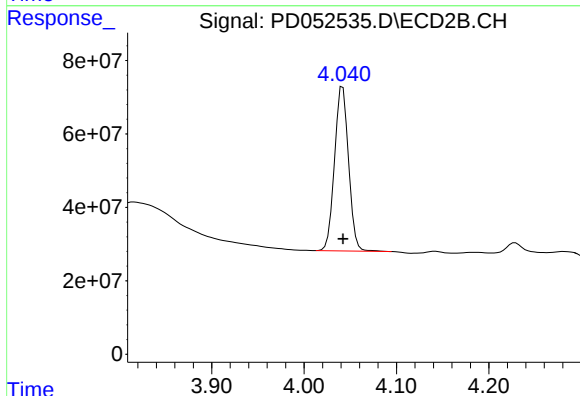


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 473262494
Conc: 14.81 ng/ml

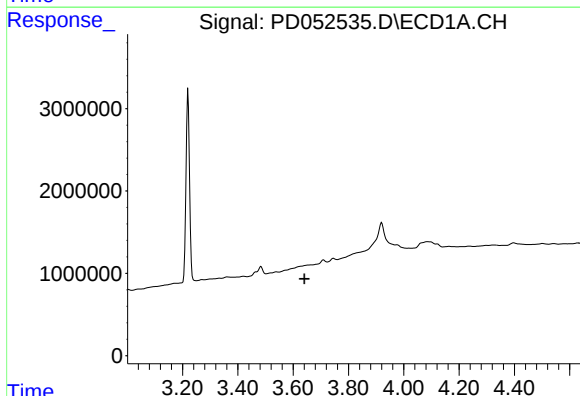


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

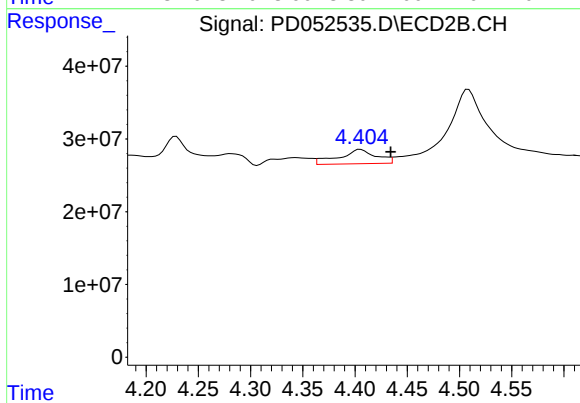

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.029 min
Response: 48847486
Conc: 1.01 ng/ml

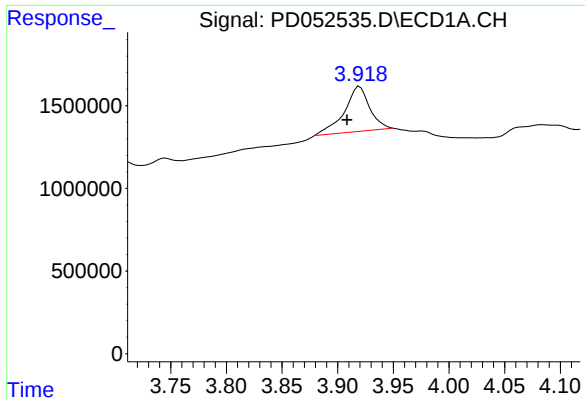

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.011 min
Response: 4339828
Conc: 1.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5G5

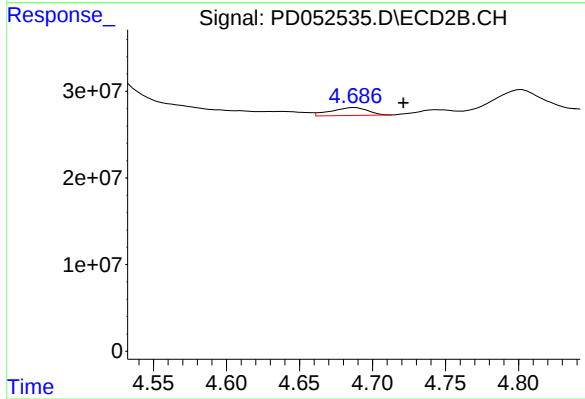


#3 gamma-BHC (Lindane)

R.T.: 4.688 min
Delta R.T.: -0.033 min
Response: 15900120
Conc: 0.36 ng/ml

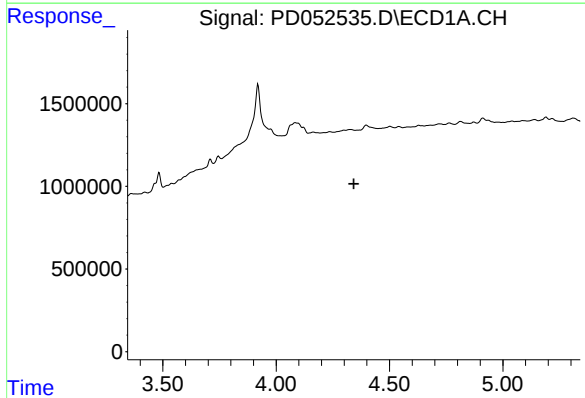


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

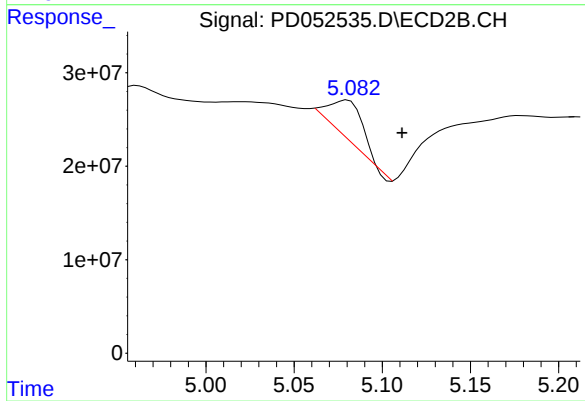

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.031 min
Response: 54375072
Conc: 1.24 ng/ml

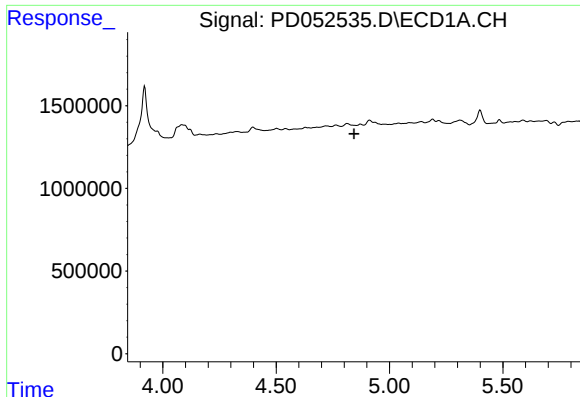

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5G5

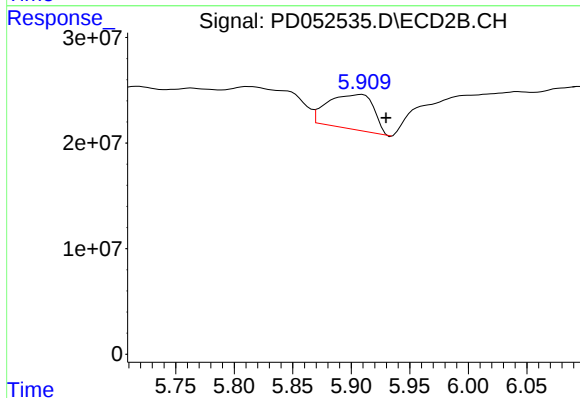


#8 Heptachlor epoxide

R.T.: 5.909 min
Delta R.T.: -0.020 min
Response: 90008906
Conc: 2.36 ng/ml

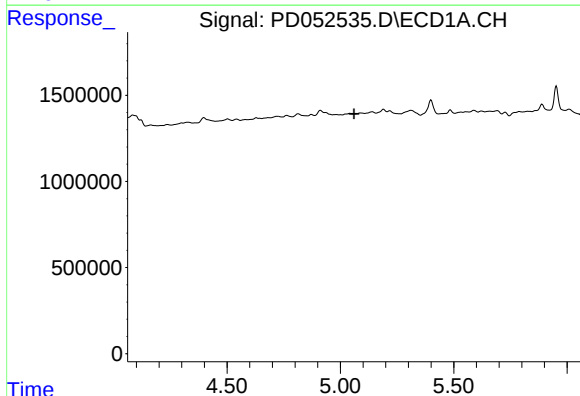


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

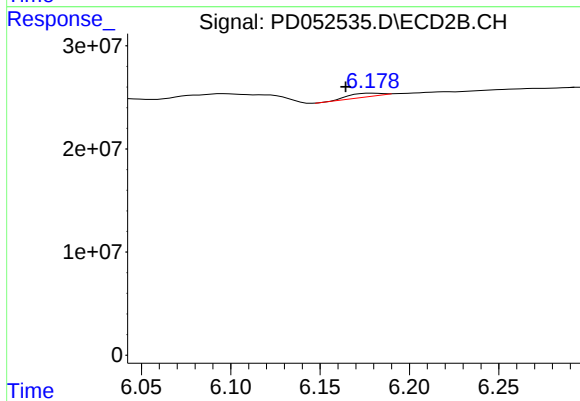

#10 trans-Chlordane


R.T.: 6.179 min
Delta R.T.: 0.015 min
Response: 4079862
Conc: 0.11 ng/ml

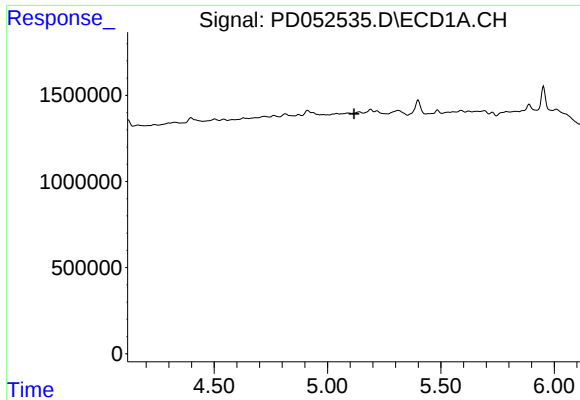

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5G5

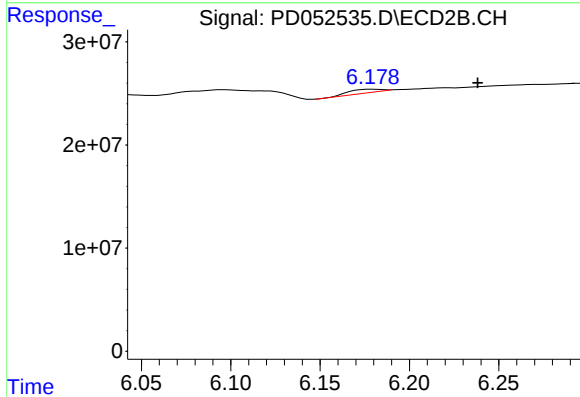


#11 cis-Chlordane

R.T.: 6.179 min
Delta R.T.: -0.059 min
Response: 4079862
Conc: 0.11 ng/ml

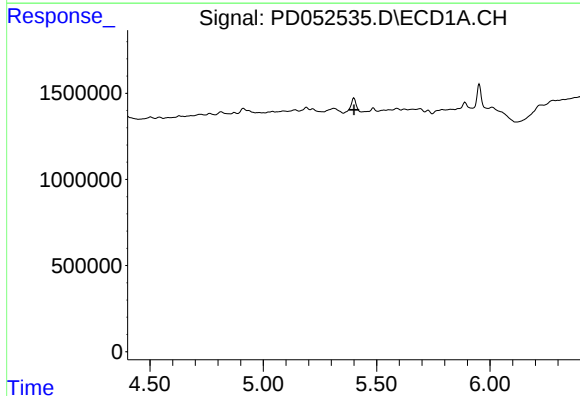


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

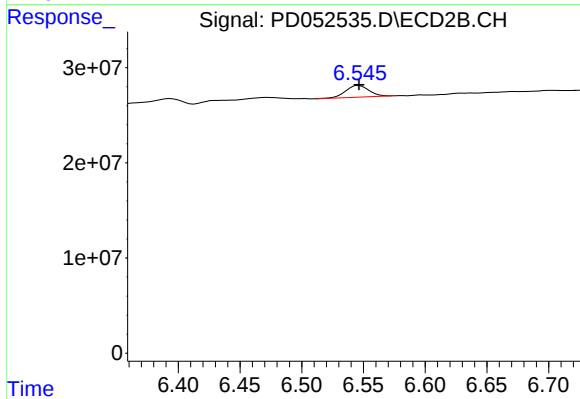

#13 Dieldrin


R.T.: 6.546 min
Delta R.T.: 0.000 min
Response: 15875605
Conc: 0.46 ng/ml

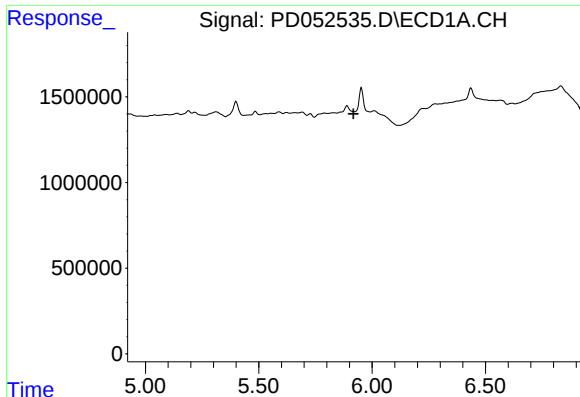

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5G5

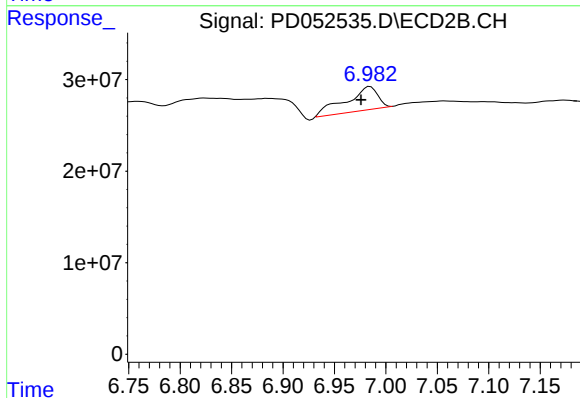


#15 Endosulfan II

R.T.: 6.985 min
Delta R.T.: 0.009 min
Response: 55062777
Conc: 1.93 ng/ml

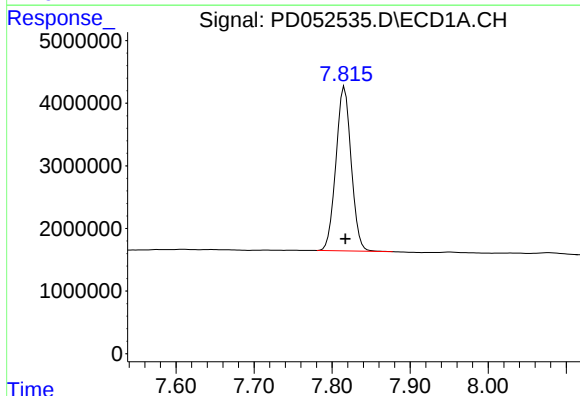

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: 0.000 min
Response: 35606538
Conc: 23.70 ng/ml

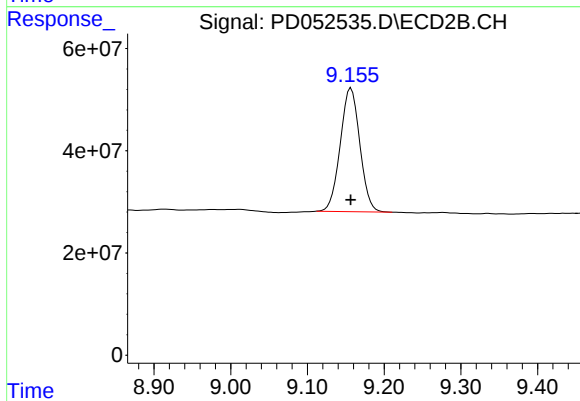

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 430280432
Conc: 22.13 ng/ml